

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
 Data File : PL047623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 17:39
 Operator : AJ\SJ
 Sample : K2515-07
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:07:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.331	3.940	215.1E6	56725008	24.248	21.250
28) SA Decachlor...	8.003	8.973	166.3E6	52306600	16.464	17.231
Target Compounds						
2) A alpha-BHC	0.000	4.301f	0	1359222	N.D.	0.365 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
Data File : PL047623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 17:39
Operator : AJ\SJ
Sample : K2515-07
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:07:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

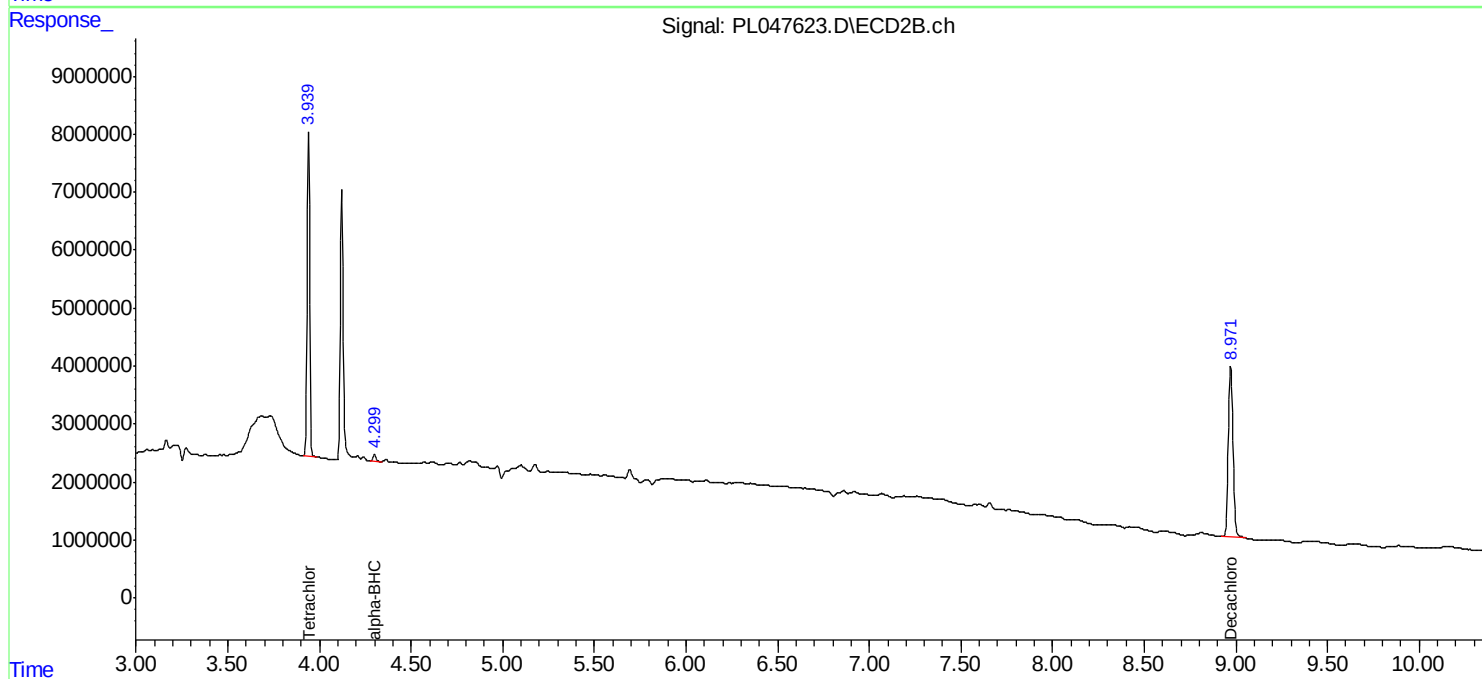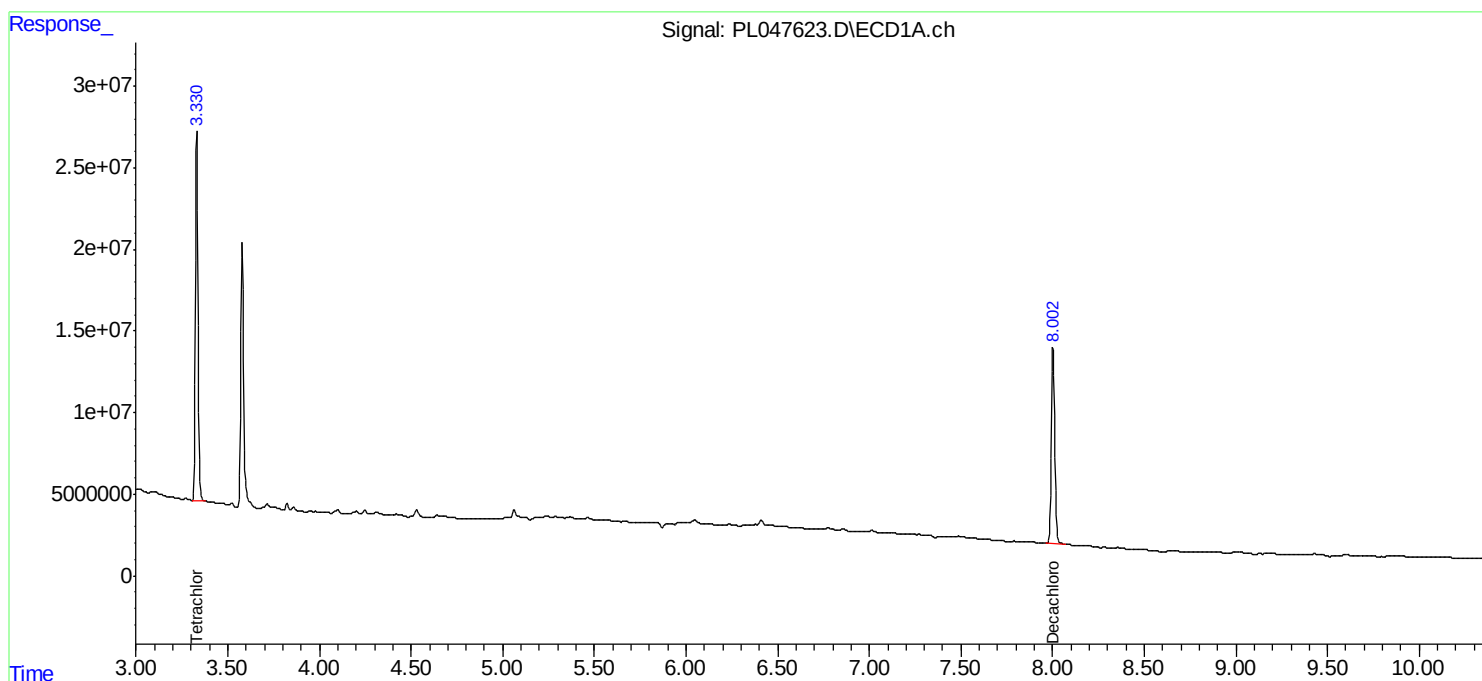


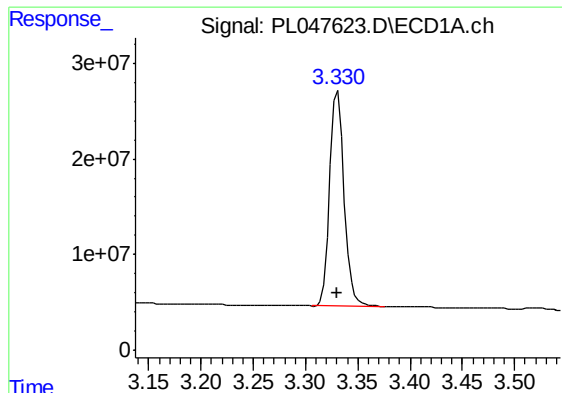

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 215144316
Conc: 24.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10

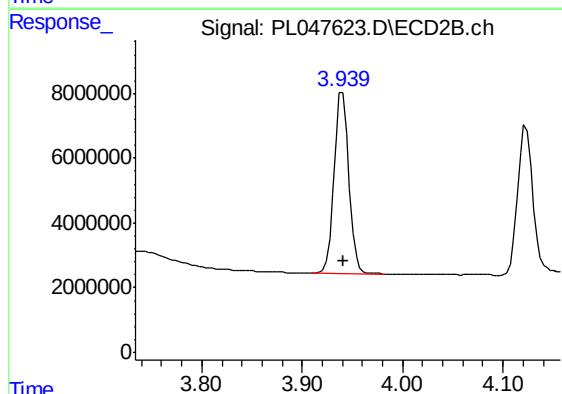


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 56725008
Conc: 21.25 ng/ml

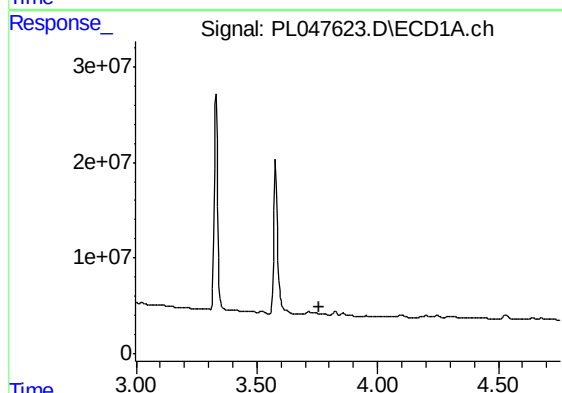


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.759 min
Response: 0
Conc: N.D.

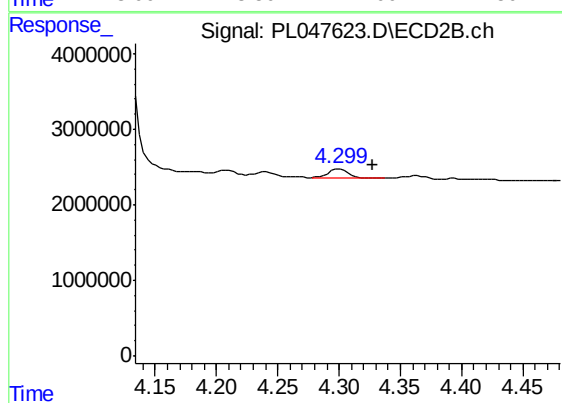

#2 alpha-BHC


R.T.: 4.301 min
Delta R.T.: -0.027 min
Response: 1359222
Conc: 0.37 ng/ml

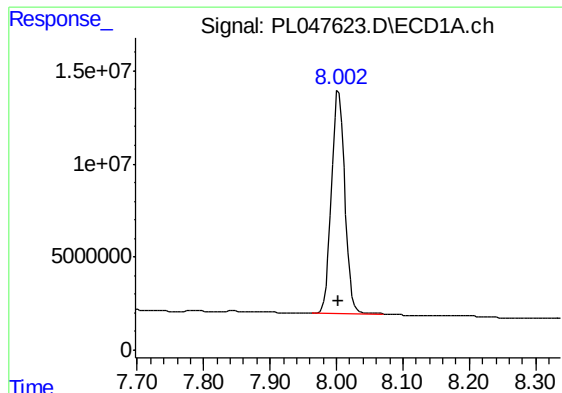

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 166314767
Conc: 16.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-10

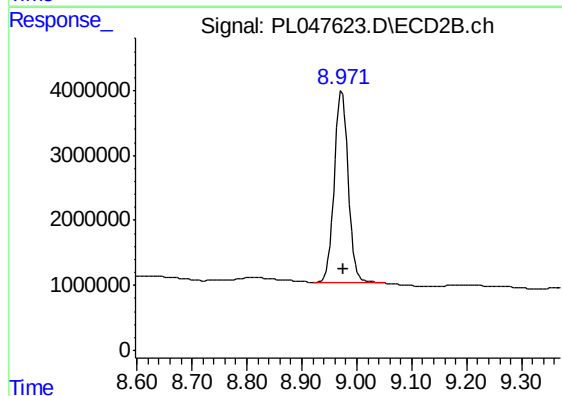

#28 Decachlorobiphenyl

R.T.: 8.973 min
Delta R.T.: -0.002 min
Response: 52306600
Conc: 17.23 ng/ml