

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
 Data File : PL047629.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2019 19:09
 Operator : AJ\SJ
 Sample : K2515-23
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: 05 Apr 23 01:09:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.331	3.940	105.9E6	28992507	11.930	10.861
28)	SA Decachlor...	8.004	8.974	110.9E6	32648093	10.982	10.755
Target Compounds							
11)	B alpha-Chl...	0.000	6.111	0	1432637	N.D.	0.448 #
26)	Chlordane-4	0.000	6.111	0	1432637	N.D.	3.033 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042219\
Data File : PL047629.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2019 19:09
Operator : AJ\SJ
Sample : K2515-23
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:09:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

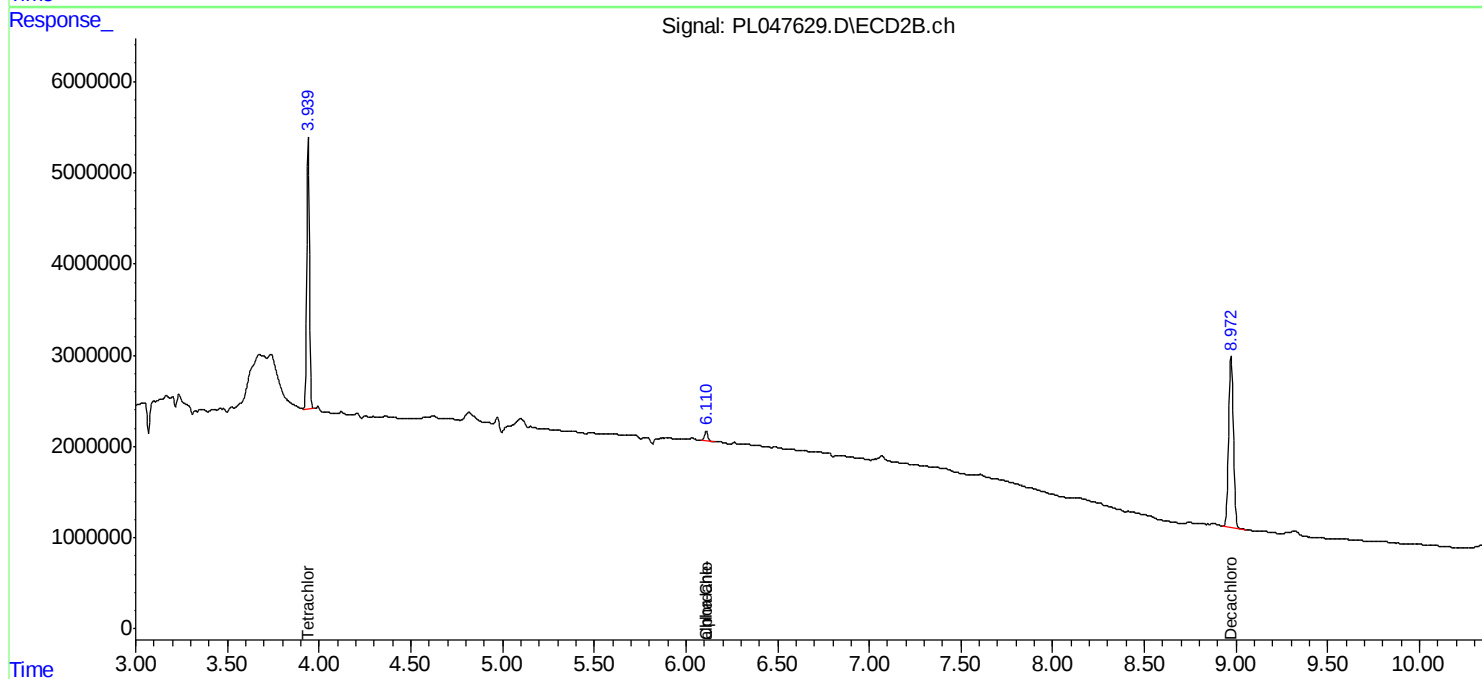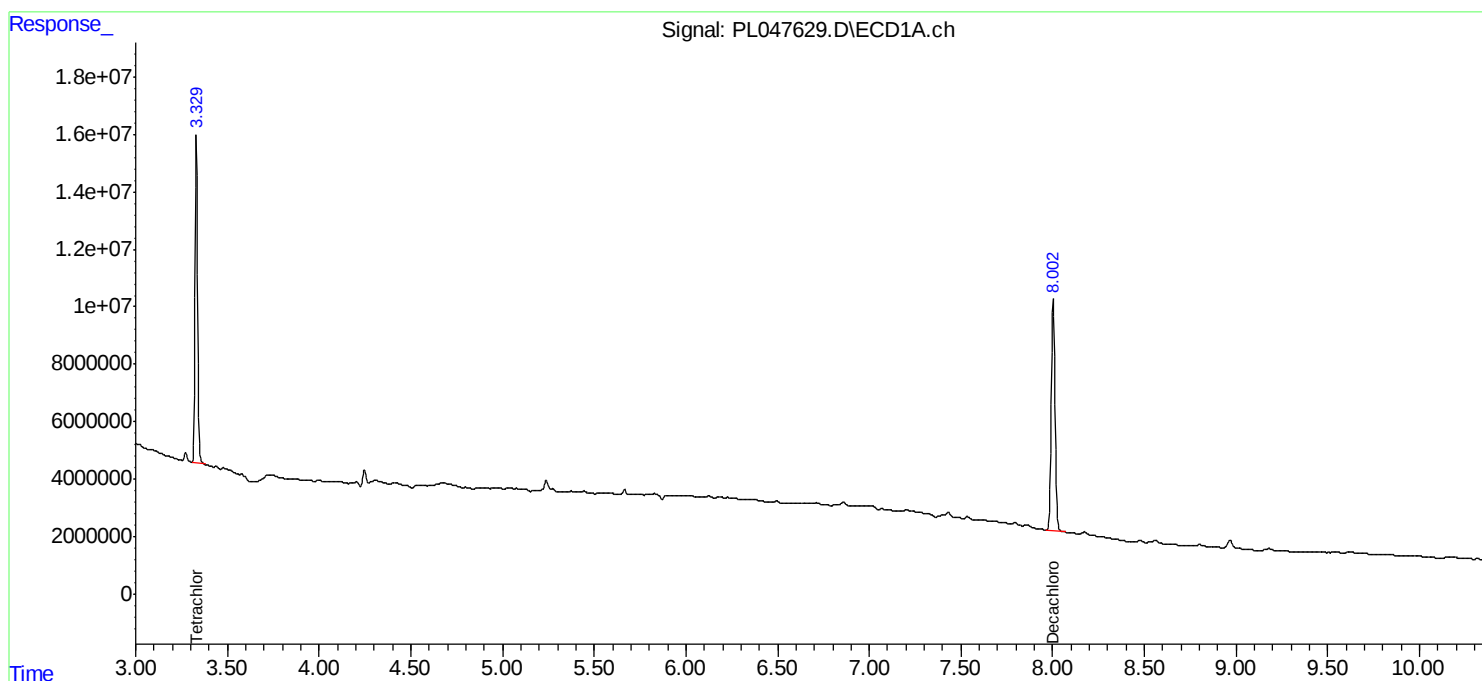


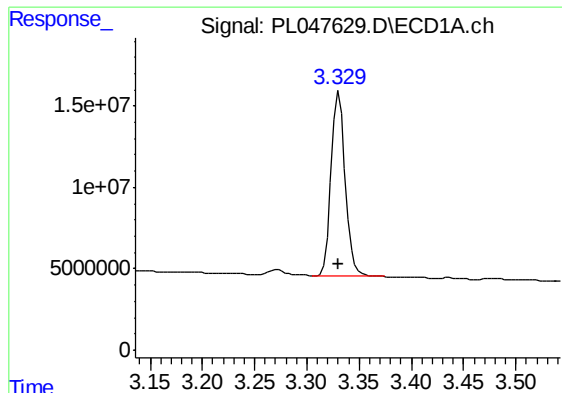

#1 Tetrachloro-m-xylene


R.T.: 3.331 min
Delta R.T.: 0.000 min
Response: 105853815
Conc: 11.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-16

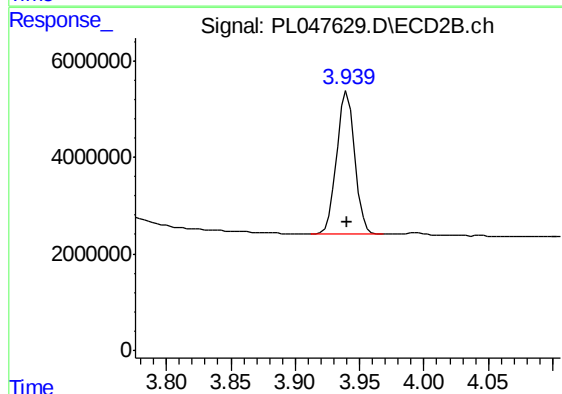


#1 Tetrachloro-m-xylene

R.T.: 3.940 min
Delta R.T.: 0.000 min
Response: 28992507
Conc: 10.86 ng/ml

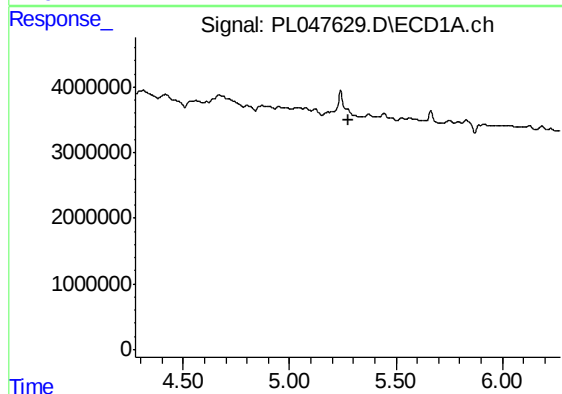


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.276 min
Response: 0
Conc: N.D.

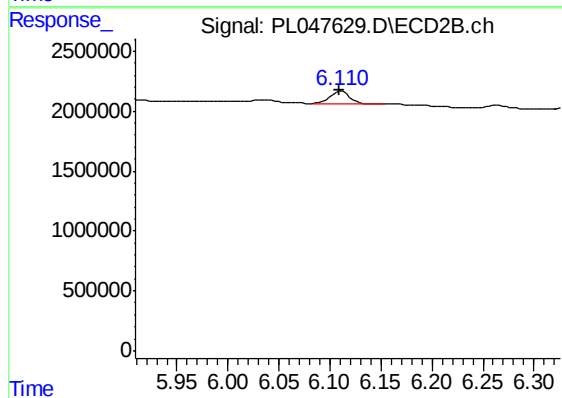

#11 alpha-Chlordane


R.T.: 6.111 min
Delta R.T.: 0.002 min
Response: 1432637
Conc: 0.45 ng/ml

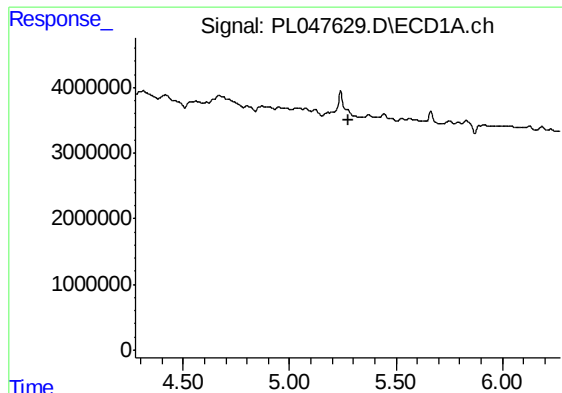

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-16

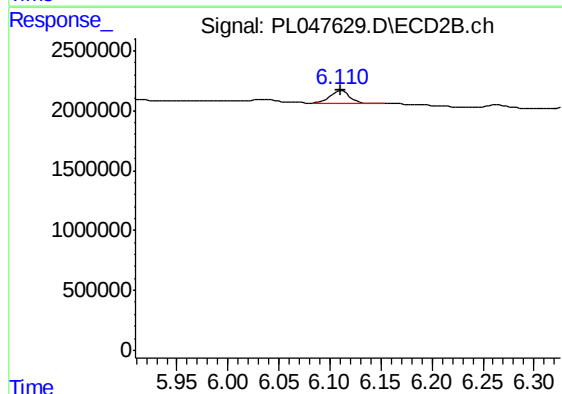


#26 Chlordane-4

R.T.: 6.111 min
Delta R.T.: 0.000 min
Response: 1432637
Conc: 3.03 ng/ml

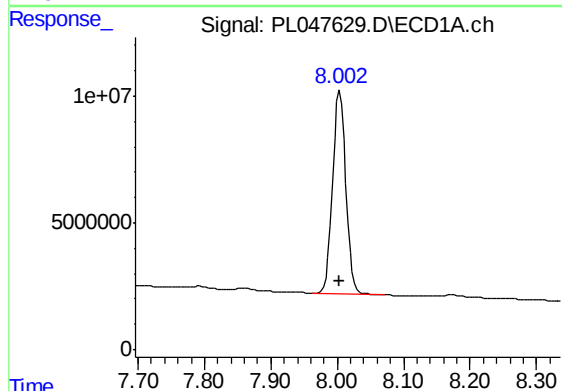

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 110934455
Conc: 10.98 ng/ml

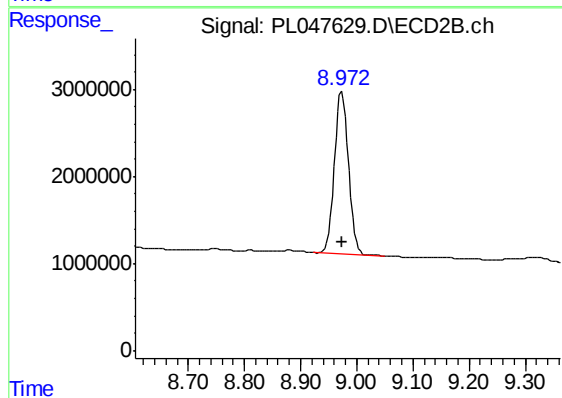

#28 Decachlorobiphenyl

R.T.: 8.974 min
Delta R.T.: -0.001 min
Response: 32648093
Conc: 10.76 ng/ml