

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
 Data File : PL058301.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 15:55
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:55:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.955	233.4E6	49250732	23.149	22.695
28)	SA Decachlor...	8.207	8.978	237.6E6	48808114	23.048	21.850
Target Compounds							
4)	MA Heptachlor	0.000	5.138	0	4920498	N.D.	1.466 #
6)	B beta-BHC	0.000	4.823f	0	623405	N.D.	0.449 #
8)	B Heptachlo...	5.189f	5.812	152843	15655463	0.011	5.798 #
14)	MA Endrin	6.014	0.000	5553357	0	0.476	N.D. #
15)	B Endosulfa...	6.253f	6.868f	5218059	1075764	0.472	0.415
16)	A 4,4'-DDD	6.135	0.000	996968	0	0.100	N.D. #
24)	Chlordane-2	4.827	0.000	7439351	0	18.427	N.D. #
27)	Chlordane-5	6.311f	0.000	9356189	0	24.734	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
Data File : PL058301.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 15:55
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:55:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

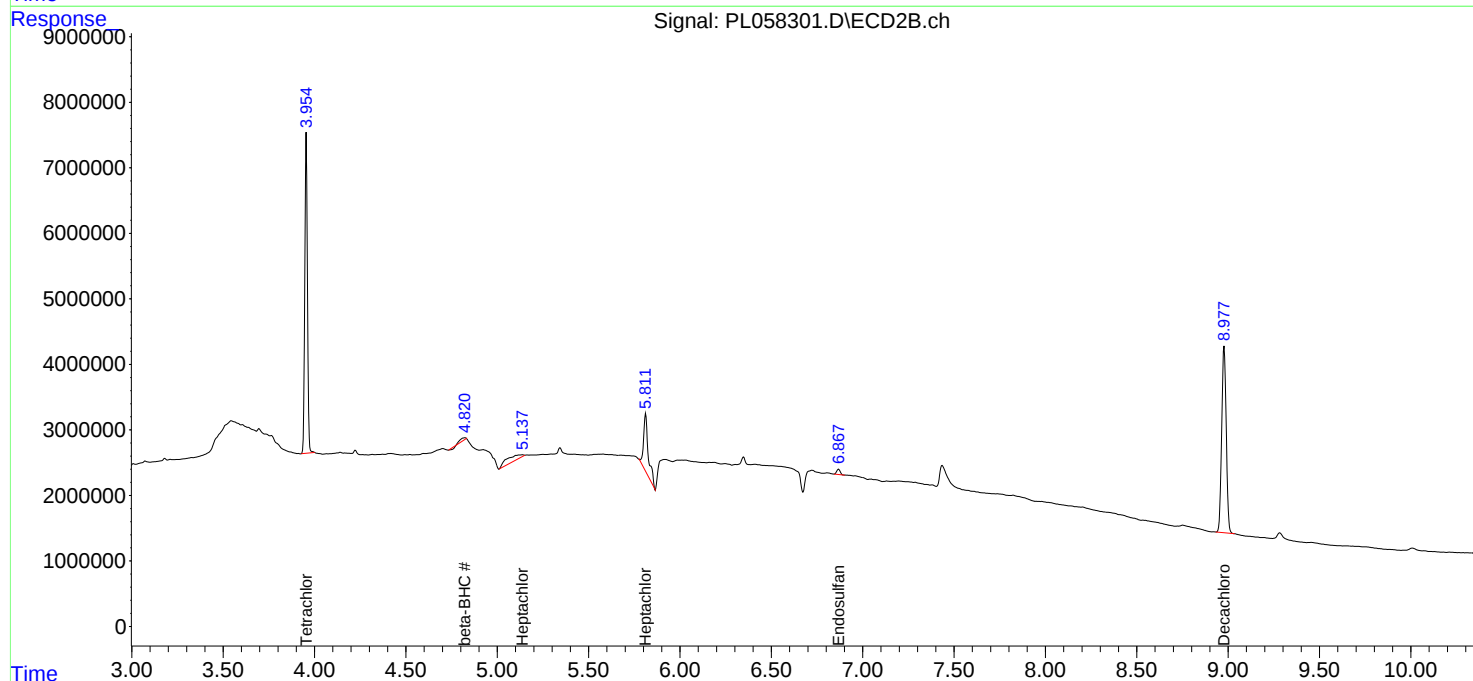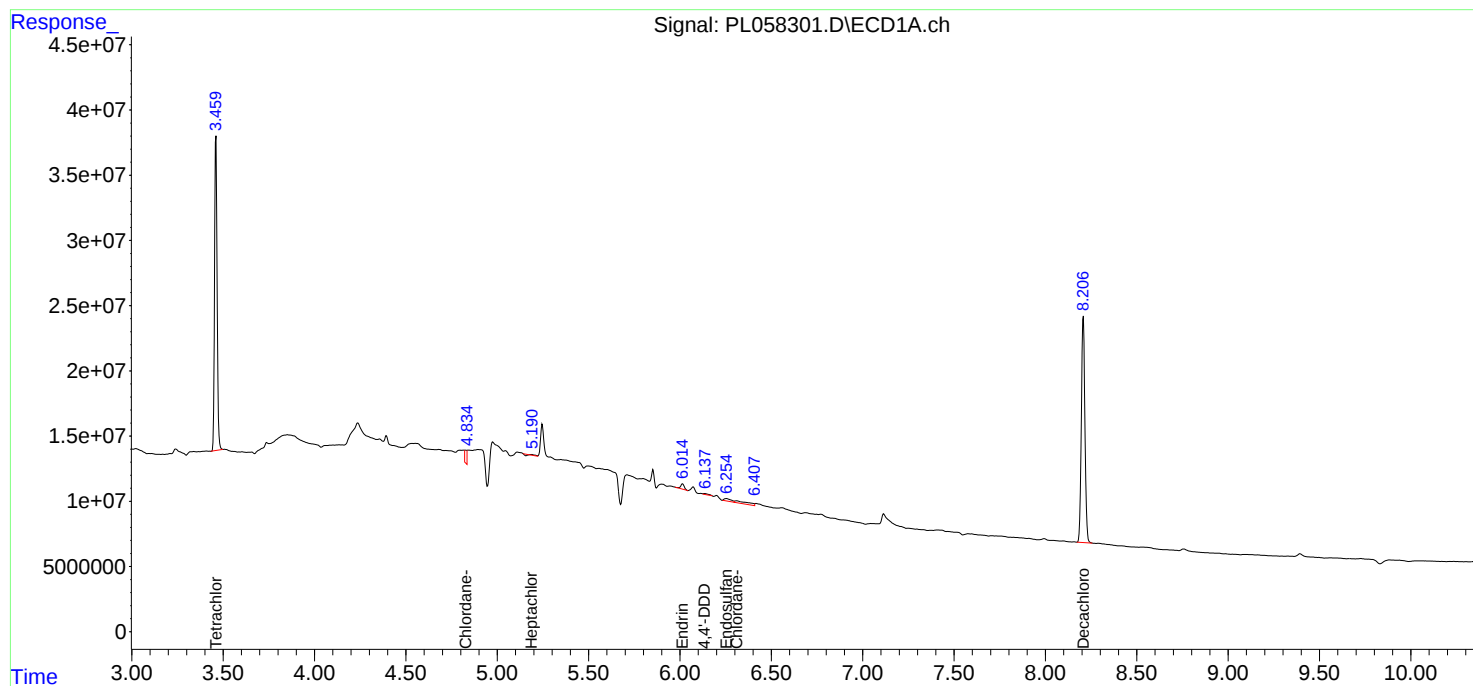


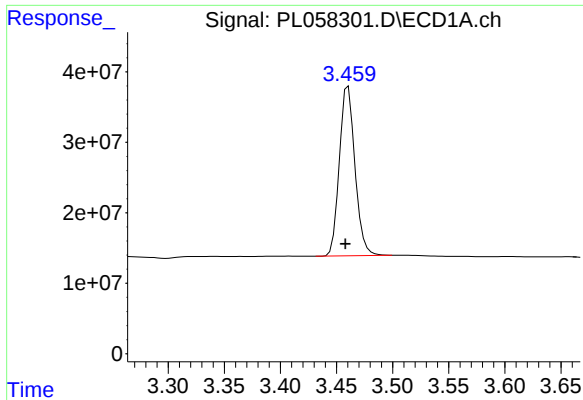

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.002 min
Response: 233362742
Conc: 23.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

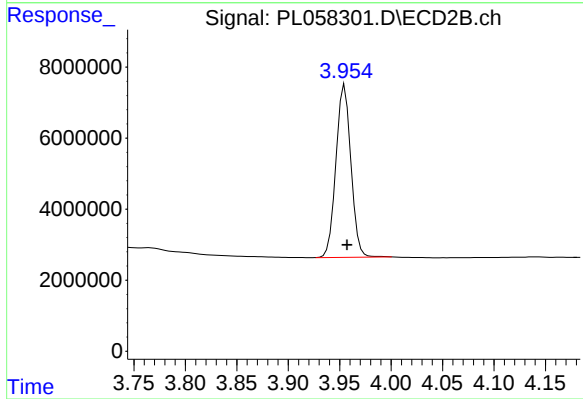


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 49250732
Conc: 22.69 ng/ml

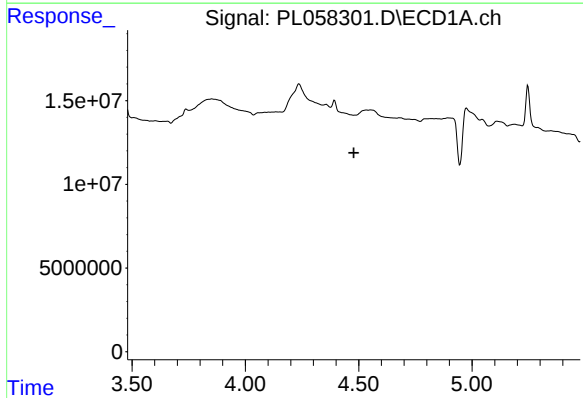


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.479 min
Response: 0
Conc: N.D.

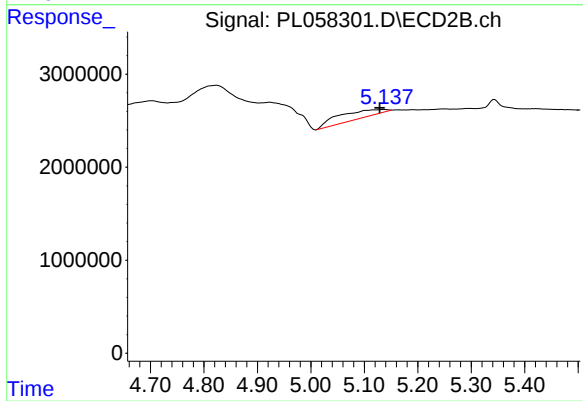

#4 Heptachlor


R.T.: 5.138 min
Delta R.T.: 0.009 min
Response: 4920498
Conc: 1.47 ng/ml

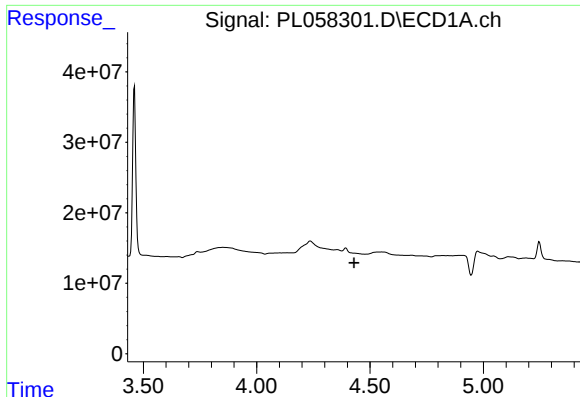

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

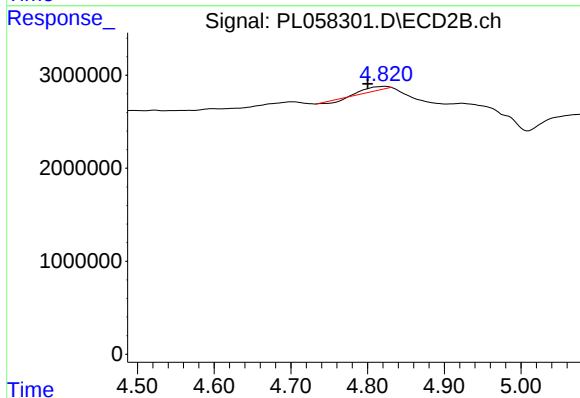


#6 beta-BHC

R.T.: 4.823 min
Delta R.T.: 0.023 min
Response: 623405
Conc: 0.45 ng/ml

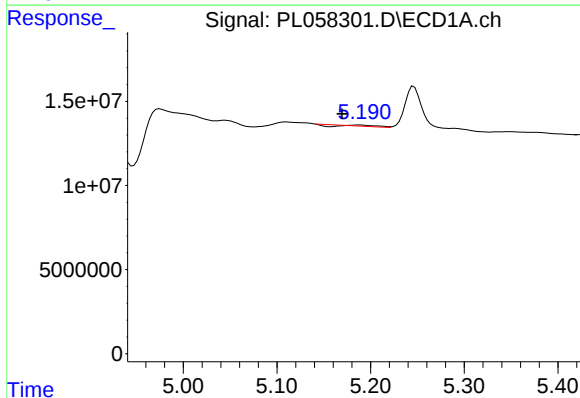


#8 Heptachlor epoxide

R.T.: 5.189 min
Delta R.T.: 0.020 min
Response: 152843
Conc: 0.01 ng/ml

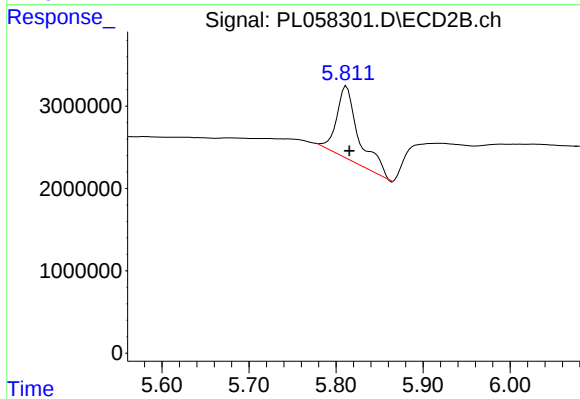

#8 Heptachlor epoxide


R.T.: 5.812 min
Delta R.T.: -0.003 min
Response: 15655463
Conc: 5.80 ng/ml

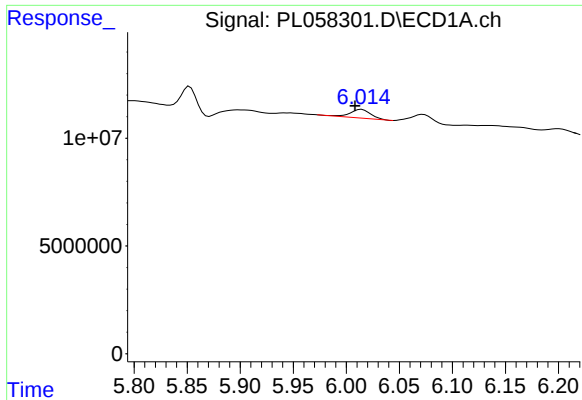

#14 Endrin


R.T.: 6.014 min
Delta R.T.: 0.006 min
Response: 5553357
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

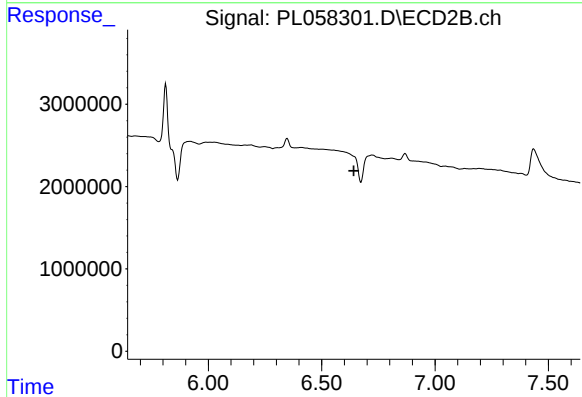


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.642 min
Response: 0
Conc: N.D.

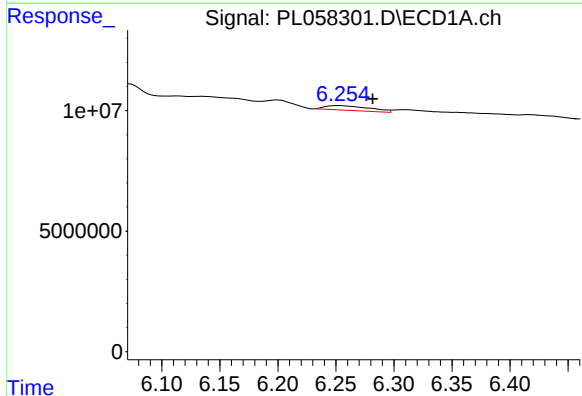


#15 Endosulfan II

R.T.: 6.253 min
Delta R.T.: -0.029 min
Response: 5218059
Conc: 0.47 ng/ml

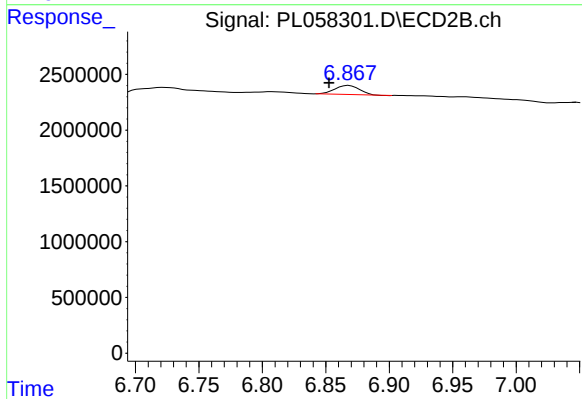

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.016 min
Response: 1075764
Conc: 0.41 ng/ml

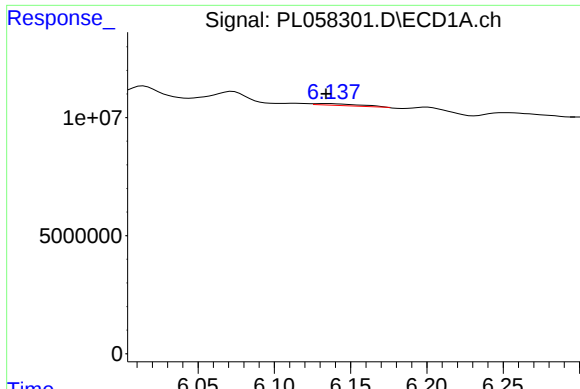

#16 4,4'-DDD


R.T.: 6.135 min
Delta R.T.: 0.001 min
Response: 996968
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

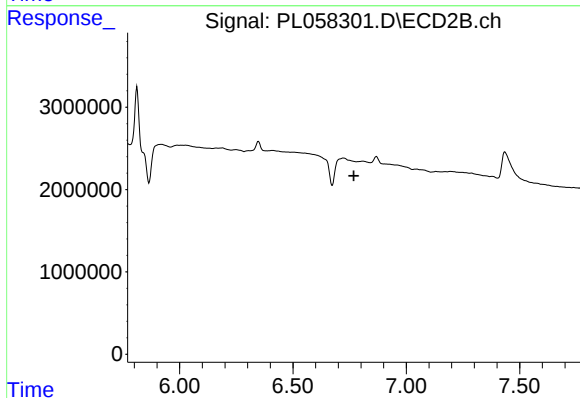


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.769 min
Response: 0
Conc: N.D.

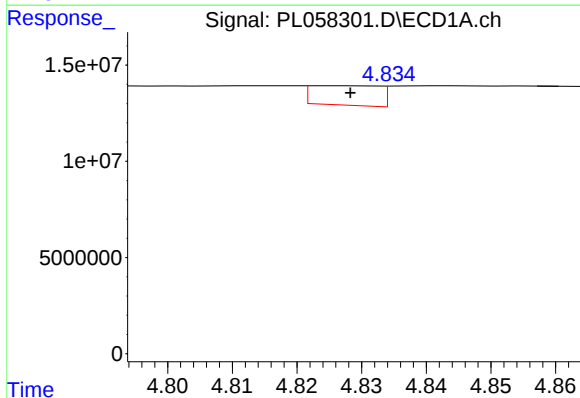


#24 Chlordane-2

R.T.: 4.827 min
Delta R.T.: -0.001 min
Response: 7439351
Conc: 18.43 ng/ml

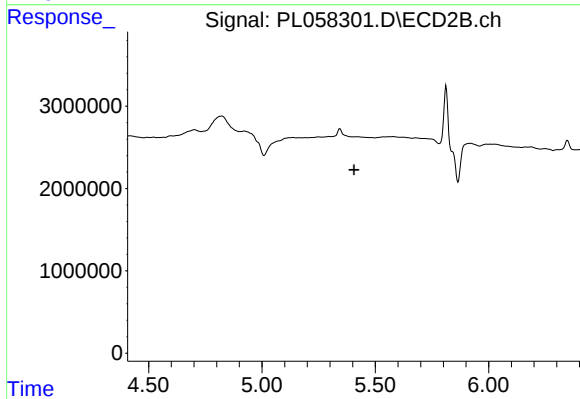

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

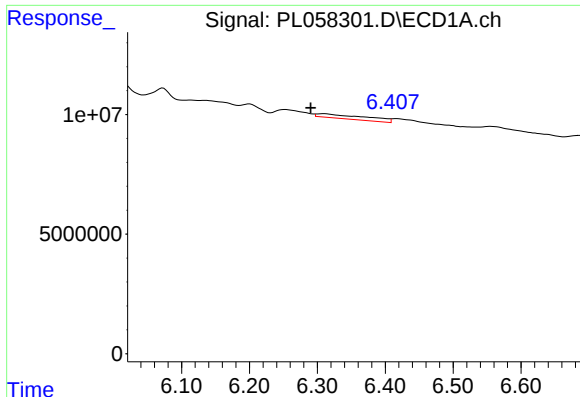

#27 Chlordane-5


R.T.: 6.311 min
Delta R.T.: 0.021 min
Response: 9356189
Conc: 24.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

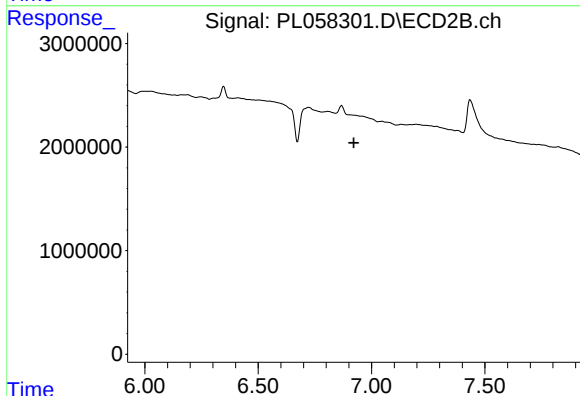


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

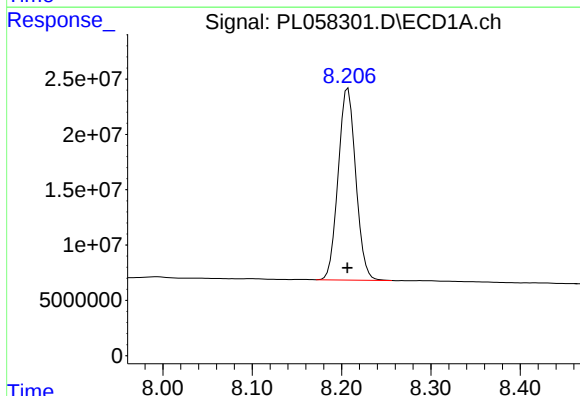

#28 Decachlorobiphenyl

R.T.: 8.207 min
Delta R.T.: 0.000 min
Response: 237593494
Conc: 23.05 ng/ml

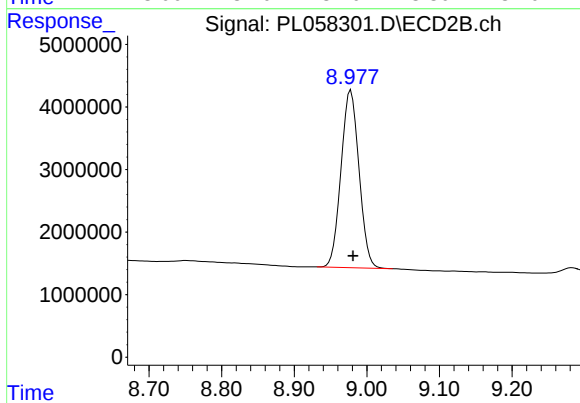

#28 Decachlorobiphenyl

R.T.: 8.978 min
Delta R.T.: -0.003 min
Response: 48808114
Conc: 21.85 ng/ml