

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
 Data File : PL058314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 19:42
 Operator : AJ\MA
 Sample : L2330-17
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PA-TWP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:59:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.954	185.1E6	40378394	18.365	18.606
28)	SA Decachlor...	8.202	8.976	175.3E6	38859365	17.007	17.396
Target Compounds							
3)	MA gamma-BHC...	4.180	0.000	1128607	0	0.078	N.D. #
4)	MA Heptachlor	0.000	5.134	0	650798	N.D.	0.194 #
5)	MB Aldrin	4.705f	0.000	2820906	0	0.192	N.D. #
7)	B delta-BHC	0.000	4.986f	0	4458150	N.D.	3.736 #
15)	B Endosulfa...	0.000	6.867	0	410911	N.D.	0.158 #
19)	B Endosulfa...	6.665	0.000	1042044	0	0.103	N.D. #
20)	A Methoxychlor	6.917	0.000	631584	0	0.115	N.D. #
21)	B Endrin ke...	7.138f	0.000	1104518	0	0.099	N.D. #
22)	Mirex	7.317f	0.000	1509612	0	0.184	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
Data File : PL058314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 19:42
Operator : AJ\MA
Sample : L2330-17
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PA-TWP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:59:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

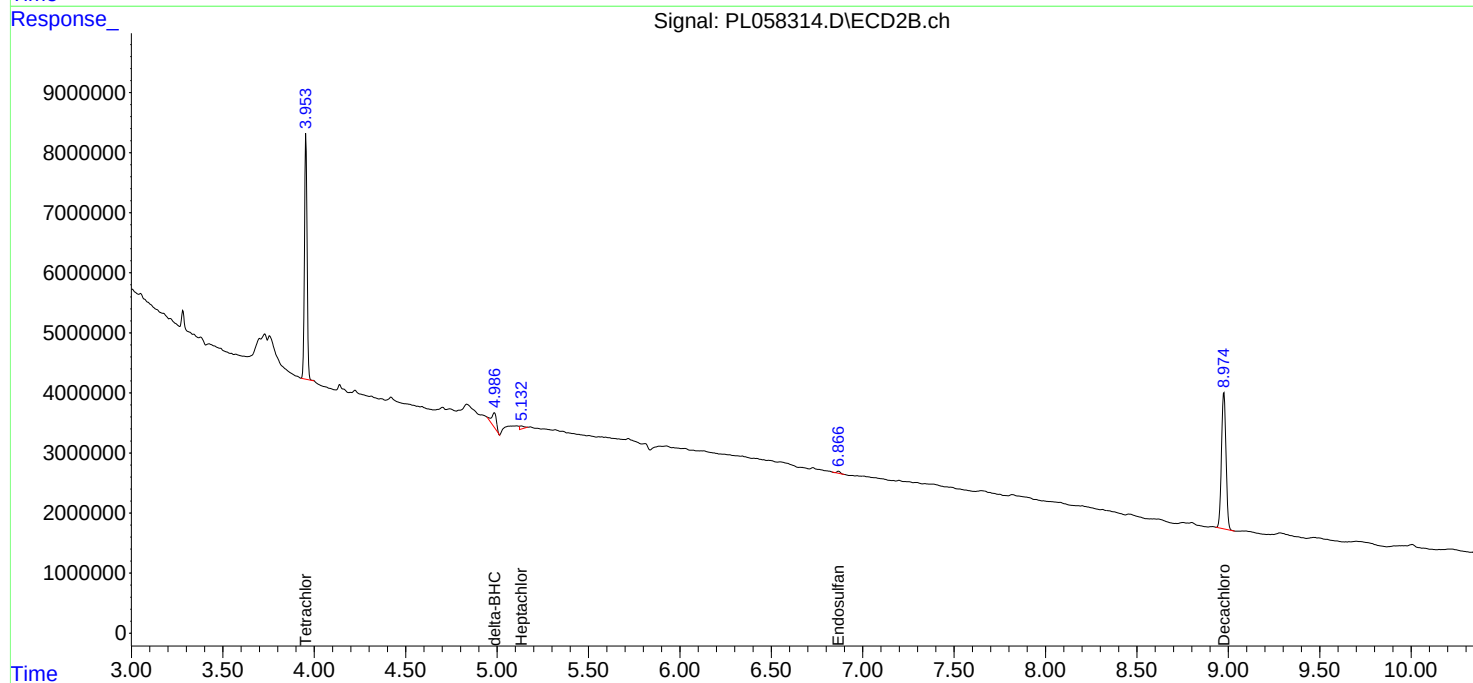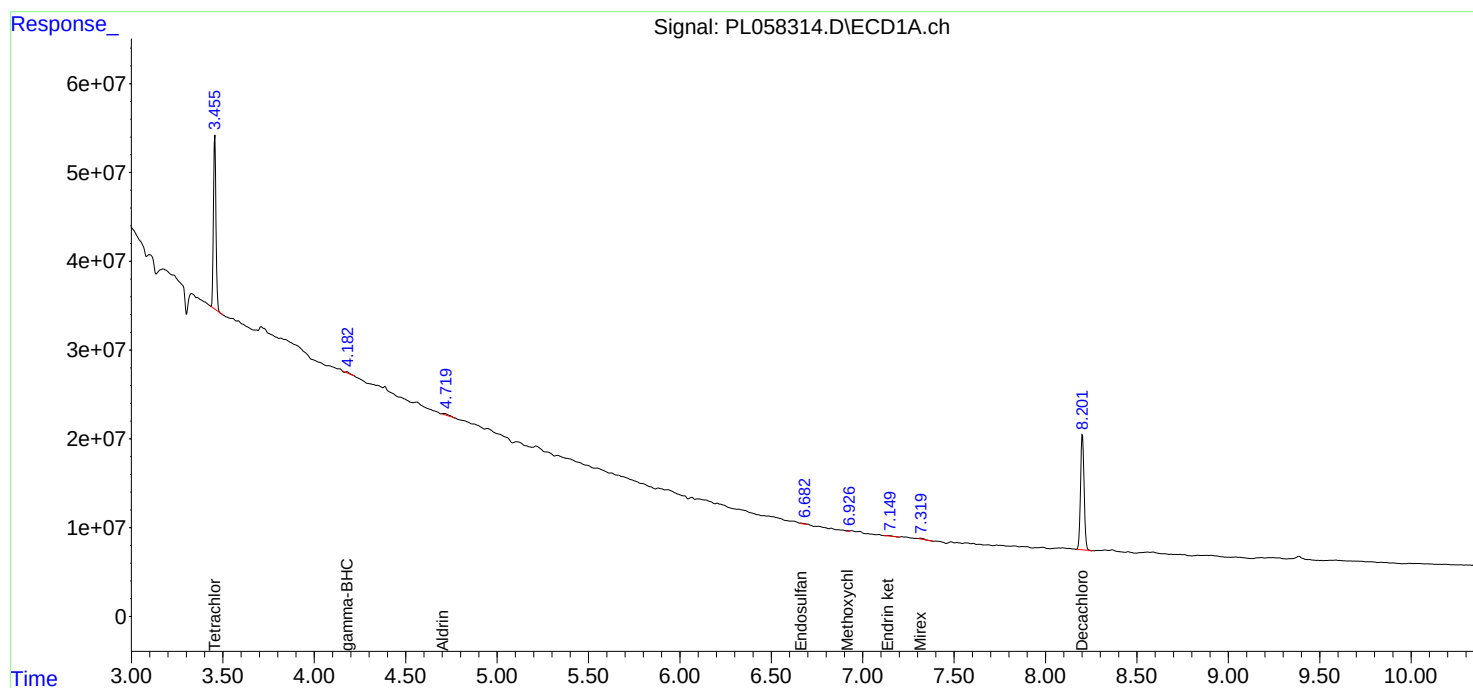


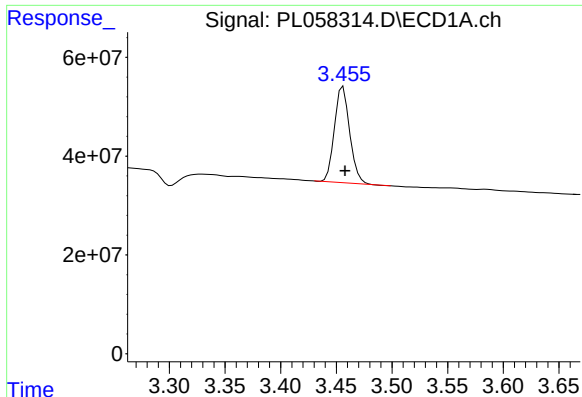

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 185138769
Conc: 18.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

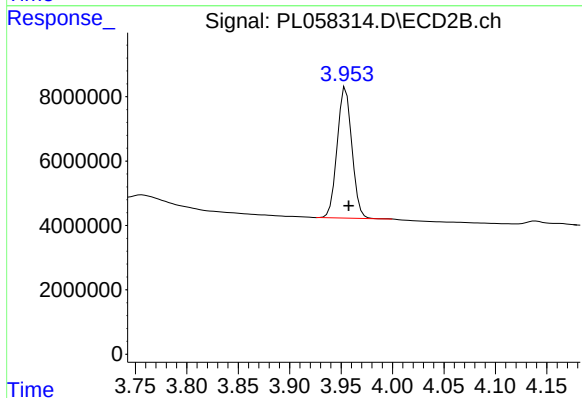


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 40378394
Conc: 18.61 ng/ml

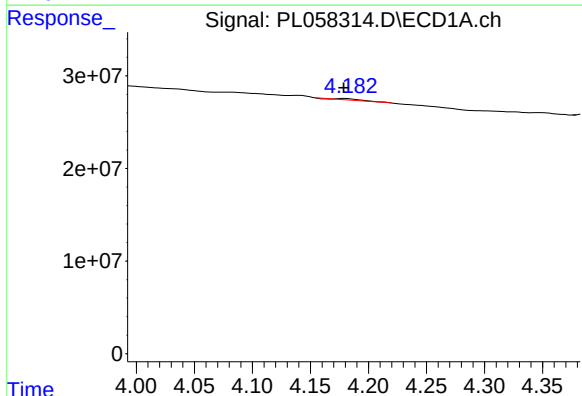


#3 gamma-BHC (Lindane)

R.T.: 4.180 min
Delta R.T.: 0.000 min
Response: 1128607
Conc: 0.08 ng/ml

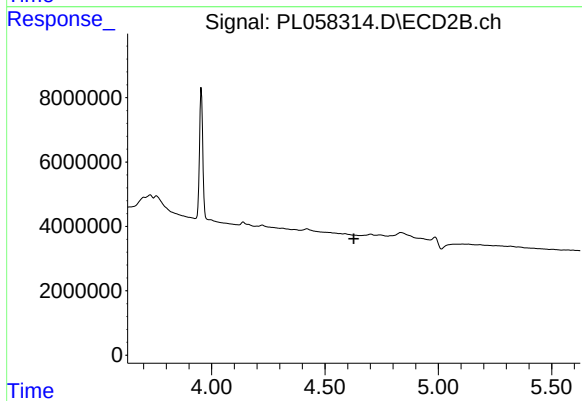

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.627 min
Response: 0
Conc: N.D.

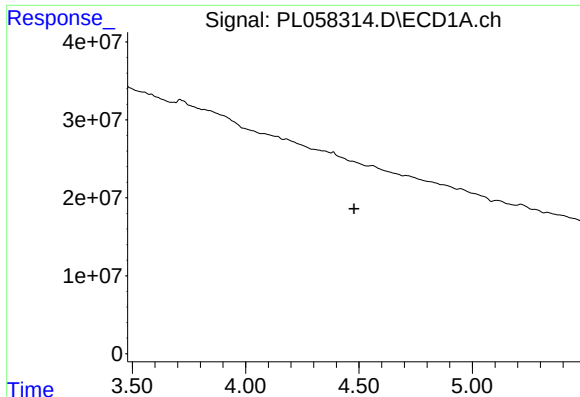

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.479 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

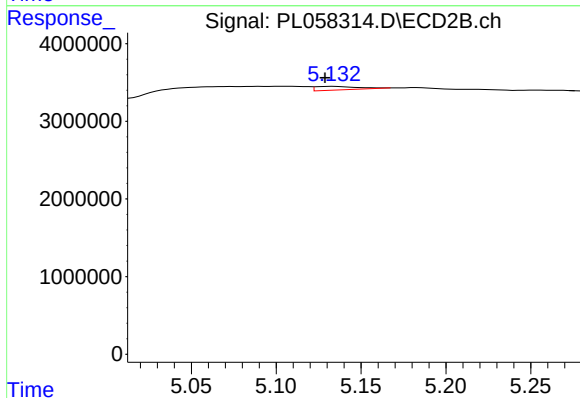


#4 Heptachlor

R.T.: 5.134 min
Delta R.T.: 0.005 min
Response: 650798
Conc: 0.19 ng/ml

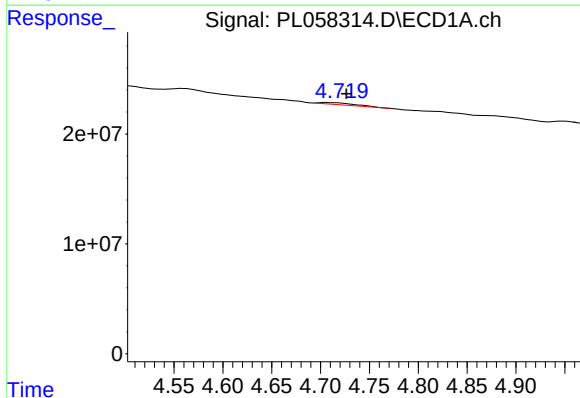


#5 Aldrin

R.T.: 4.705 min
Delta R.T.: -0.021 min
Response: 2820906
Conc: 0.19 ng/ml

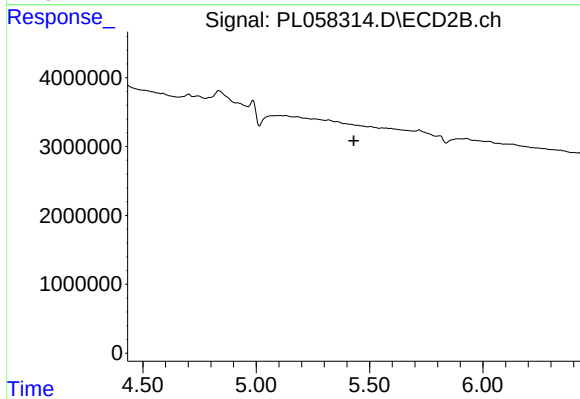

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.431 min
Response: 0
Conc: N.D.

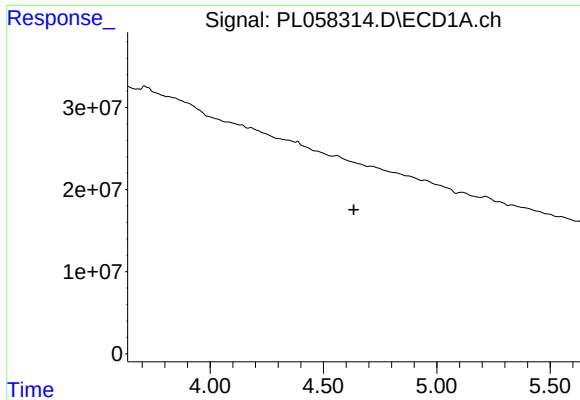

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

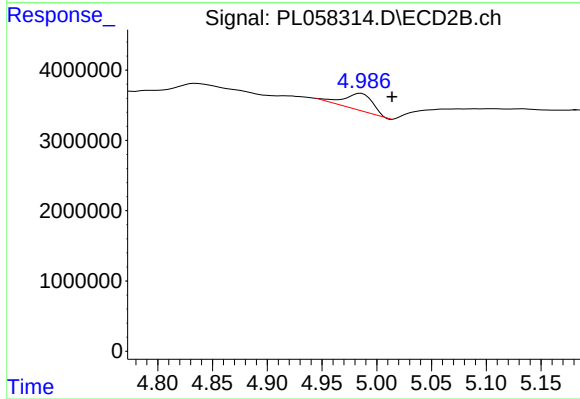


#7 delta-BHC

R.T.: 4.986 min
Delta R.T.: -0.028 min
Response: 4458150
Conc: 3.74 ng/ml

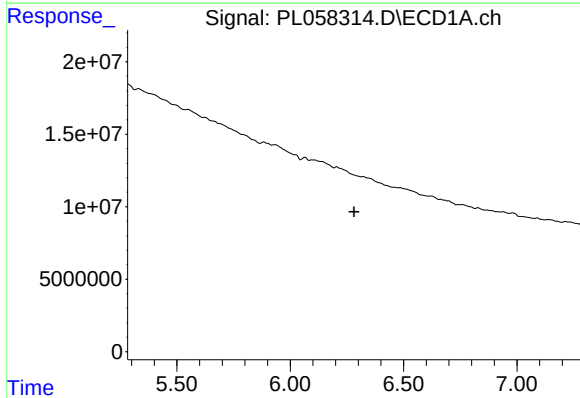


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

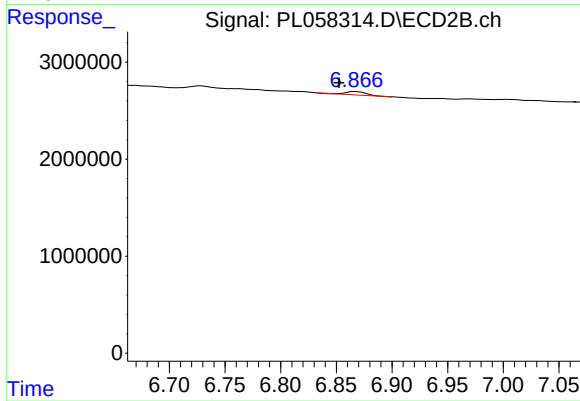

#15 Endosulfan II


R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 410911
Conc: 0.16 ng/ml

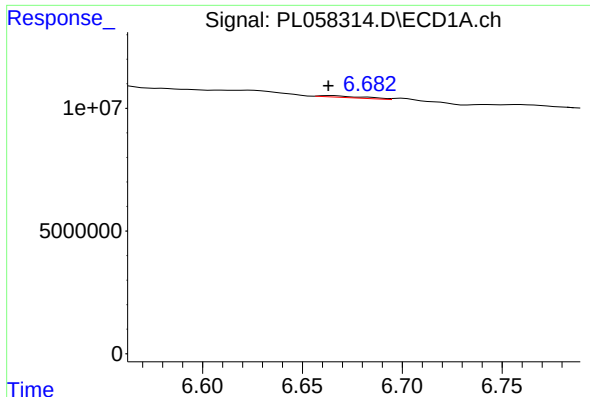

#19 Endosulfan Sulfate


R.T.: 6.665 min
Delta R.T.: 0.002 min
Response: 1042044
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

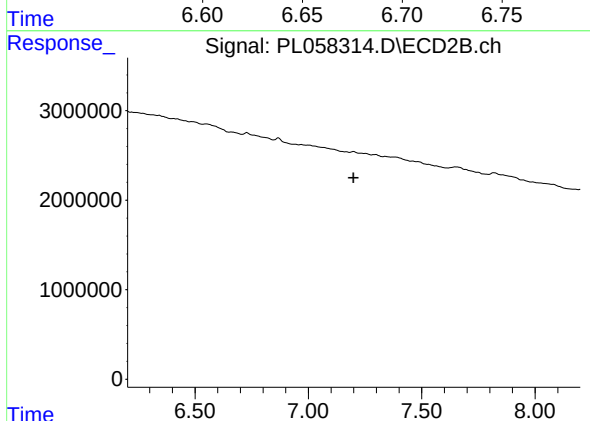


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

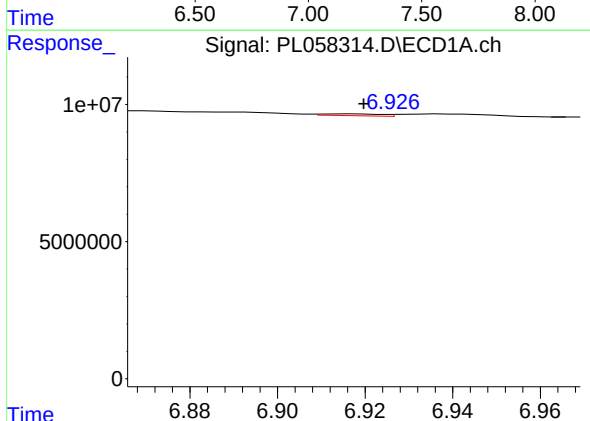


#20 Methoxychlor

R.T.: 6.917 min
Delta R.T.: -0.003 min
Response: 631584
Conc: 0.11 ng/ml

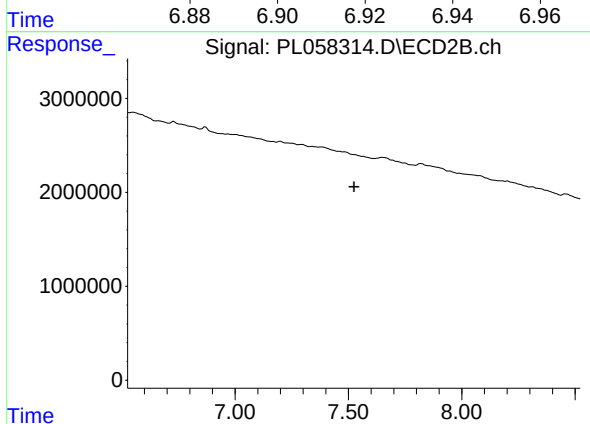

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.525 min
Response: 0
Conc: N.D.

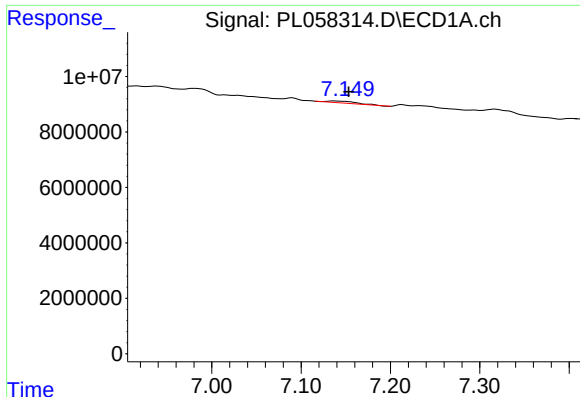

#21 Endrin ketone


R.T.: 7.138 min
Delta R.T.: -0.016 min
Response: 1104518
Conc: 0.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

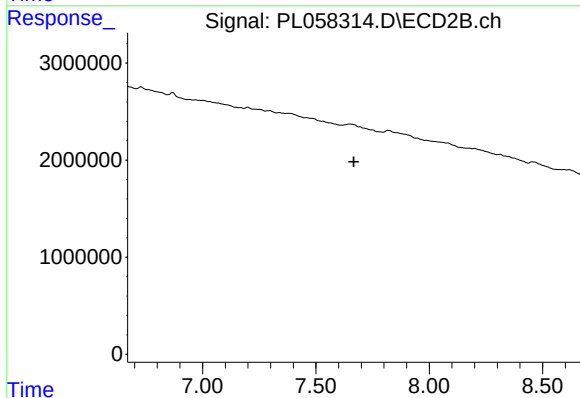


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.667 min
Response: 0
Conc: N.D.

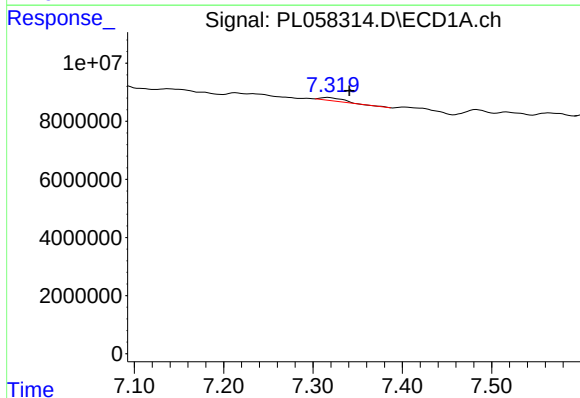


#22 Mirex

R.T.: 7.317 min
Delta R.T.: -0.024 min
Response: 1509612
Conc: 0.18 ng/ml

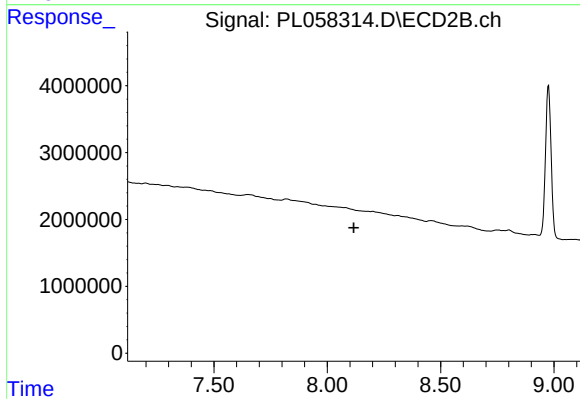

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 8.117 min
Response: 0
Conc: N.D.

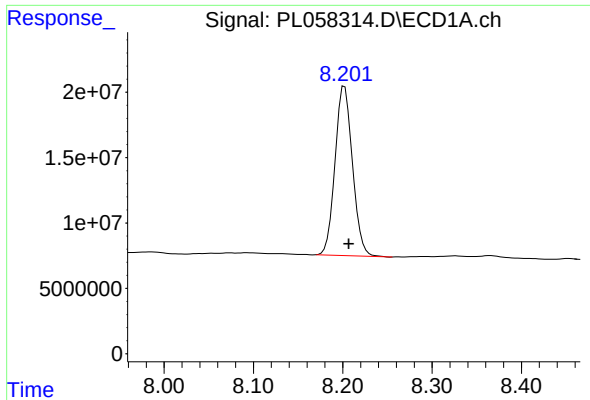

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 175315628
Conc: 17.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PA-TWP-1

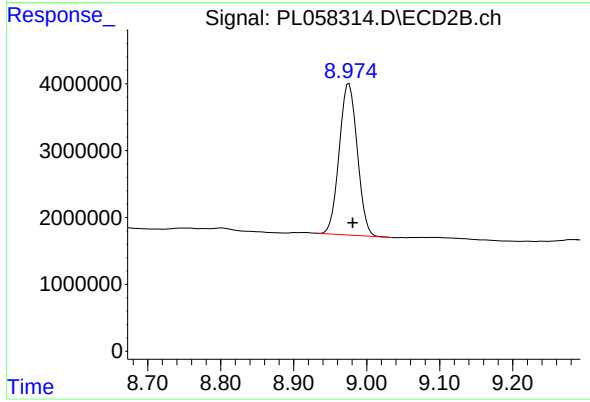

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 38859365
Conc: 17.40 ng/ml