

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
 Data File : PL058305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 17:07
 Operator : AJ\MA
 Sample : L2351-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-17A

Manual Integrations
 APPROVED

mohammad
 4/23/2020 2:14:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:56:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.954	110.0E6	23278725	10.911m	10.727
28)	SA Decachlor...	8.203	8.977	115.2E6	26345797	11.172	11.794

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
Data File : PL058305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 17:07
Operator : AJ\MA
Sample : L2351-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-17A


Manual Integrations
APPROVED

mohammad
4/23/2020 2:14:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:56:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

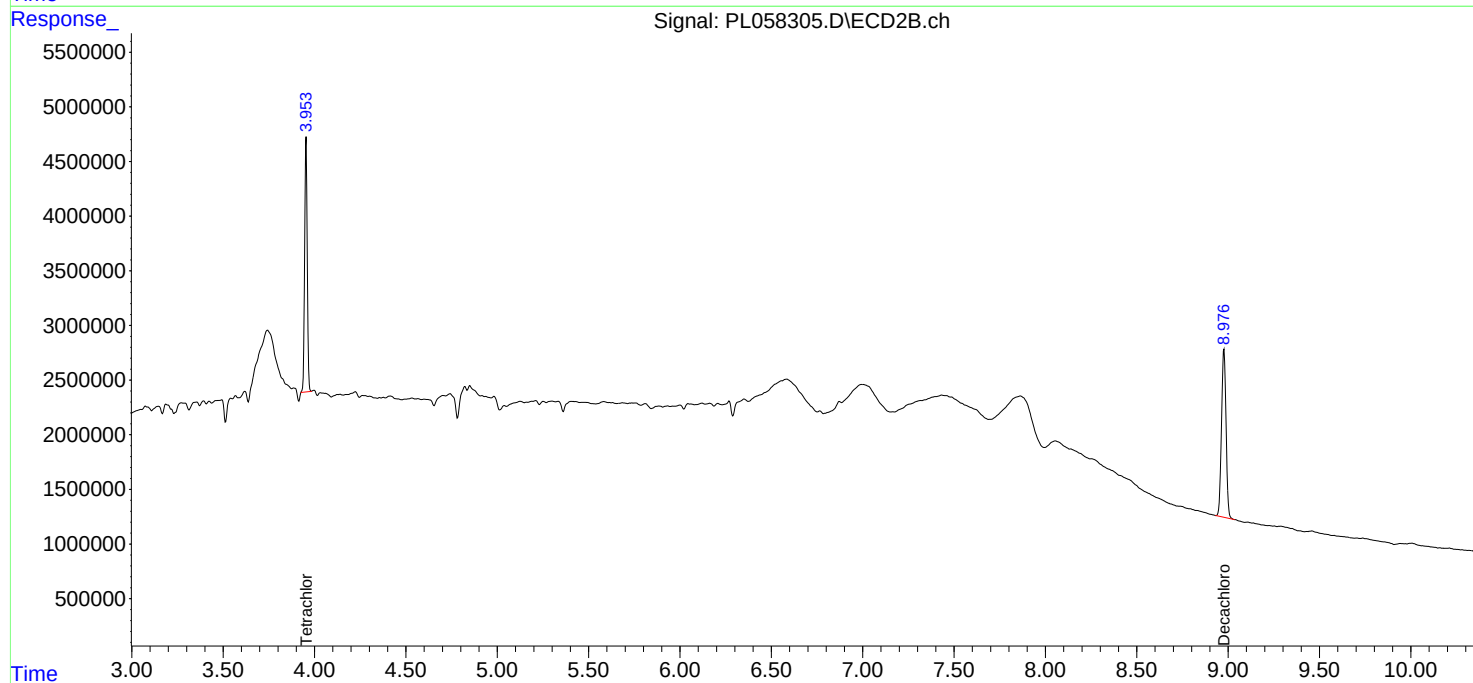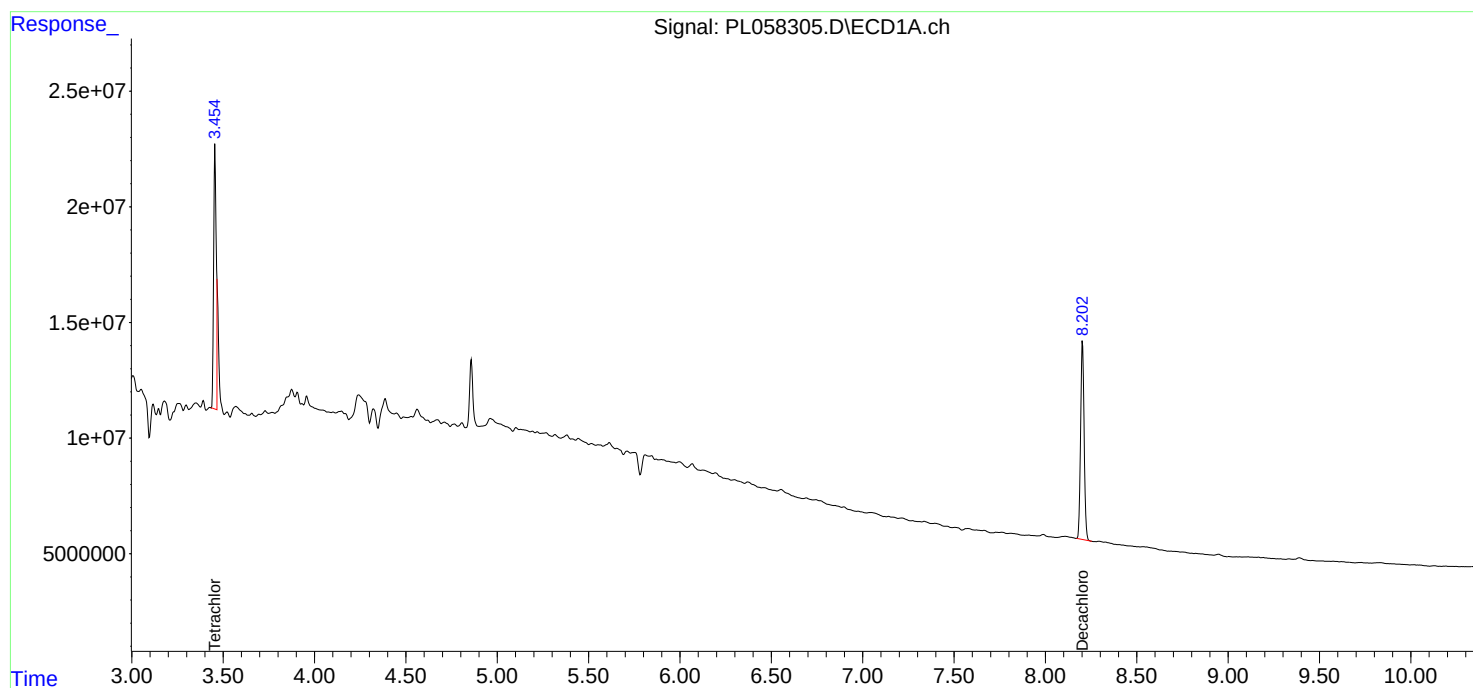

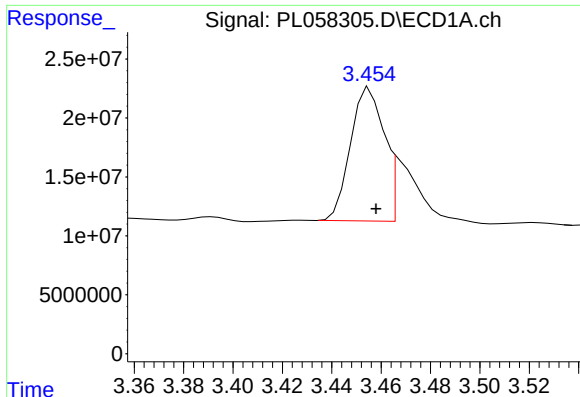


#1 Tetrachloro-m-xylene

R.T.: 3.454 min
Delta R.T.: -0.004 min
Response: 109992696
Conc: 10.91 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-17A


Manual Integrations
APPROVED

mohammad
4/23/2020 2:14:28 PM

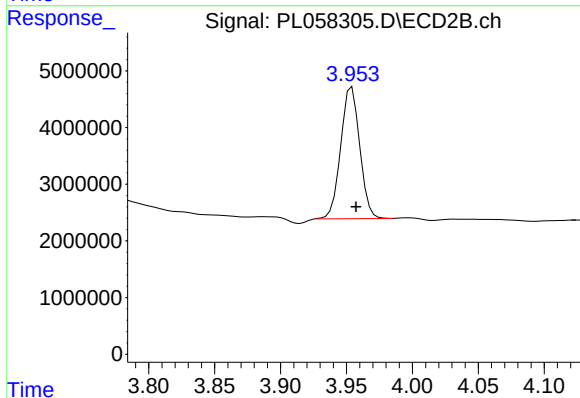


#1 Tetrachloro-m-xylene

R.T.: 3.954 min
Delta R.T.: -0.003 min
Response: 23278725
Conc: 10.73 ng/ml

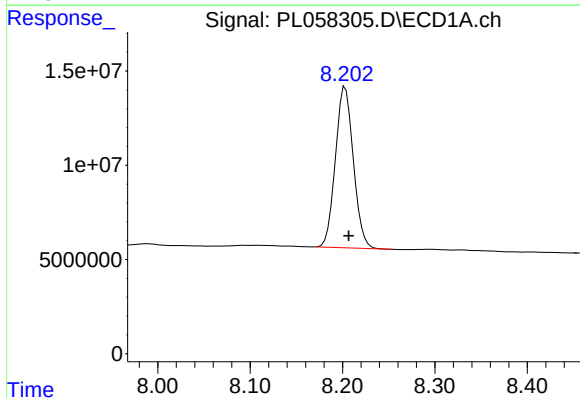

#28 Decachlorobiphenyl

R.T.: 8.203 min
Delta R.T.: -0.004 min
Response: 115163402
Conc: 11.17 ng/ml

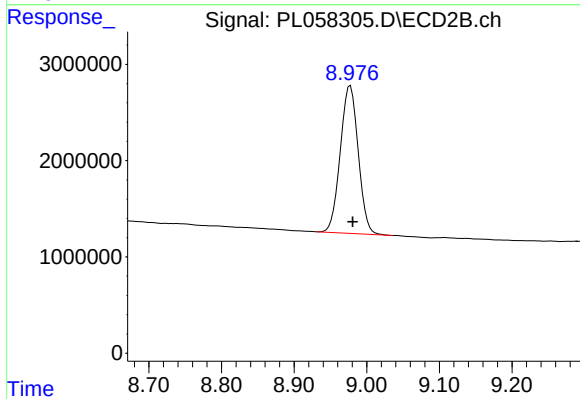

#28 Decachlorobiphenyl

R.T.: 8.977 min
Delta R.T.: -0.003 min
Response: 26345797
Conc: 11.79 ng/ml