

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
 Data File : PL058313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2020 19:28
 Operator : AJ\MA
 Sample : L2375-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-16A

Manual Integrations
 APPROVED

mohammad
 4/23/2020 2:14:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:59:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	3.953	239.7E6	14418921	23.773m	6.644m#
28)	SA Decachlor...	8.202	8.976	84439008	20354570	8.191	9.112

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042220\
Data File : PL058313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2020 19:28
Operator : AJ\MA
Sample : L2375-02
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-16A


Manual Integrations
APPROVED

mohammad
4/23/2020 2:14:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:59:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

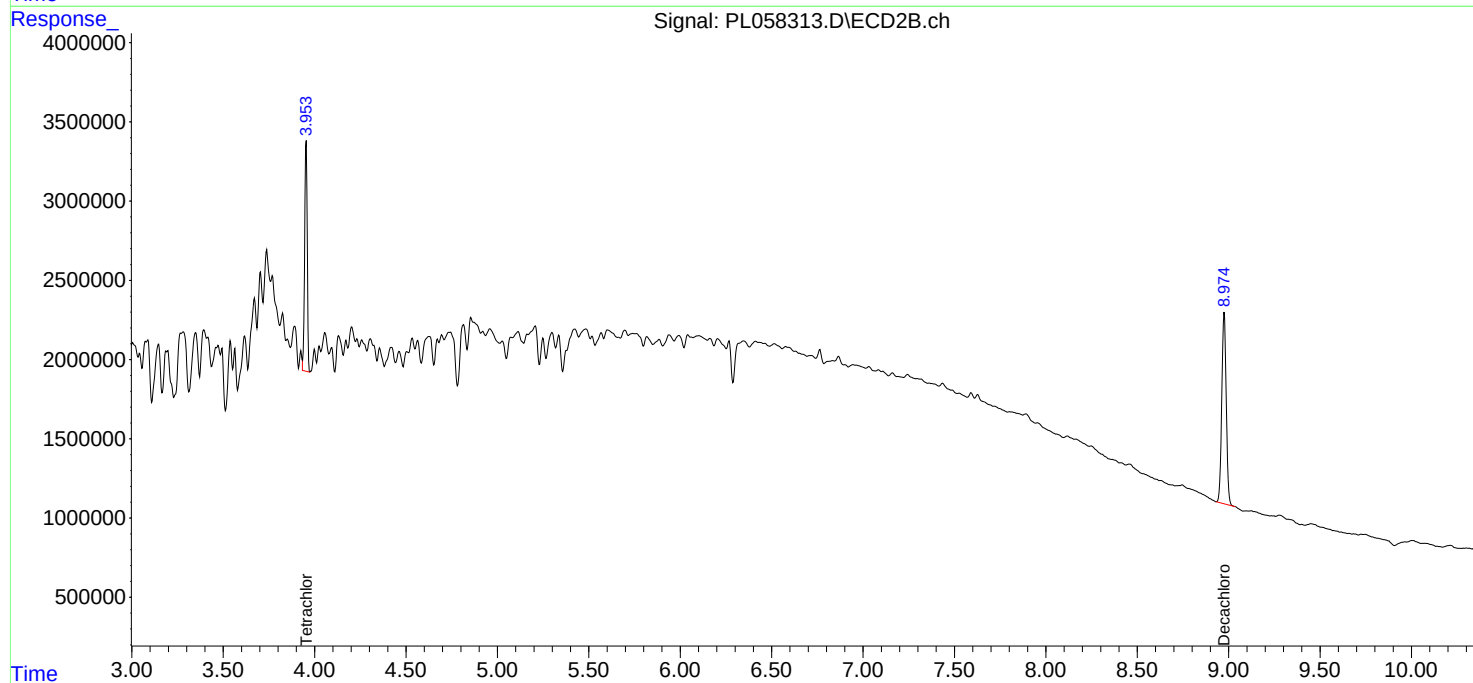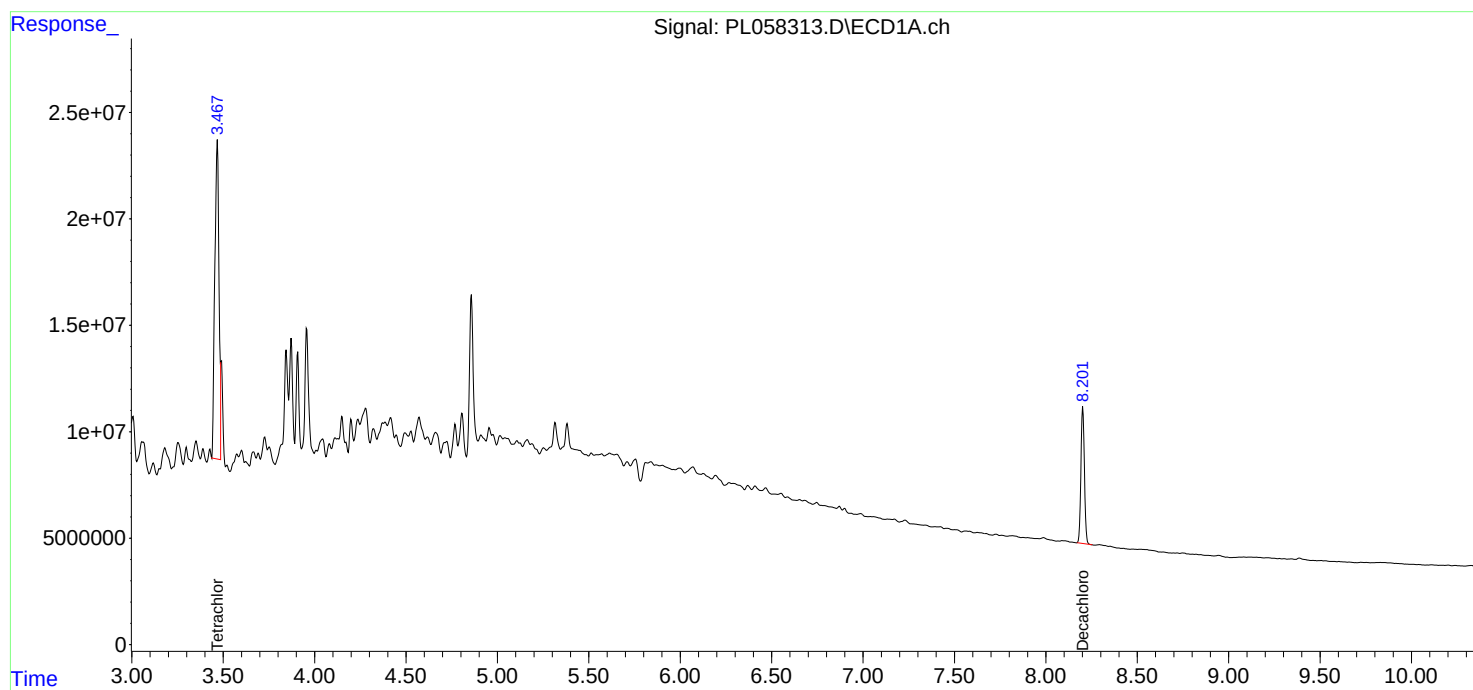

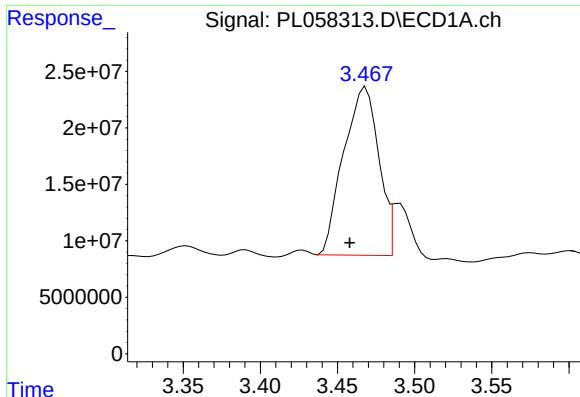


#1 Tetrachloro-m-xylene

R.T.: 3.467 min
Delta R.T.: 0.009 min
Response: 239654784
Conc: 23.77 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-16A


Manual Integrations
APPROVED

mohammad
4/23/2020 2:14:30 PM

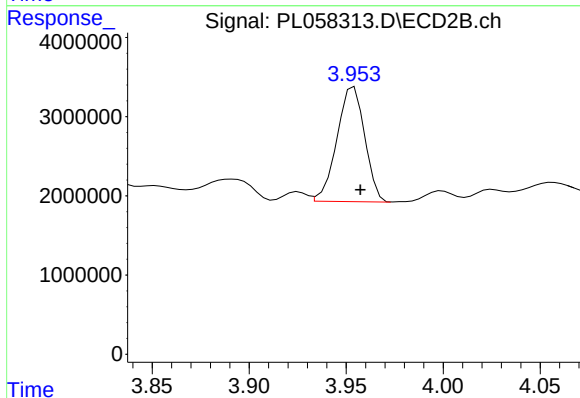


#1 Tetrachloro-m-xylene

R.T.: 3.953 min
Delta R.T.: -0.005 min
Response: 14418921
Conc: 6.64 ng/ml m

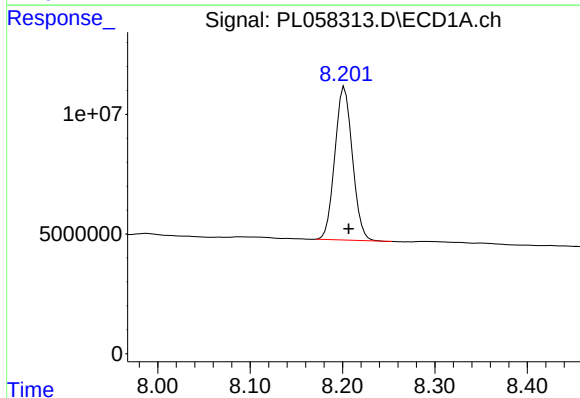

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.004 min
Response: 84439008
Conc: 8.19 ng/ml

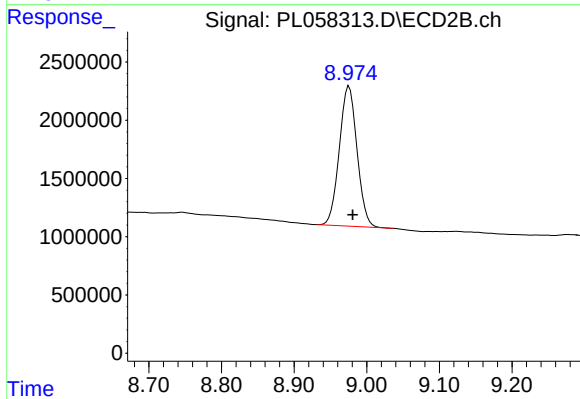

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 20354570
Conc: 9.11 ng/ml