

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:49
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:17:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:16:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.153	74359305	98194273	23.480	23.781
28)	SA Decachlor...	8.267	9.352	58016611	83975614	25.030	25.126
Target Compounds							
23)	Chlordane-1	4.302	5.173	26127557	45558291	253.099	245.824
24)	Chlordane-2	4.802	5.651	31021554	45943554	256.701	251.793
25)	Chlordane-3	5.371	6.309	79047965	167.3E6	241.145	232.466
26)	Chlordane-4	5.429	6.383	69511113	201.9E6	240.552	236.781
27)	Chlordane-5	6.269	7.206	26950644	34486790	245.541	239.633


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:49
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:17:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:16:42 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

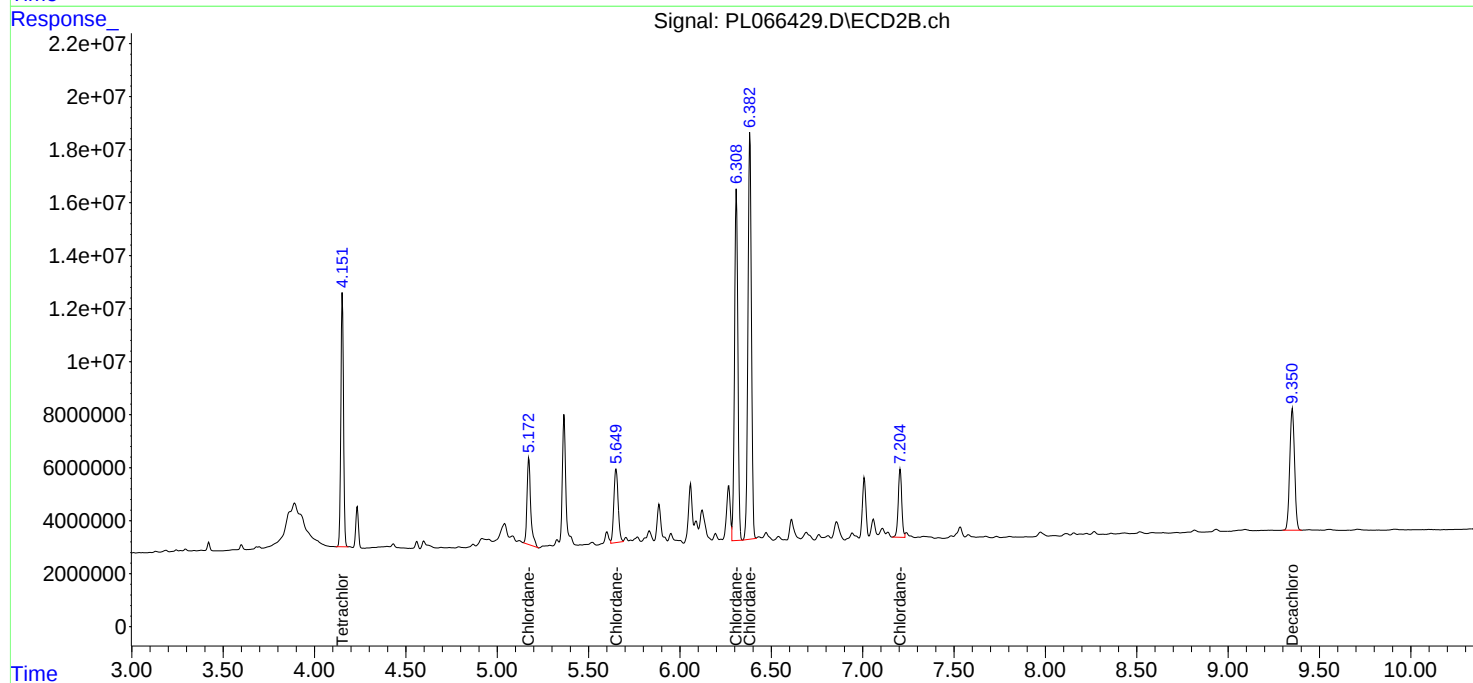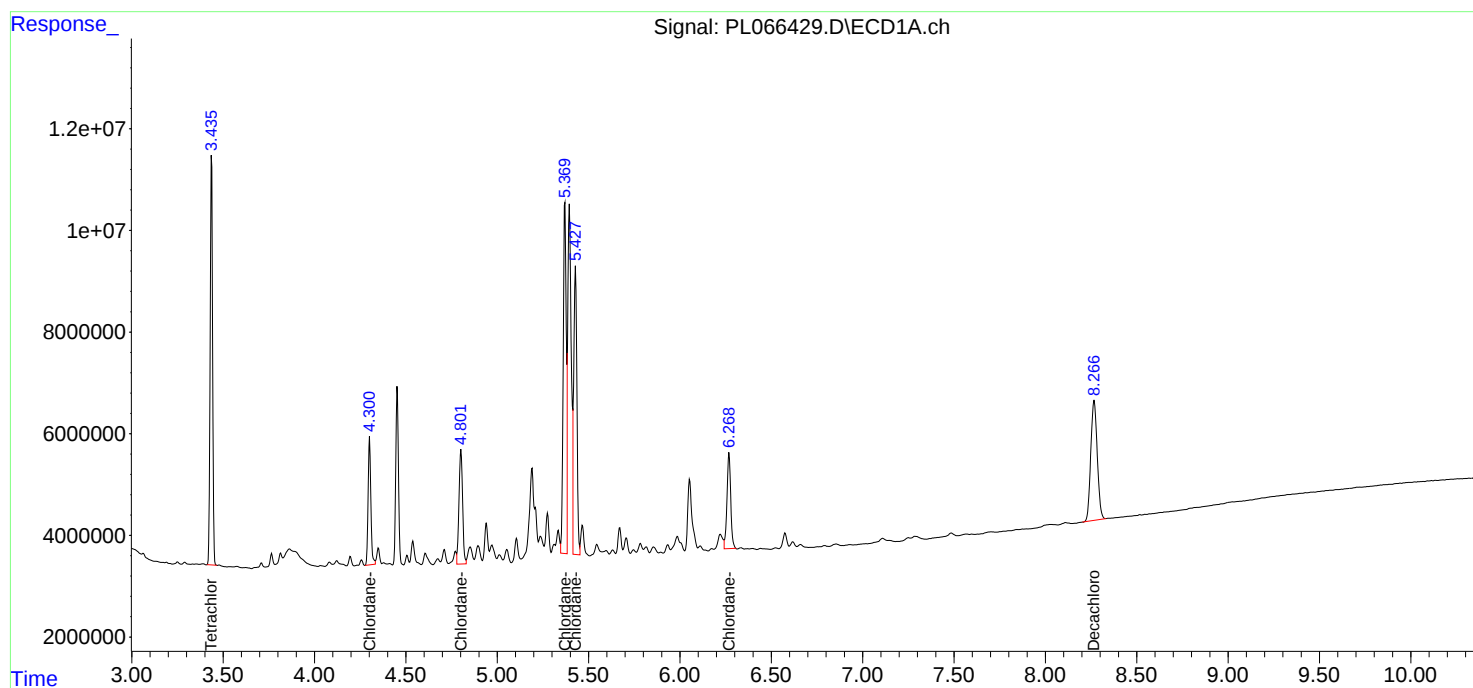

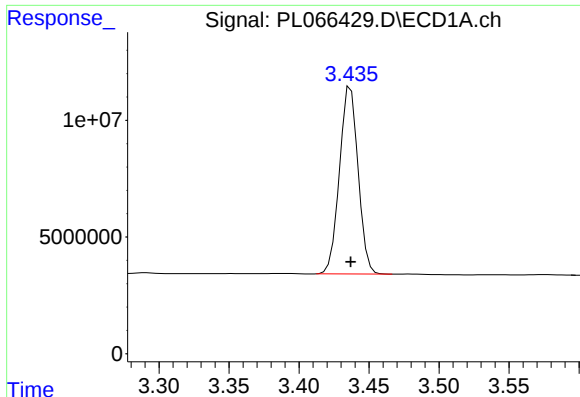


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 74359305
Conc: 23.48 ng/ml

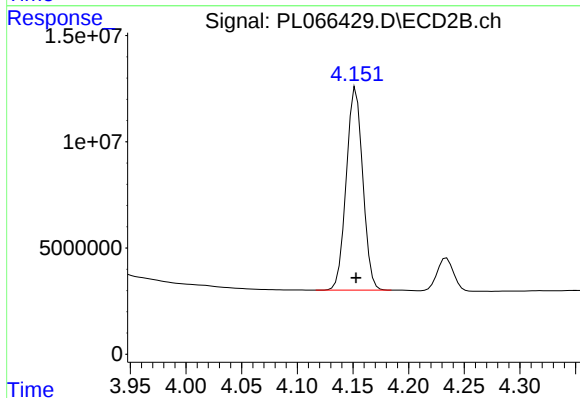


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 98194273
Conc: 23.78 ng/ml

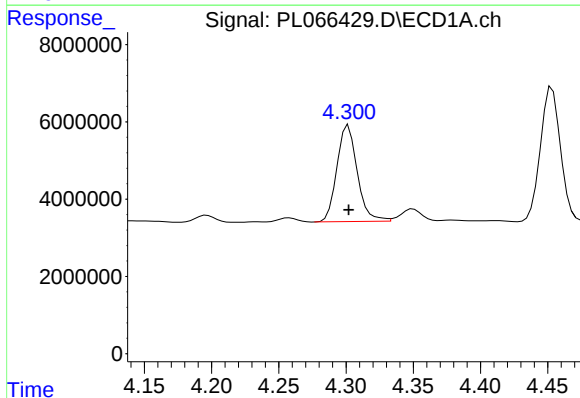


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 26127557
Conc: 253.10 ng/ml

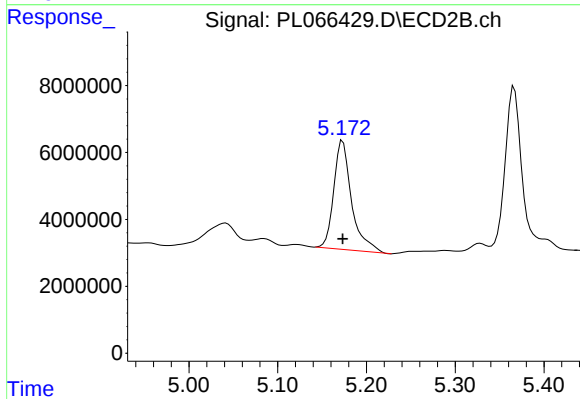


#23 Chlordane-1

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 45558291
Conc: 245.82 ng/ml

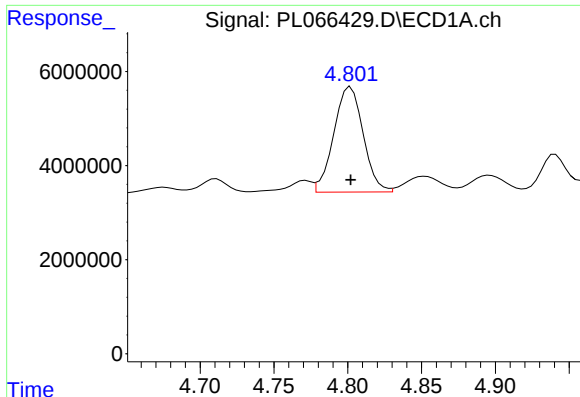


#24 Chlordane-2

R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 31021554
Conc: 256.70 ng/ml

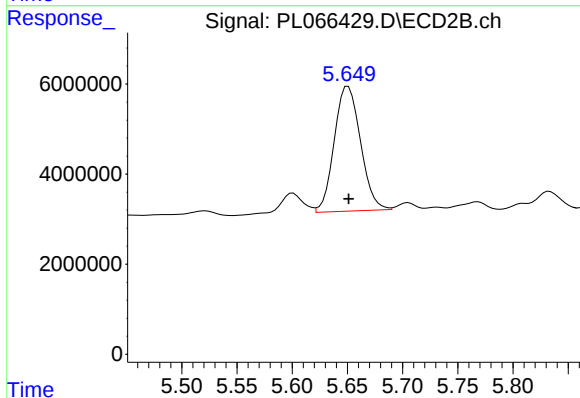


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 45943554
Conc: 251.79 ng/ml

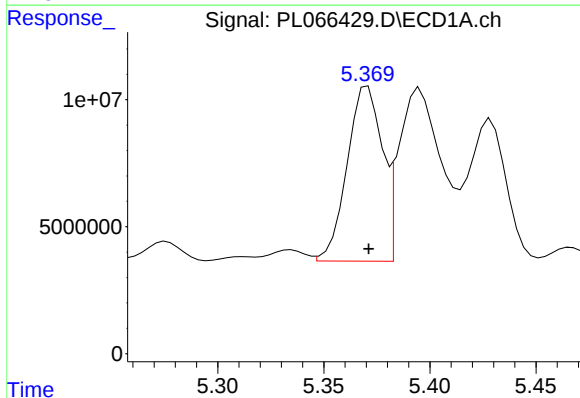


#25 Chlordane-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 79047965
Conc: 241.14 ng/ml

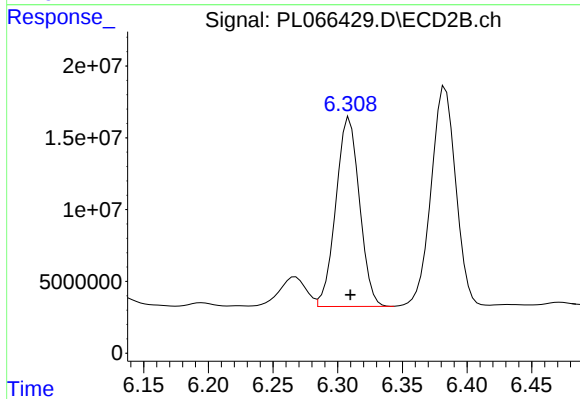


#25 Chlordane-3

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 167290608
Conc: 232.47 ng/ml

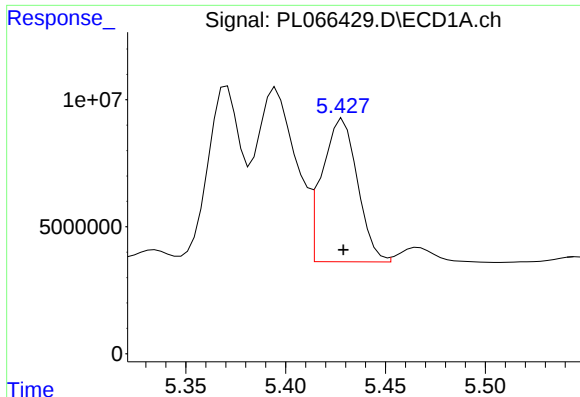


#26 Chlordane-4

R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 69511113
Conc: 240.55 ng/ml

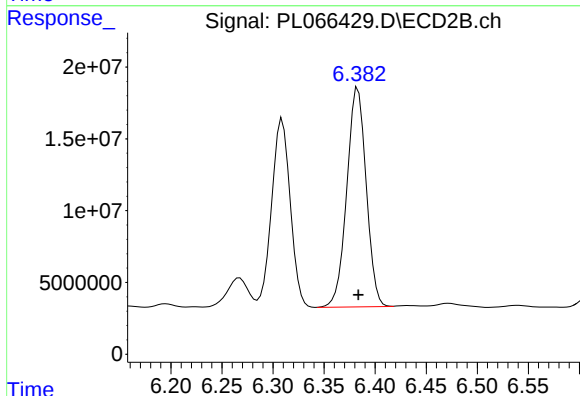


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 201895785
Conc: 236.78 ng/ml

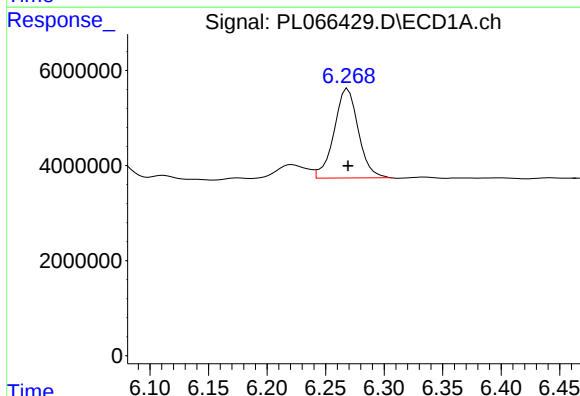


#27 Chlordane-5

R.T.: 6.269 min
Delta R.T.: 0.000 min
Response: 26950644
Conc: 245.54 ng/ml

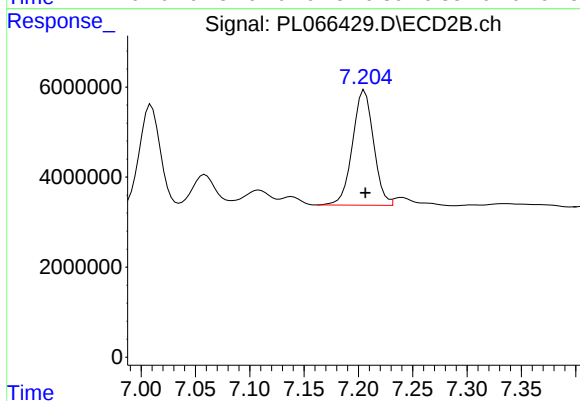


#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 34486790
Conc: 239.63 ng/ml

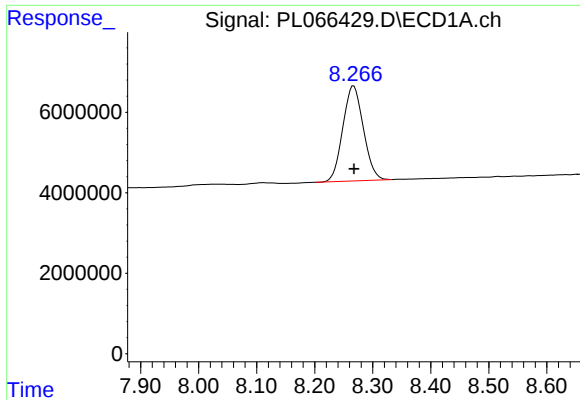

#28 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 58016611
Conc: 25.03 ng/ml

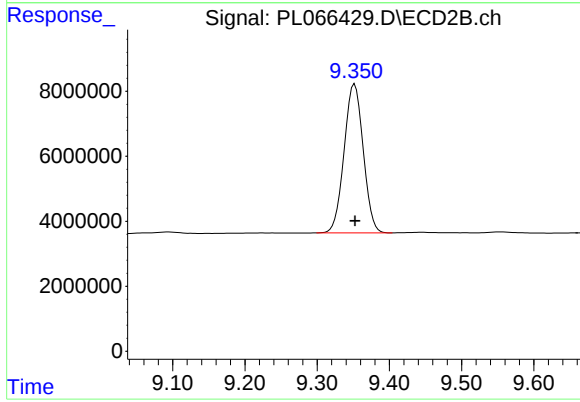

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 83975614
Conc: 25.13 ng/ml