

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 21:04
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:17:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:16:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.152	14718564	19276044	4.648	4.668
28)	SA Decachlor...	8.267	9.352	11583836	17282128	4.998	5.171
Target Compounds							
23)	Chlordane-1	4.302	5.173	5726819	13018313	55.476	70.244 #
24)	Chlordane-2	4.801	5.650	6796436	9441913	56.240	51.746
25)	Chlordane-3	5.370	6.309	15316831	31896912	46.726	44.324
26)	Chlordane-4	5.428	6.383	13303323	39473575	46.038	46.294
27)	Chlordane-5	6.268	7.205	7525927	6141776	68.567	42.676 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 21:04
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:17:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:16:42 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

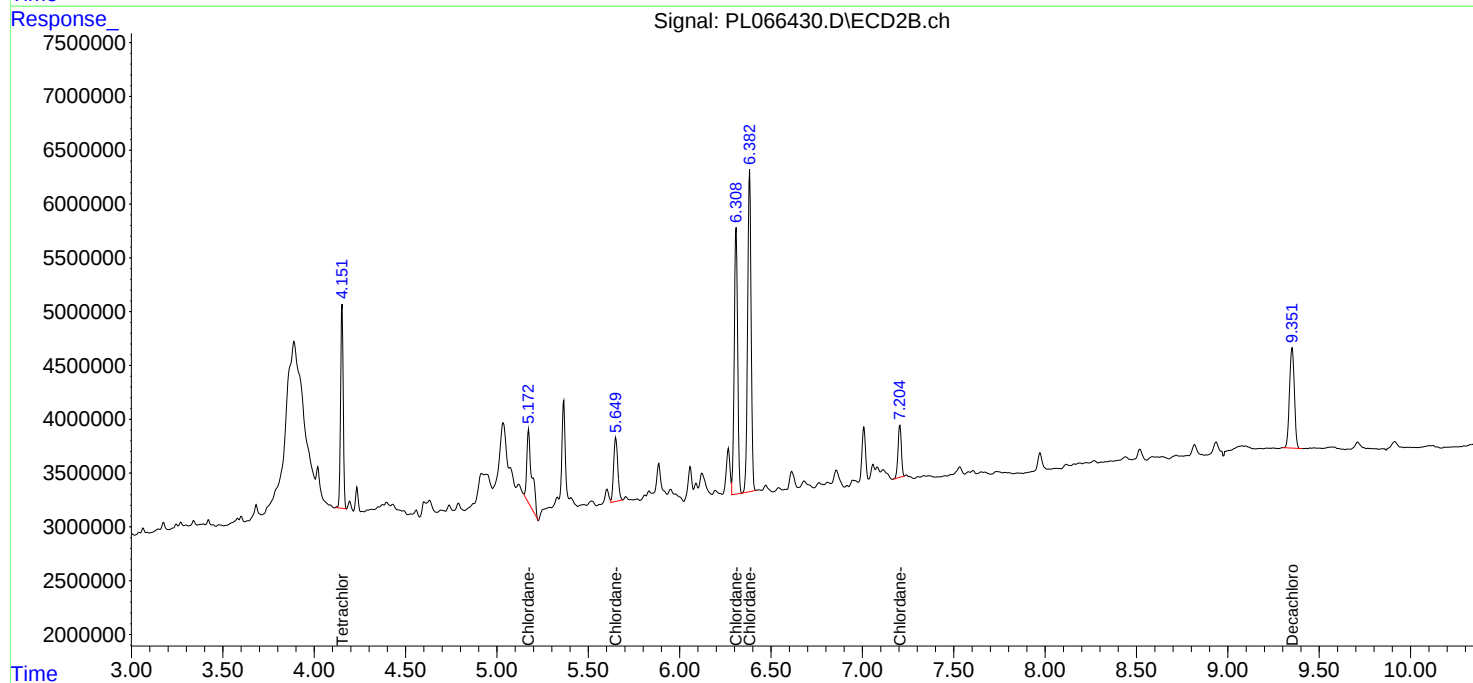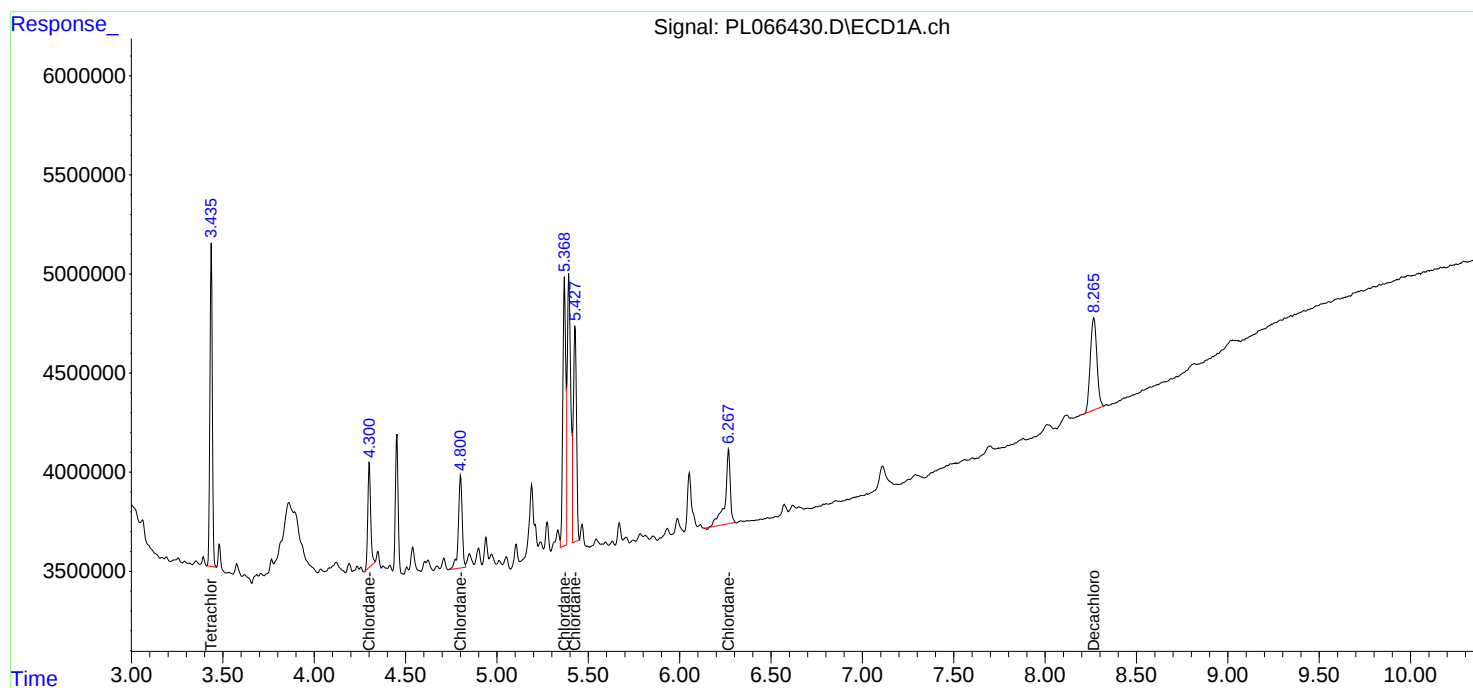

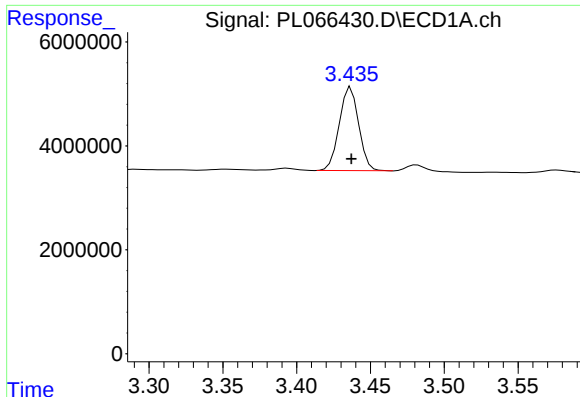


#1 Tetrachloro-m-xylene

R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 14718564
Conc: 4.65 ng/ml

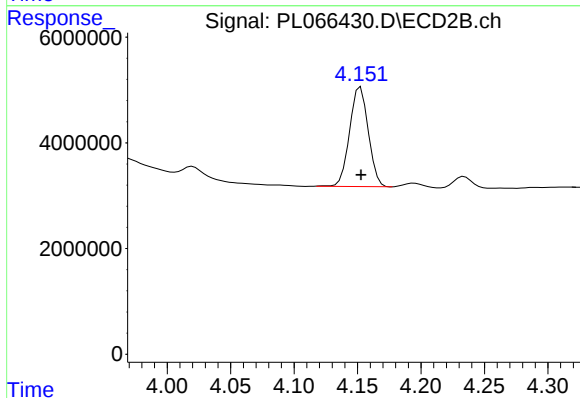


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 19276044
Conc: 4.67 ng/ml

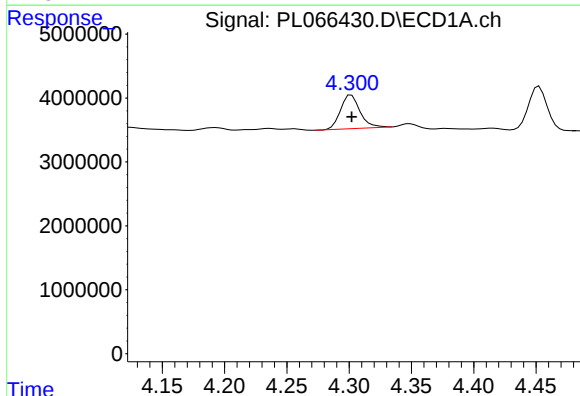


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 5726819
Conc: 55.48 ng/ml

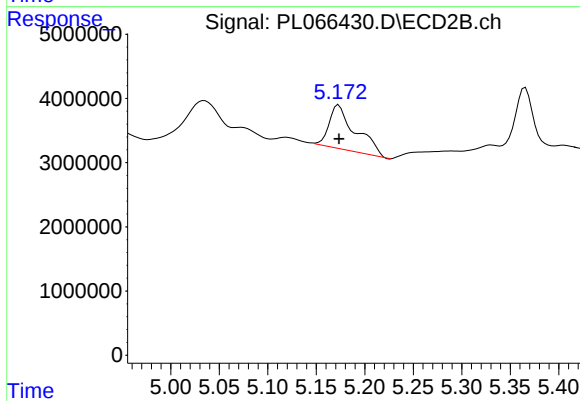


#23 Chlordane-1

R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 13018313
Conc: 70.24 ng/ml

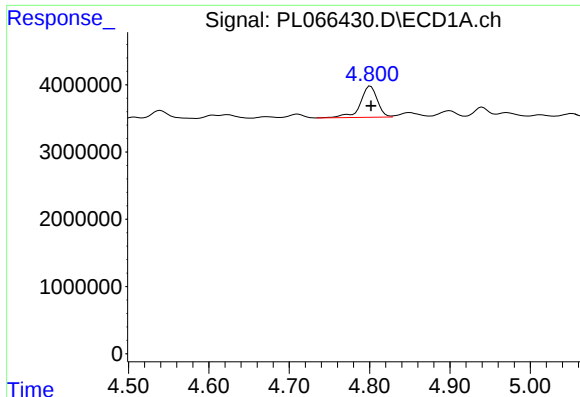


#24 Chlordane-2

R.T.: 4.801 min
Delta R.T.: 0.000 min
Response: 6796436
Conc: 56.24 ng/ml

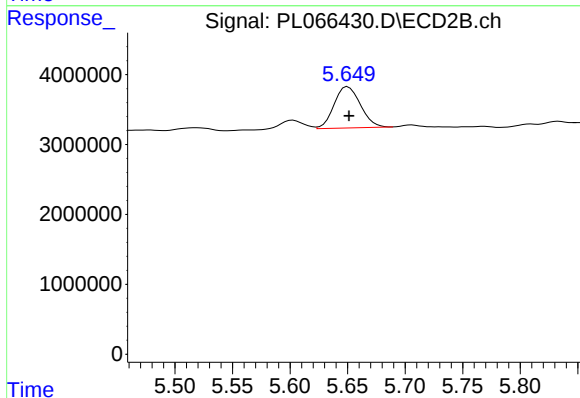


#24 Chlordane-2

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 9441913
Conc: 51.75 ng/ml

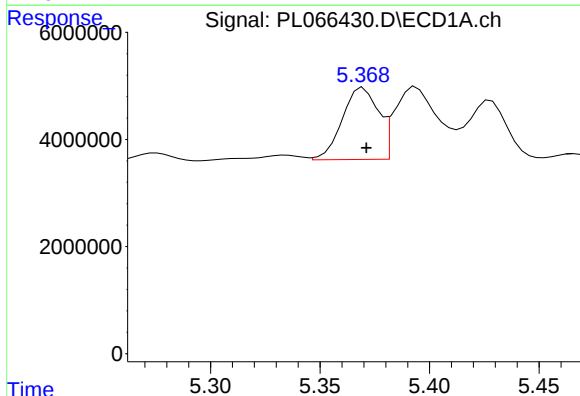


#25 Chlordane-3

R.T.: 5.370 min
Delta R.T.: -0.001 min
Response: 15316831
Conc: 46.73 ng/ml

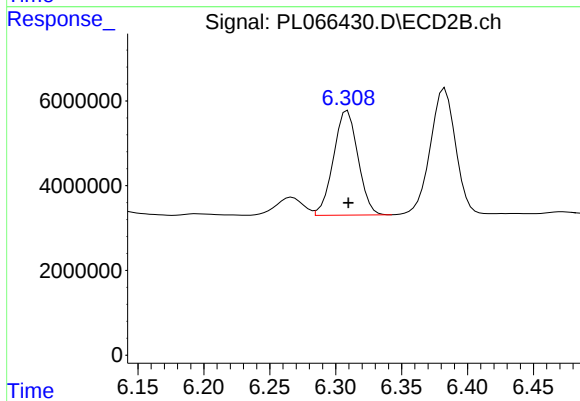


#25 Chlordane-3

R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 31896912
Conc: 44.32 ng/ml

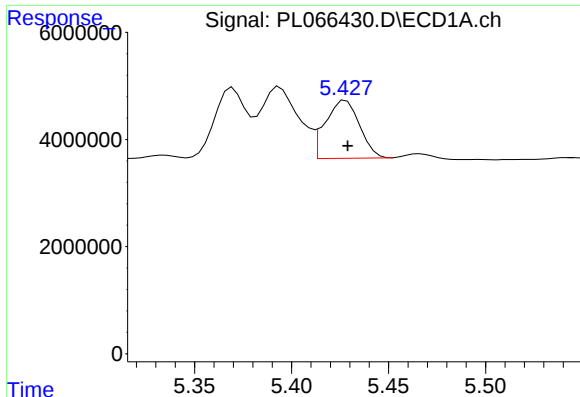


#26 Chlordane-4

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 13303323
Conc: 46.04 ng/ml

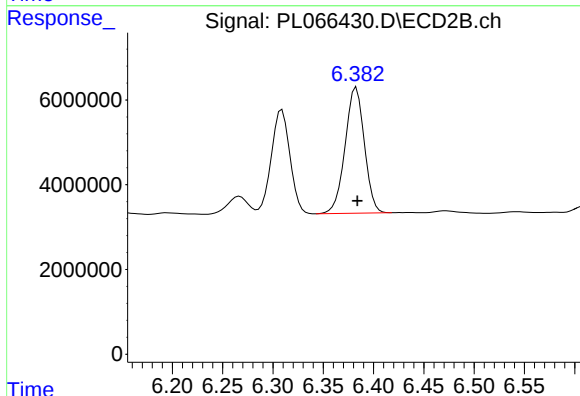


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 39473575
Conc: 46.29 ng/ml

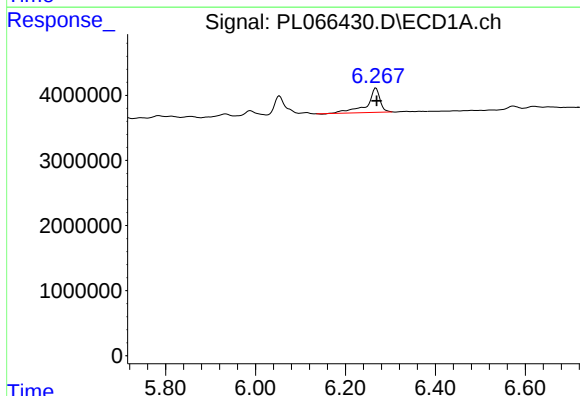


#27 Chlordane-5

R.T.: 6.268 min
Delta R.T.: -0.001 min
Response: 7525927
Conc: 68.57 ng/ml

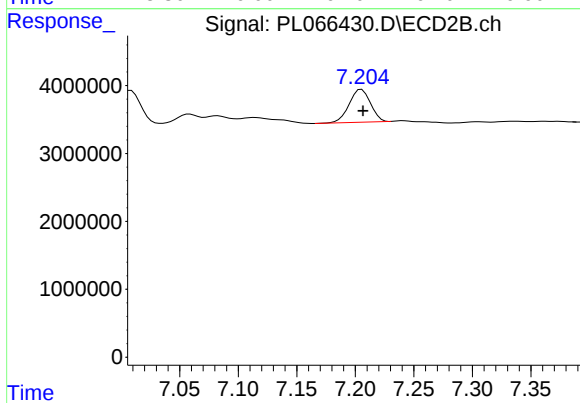


#27 Chlordane-5

R.T.: 7.205 min
Delta R.T.: -0.001 min
Response: 6141776
Conc: 42.68 ng/ml

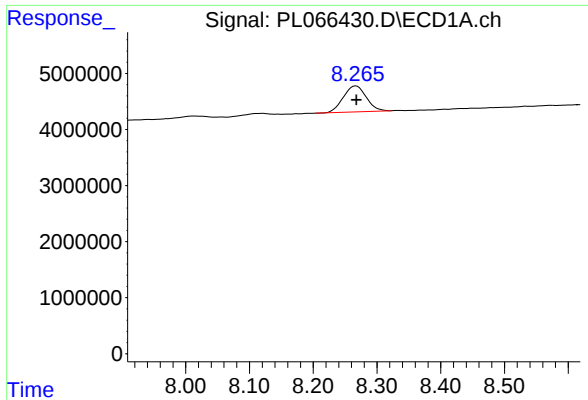

#28 Decachlorobiphenyl

R.T.: 8.267 min
Delta R.T.: 0.000 min
Response: 11583836
Conc: 5.00 ng/ml

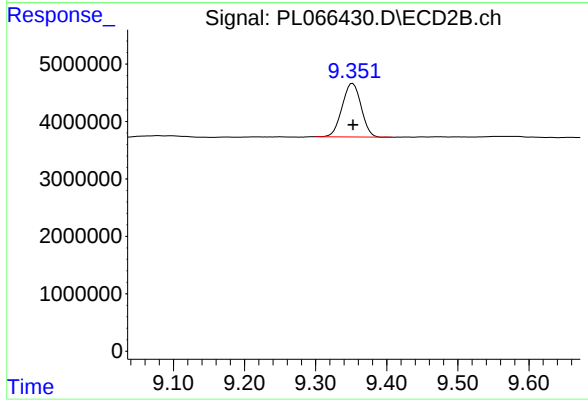

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 17282128
Conc: 5.17 ng/ml