

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 18:40
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 01:03:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:52:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.438	4.153	62763838	86654631	21.203	20.734
28)	SA Decachlor...	8.269	9.349	51951730	69727317	20.248	20.275
Target Compounds							
9)	A Endosulfan I	5.480	6.437	32256244	42743931	9.660	9.508
10)	B gamma-Chl...	5.371	6.310	34482502	44826498	9.543	9.106
12)	B 4,4'-DDE	5.603	6.538	64141589	85350411	19.547	19.136
13)	MA Dieldrin	5.726	6.699	69759535	89658681	20.353	19.882
19)	B Endosulfa...	6.657	7.486	57265863	71261223	18.904	18.642
20)	A Methoxychlor	6.956	7.800	126.3E6	174.2E6	94.823	88.902
21)	B Endrin ke...	7.154	7.967	65100052	73637388	20.149	18.482



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 18:40
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 01:03:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:52:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

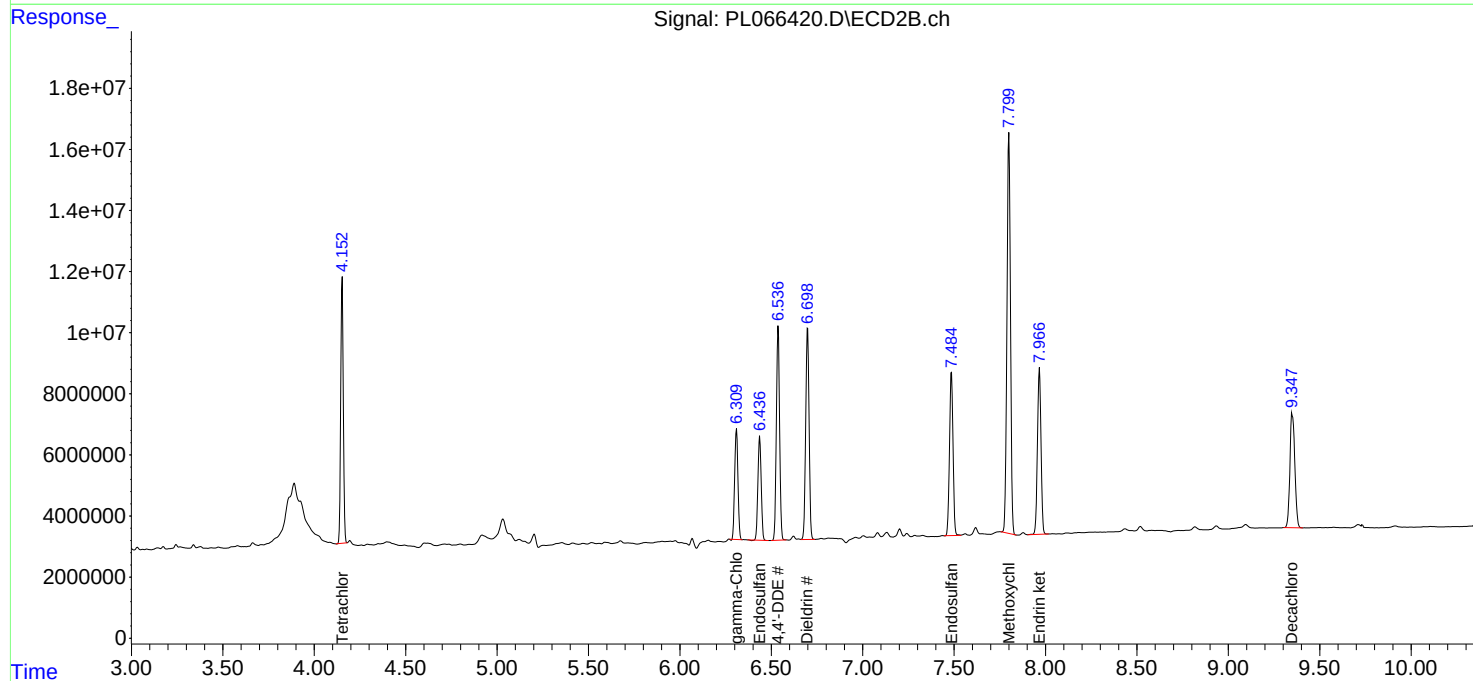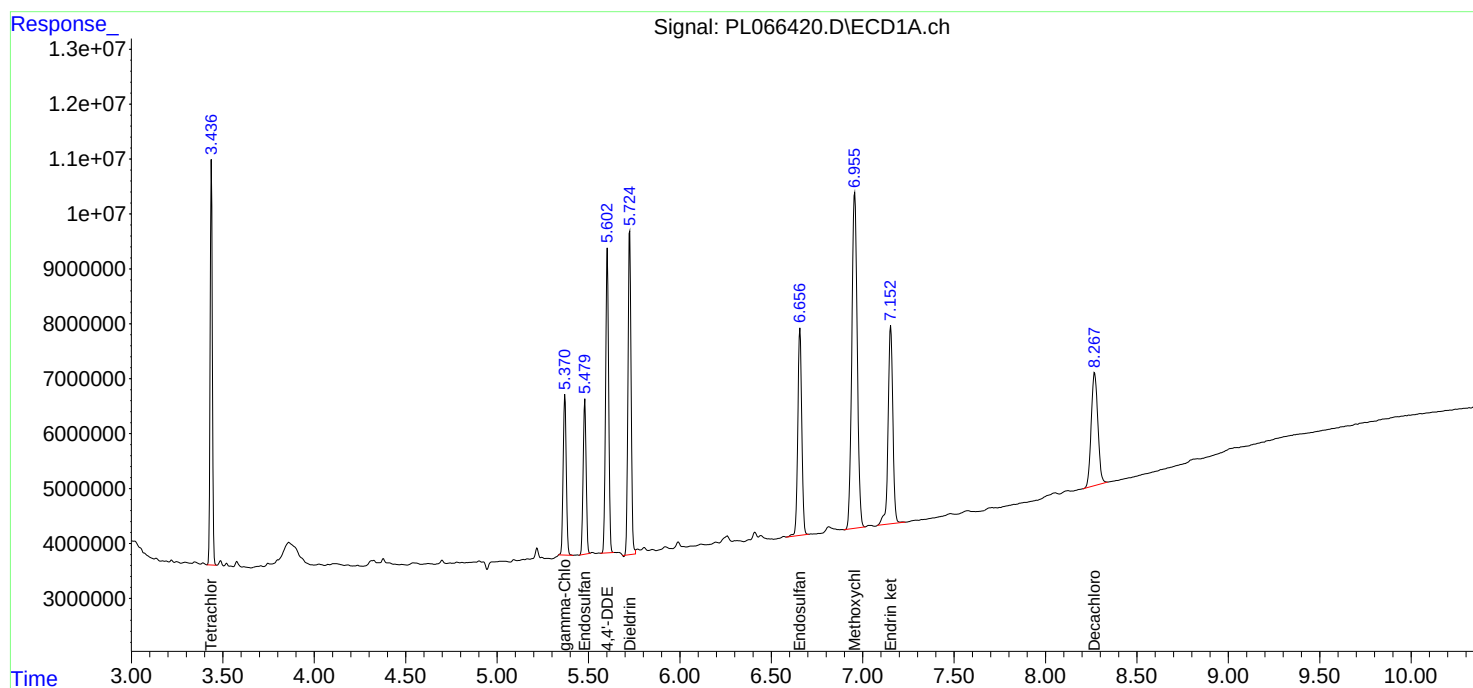


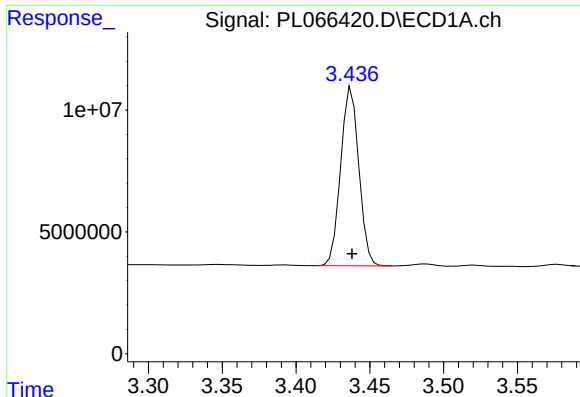

#1 Tetrachloro-m-xylene


R.T.: 3.438 min
Delta R.T.: 0.000 min
Response: 62763838
Conc: 21.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

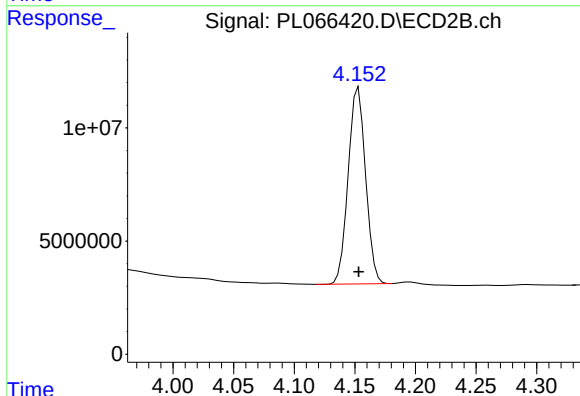


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 86654631
Conc: 20.73 ng/ml

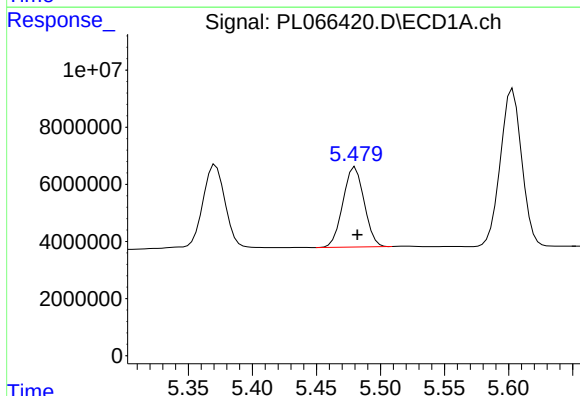


#9 Endosulfan I

R.T.: 5.480 min
Delta R.T.: -0.002 min
Response: 32256244
Conc: 9.66 ng/ml

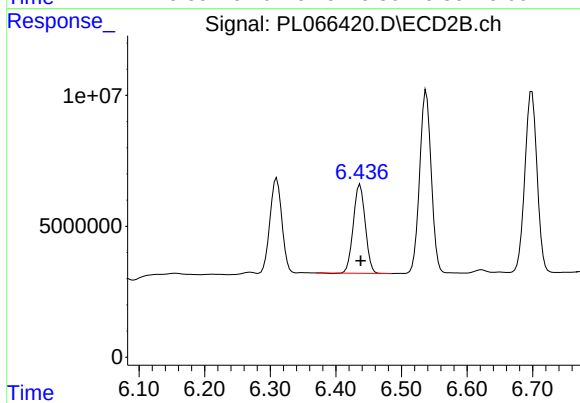

#9 Endosulfan I


R.T.: 6.437 min
Delta R.T.: -0.001 min
Response: 42743931
Conc: 9.51 ng/ml

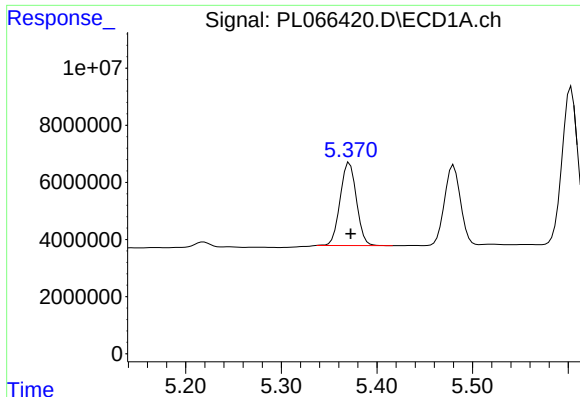

#10 gamma-Chlordane


R.T.: 5.371 min
Delta R.T.: -0.001 min
Response: 34482502
Conc: 9.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

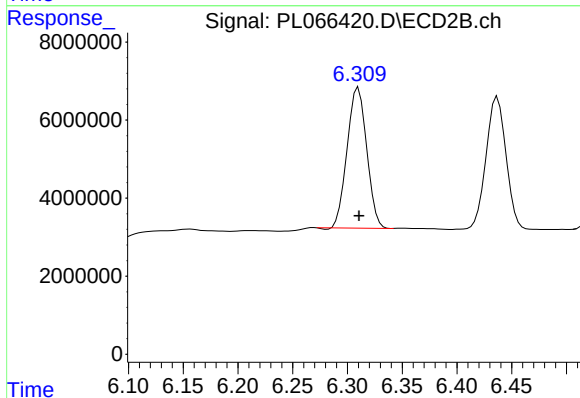


#10 gamma-Chlordane

R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 44826498
Conc: 9.11 ng/ml

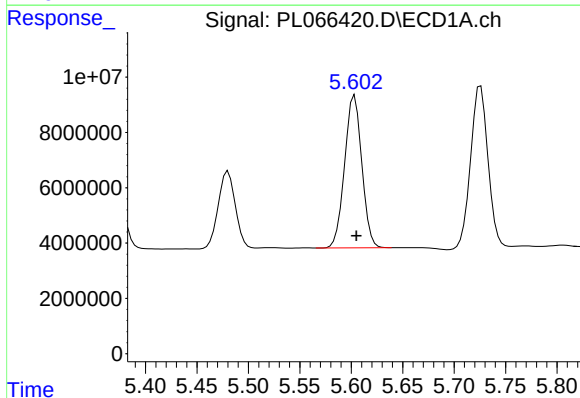


#12 4,4'-DDE

R.T.: 5.603 min
Delta R.T.: -0.002 min
Response: 64141589
Conc: 19.55 ng/ml

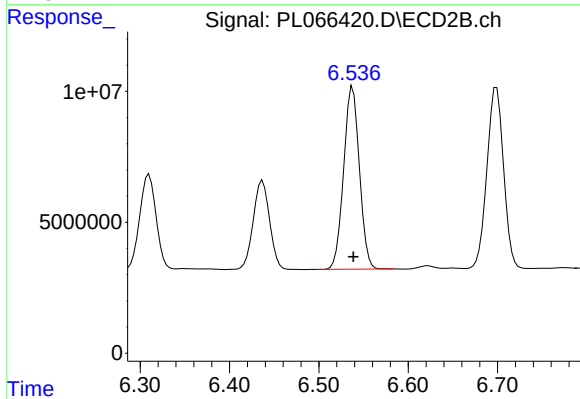

#12 4,4'-DDE


R.T.: 6.538 min
Delta R.T.: 0.000 min
Response: 85350411
Conc: 19.14 ng/ml

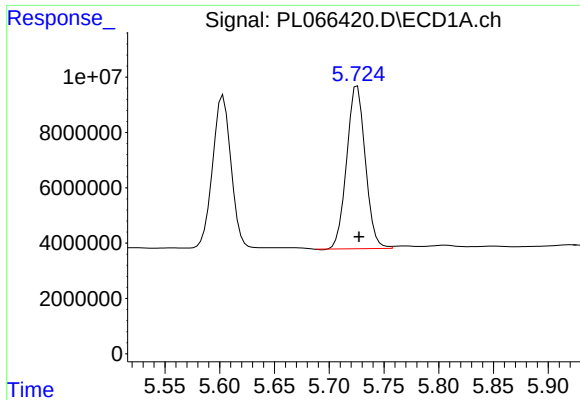

#13 Dieldrin


R.T.: 5.726 min
Delta R.T.: -0.002 min
Response: 69759535
Conc: 20.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

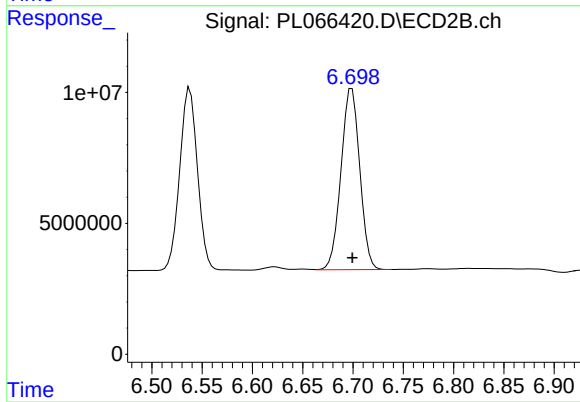


#13 Dieldrin

R.T.: 6.699 min
Delta R.T.: 0.000 min
Response: 89658681
Conc: 19.88 ng/ml

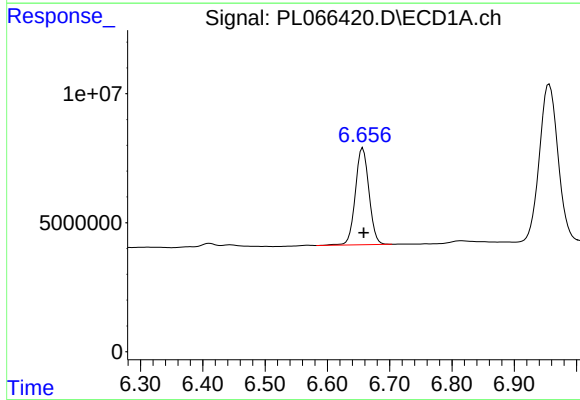


#19 Endosulfan Sulfate

R.T.: 6.657 min
Delta R.T.: -0.002 min
Response: 57265863
Conc: 18.90 ng/ml

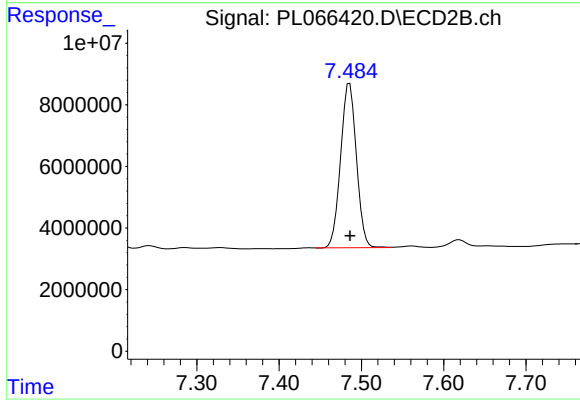

#19 Endosulfan Sulfate


R.T.: 7.486 min
Delta R.T.: 0.000 min
Response: 71261223
Conc: 18.64 ng/ml

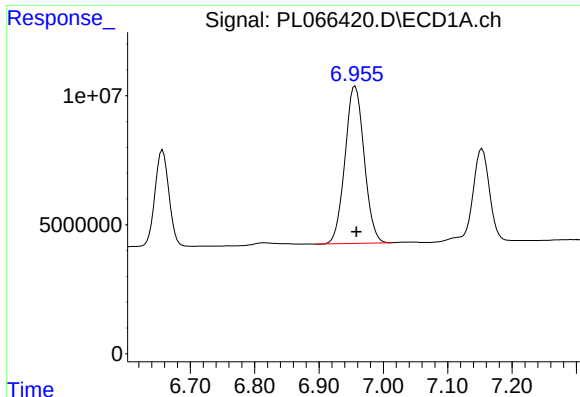

#20 Methoxychlor


R.T.: 6.956 min
Delta R.T.: -0.002 min
Response: 126265822
Conc: 94.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

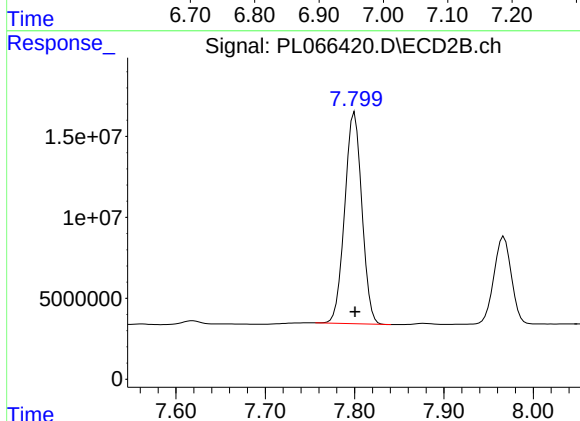


#20 Methoxychlor

R.T.: 7.800 min
Delta R.T.: 0.000 min
Response: 174194208
Conc: 88.90 ng/ml

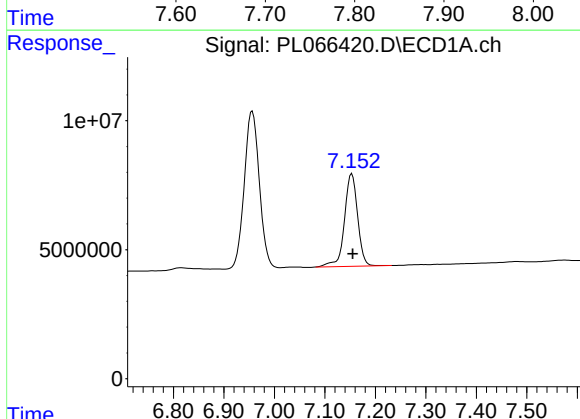


#21 Endrin ketone

R.T.: 7.154 min
Delta R.T.: -0.001 min
Response: 65100052
Conc: 20.15 ng/ml

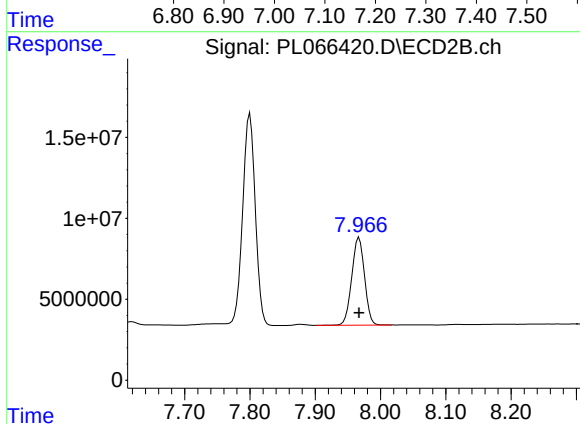

#21 Endrin ketone


R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 73637388
Conc: 18.48 ng/ml

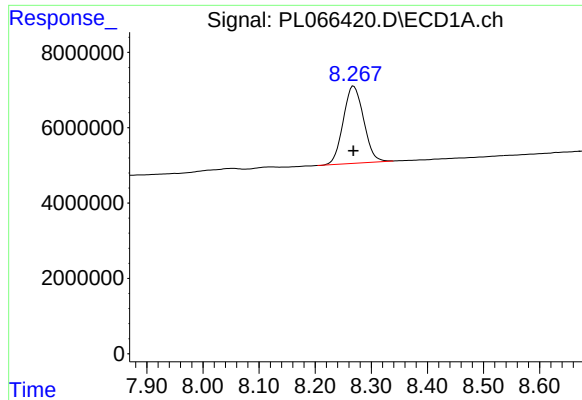

#28 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: 0.000 min
Response: 51951730
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
RESCHK

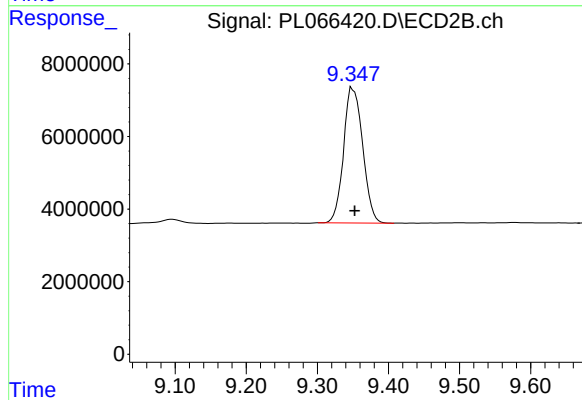

#28 Decachlorobiphenyl

R.T.: 9.349 min
Delta R.T.: -0.004 min
Response: 69727317
Conc: 20.27 ng/ml