

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:06
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:17:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:16:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.153	312.7E6	381.8E6	98.751	92.459
28)	SA Decachlor...	8.271	9.352	217.6E6	300.9E6	93.894	90.044
Target Compounds							
23)	Chlordane-1	4.302	5.174	98449818	171.8E6	953.689	927.237
24)	Chlordane-2	4.803	5.651	111.5E6	165.7E6	922.927	908.063
25)	Chlordane-3	5.372	6.310	322.1E6	688.0E6	982.456	956.012
26)	Chlordane-4	5.430	6.383	281.3E6	803.4E6	973.458	942.178
27)	Chlordane-5	6.270	7.206	104.1E6	136.2E6	948.751	946.363



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:06
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:17:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:16:42 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

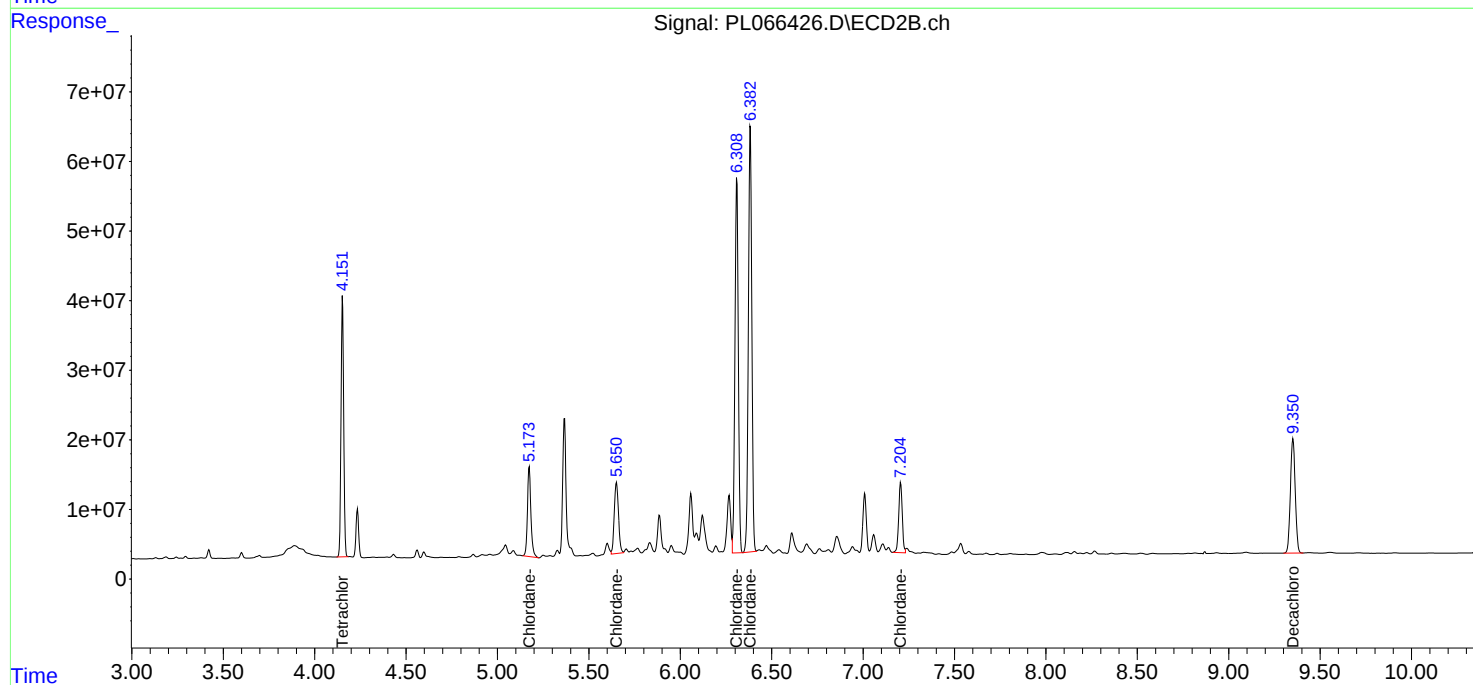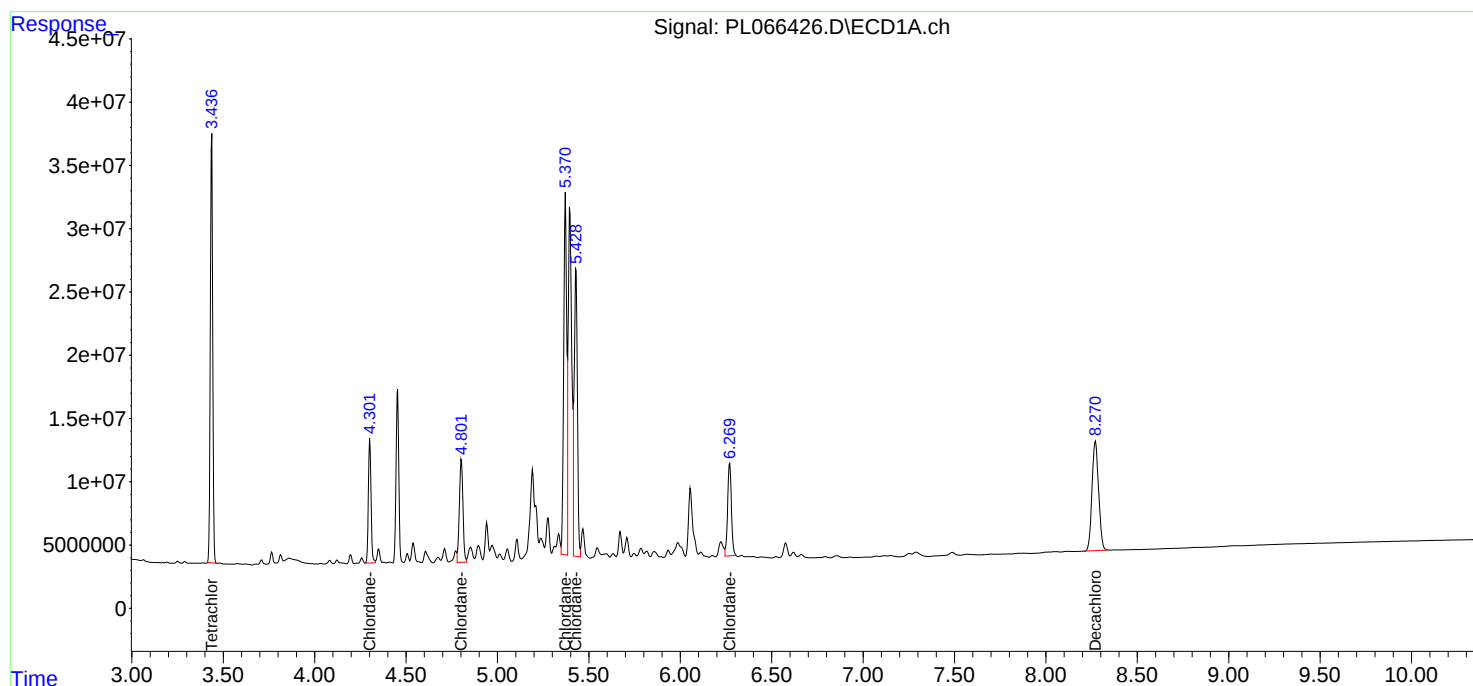


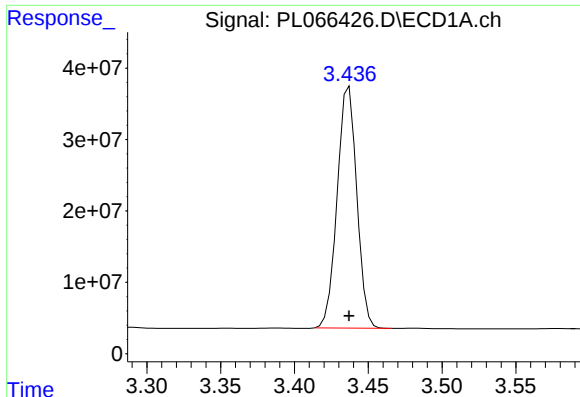

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 312740136
Conc: 98.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

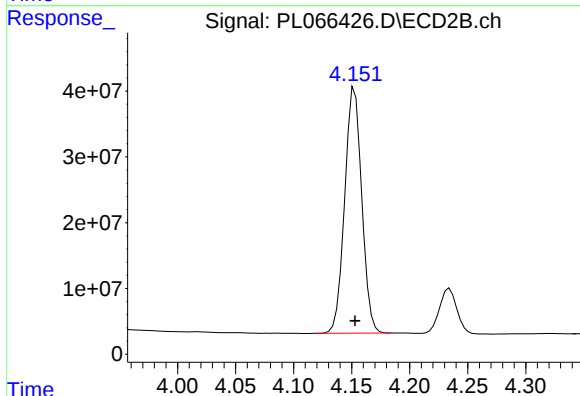


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 381773519
Conc: 92.46 ng/ml

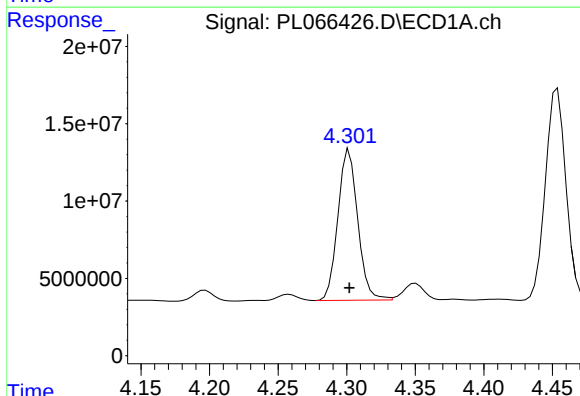


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 98449818
Conc: 953.69 ng/ml

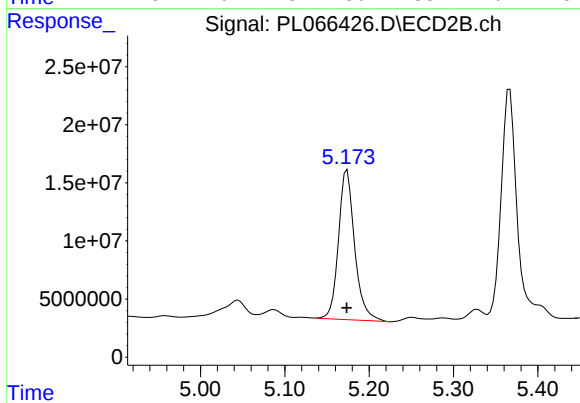

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 171843731
Conc: 927.24 ng/ml

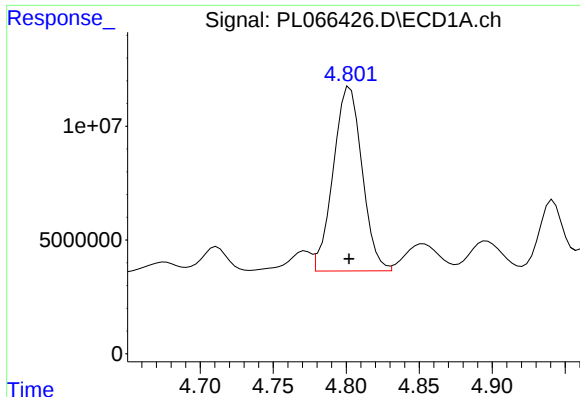

#24 Chlordane-2


R.T.: 4.803 min
Delta R.T.: 0.000 min
Response: 111532842
Conc: 922.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

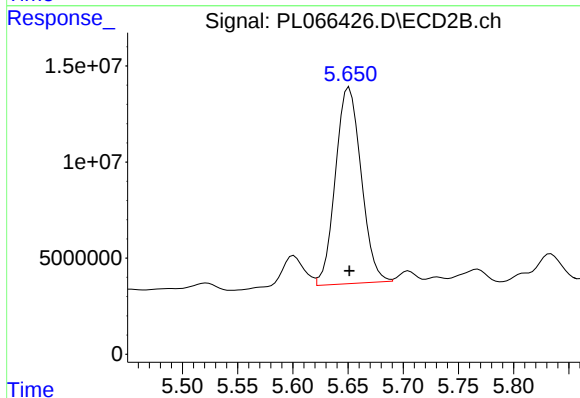


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 165690340
Conc: 908.06 ng/ml

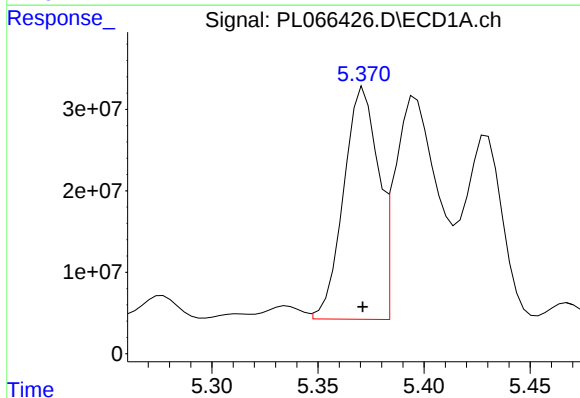


#25 Chlordane-3

R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 322051829
Conc: 982.46 ng/ml

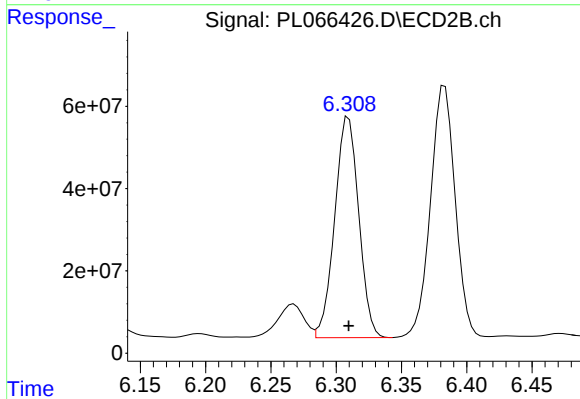

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 687978144
Conc: 956.01 ng/ml

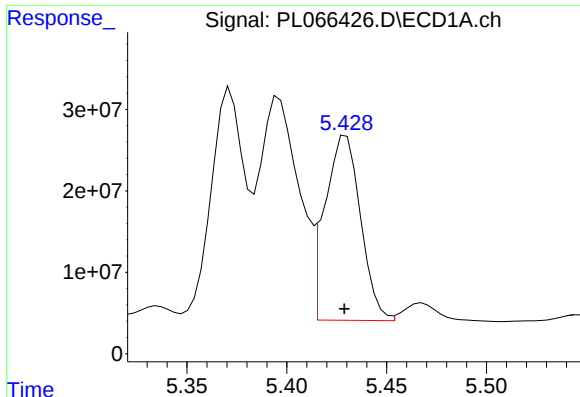

#26 Chlordane-4


R.T.: 5.430 min
Delta R.T.: 0.000 min
Response: 281294813
Conc: 973.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

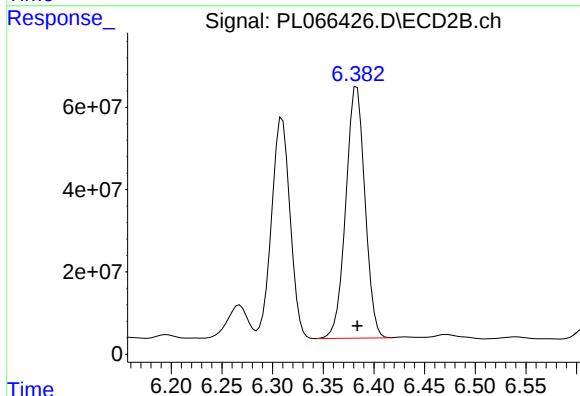


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 803364244
Conc: 942.18 ng/ml

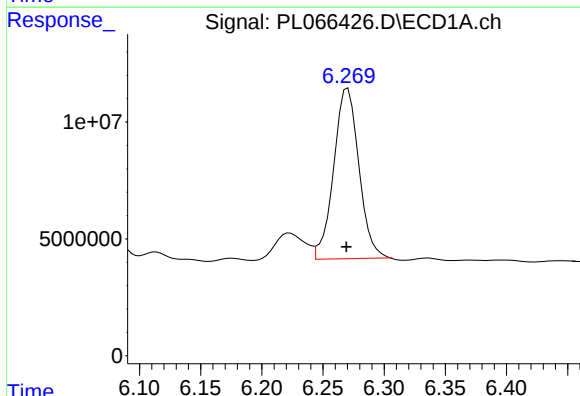


#27 Chlordane-5

R.T.: 6.270 min
Delta R.T.: 0.001 min
Response: 104135150
Conc: 948.75 ng/ml

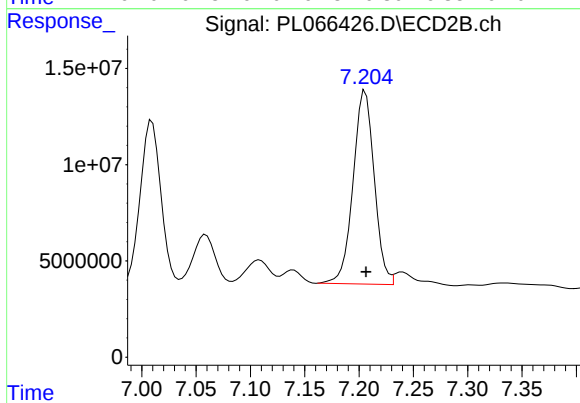

#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 136195844
Conc: 946.36 ng/ml

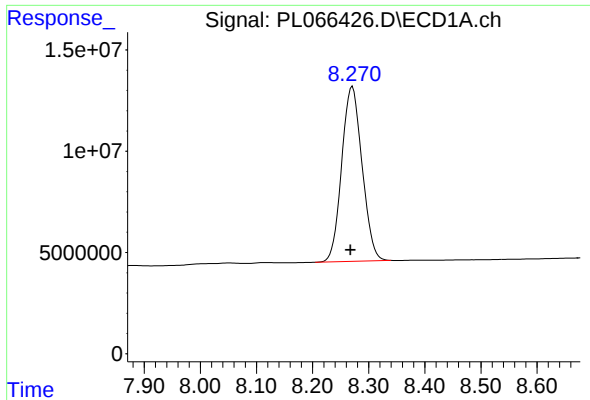

#28 Decachlorobiphenyl


R.T.: 8.271 min

Delta R.T.: 0.003 min

Response: 217634736

Conc: 93.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

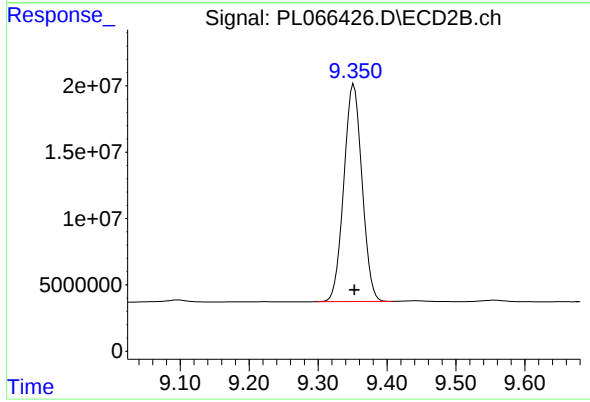

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 300946513

Conc: 90.04 ng/ml