

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:20
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:17:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:16:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.152	237.4E6	300.7E6	74.975	72.816
28)	SA Decachlor...	8.269	9.352	169.2E6	241.9E6	73.009	72.383
Target Compounds							
23)	Chlordane-1	4.302	5.173	76043858	132.2E6	736.641	713.091
24)	Chlordane-2	4.802	5.650	87381072	129.9E6	723.073	712.150
25)	Chlordane-3	5.371	6.309	250.8E6	534.9E6	764.957	743.353
26)	Chlordane-4	5.429	6.383	215.0E6	628.3E6	744.138	736.882
27)	Chlordane-5	6.269	7.206	80948667	107.2E6	737.505	744.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066427.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:20
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:17:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:16:42 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

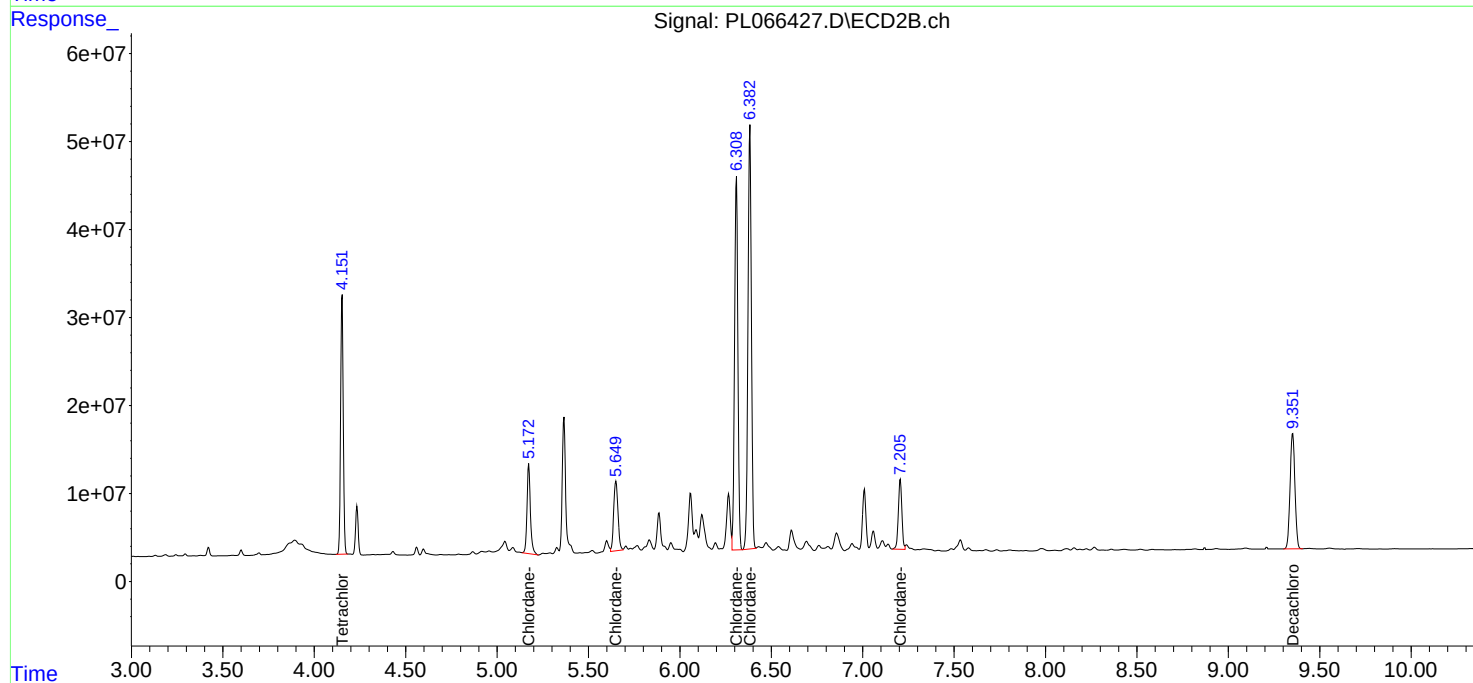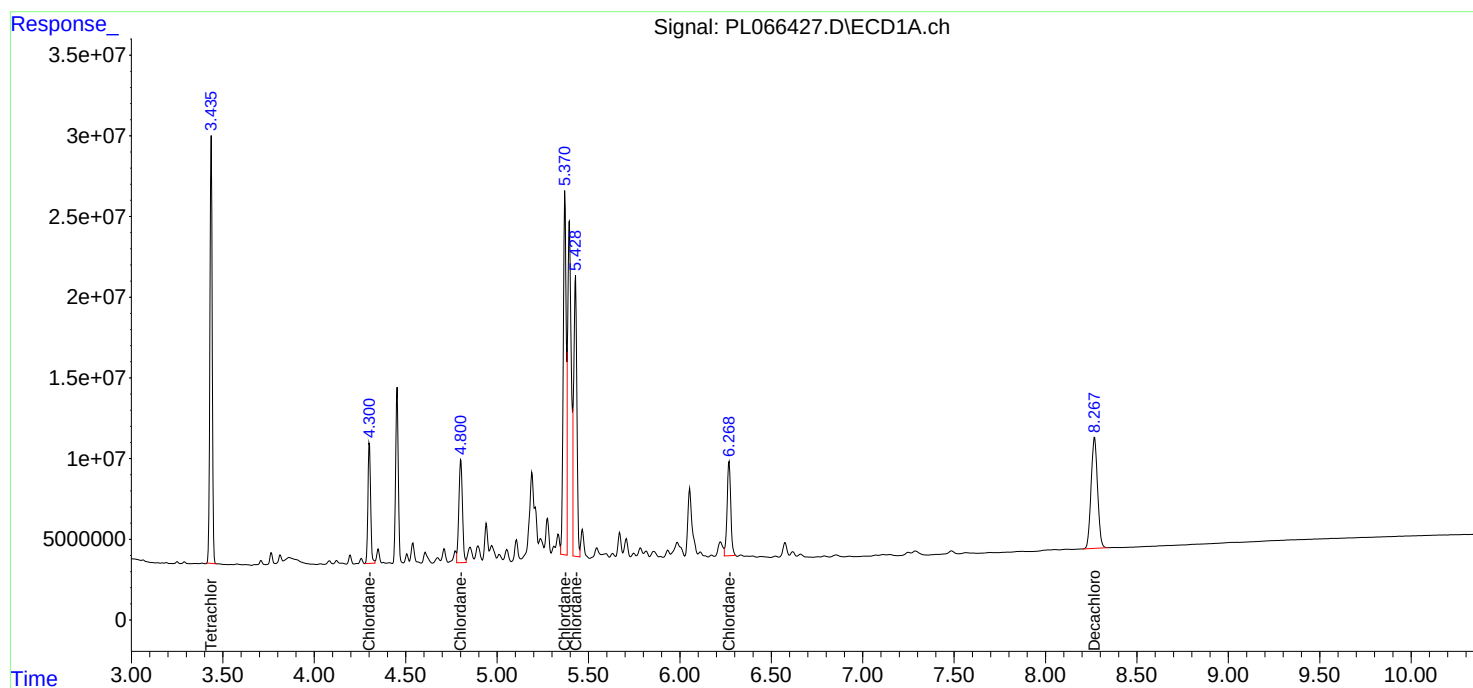


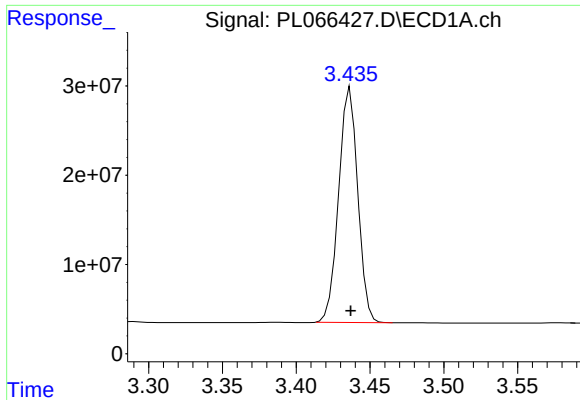

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 237441717
Conc: 74.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

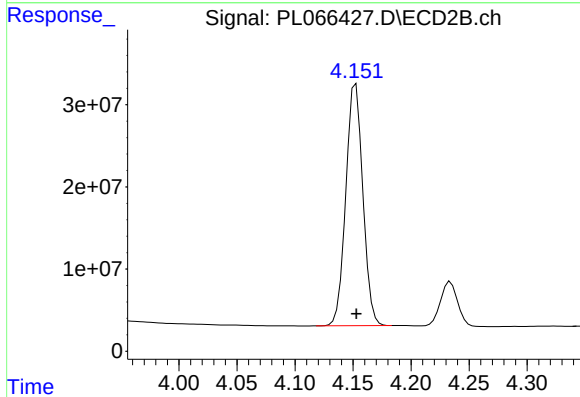


#1 Tetrachloro-m-xylene

R.T.: 4.152 min
Delta R.T.: 0.000 min
Response: 300663302
Conc: 72.82 ng/ml

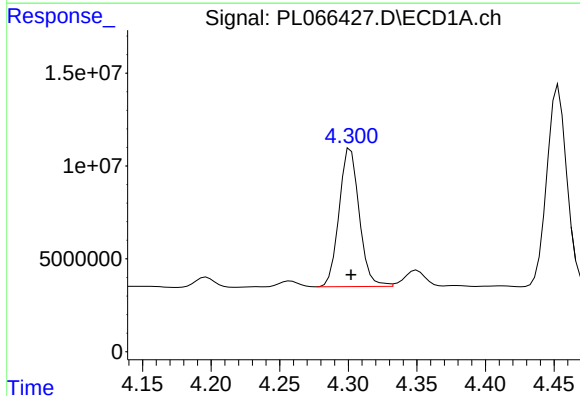


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 76043858
Conc: 736.64 ng/ml

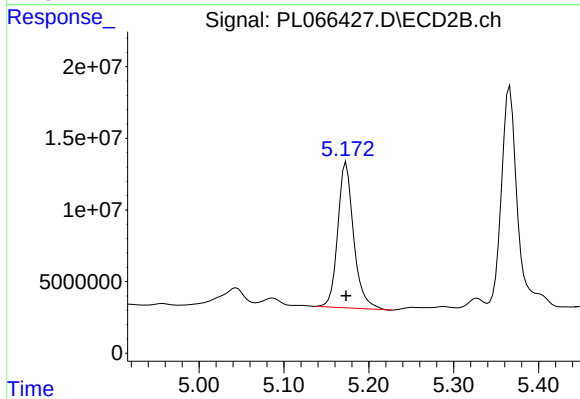

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 132156333
Conc: 713.09 ng/ml

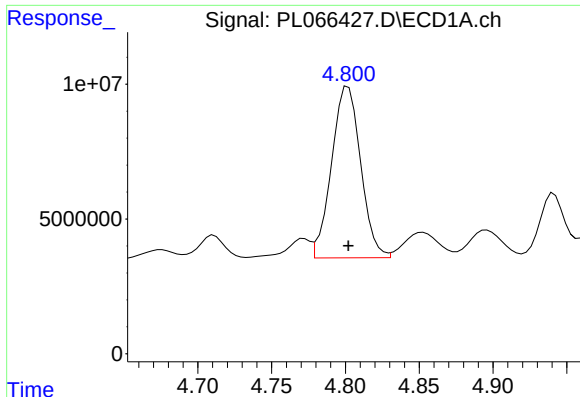

#24 Chlordane-2


R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 87381072
Conc: 723.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

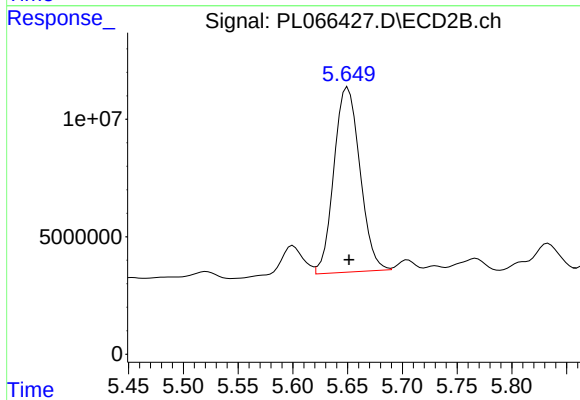


#24 Chlordane-2

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 129942927
Conc: 712.15 ng/ml

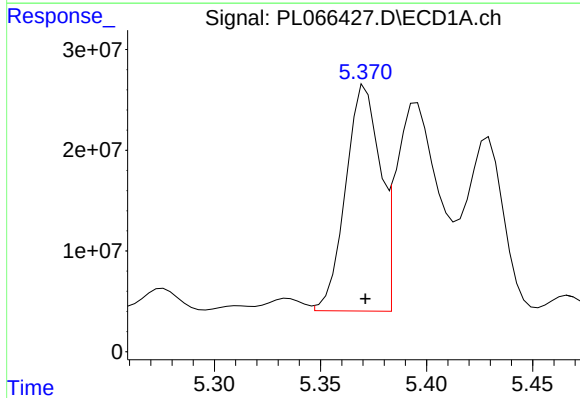


#25 Chlordane-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 250755021
Conc: 764.96 ng/ml

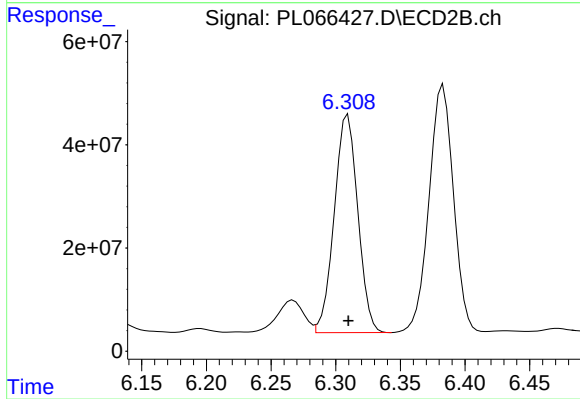

#25 Chlordane-3


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 534942163
Conc: 743.35 ng/ml

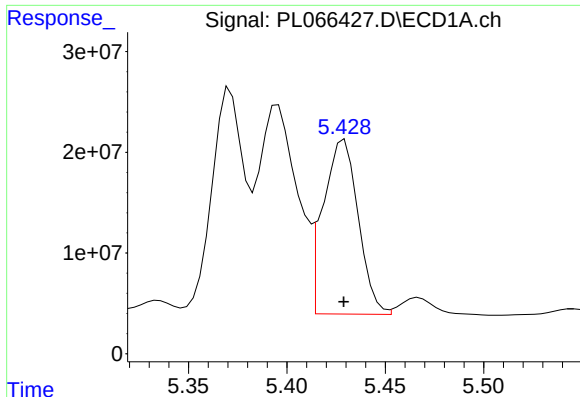

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 215029375
Conc: 744.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

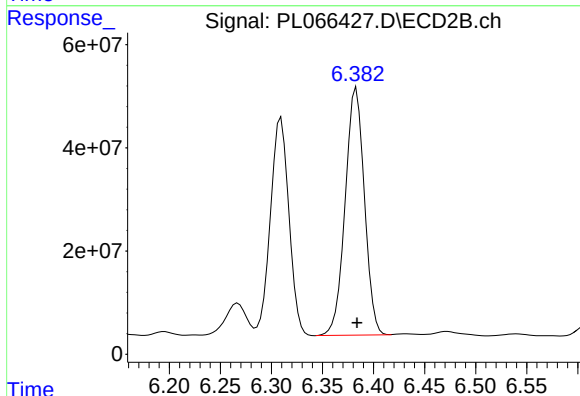


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 628315266
Conc: 736.88 ng/ml

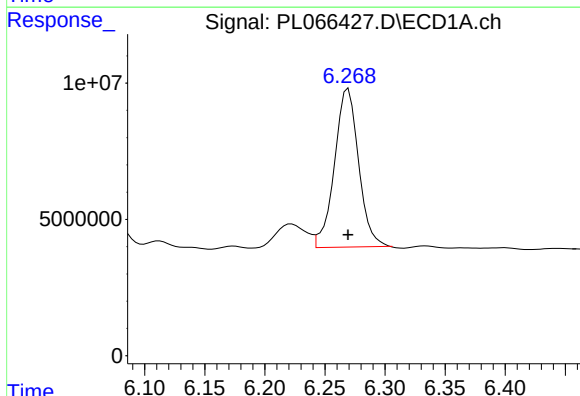


#27 Chlordane-5

R.T.: 6.269 min
Delta R.T.: 0.000 min
Response: 80948667
Conc: 737.50 ng/ml

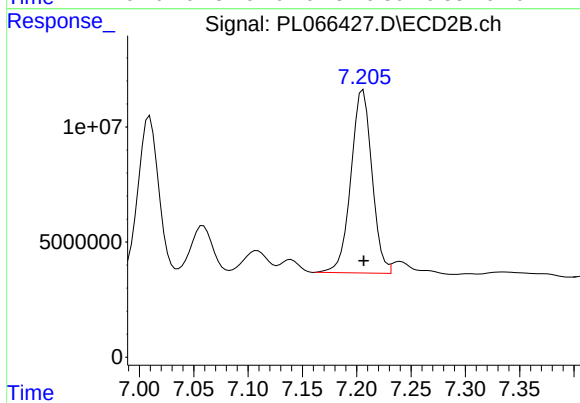

#27 Chlordane-5


R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 107192595
Conc: 744.83 ng/ml

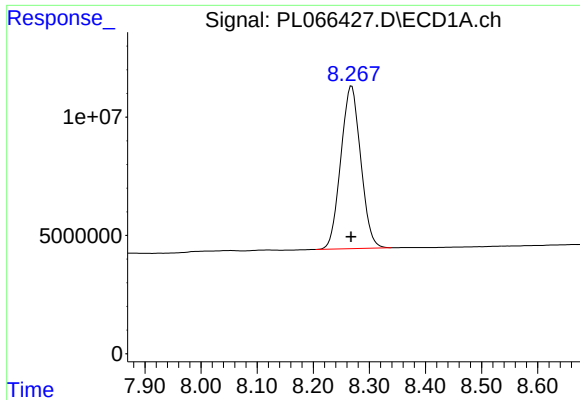

#28 Decachlorobiphenyl

R.T.: 8.269 min
Delta R.T.: 0.000 min
Response: 169226569
Conc: 73.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

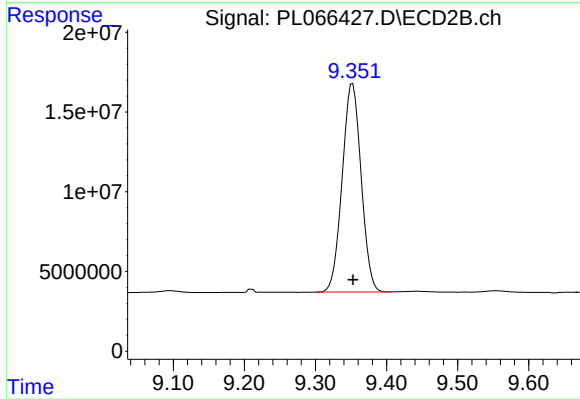

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 241919336
Conc: 72.38 ng/ml