

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
 Data File : PL066428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2021 20:35
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 00:17:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 23 00:16:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.437	4.153	158.3E6	206.5E6	50.000	50.000
28)	SA Decachlor...	8.268	9.353	115.9E6	167.1E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.302	5.173	51615246	92664437	500.000	500.000
24)	Chlordane-2	4.802	5.651	60423405	91232816	500.000	500.000
25)	Chlordane-3	5.371	6.310	163.9E6	359.8E6	500.000	500.000
26)	Chlordane-4	5.429	6.384	144.5E6	426.3E6	500.000	500.000
27)	Chlordane-5	6.269	7.207	54880105	71957491	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042221\
Data File : PL066428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2021 20:35
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 00:17:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042221.M
Quant Title : GC Extractables
QLast Update : Fri Apr 23 00:16:42 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

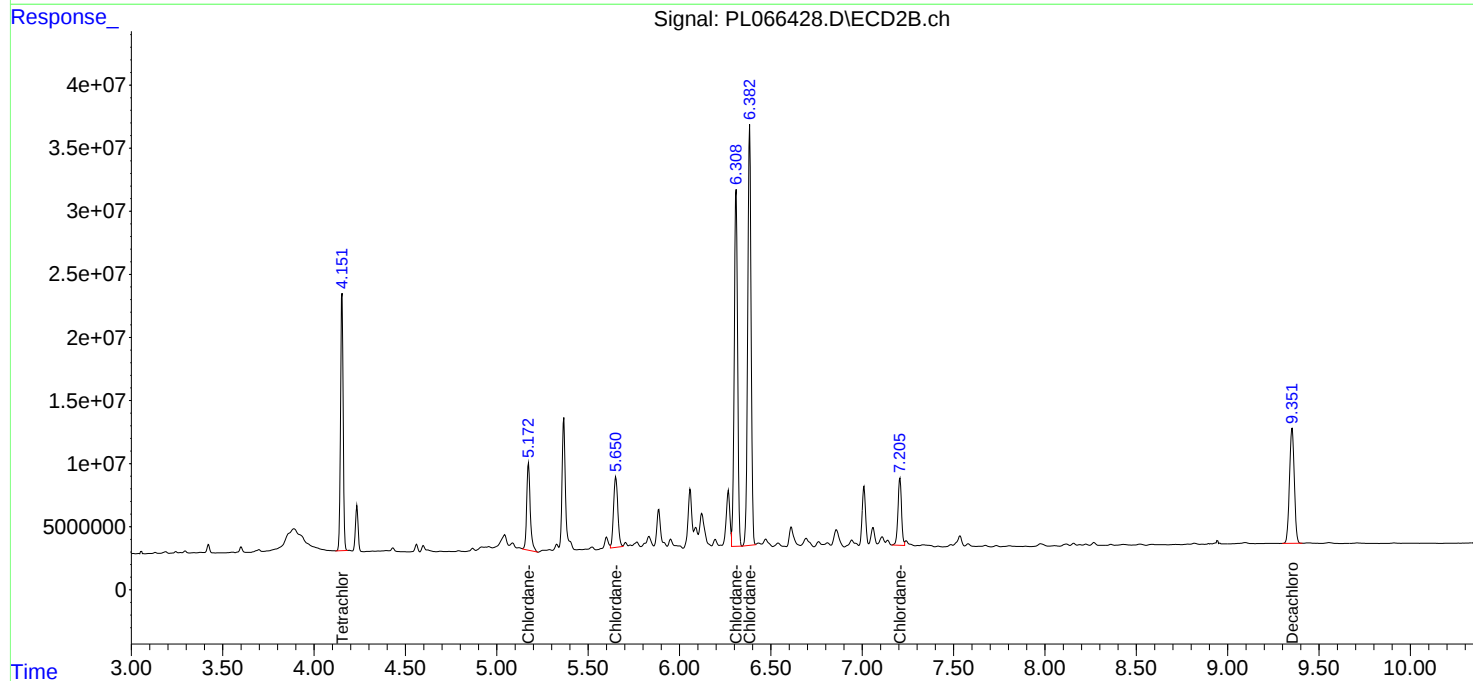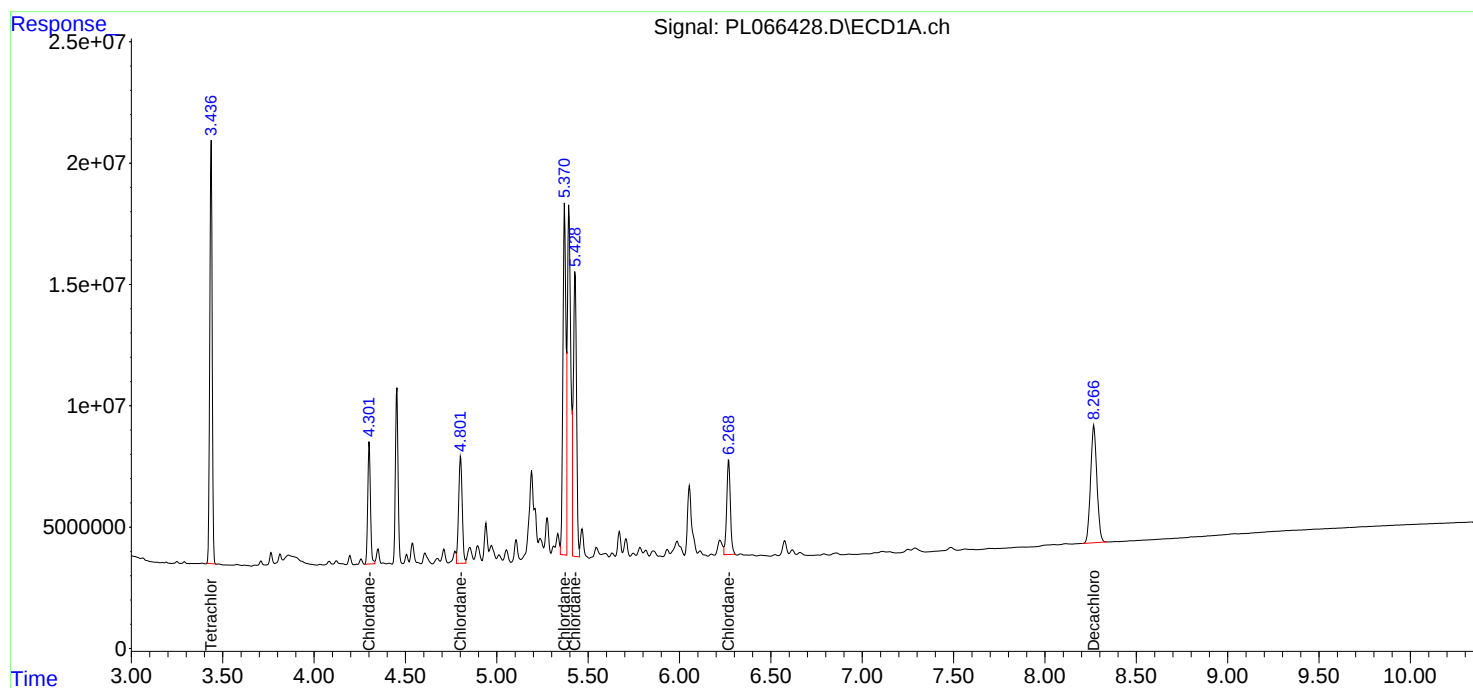


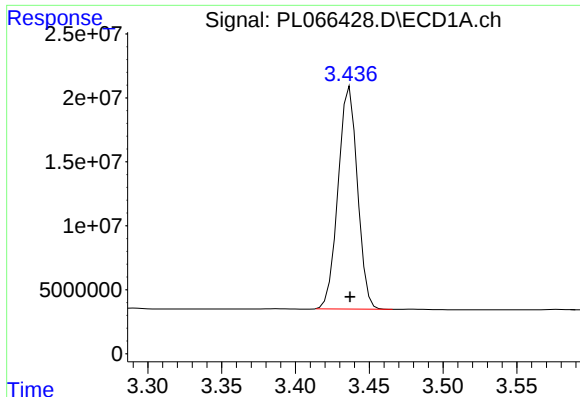

#1 Tetrachloro-m-xylene


R.T.: 3.437 min
Delta R.T.: 0.000 min
Response: 158348028
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

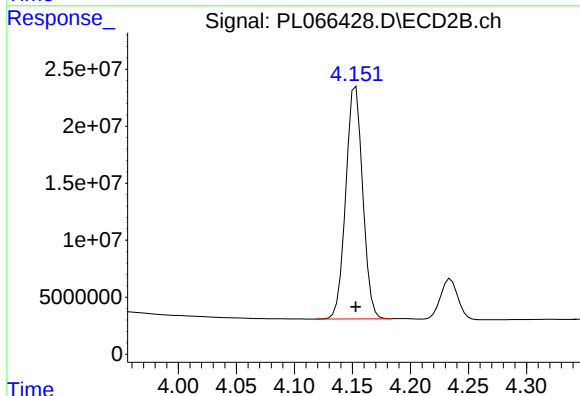


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 206455408
Conc: 50.00 ng/ml

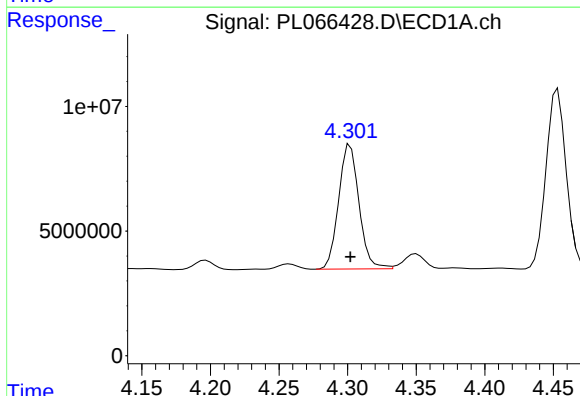


#23 Chlordane-1

R.T.: 4.302 min
Delta R.T.: 0.000 min
Response: 51615246
Conc: 500.00 ng/ml

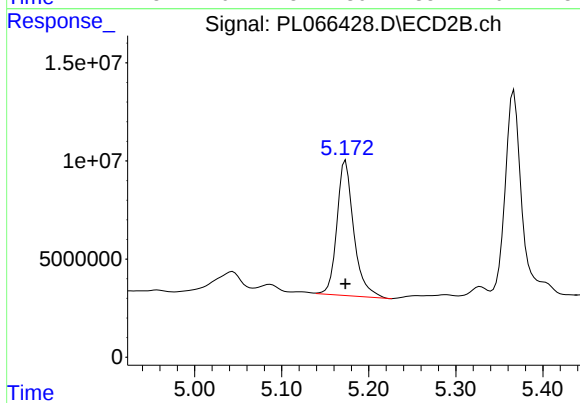

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 92664437
Conc: 500.00 ng/ml

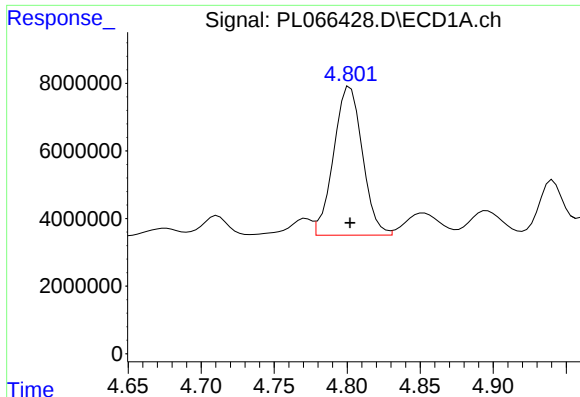

#24 Chlordane-2


R.T.: 4.802 min
Delta R.T.: 0.000 min
Response: 60423405
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

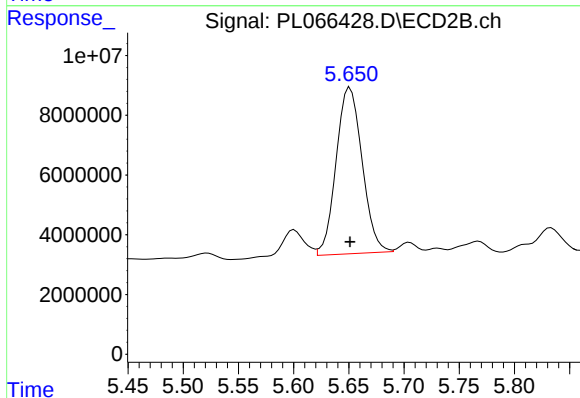


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 91232816
Conc: 500.00 ng/ml

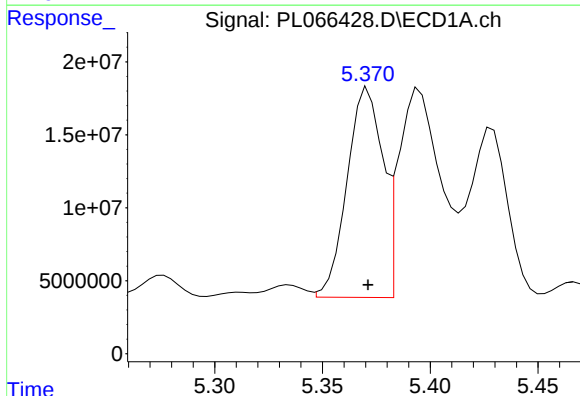


#25 Chlordane-3

R.T.: 5.371 min
Delta R.T.: 0.000 min
Response: 163901327
Conc: 500.00 ng/ml

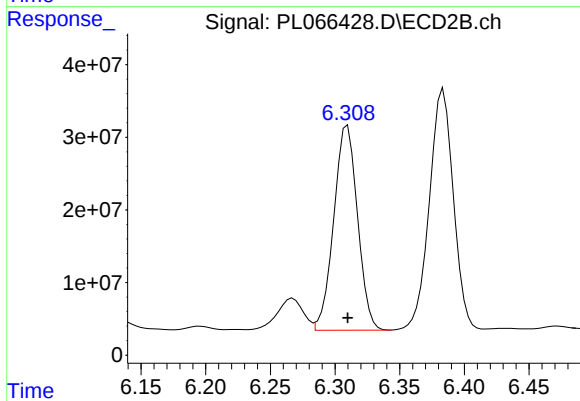

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 359816815
Conc: 500.00 ng/ml

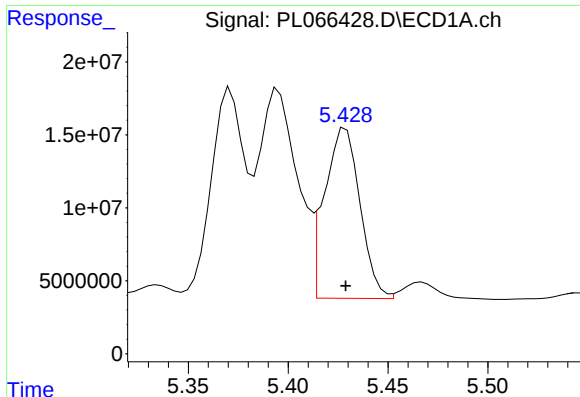

#26 Chlordane-4


R.T.: 5.429 min
Delta R.T.: 0.000 min
Response: 144482221
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

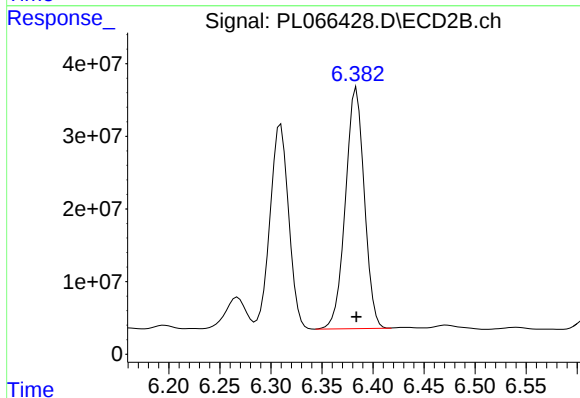


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 426333723
Conc: 500.00 ng/ml

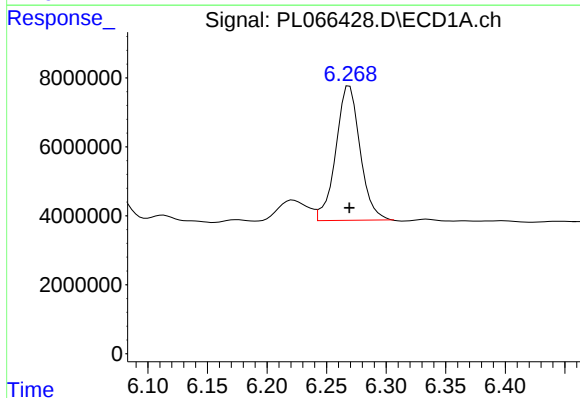


#27 Chlordane-5

R.T.: 6.269 min
Delta R.T.: 0.000 min
Response: 54880105
Conc: 500.00 ng/ml

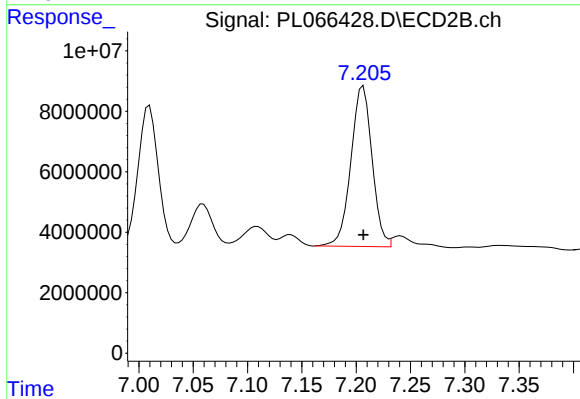

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 71957491
Conc: 500.00 ng/ml

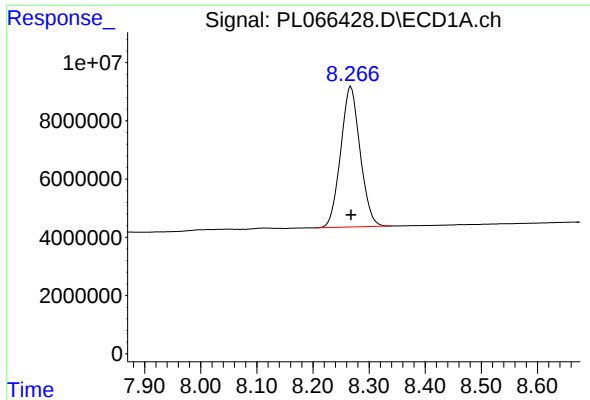

#28 Decachlorobiphenyl

R.T.: 8.268 min
Delta R.T.: 0.000 min
Response: 115894420
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

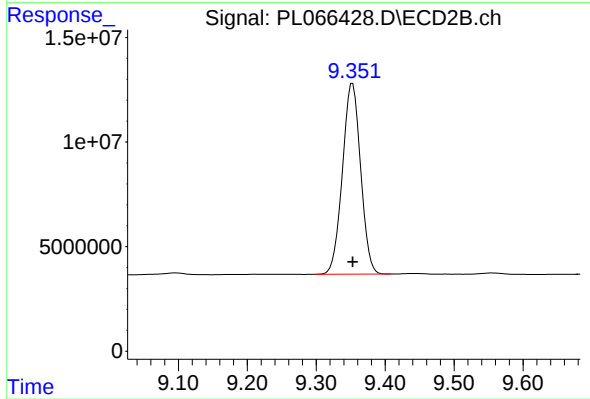

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 167111471
Conc: 50.00 ng/ml