

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042222\
 Data File : PL074297.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2022 13:09
 Operator : AR\AJ
 Sample : PB144296BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB144296BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 04/25/2022
 Supervised By : mohammad ahmed 04/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 22 23:05:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.488	6403734	34235333	19.819	19.201
28)	SA Decachlor...	10.400	11.328	10131144	35596572	19.482m	20.153

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042222\
Data File : PL074297.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2022 13:09
Operator : AR\AJ
Sample : PB144296BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB144296BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/25/2022
Supervised By : mohammad ahmed 04/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 22 23:05:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

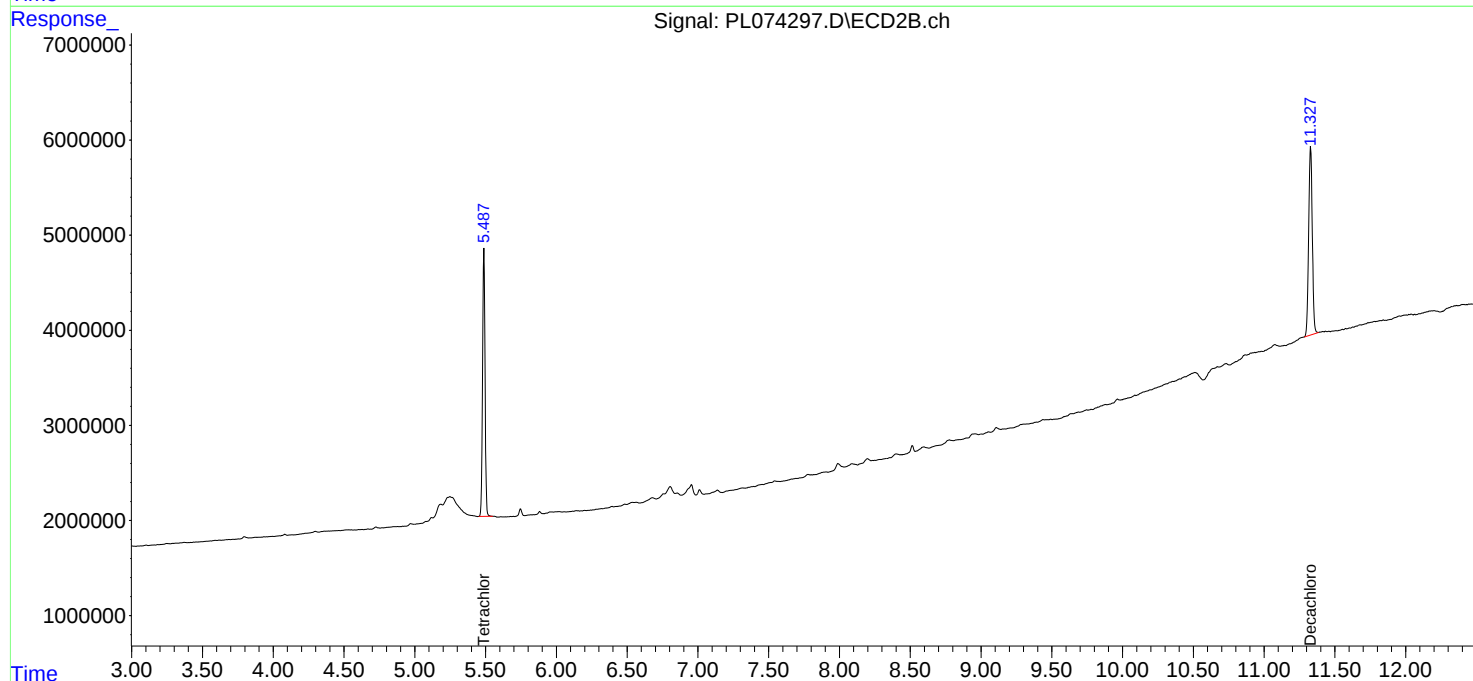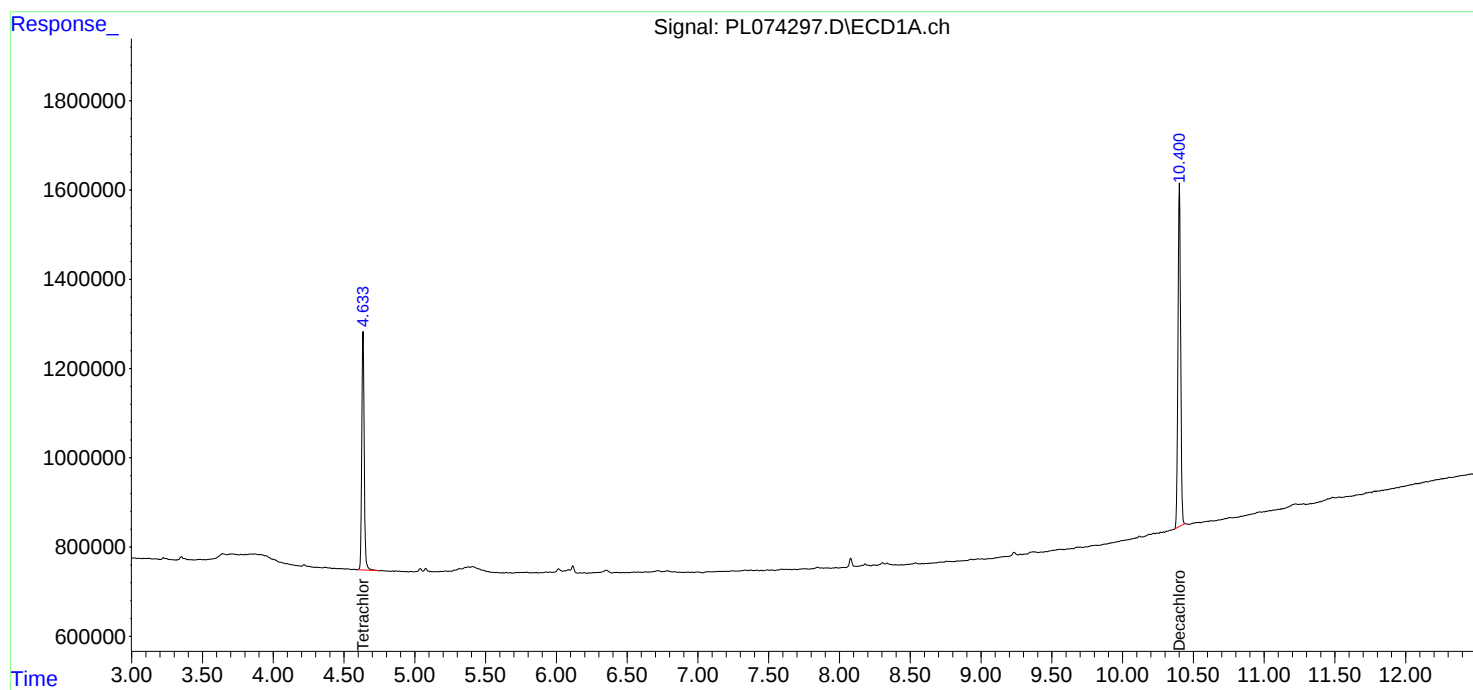

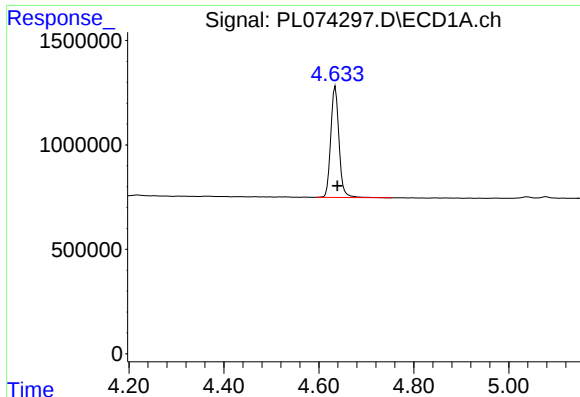


#1 Tetrachloro-m-xylene

R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 6403734
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB144296BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/25/2022
Supervised By :mohammad ahmed 04/25/2022

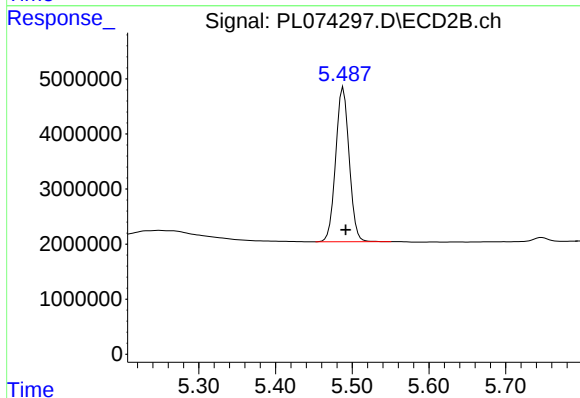


#1 Tetrachloro-m-xylene

R.T.: 5.488 min
Delta R.T.: -0.003 min
Response: 34235333
Conc: 19.20 ng/ml

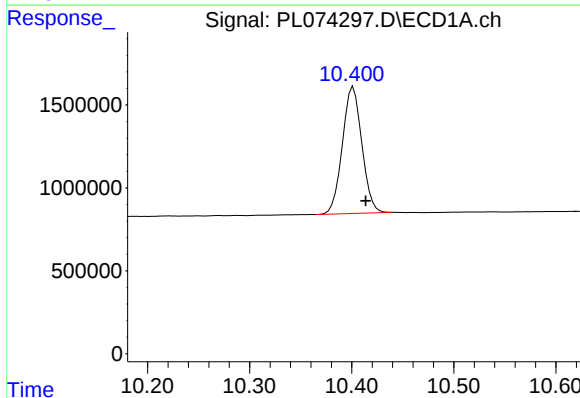

#28 Decachlorobiphenyl

R.T.: 10.400 min
Delta R.T.: -0.014 min
Response: 10131144
Conc: 19.48 ng/ml m

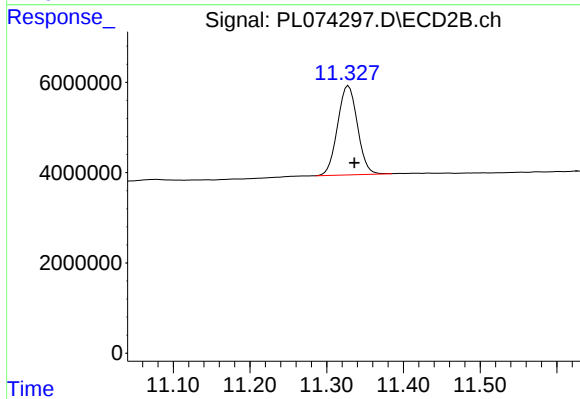

#28 Decachlorobiphenyl

R.T.: 11.328 min
Delta R.T.: -0.008 min
Response: 35596572
Conc: 20.15 ng/ml