

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042224\
 Data File : PL089113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Apr 2024 15:06
 Operator : AR\AJ
 Sample : P2177-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LKWD-BACKFILL-20

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 04:32:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 15 18:43:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.550	2.797	43072364	25854417	20.266	19.397
28)	SA Decachlor...	9.065	7.950	25950790	25007377	20.373	18.675

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042224\
Data File : PL089113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Apr 2024 15:06
Operator : AR\AJ
Sample : P2177-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-20

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 04:32:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041524.M
Quant Title : GC Extractables
QLast Update : Mon Apr 15 18:43:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

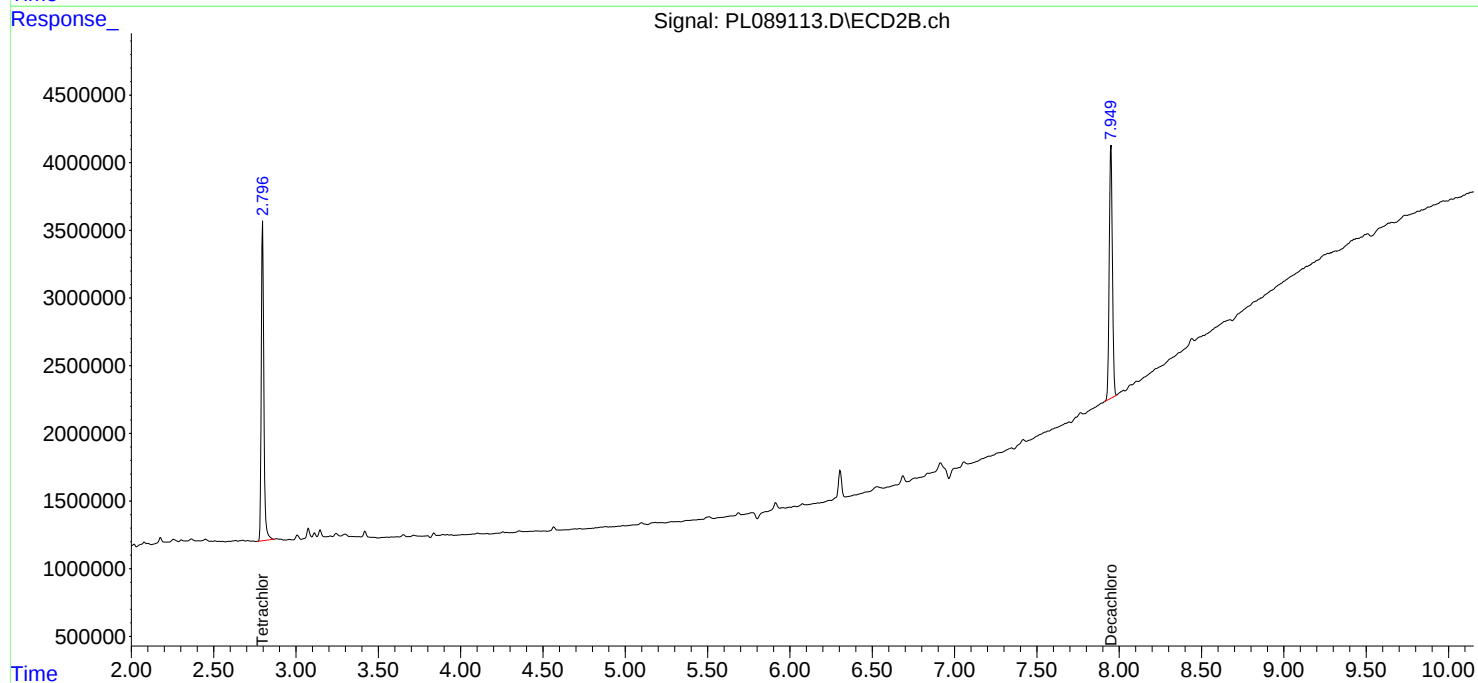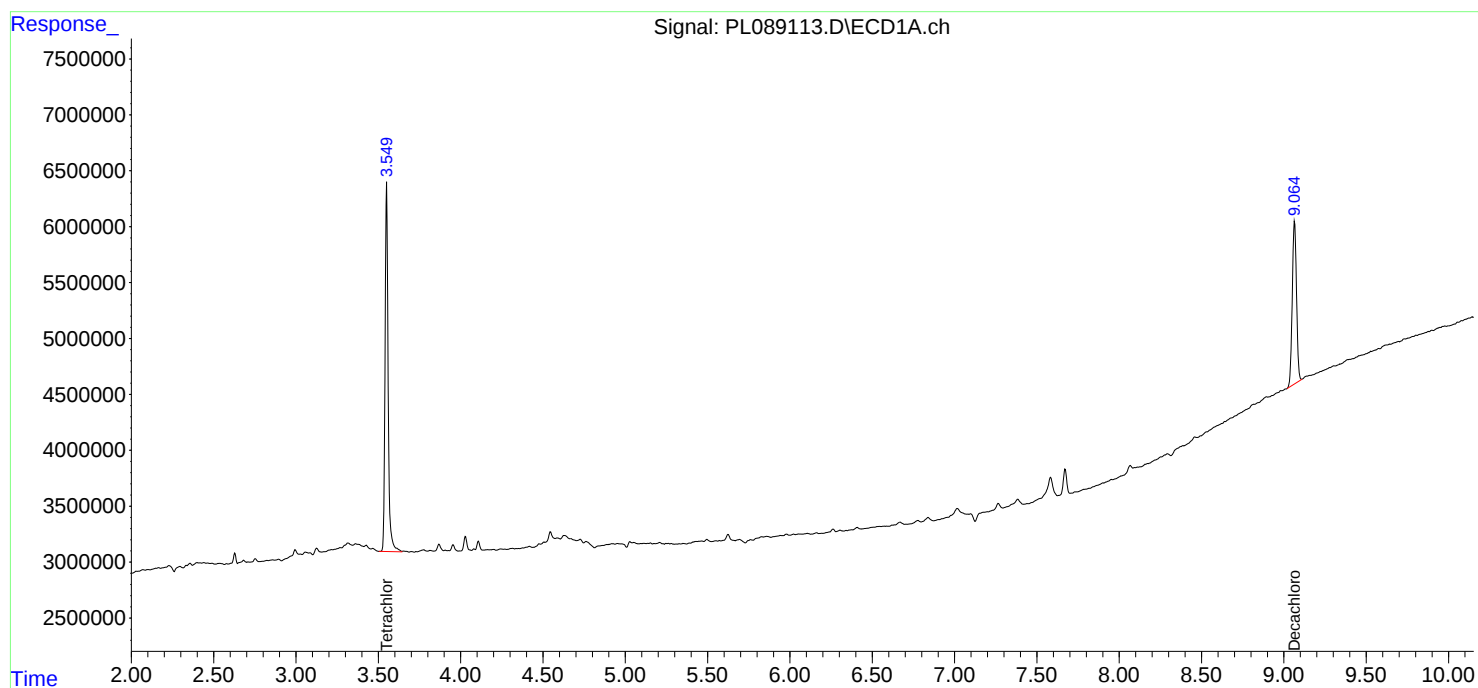


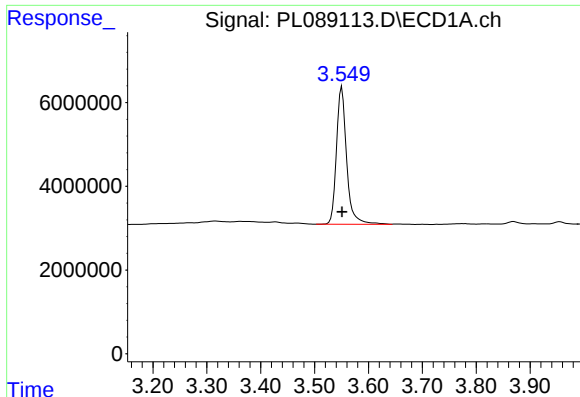

#1 Tetrachloro-m-xylene


R.T.: 3.550 min
Delta R.T.: 0.000 min
Response: 43072364
Conc: 20.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
LKWD-BACKFILL-20

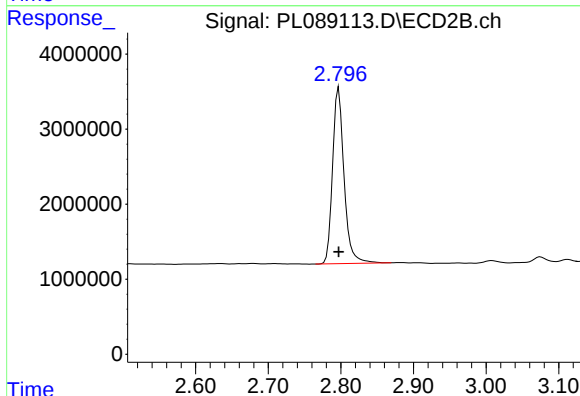


#1 Tetrachloro-m-xylene

R.T.: 2.797 min
Delta R.T.: 0.000 min
Response: 25854417
Conc: 19.40 ng/ml

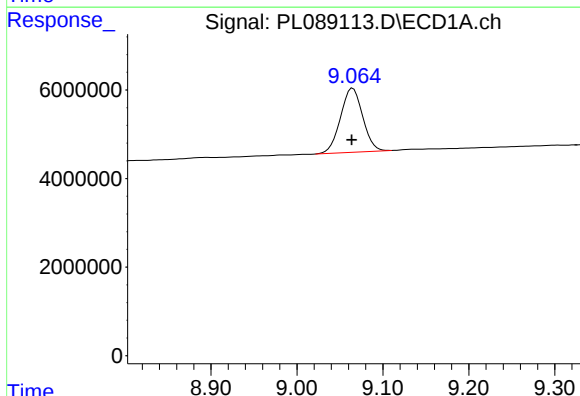

#28 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.001 min
Response: 25950790
Conc: 20.37 ng/ml

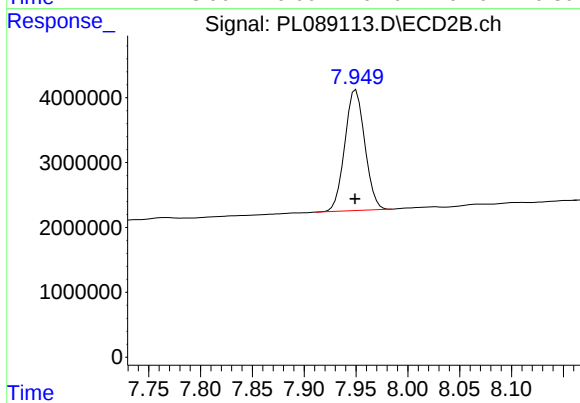

#28 Decachlorobiphenyl

R.T.: 7.950 min
Delta R.T.: 0.000 min
Response: 25007377
Conc: 18.67 ng/ml