

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047636.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 11:34
 Operator : AJ\SJ
 Sample : K2515-24
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-16

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 00:55:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.335	3.942	182.1E6	47570930	20.529	17.821
28)	SA Decachlor...	8.009	8.983	177.5E6	49175322	17.574	16.200
Target Compounds							
4)	MA Heptachlor	0.000	5.125	0	2013132	N.D.	0.546 #
7)	B delta-BHC	0.000	4.977f	0	2102152	N.D.	0.783 #
17)	MA 4,4'-DDT	0.000	7.073f	0	1855466	N.D.	0.747 #
23)	Chlordane-1	4.187	0.000	6305702	0	16.026	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047636.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 11:34
Operator : AJ\SJ
Sample : K2515-24
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-16

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 00:55:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

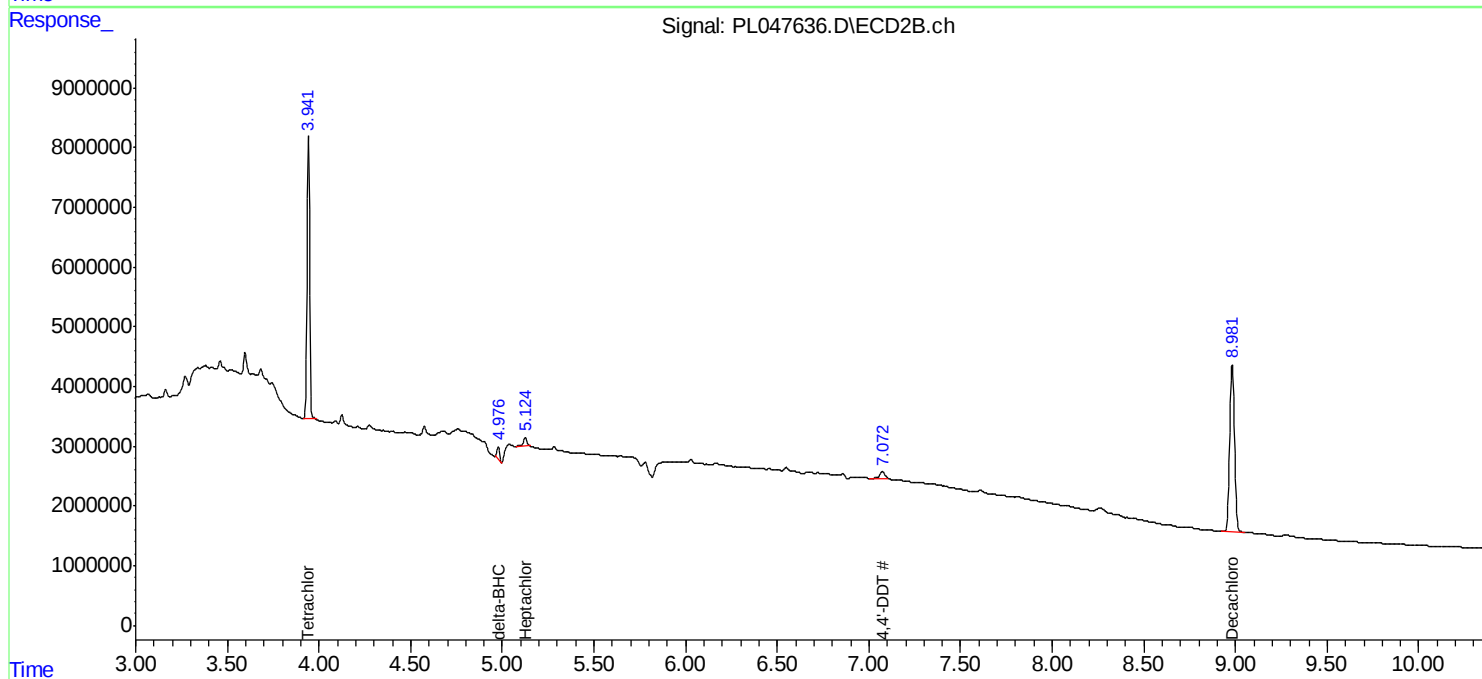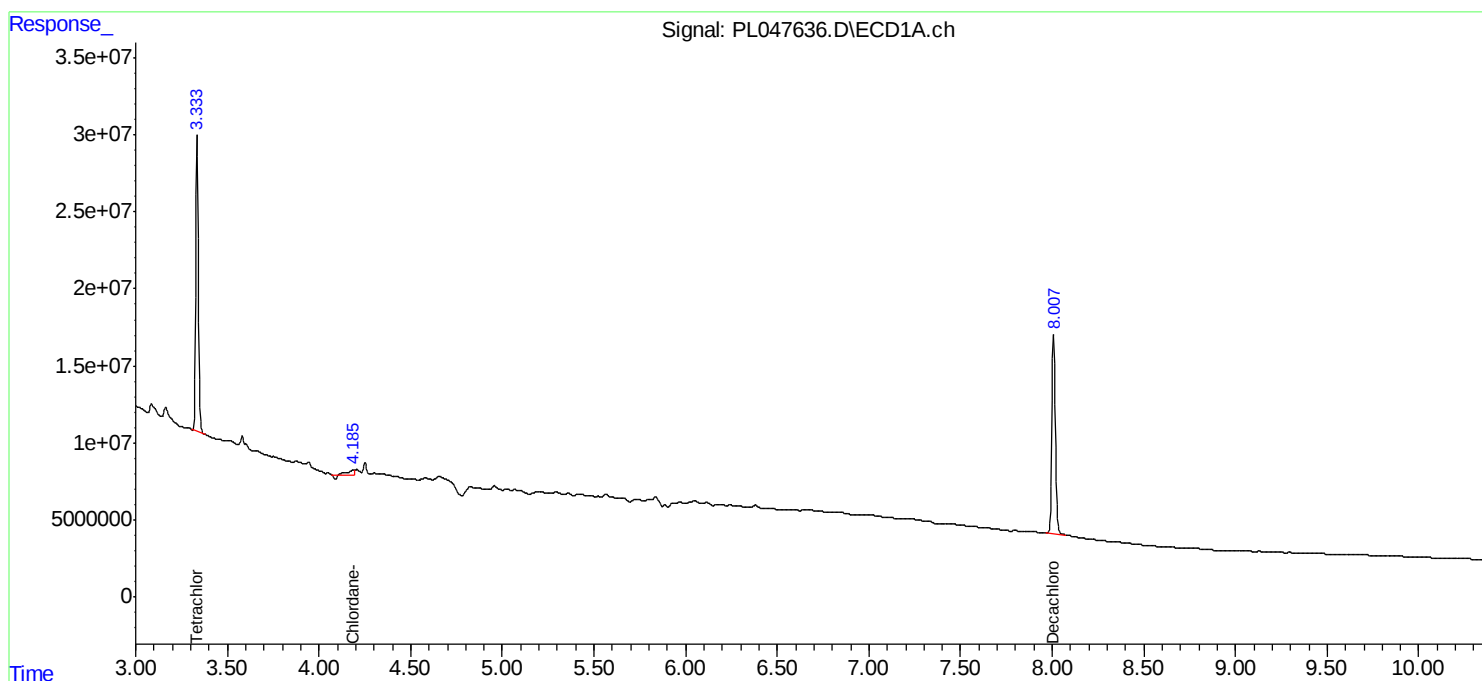


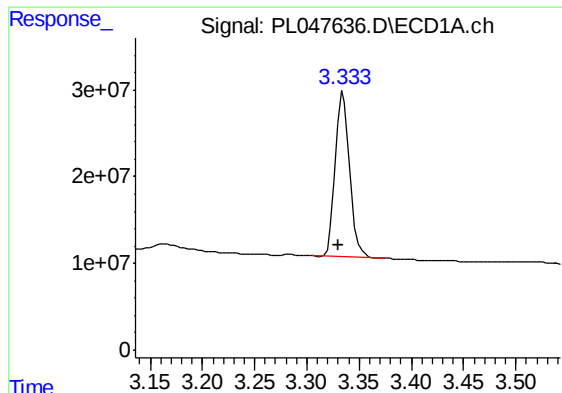

#1 Tetrachloro-m-xylene


R.T.: 3.335 min
Delta R.T.: 0.005 min
Response: 182148953
Conc: 20.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-16

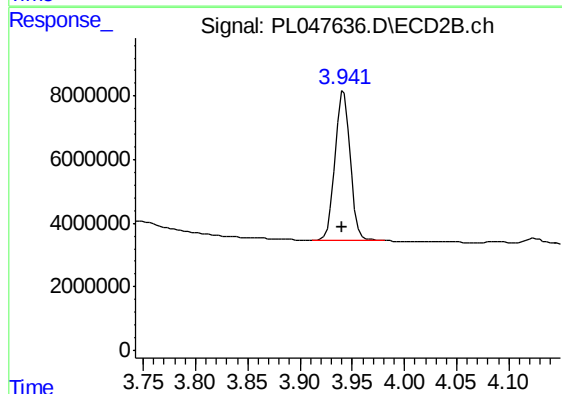


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.001 min
Response: 47570930
Conc: 17.82 ng/ml

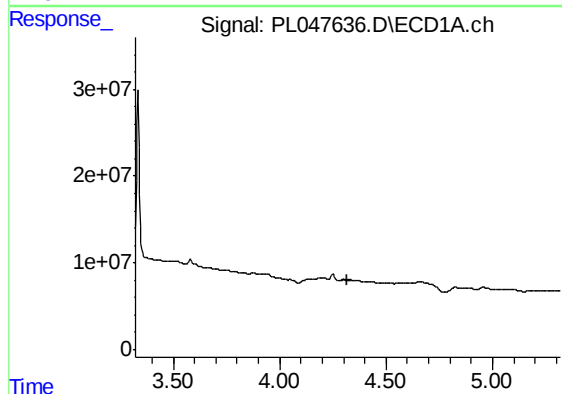


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.320 min
Response: 0
Conc: N.D.

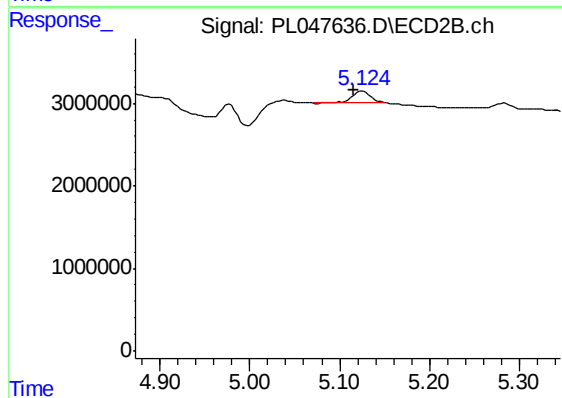

#4 Heptachlor


R.T.: 5.125 min
Delta R.T.: 0.010 min
Response: 2013132
Conc: 0.55 ng/ml

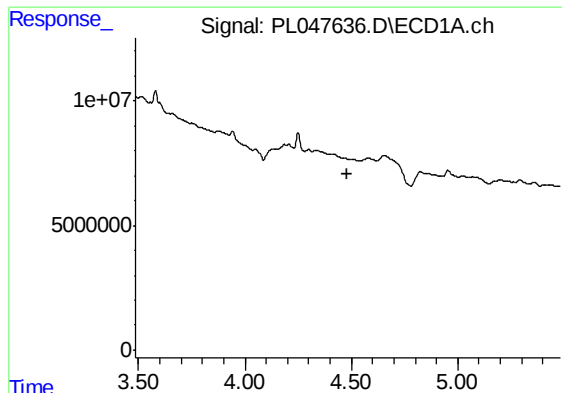

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.483 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-16

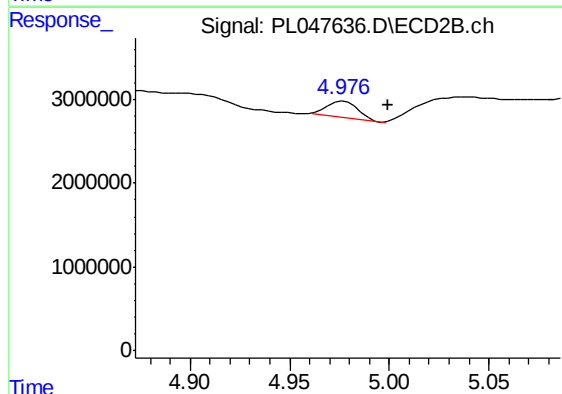


#7 delta-BHC

R.T.: 4.977 min
Delta R.T.: -0.022 min
Response: 2102152
Conc: 0.78 ng/ml

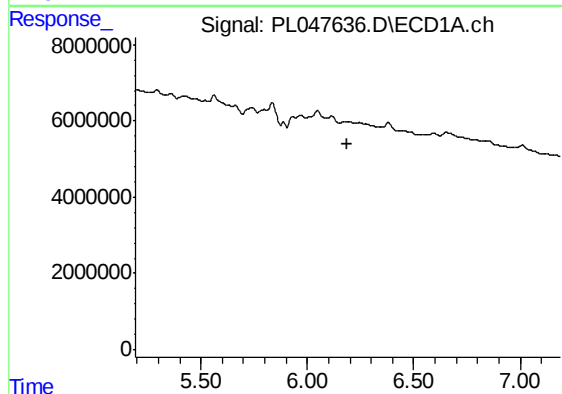


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.190 min
Response: 0
Conc: N.D.

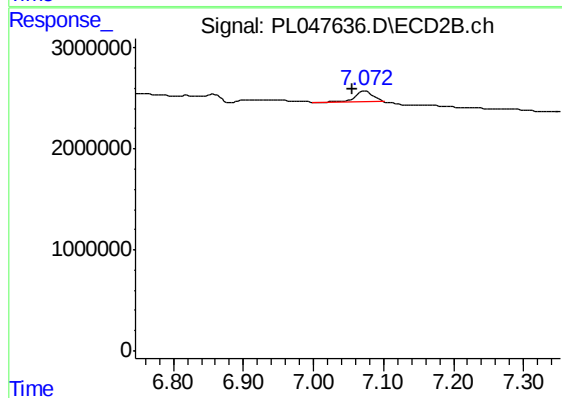

#17 4,4'-DDT


R.T.: 7.073 min
Delta R.T.: 0.018 min
Response: 1855466
Conc: 0.75 ng/ml

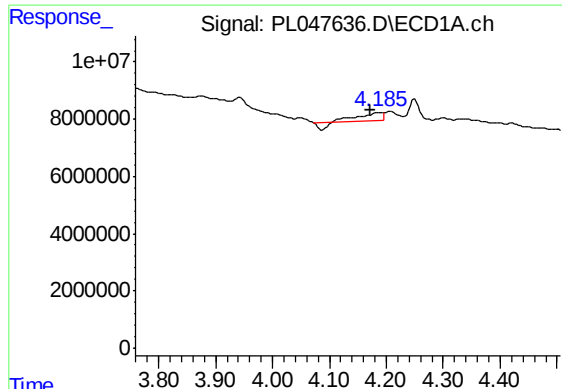

#23 Chlordane-1


R.T.: 4.187 min
Delta R.T.: 0.014 min
Response: 6305702
Conc: 16.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-16

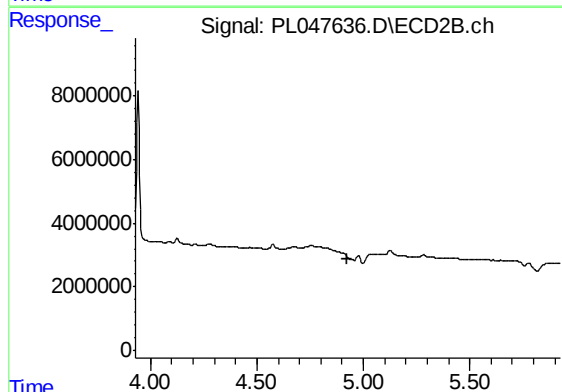


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.927 min
Response: 0
Conc: N.D.

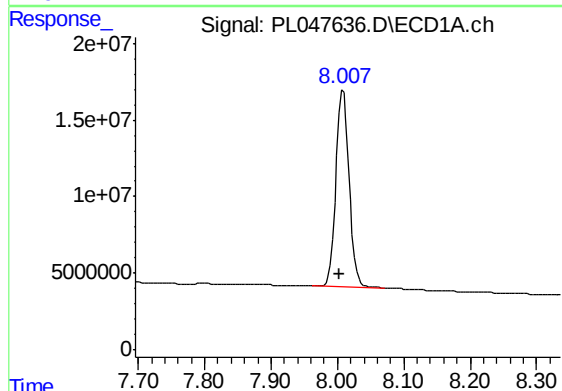

#28 Decachlorobiphenyl

R.T.: 8.009 min
Delta R.T.: 0.006 min
Response: 177527390
Conc: 17.57 ng/ml

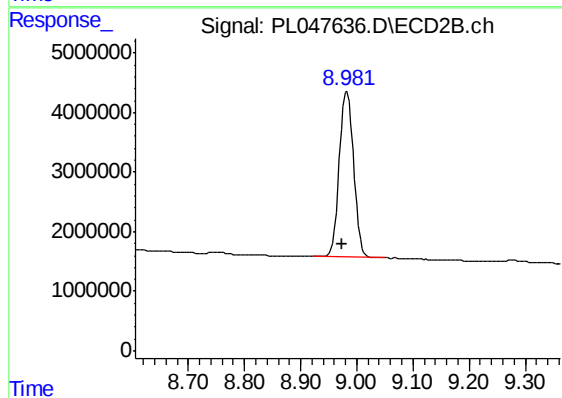

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: 0.008 min
Response: 49175322
Conc: 16.20 ng/ml