

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 12:04
 Operator : AJ\SJ
 Sample : K2515-03RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-15RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 00:55:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.941	46098635	12294839	5.196	4.606
28)	SA Decachlor...	8.002	8.979	103.5E6	28874903	10.246	9.512
Target Compounds							
10)	B gamma-Chl...	5.240f	0.000	10188189	0	0.833	N.D. #
11)	B alpha-Chl...	0.000	6.115	0	2910892	N.D.	0.909 #
25)	Chlordane-3	5.240f	0.000	10188189	0	7.431	N.D. #
26)	Chlordane-4	0.000	6.115	0	2910892	N.D.	6.162 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 12:04
Operator : AJ\SJ
Sample : K2515-03RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-15RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 00:55:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

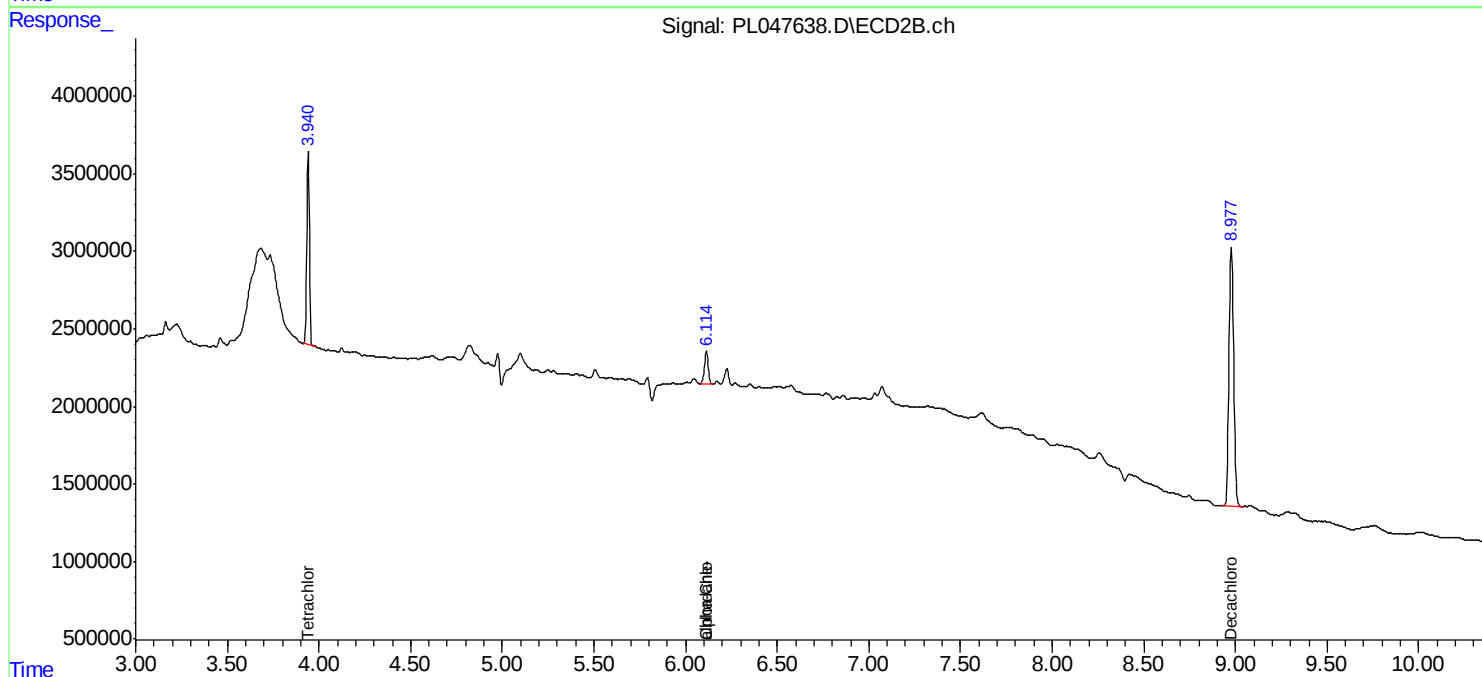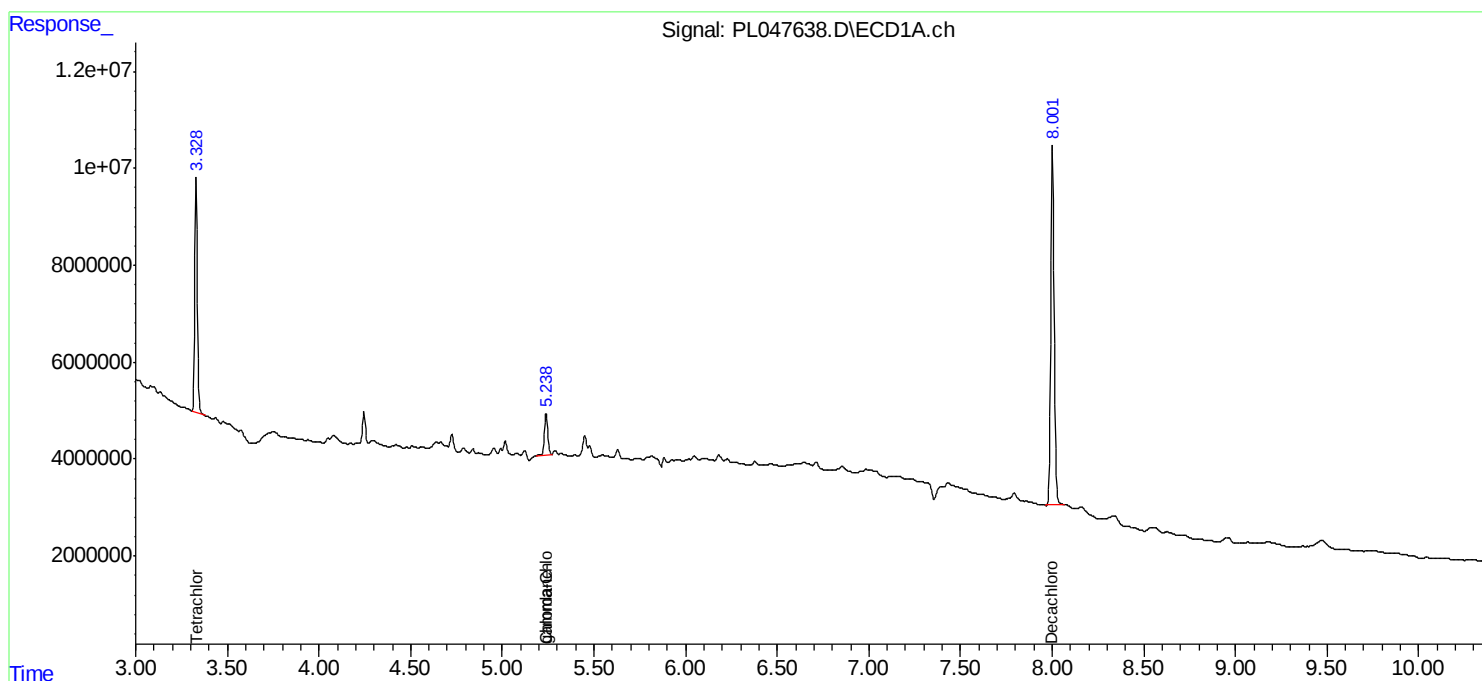


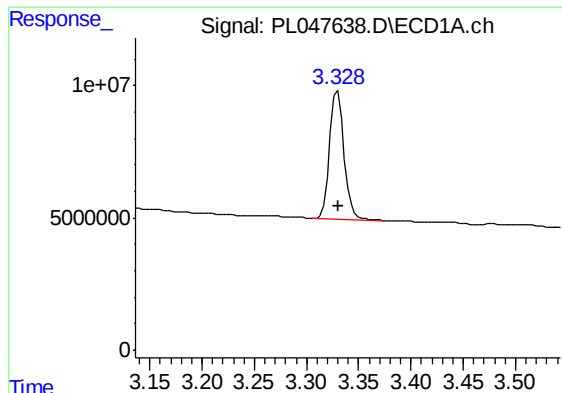

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 46098635
Conc: 5.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-15RE

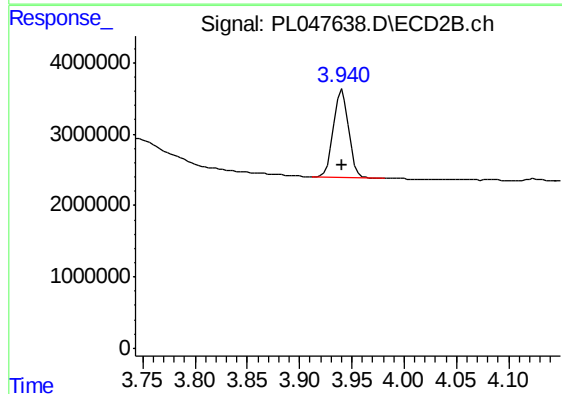


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 12294839
Conc: 4.61 ng/ml

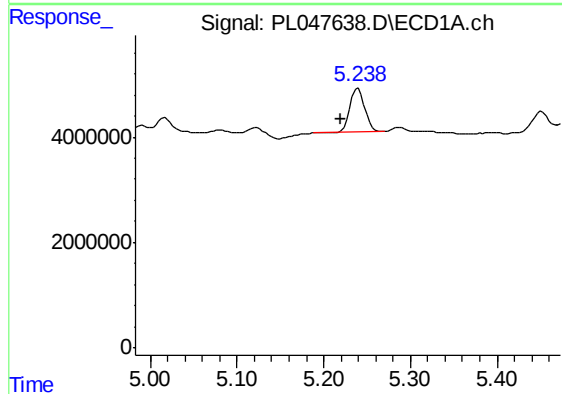


#10 gamma-Chlordane

R.T.: 5.240 min
Delta R.T.: 0.020 min
Response: 10188189
Conc: 0.83 ng/ml

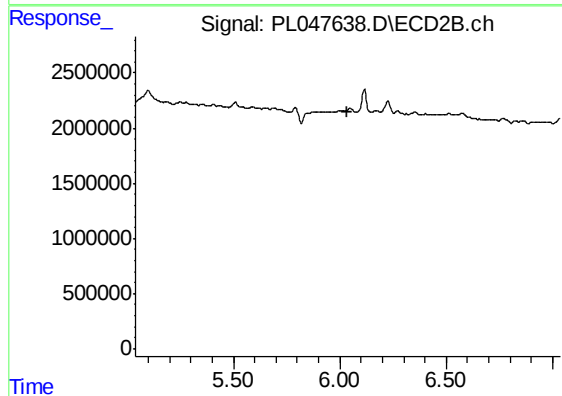

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.037 min
Response: 0
Conc: N.D.

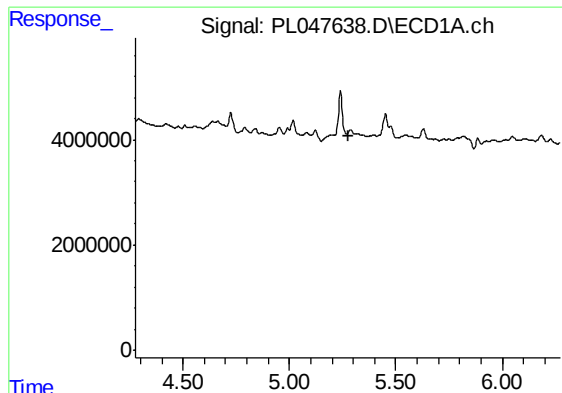

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15RE

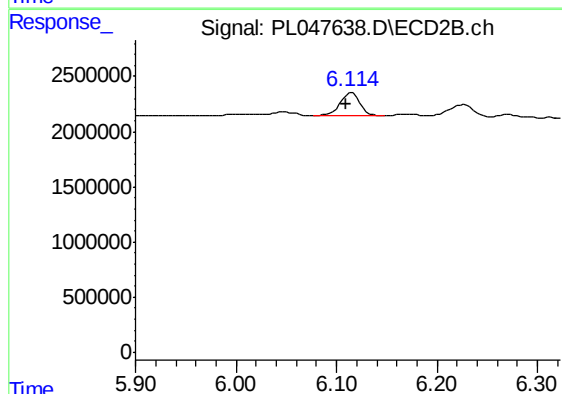


#11 alpha-Chlordane

R.T.: 6.115 min
Delta R.T.: 0.006 min
Response: 2910892
Conc: 0.91 ng/ml

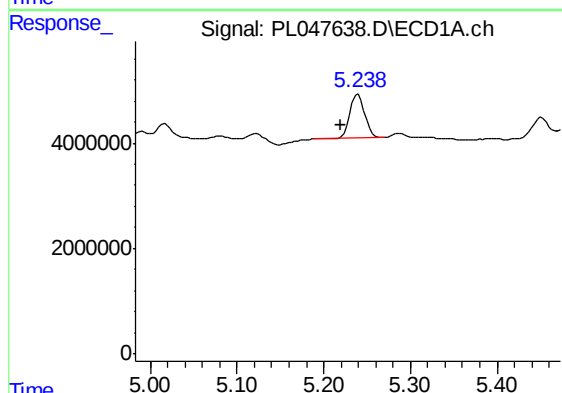


#25 Chlordane-3

R.T.: 5.240 min
Delta R.T.: 0.019 min
Response: 10188189
Conc: 7.43 ng/ml

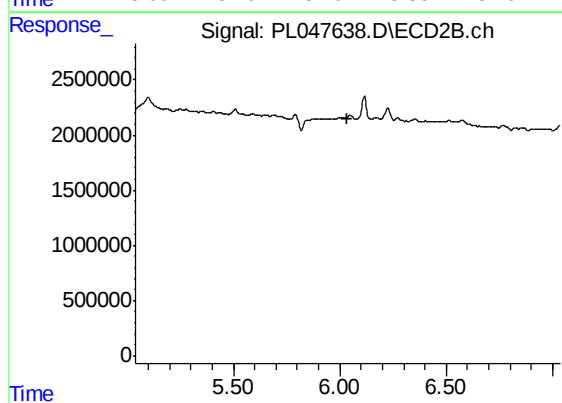

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.037 min
Response: 0
Conc: N.D.

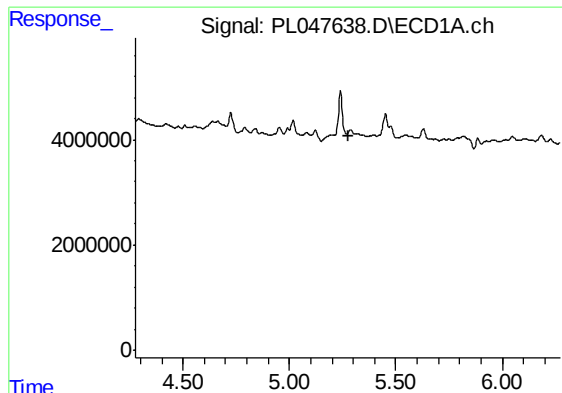

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-15RE

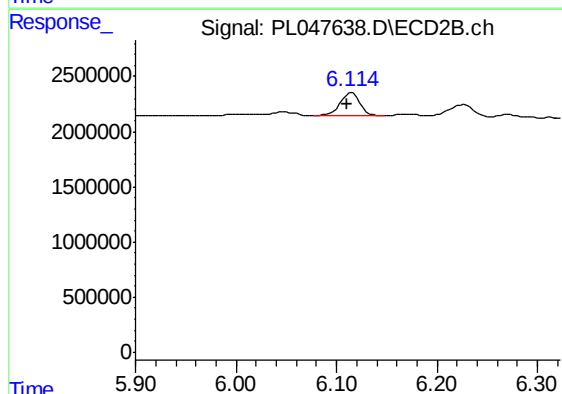


#26 Chlordane-4

R.T.: 6.115 min
Delta R.T.: 0.005 min
Response: 2910892
Conc: 6.16 ng/ml

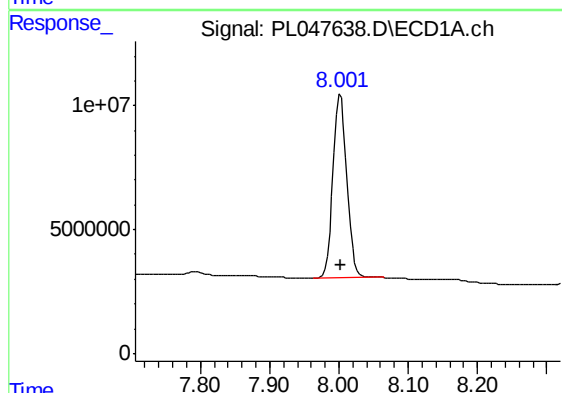

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 103499541
Conc: 10.25 ng/ml

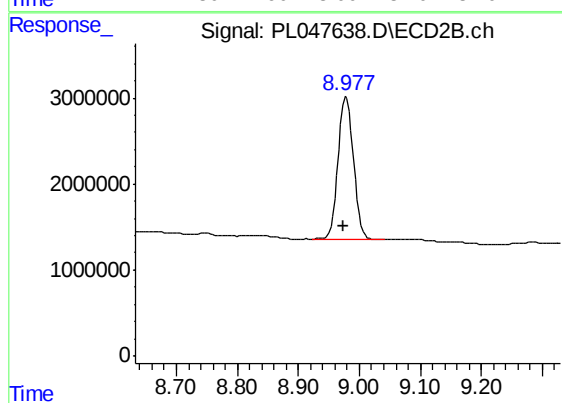

#28 Decachlorobiphenyl

R.T.: 8.979 min
Delta R.T.: 0.004 min
Response: 28874903
Conc: 9.51 ng/ml