

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 17:27
 Operator : AJ\SJ
 Sample : K2522-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WELL-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:00:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.941	163.2E6	42516833	18.393	15.927
28)	SA Decachlor...	8.003	8.982	146.8E6	41144296	14.534	13.554
Target Compounds							
2)	A alpha-BHC	3.775f	0.000	19259670	0	1.373	N.D. #
3)	MA gamma-BHC...	4.044	0.000	9561213	0	0.790	N.D. #
7)	B delta-BHC	0.000	5.028f	0	754472	N.D.	0.281 #
9)	A Endosulfan I	0.000	6.173	0	3552842	N.D.	1.198 #
11)	B alpha-Chl...	5.288	0.000	23204585	0	1.931	N.D. #
15)	B Endosulfa...	6.114f	0.000	29782890	0	2.813	N.D. #
26)	Chlordane-4	5.288	0.000	23204585	0	18.307	N.D. #
27)	Chlordane-5	6.114f	0.000	29782890	0	76.306	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 17:27
Operator : AJ\SJ
Sample : K2522-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WELL-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:00:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

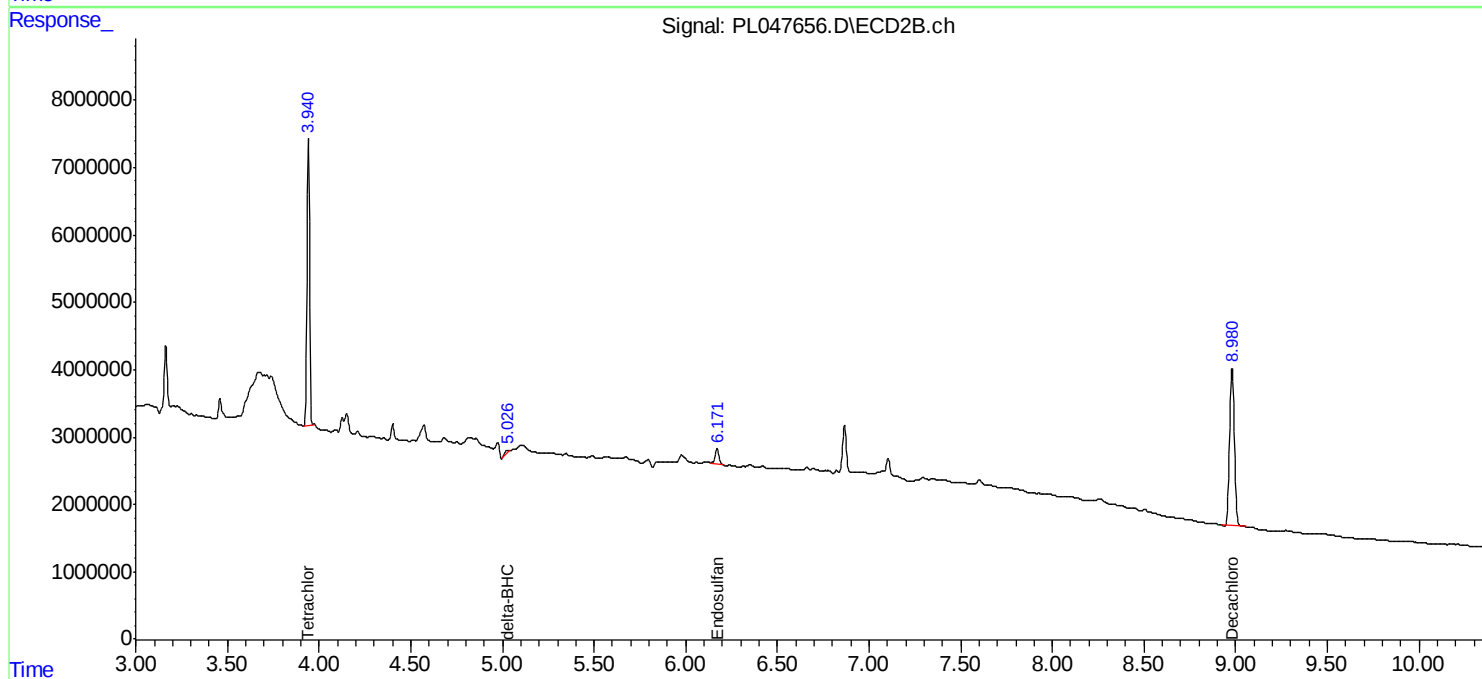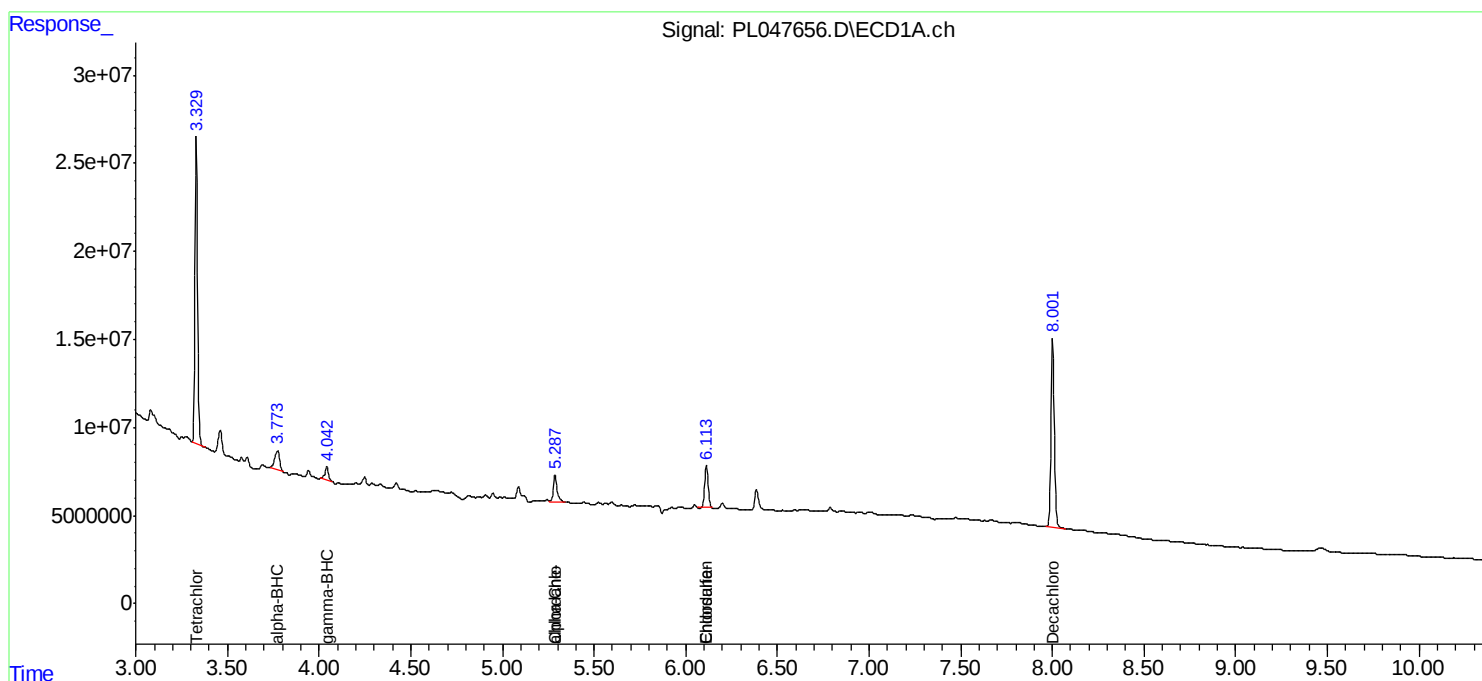


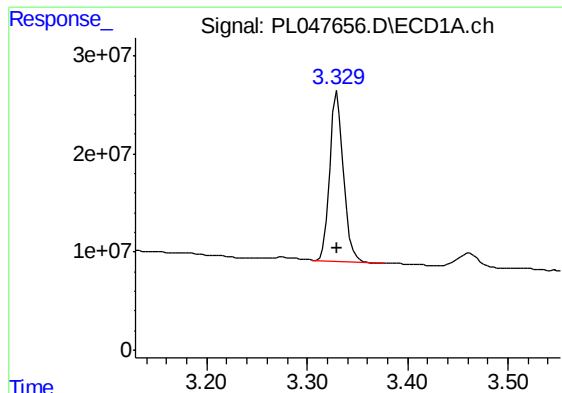

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 163196572
Conc: 18.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-1

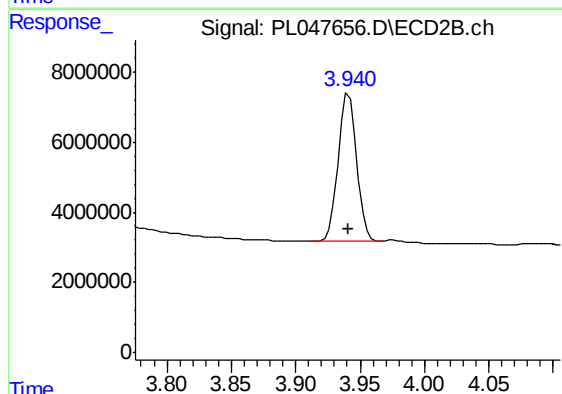


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 42516833
Conc: 15.93 ng/ml

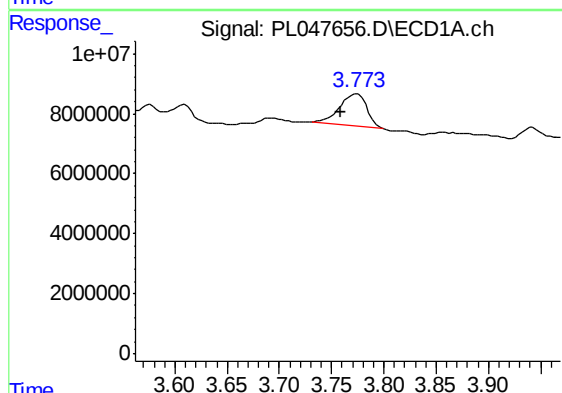


#2 alpha-BHC

R.T.: 3.775 min
Delta R.T.: 0.016 min
Response: 19259670
Conc: 1.37 ng/ml

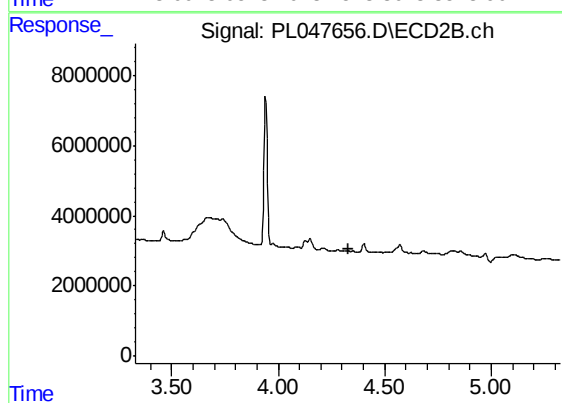

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.328 min
Response: 0
Conc: N.D.

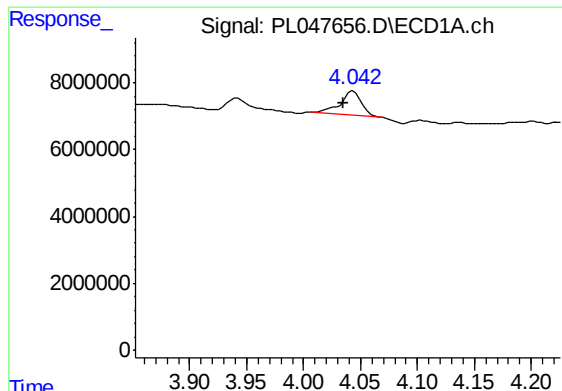

#3 gamma-BHC (Lindane)


R.T.: 4.044 min
Delta R.T.: 0.009 min
Response: 9561213
Conc: 0.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-1

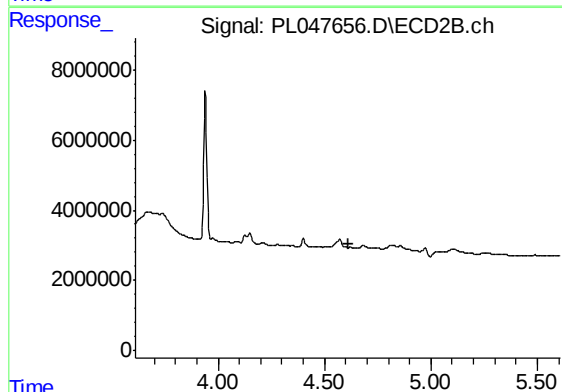


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.611 min
Response: 0
Conc: N.D.

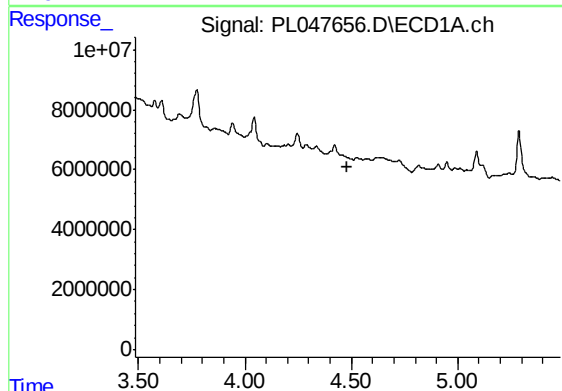


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

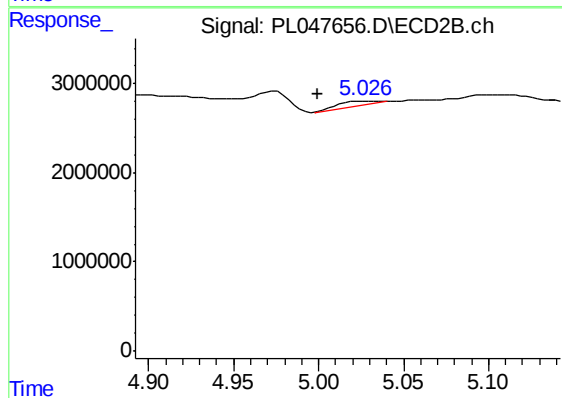

#7 delta-BHC


R.T.: 5.028 min
Delta R.T.: 0.029 min
Response: 754472
Conc: 0.28 ng/ml

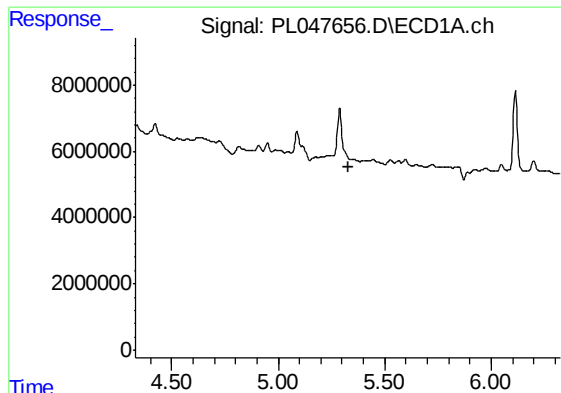

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WELL-1

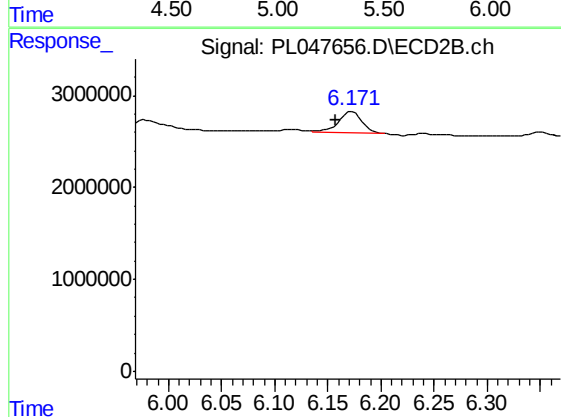


#9 Endosulfan I

R.T.: 6.173 min
Delta R.T.: 0.015 min
Response: 3552842
Conc: 1.20 ng/ml

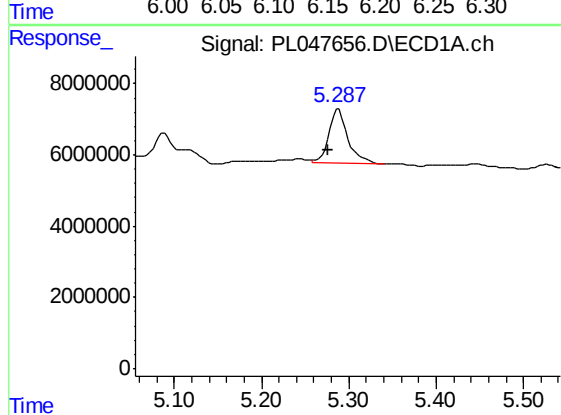


#11 alpha-Chlordane

R.T.: 5.288 min
Delta R.T.: 0.012 min
Response: 23204585
Conc: 1.93 ng/ml

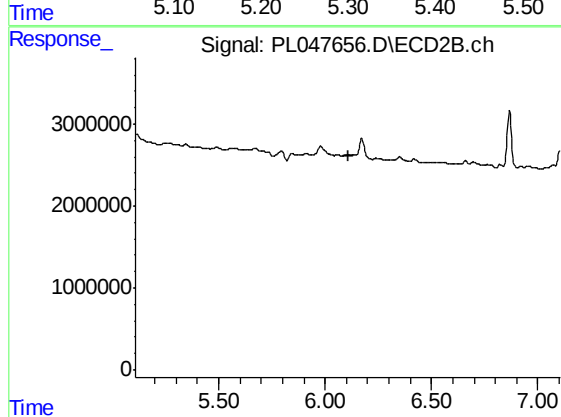

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

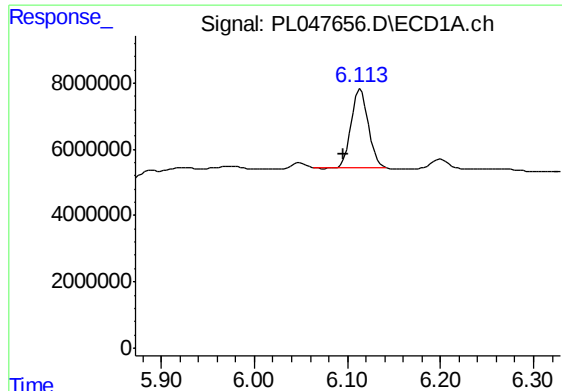

#15 Endosulfan II


R.T.: 6.114 min
Delta R.T.: 0.019 min
Response: 29782890
Conc: 2.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-1

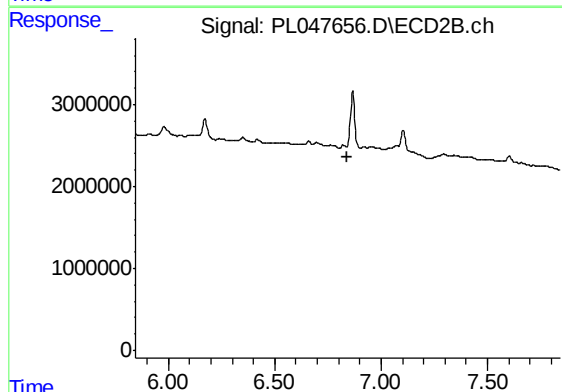


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.842 min
Response: 0
Conc: N.D.

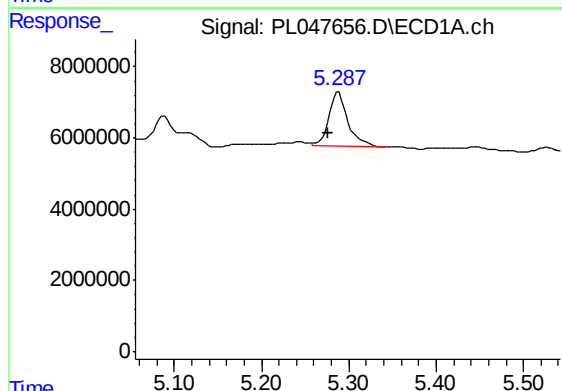


#26 Chlordane-4

R.T.: 5.288 min
Delta R.T.: 0.013 min
Response: 23204585
Conc: 18.31 ng/ml

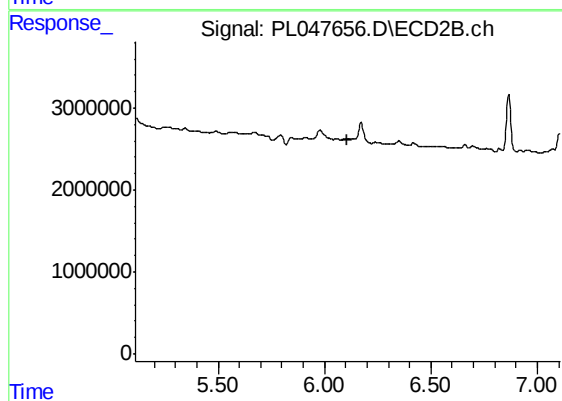

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.110 min
Response: 0
Conc: N.D.

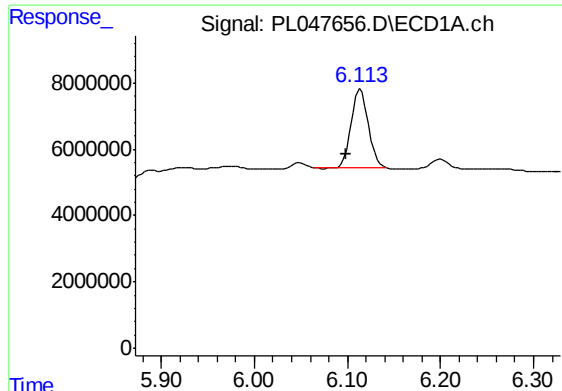

#27 Chlordane-5


R.T.: 6.114 min
Delta R.T.: 0.015 min
Response: 29782890
Conc: 76.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-1

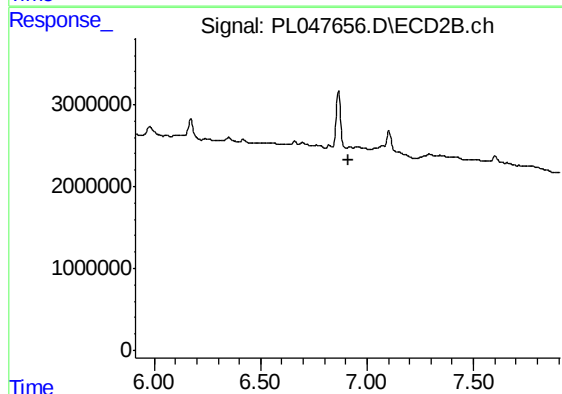


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

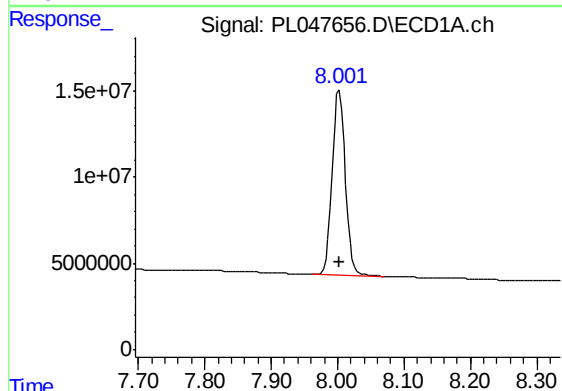

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 146811967
Conc: 14.53 ng/ml

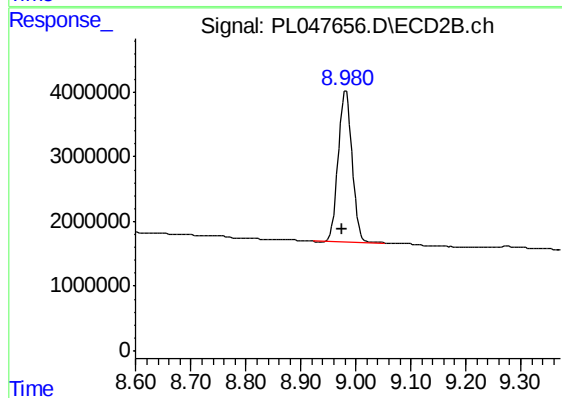

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.007 min
Response: 41144296
Conc: 13.55 ng/ml