

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047657.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 17:42
 Operator : AJ\SJ
 Sample : K2522-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WELL-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:00:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	183.6E6	49796244	20.690	18.654
28)	SA Decachlor...	8.003	8.981	152.3E6	41969902	15.076	13.826
Target Compounds							
3)	MA gamma-BHC...	4.043	0.000	9775034	0	0.808	N.D. #
8)	B Heptachlo...	5.009	0.000	59694609	0	5.098	N.D. #
9)	A Endosulfan I	0.000	6.173	0	2640671	N.D.	0.890 #
10)	B gamma-Chl...	0.000	6.056f	0	16835877	N.D.	5.326 #
11)	B alpha-Chl...	5.287	0.000	28125797	0	2.340	N.D. #
13)	MA Dieldrin	5.597f	0.000	59124781	0	4.964	N.D. #
15)	B Endosulfa...	6.114f	6.866f	23404590	3012824	2.210	1.086 #
25)	Chlordane-3	0.000	6.056f	0	16835877	N.D.	41.964 #
26)	Chlordane-4	5.287	0.000	28125797	0	22.189	N.D. #
27)	Chlordane-5	6.114f	0.000	23404590	0	59.964	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047657.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 17:42
Operator : AJ\SJ
Sample : K2522-04
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
WELL-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:00:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

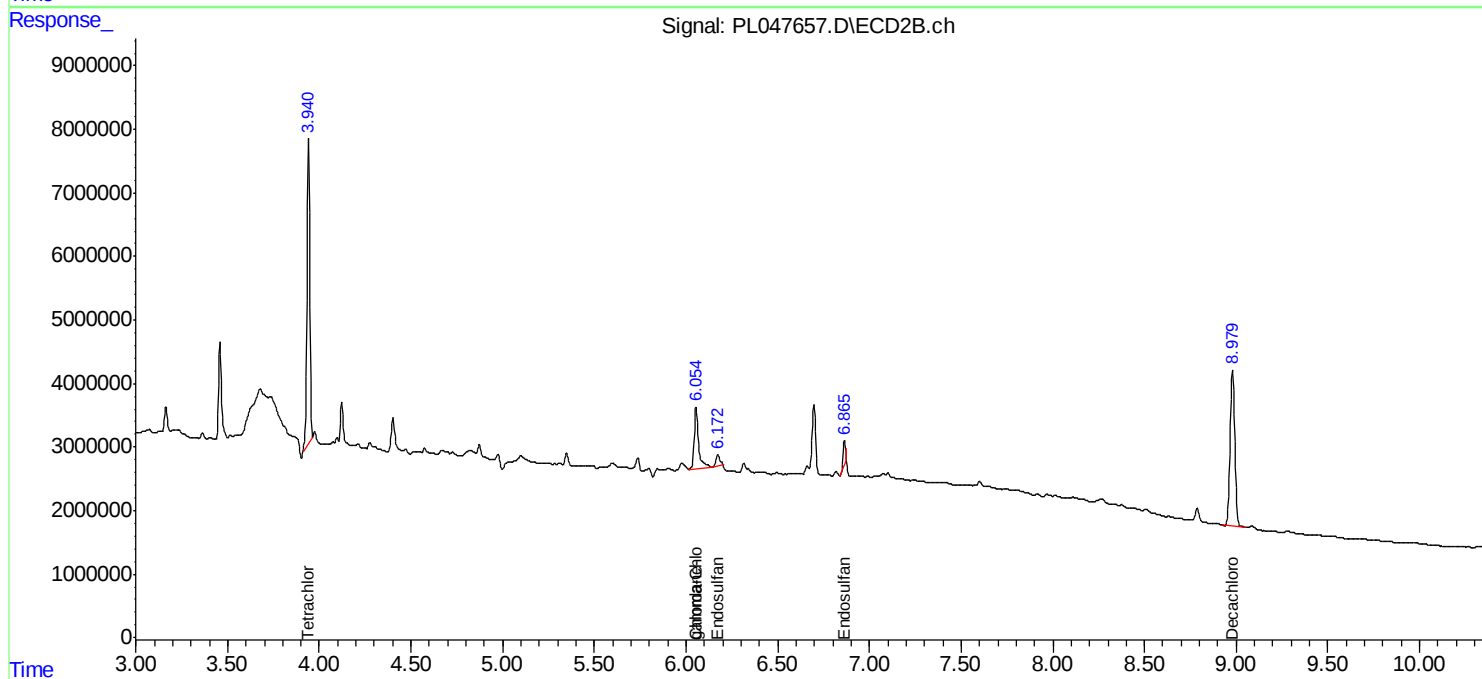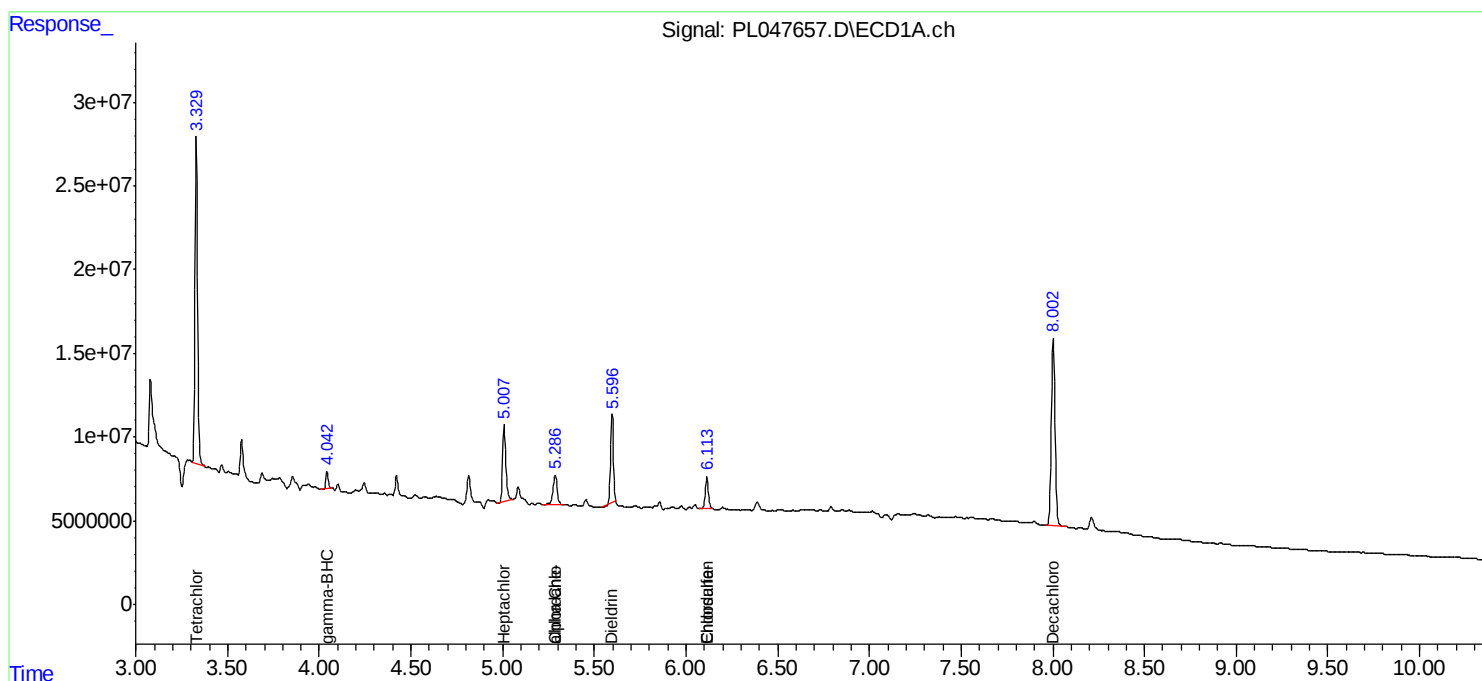


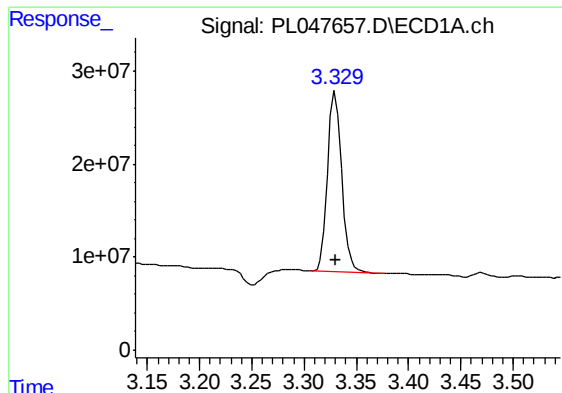

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 183577571
Conc: 20.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-2

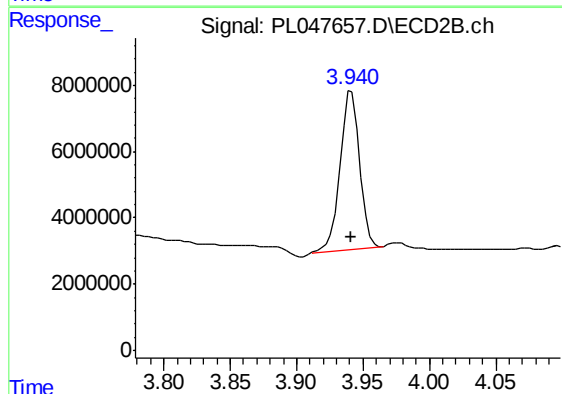


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 49796244
Conc: 18.65 ng/ml

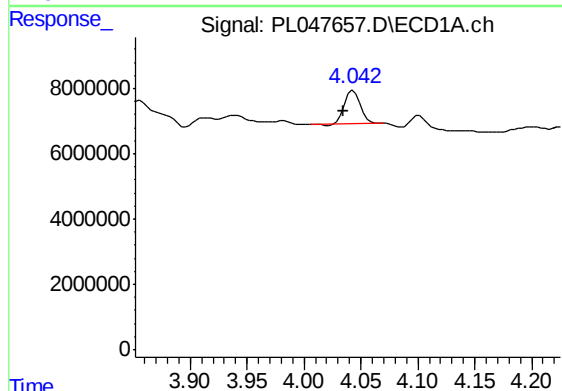


#3 gamma-BHC (Lindane)

R.T.: 4.043 min
Delta R.T.: 0.009 min
Response: 9775034
Conc: 0.81 ng/ml

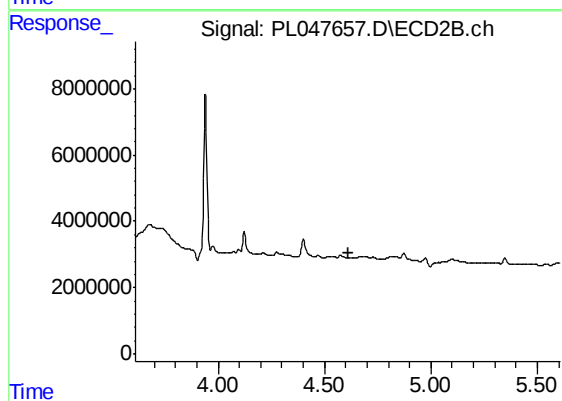

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.611 min
Response: 0
Conc: N.D.

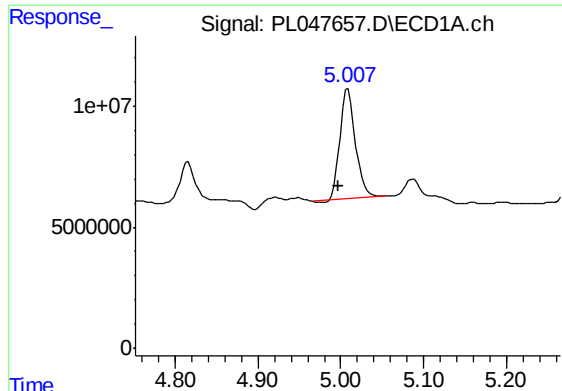

#8 Heptachlor epoxide


R.T.: 5.009 min
Delta R.T.: 0.012 min
Response: 59694609
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-2

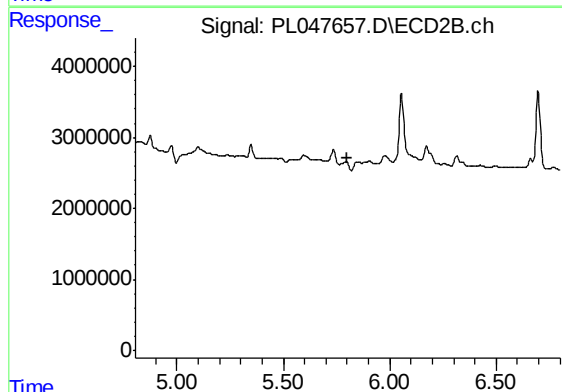


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.803 min
Response: 0
Conc: N.D.

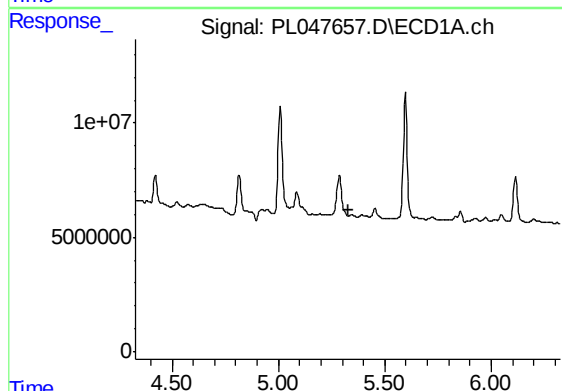


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

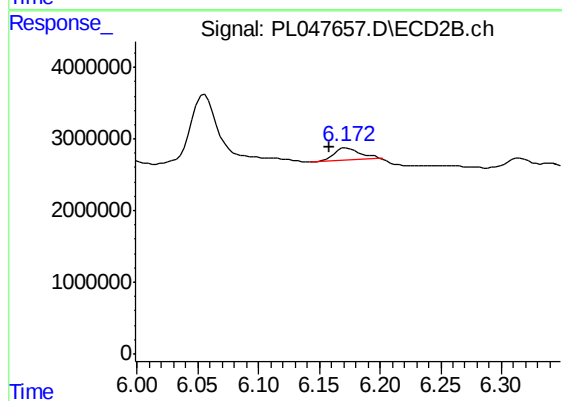

#9 Endosulfan I


R.T.: 6.173 min
Delta R.T.: 0.015 min
Response: 2640671
Conc: 0.89 ng/ml

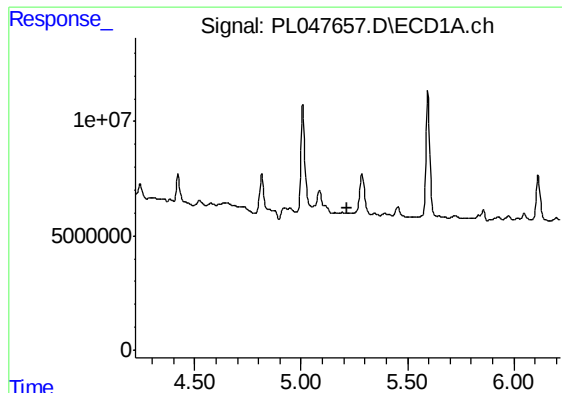

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WELL-2

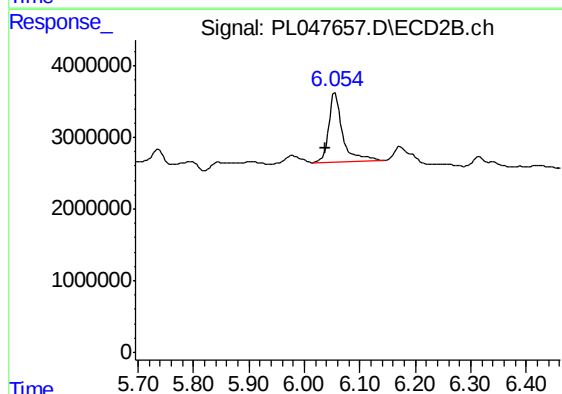


#10 gamma-Chlordane

R.T.: 6.056 min
Delta R.T.: 0.019 min
Response: 16835877
Conc: 5.33 ng/ml

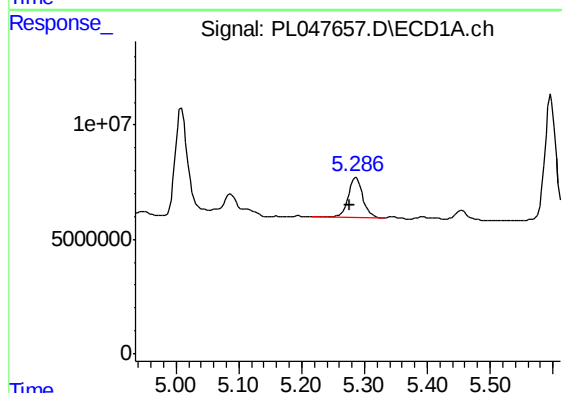


#11 alpha-Chlordane

R.T.: 5.287 min
Delta R.T.: 0.011 min
Response: 28125797
Conc: 2.34 ng/ml

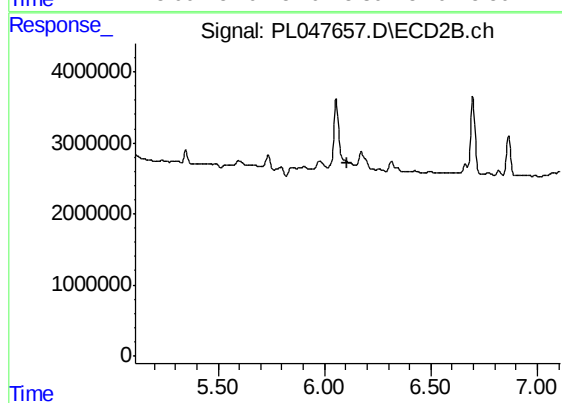

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.109 min
Response: 0
Conc: N.D.

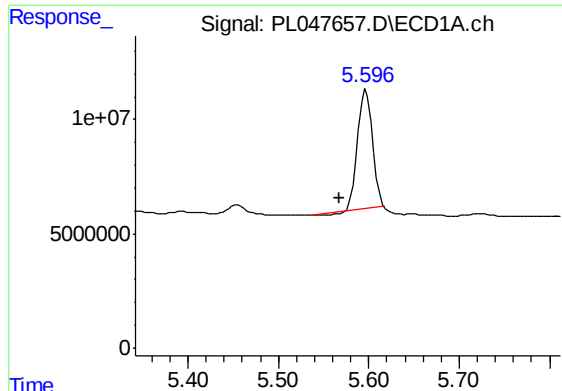

#13 Dielddrin


R.T.: 5.597 min
Delta R.T.: 0.030 min
Response: 59124781
Conc: 4.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-2

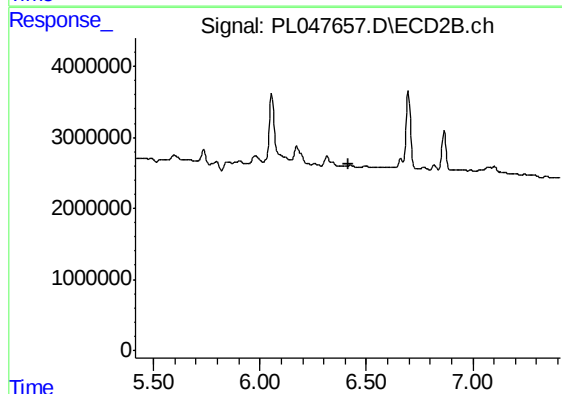


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

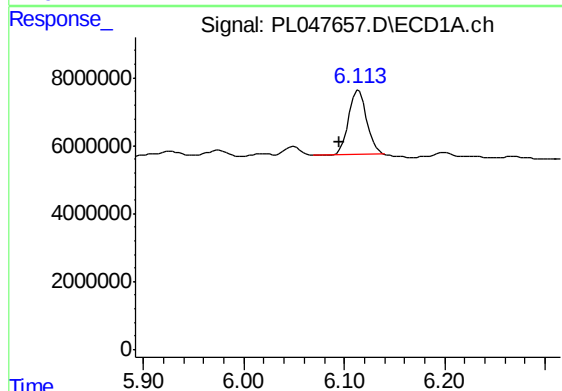


#15 Endosulfan II

R.T.: 6.114 min
Delta R.T.: 0.019 min
Response: 23404590
Conc: 2.21 ng/ml

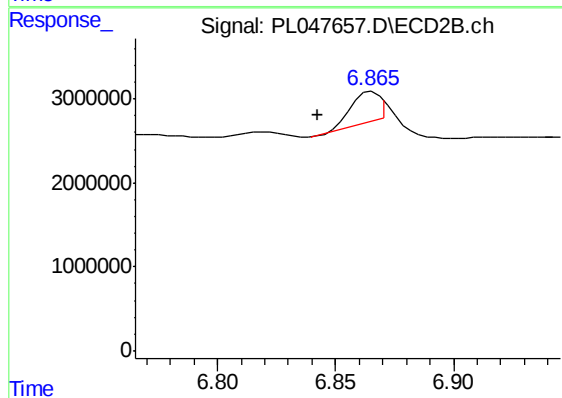

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.024 min
Response: 3012824
Conc: 1.09 ng/ml

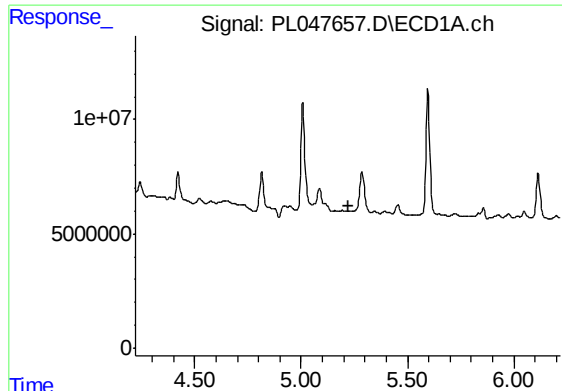

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 5.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
WELL-2

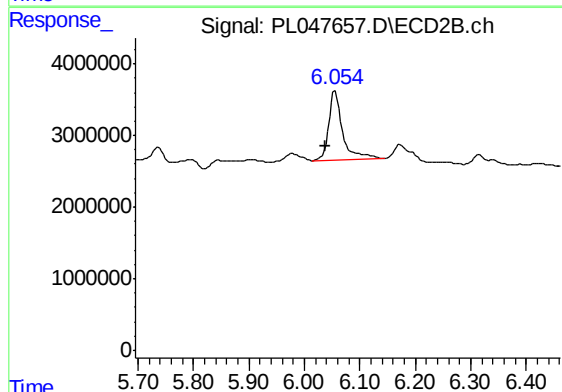


#25 Chlordane-3

R.T.: 6.056 min
Delta R.T.: 0.019 min
Response: 16835877
Conc: 41.96 ng/ml

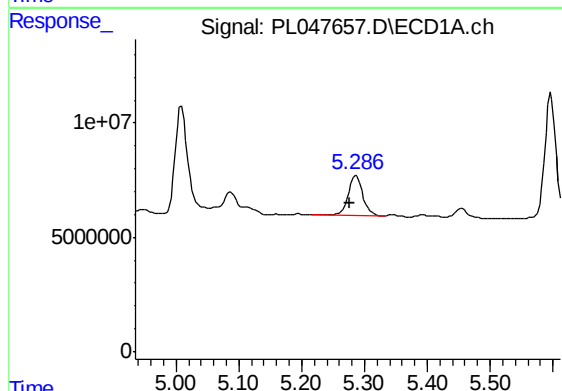


#26 Chlordane-4

R.T.: 5.287 min
Delta R.T.: 0.011 min
Response: 28125797
Conc: 22.19 ng/ml

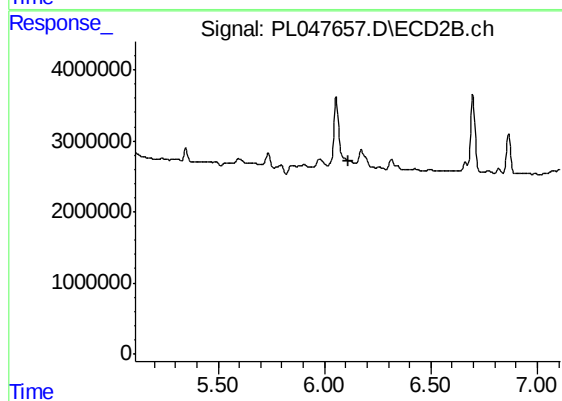

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.110 min
Response: 0
Conc: N.D.

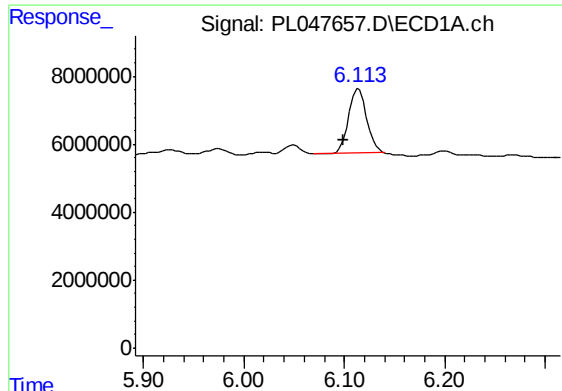

#27 Chlordane-5


R.T.: 6.114 min
Delta R.T.: 0.016 min
Response: 23404590
Conc: 59.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
WELL-2

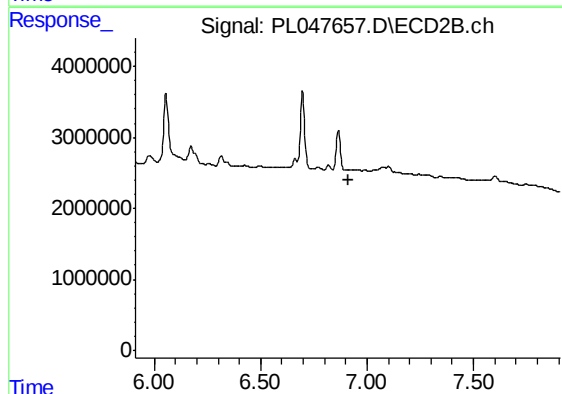


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.912 min
Response: 0
Conc: N.D.

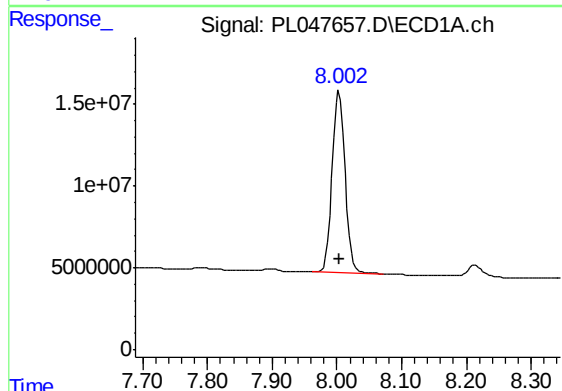

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 152292156
Conc: 15.08 ng/ml

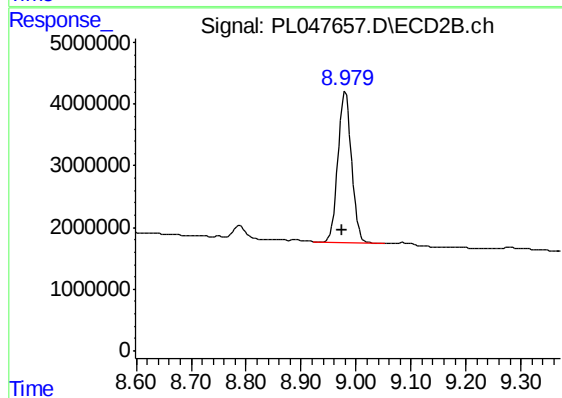

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.006 min
Response: 41969902
Conc: 13.83 ng/ml