

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 18:12
 Operator : AJ\SJ
 Sample : K2532-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:00:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	193.3E6	50989628	21.790	19.101
28)	SA Decachlor...	8.003	8.981	218.6E6	59812559	21.641	19.704
Target Compounds							
23)	Chlordane-1	4.197f	0.000	13227181	0	33.618	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 18:12
Operator : AJ\SJ
Sample : K2532-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:00:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

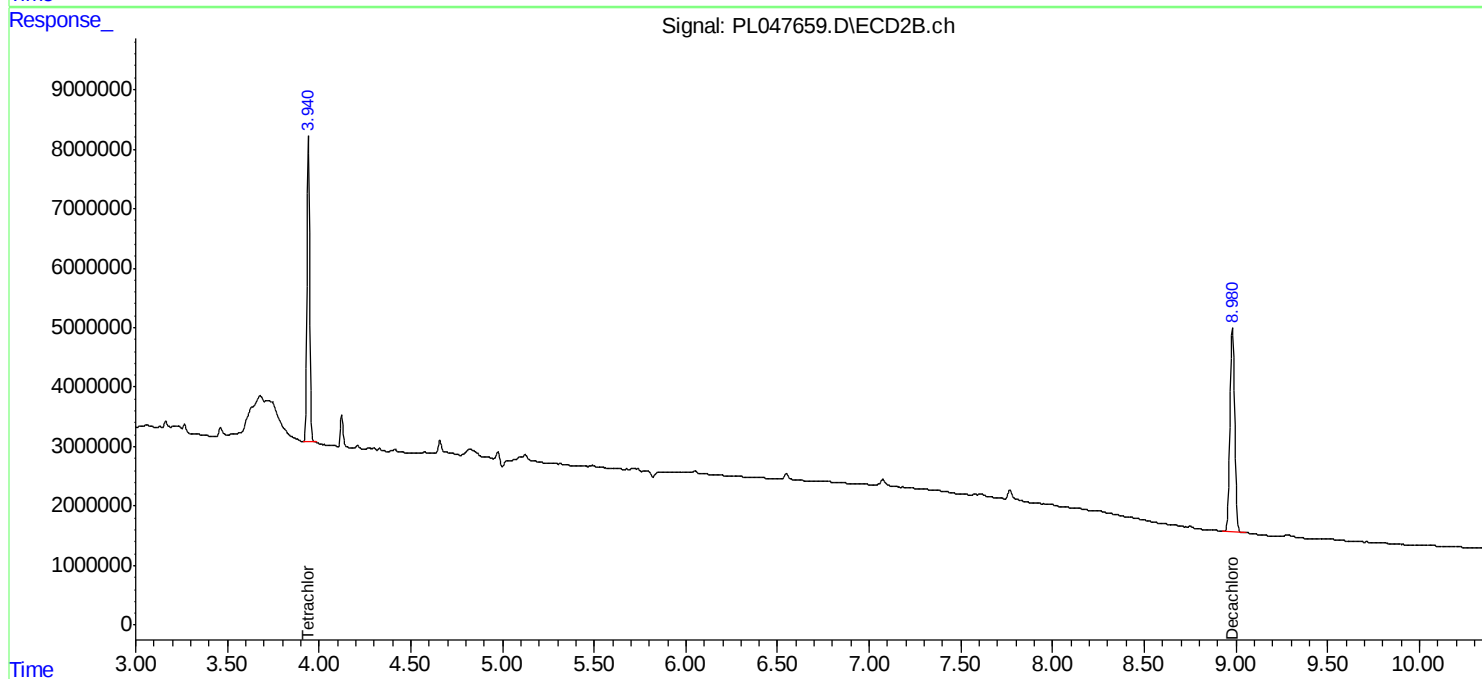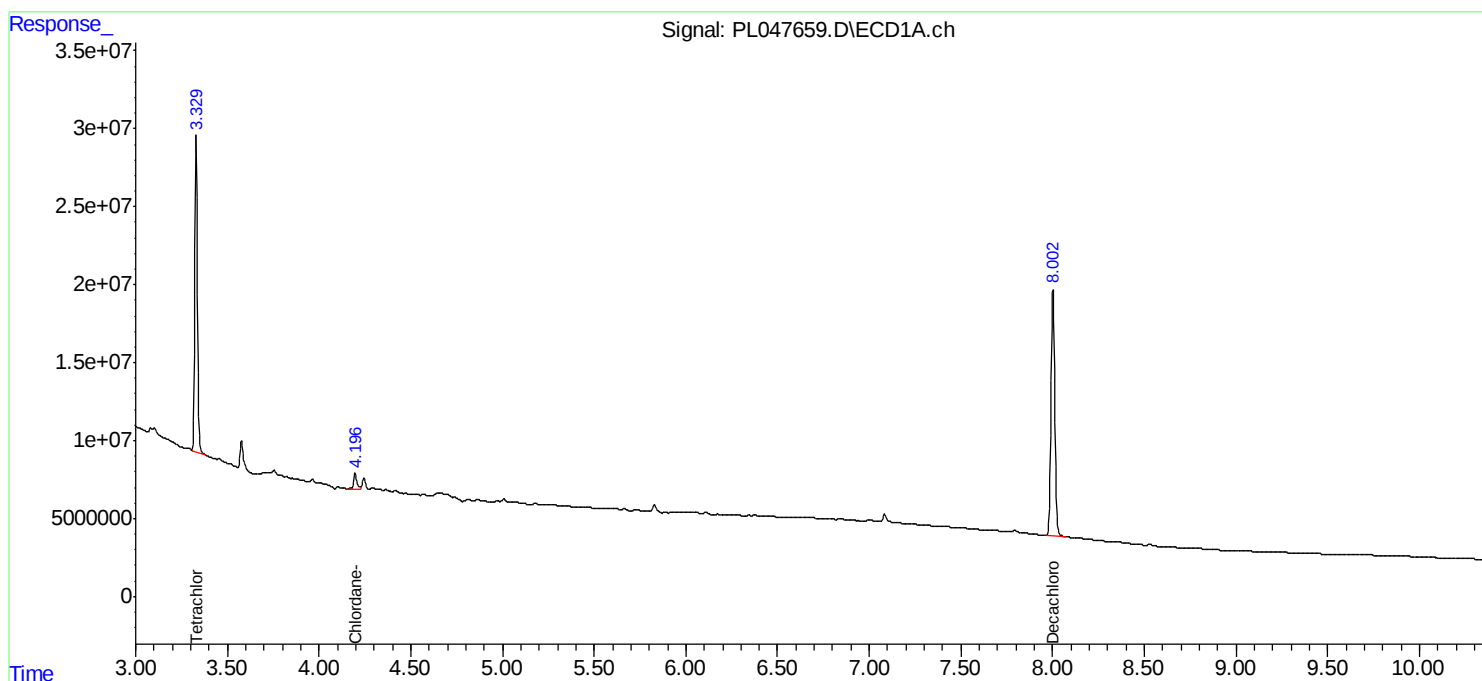


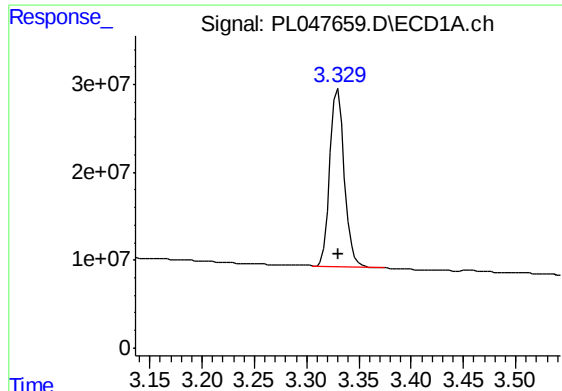

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 193333821
Conc: 21.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14

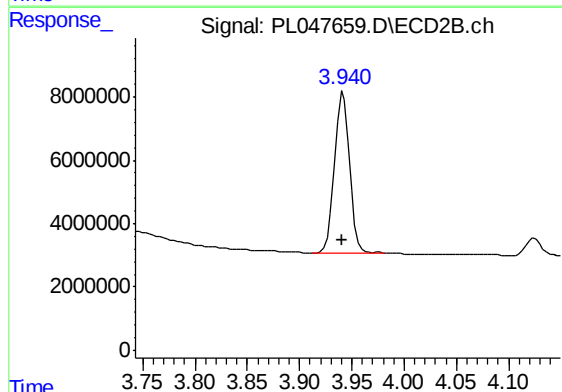


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.001 min
Response: 50989628
Conc: 19.10 ng/ml

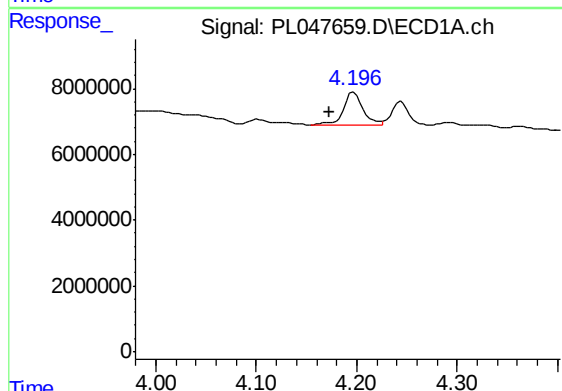


#23 Chlordane-1

R.T.: 4.197 min
Delta R.T.: 0.024 min
Response: 13227181
Conc: 33.62 ng/ml

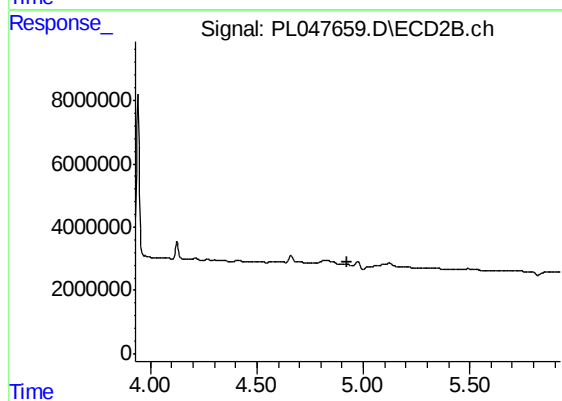

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.927 min
Response: 0
Conc: N.D.

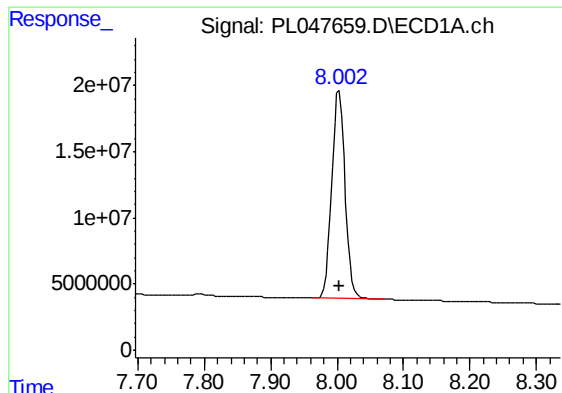

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 218601720
Conc: 21.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14

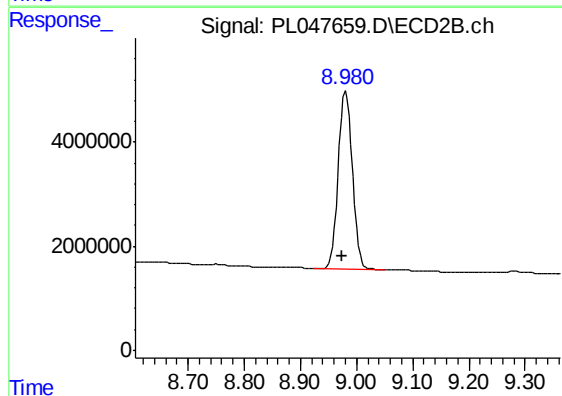

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.006 min
Response: 59812559
Conc: 19.70 ng/ml