

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
 Data File : PL047681.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2019 23:45
 Operator : AJ\SJ
 Sample : K2532-04
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 01:06:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 19 16:51:53 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	208.7E6	53795990	23.524	20.153
28)	SA Decachlor...	8.003	8.981	211.3E6	56999222	20.919	18.777
Target Compounds							
7)	B delta-BHC	0.000	4.977f	0	2214838	N.D.	0.825 #
10)	B gamma-Chl...	0.000	6.030	0	3533960	N.D.	1.118 #
13)	MA Dieldrin	5.557	0.000	8939800	0	0.751	N.D. #
25)	Chlordane-3	0.000	6.030	0	3533960	N.D.	8.808 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042319\
Data File : PL047681.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2019 23:45
Operator : AJ\SJ
Sample : K2532-04
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 01:06:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041919.M
Quant Title : GC Extractables
QLast Update : Fri Apr 19 16:51:53 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

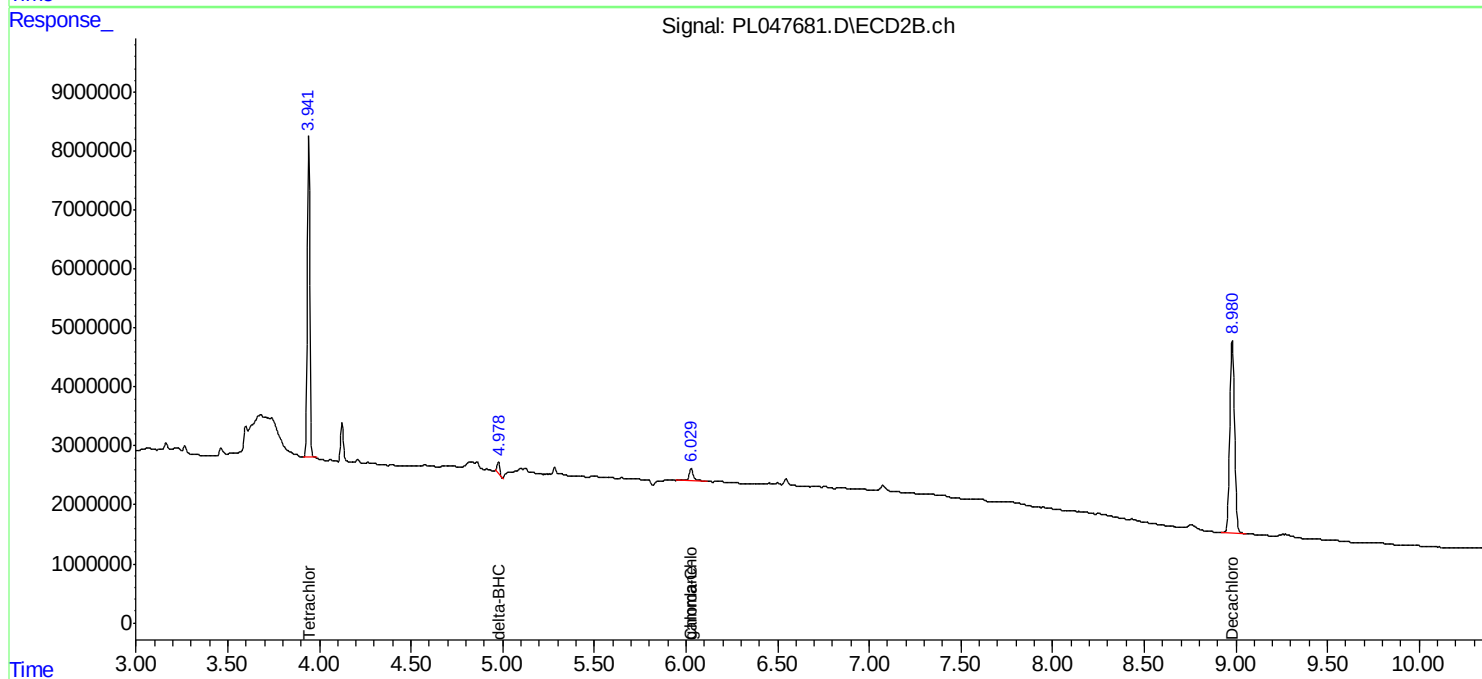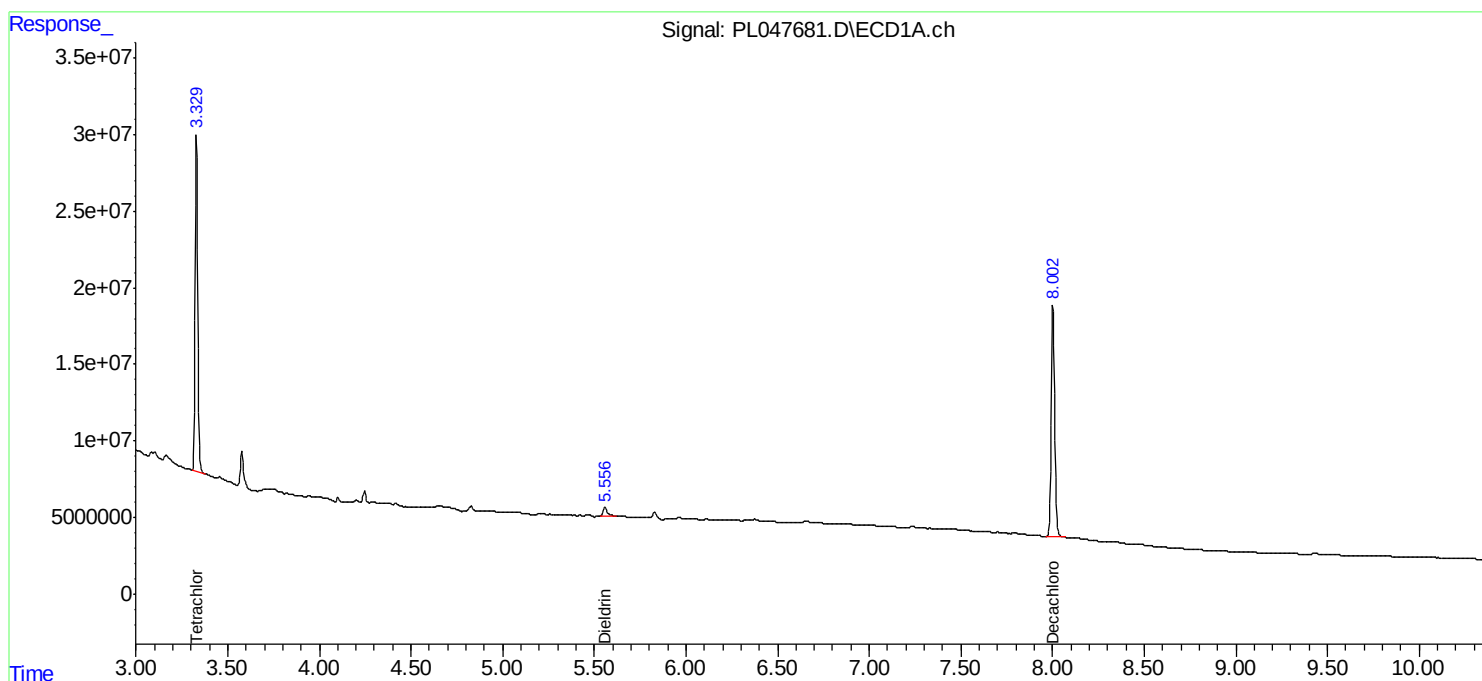


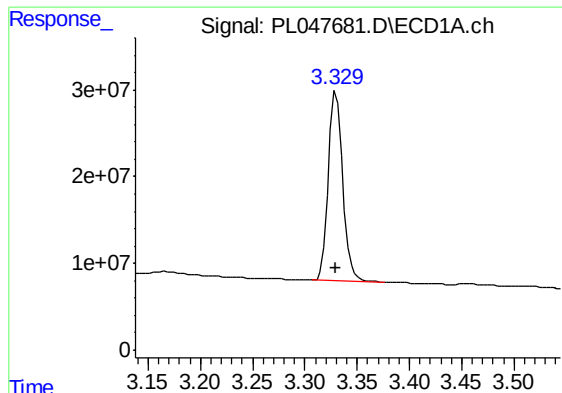

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 208721032
Conc: 23.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-5

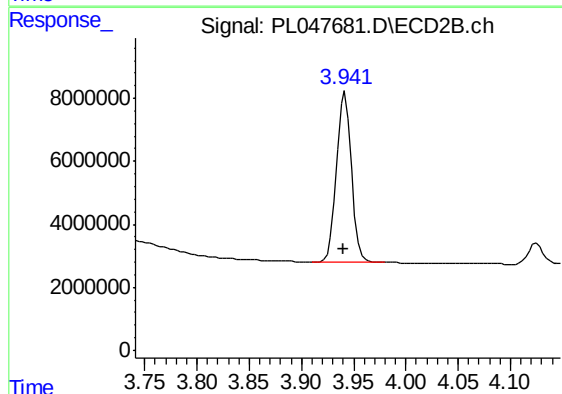


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.001 min
Response: 53795990
Conc: 20.15 ng/ml

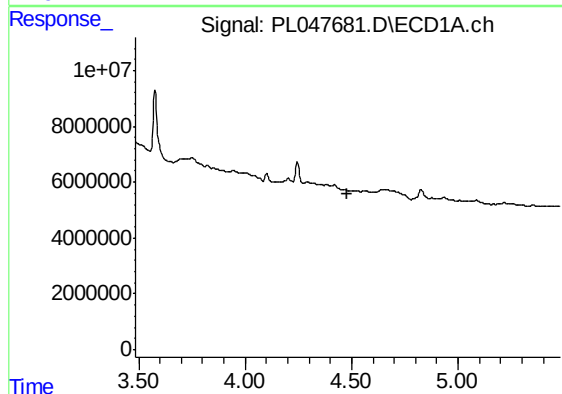


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

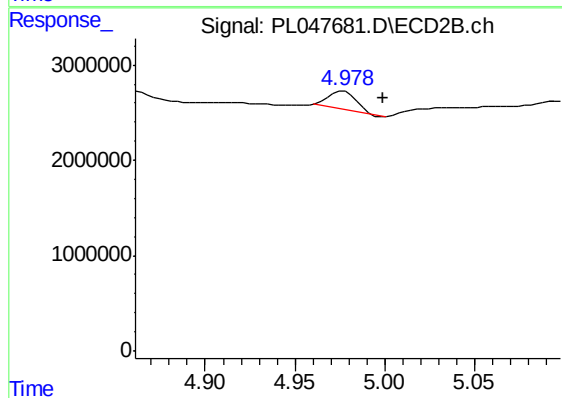

#7 delta-BHC


R.T.: 4.977 min
Delta R.T.: -0.022 min
Response: 2214838
Conc: 0.83 ng/ml

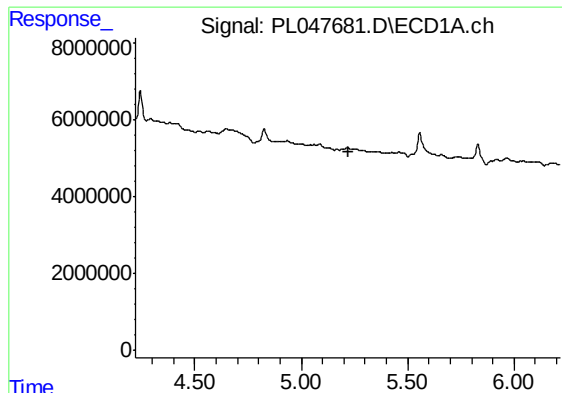

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-5

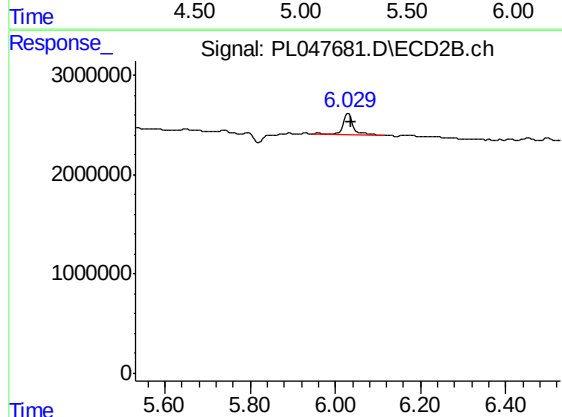


#10 gamma-Chlordane

R.T.: 6.030 min
Delta R.T.: -0.007 min
Response: 3533960
Conc: 1.12 ng/ml

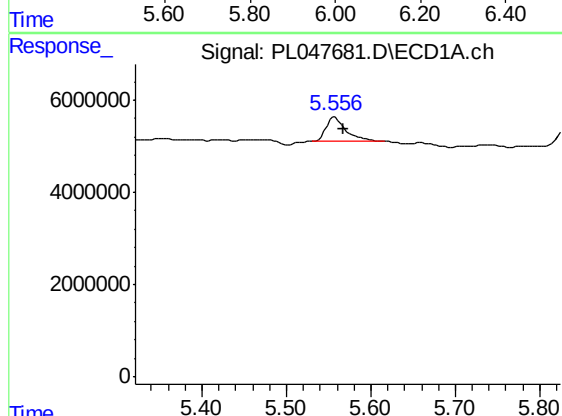


#13 Dieldrin

R.T.: 5.557 min
Delta R.T.: -0.010 min
Response: 8939800
Conc: 0.75 ng/ml

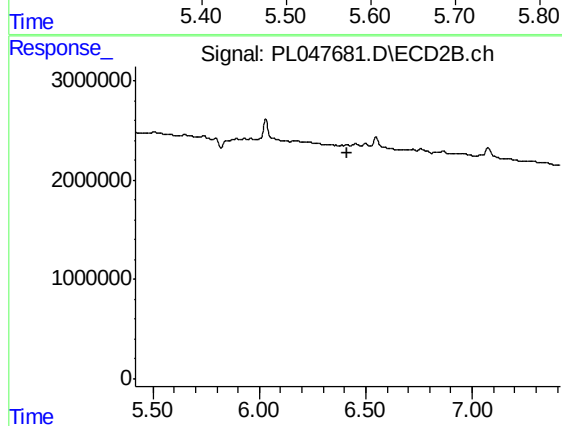

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

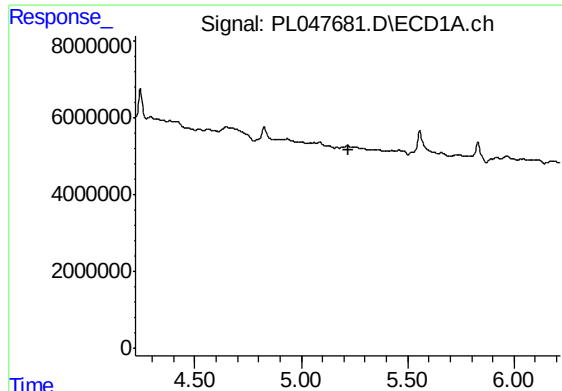

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-5

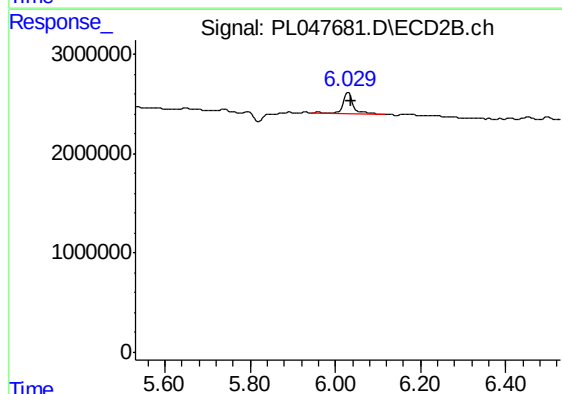


#25 Chlordane-3

R.T.: 6.030 min
Delta R.T.: -0.007 min
Response: 3533960
Conc: 8.81 ng/ml

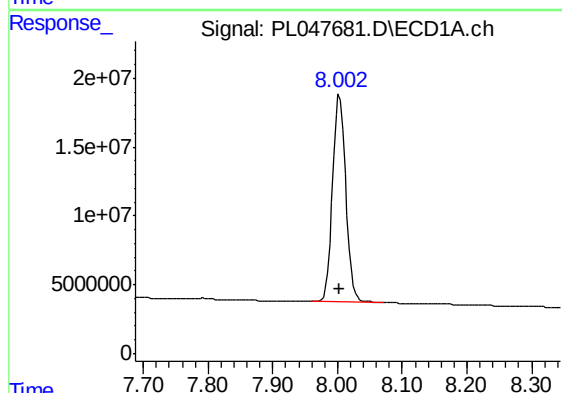

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 211313294
Conc: 20.92 ng/ml

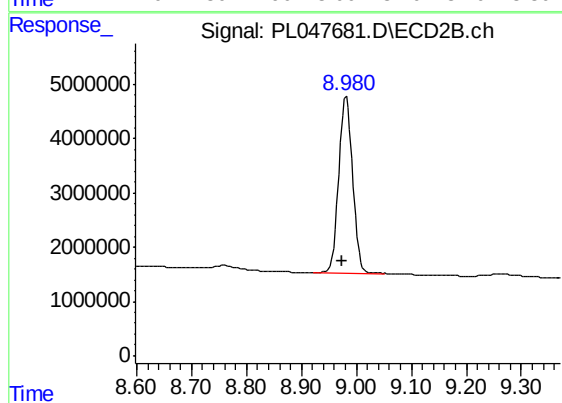

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.007 min
Response: 56999222
Conc: 18.78 ng/ml