

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0042320\
 Data File : P0068022.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Apr 2020 20:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 05:17:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.915	3.936	481313	791783	20.211	23.623
2) SA Decachlor...	10.883	9.215	674664	749194	19.818	18.120
Target Compounds						
34) L7 AR-1260-4	8.741	0.000	32798	0	21.342	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0042320\
Data File : P0068022.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Apr 2020 20:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 05:17:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

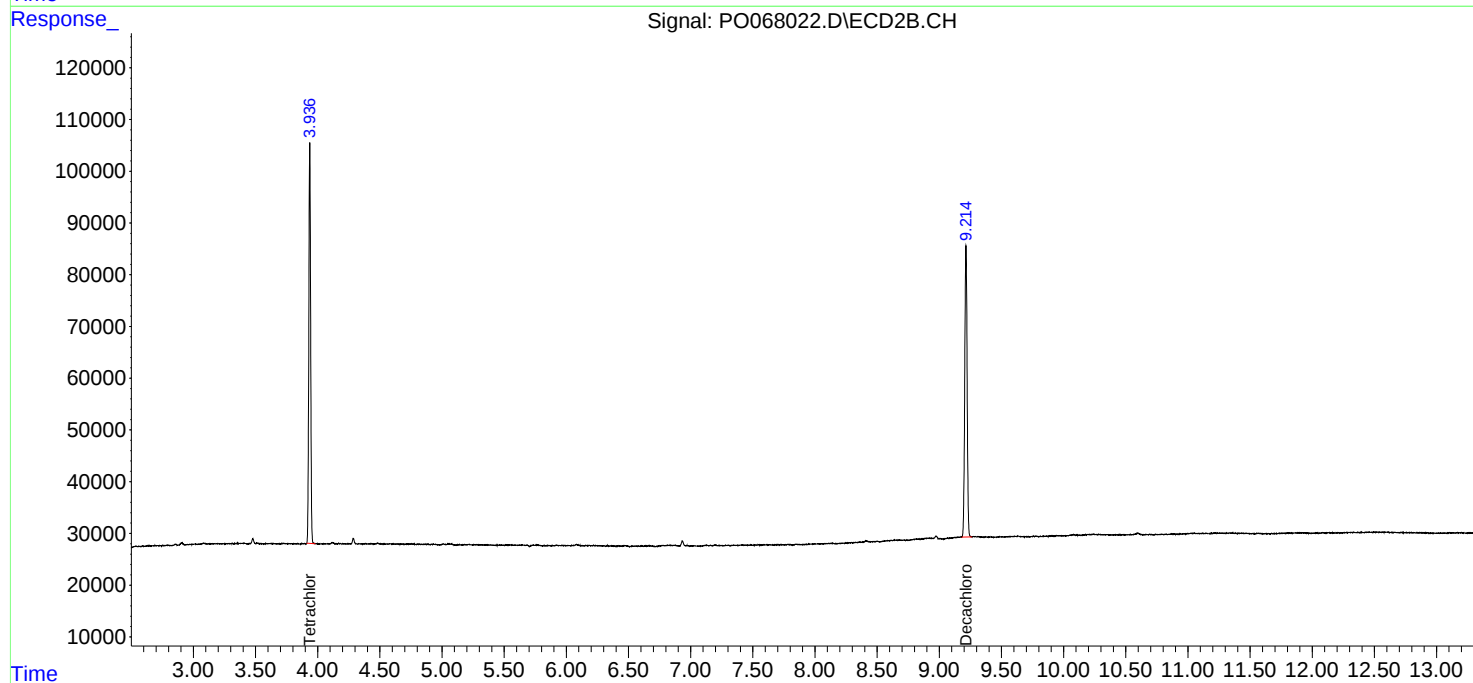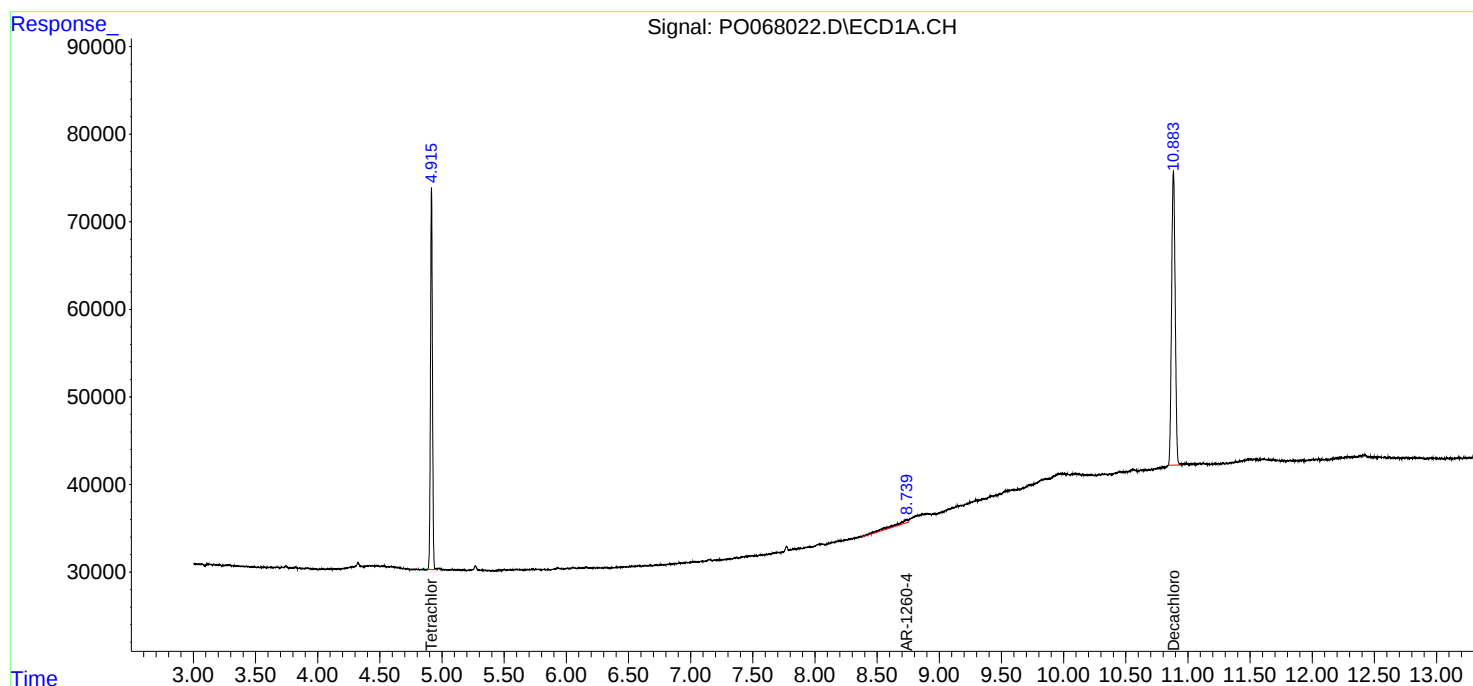


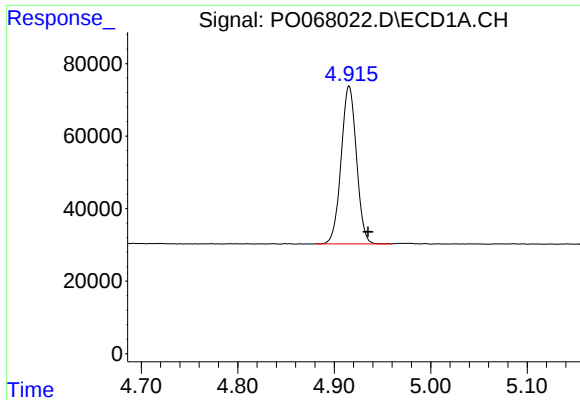

#1 Tetrachloro-m-xylene


R.T.: 4.915 min
Delta R.T.: -0.020 min
Response: 481313
Conc: 20.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

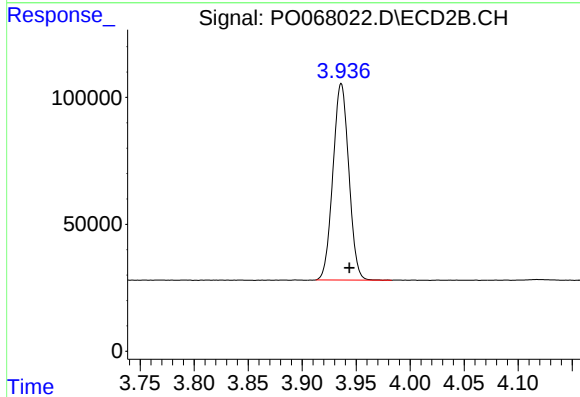


#1 Tetrachloro-m-xylene

R.T.: 3.936 min
Delta R.T.: -0.008 min
Response: 791783
Conc: 23.62 ng/ml

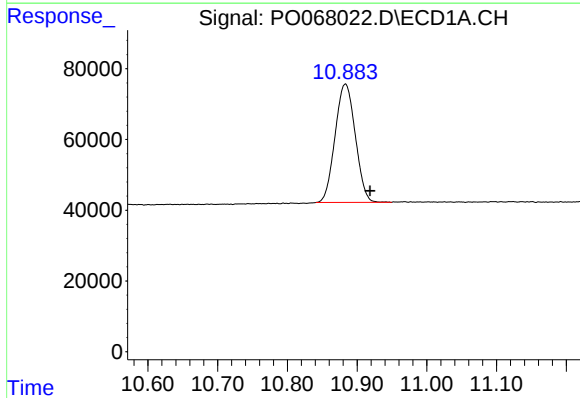


#2 Decachlorobiphenyl

R.T.: 10.883 min
Delta R.T.: -0.036 min
Response: 674664
Conc: 19.82 ng/ml

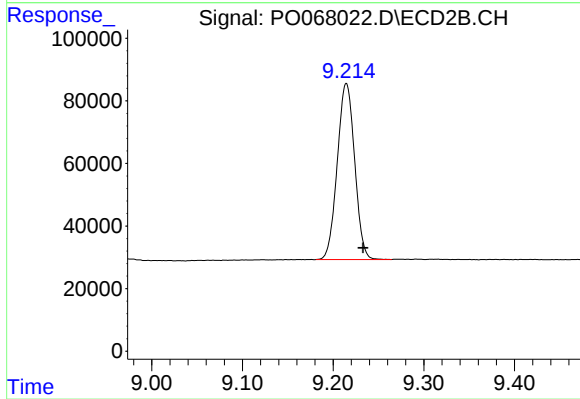

#2 Decachlorobiphenyl


R.T.: 9.215 min
Delta R.T.: -0.019 min
Response: 749194
Conc: 18.12 ng/ml

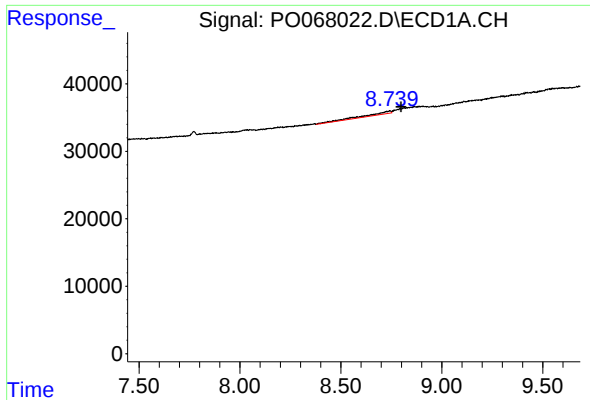

#34 AR-1260-4

R.T.: 8.741 min
Delta R.T.: -0.056 min
Response: 32798
Conc: 21.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

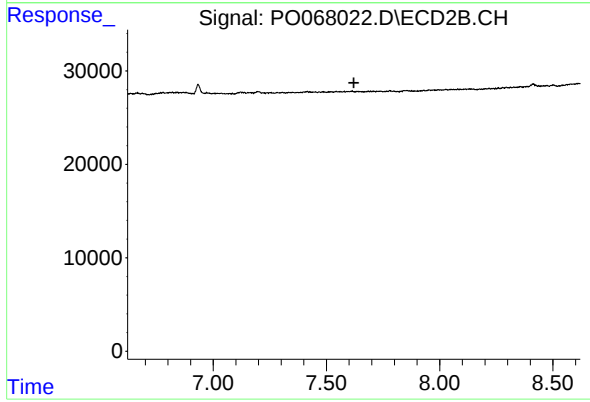

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.621 min
Response: 0
Conc: N.D.