

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 10:05
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 05:37:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 05:35:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) A	alpha-BHC	3.872	0.000	2930918	0	0.585	N.D. #
4) MA	Heptachlor	4.417f	0.000	2043294	0	0.484	N.D. #
6) B	beta-BHC	4.417f	5.029	2043294	7766207	1.009	2.903 #
10) B	gamma-Chl...	0.000	6.309	0	6719166	N.D.	1.554 #
11) B	alpha-Chl...	0.000	6.401f	0	3852571	N.D.	0.901 #
15) B	Endosulfa...	6.206f	0.000	604082	0	0.189	N.D. #
21) B	Endrin ke...	0.000	7.971	0	2754629	N.D.	0.726 #
23)	Chlordane-1	4.315f	5.199f	3952559	5254463	30.213	32.419
25)	Chlordane-3	0.000	6.309	0	6719166	N.D.	11.040 #
26)	Chlordane-4	0.000	6.401f	0	3852571	N.D.	5.303 #
27)	Chlordane-5	6.206f	0.000	604082	0	4.579	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066434.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 10:05
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 05:37:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 05:35:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

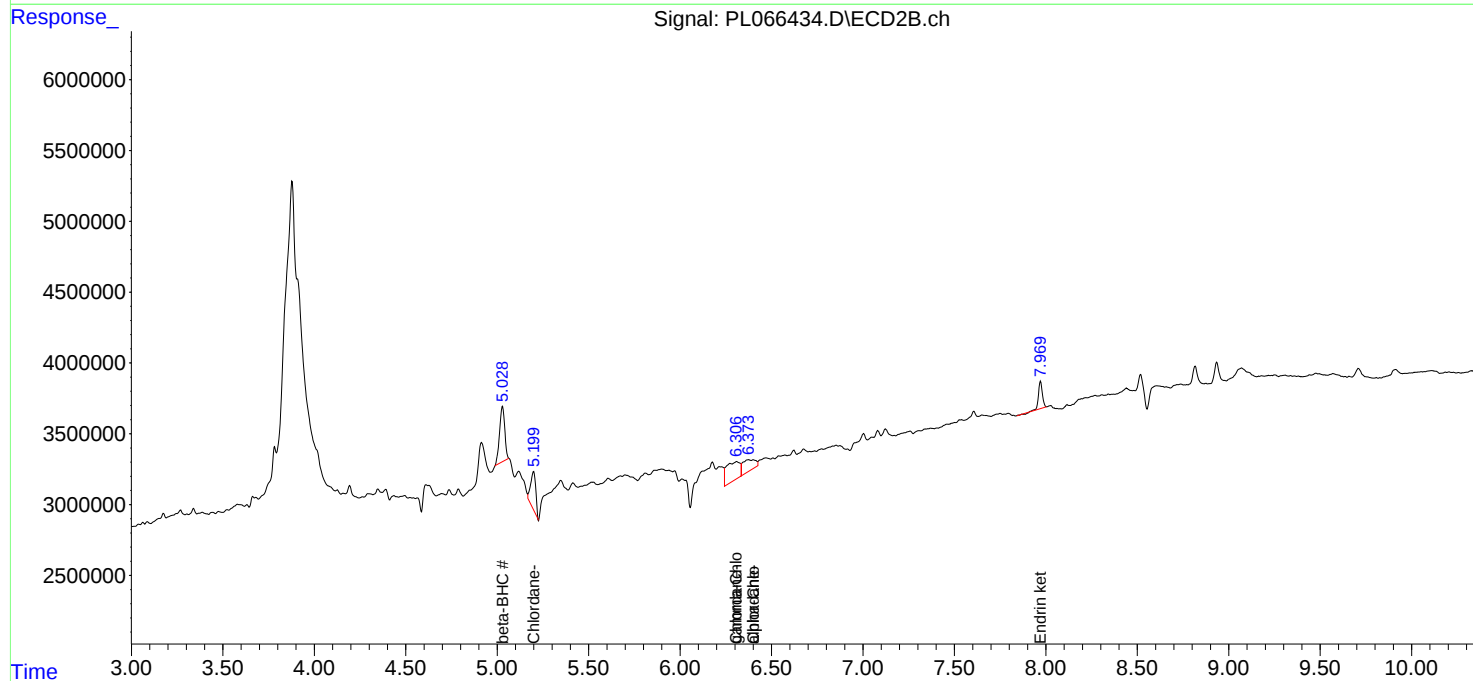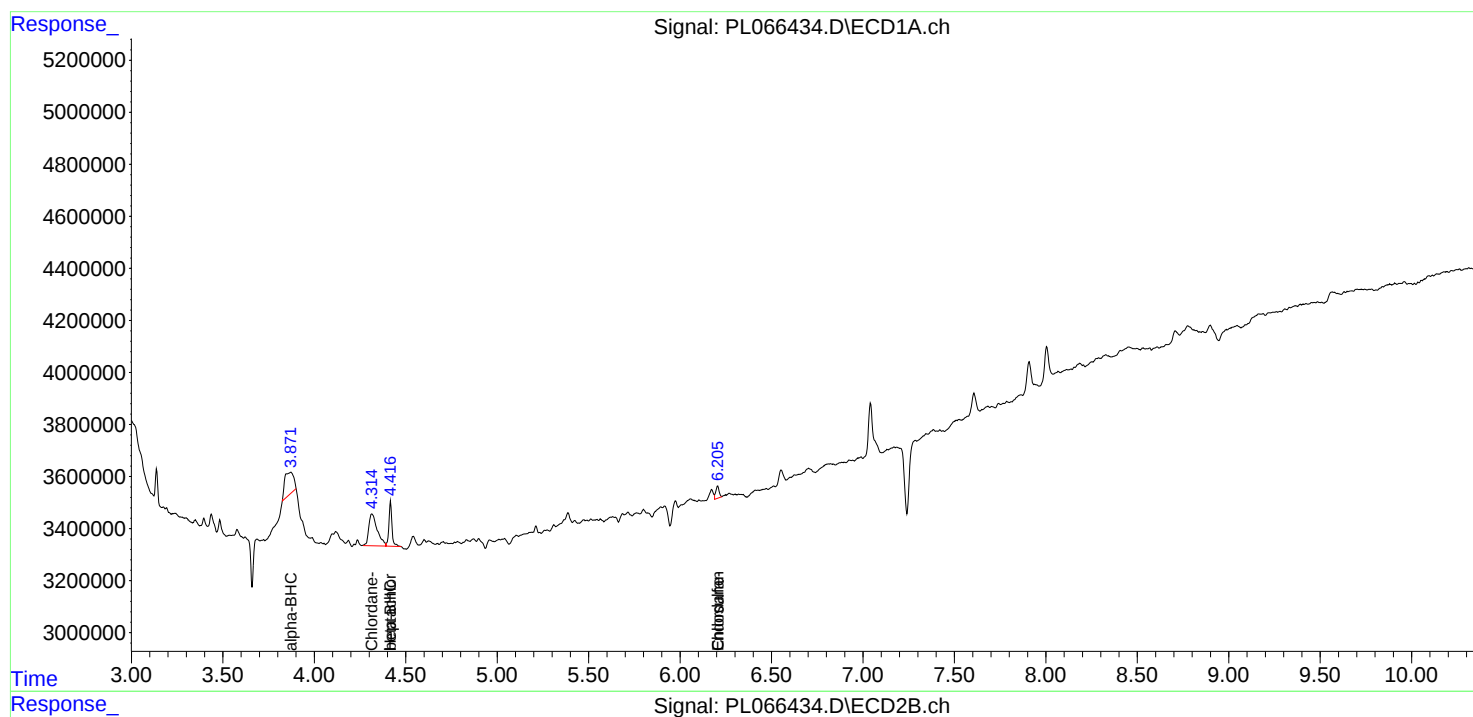


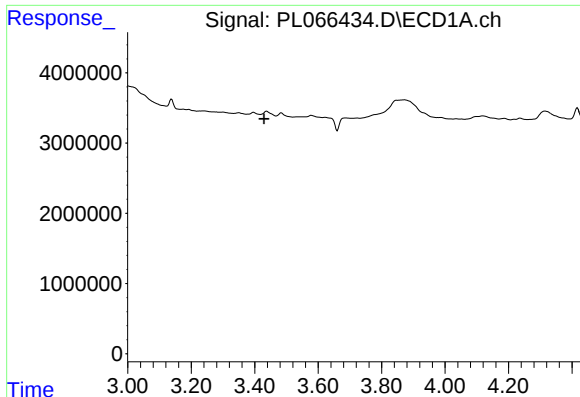

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

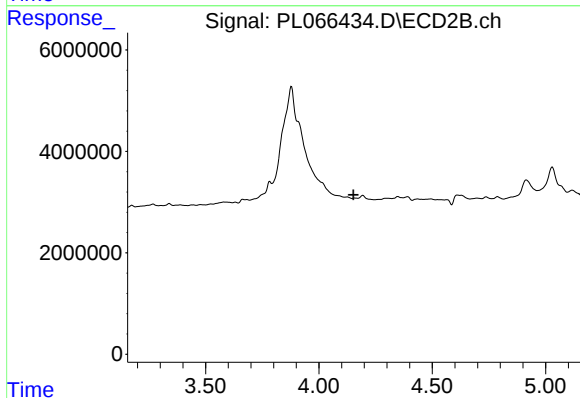


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.153 min
Response: 0
Conc: N.D.

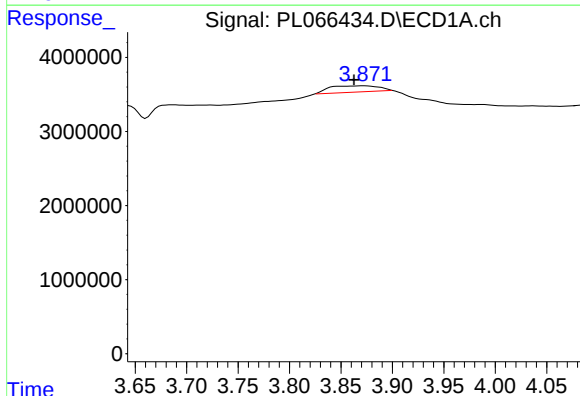


#2 alpha-BHC

R.T.: 3.872 min
Delta R.T.: 0.009 min
Response: 2930918
Conc: 0.58 ng/ml

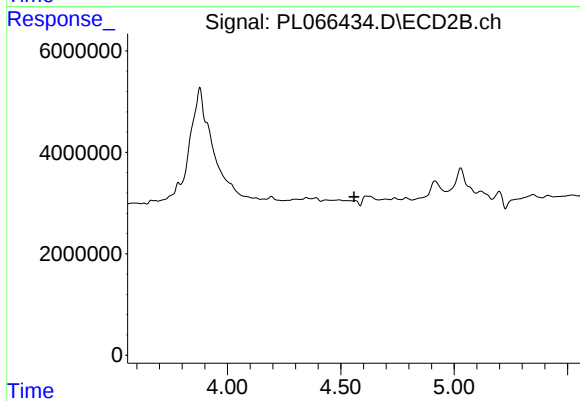

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.558 min
Response: 0
Conc: N.D.

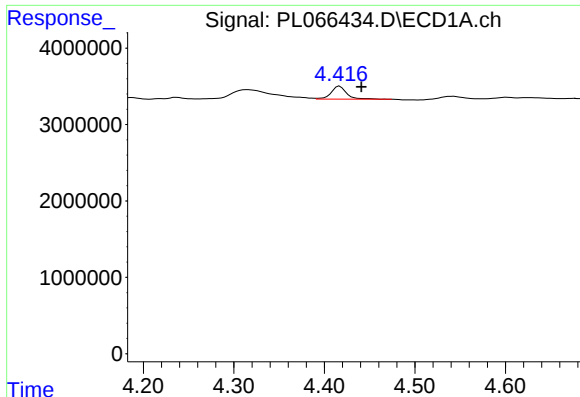

#4 Heptachlor


R.T.: 4.417 min
Delta R.T.: -0.024 min
Response: 2043294
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

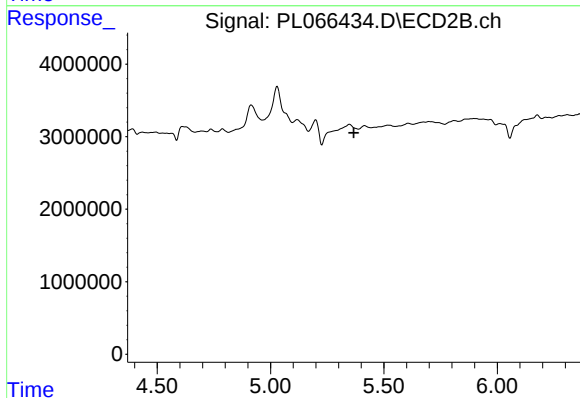


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.367 min
Response: 0
Conc: N.D.

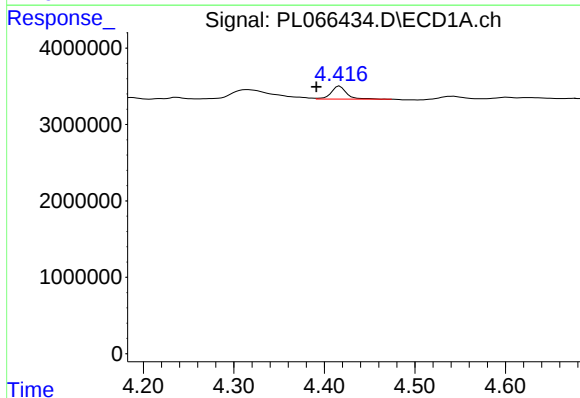


#6 beta-BHC

R.T.: 4.417 min
Delta R.T.: 0.026 min
Response: 2043294
Conc: 1.01 ng/ml

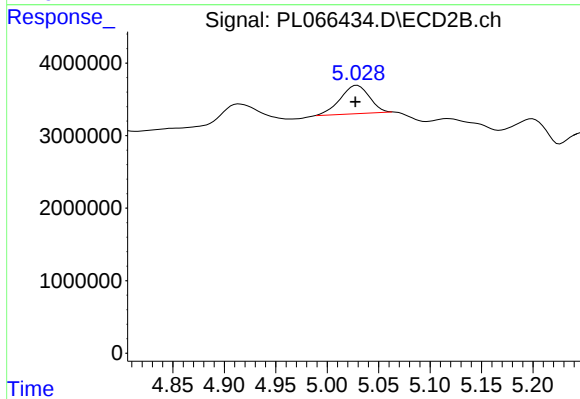

#6 beta-BHC


R.T.: 5.029 min
Delta R.T.: 0.002 min
Response: 7766207
Conc: 2.90 ng/ml

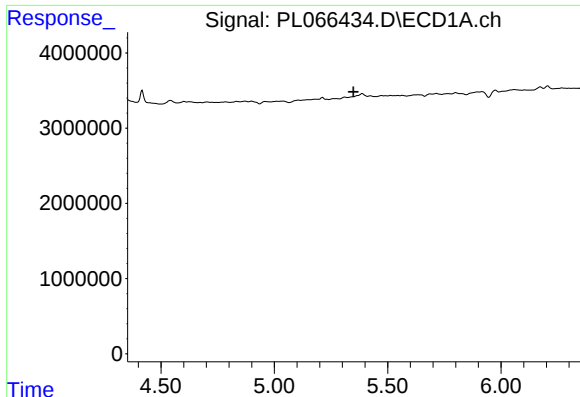

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

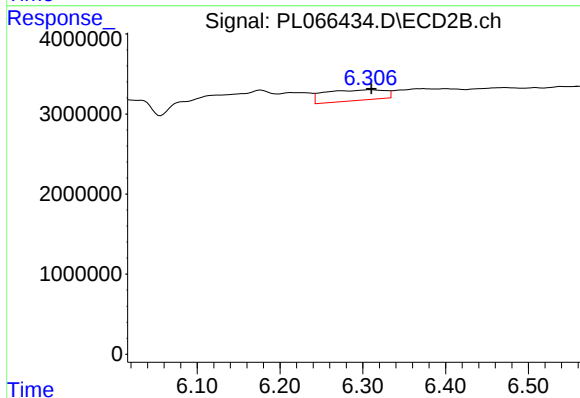


#10 gamma-Chlordane

R.T.: 6.309 min
Delta R.T.: -0.001 min
Response: 6719166
Conc: 1.55 ng/ml

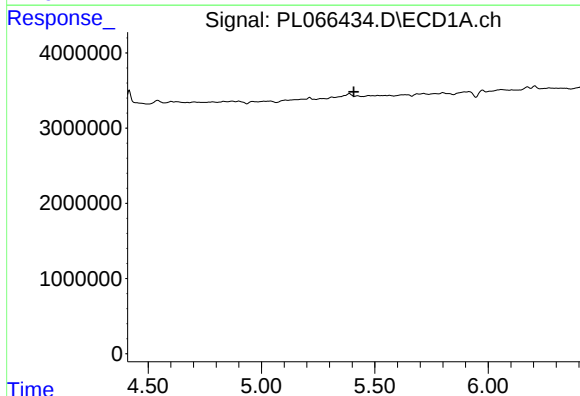


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

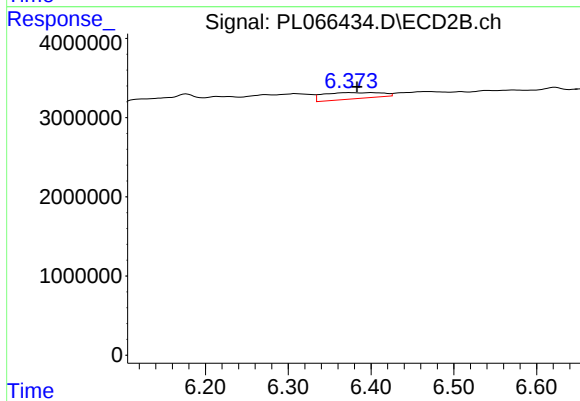

#11 alpha-Chlordane


R.T.: 6.401 min
Delta R.T.: 0.017 min
Response: 3852571
Conc: 0.90 ng/ml

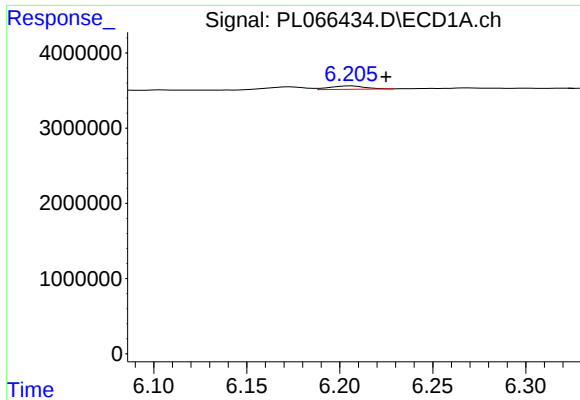

#15 Endosulfan II


R.T.: 6.206 min
Delta R.T.: -0.019 min
Response: 604082
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

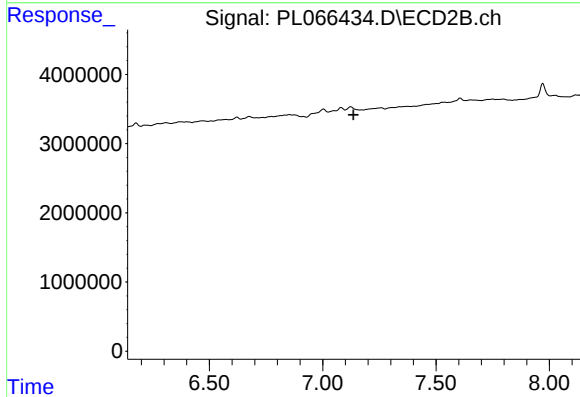


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

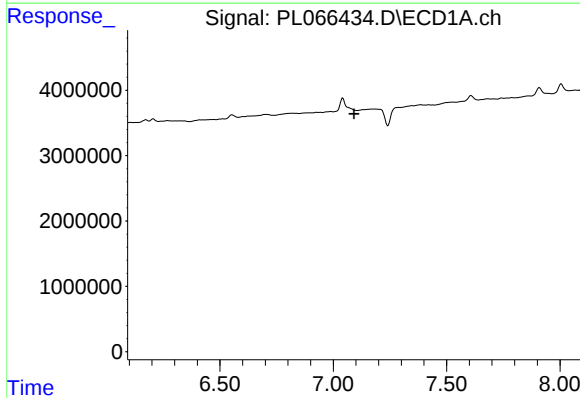


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

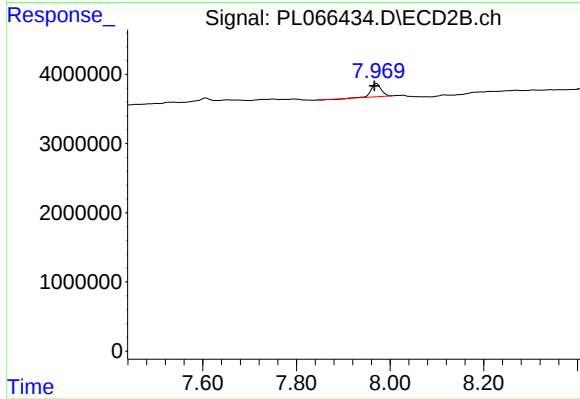

#21 Endrin ketone


R.T.: 7.971 min
Delta R.T.: 0.004 min
Response: 2754629
Conc: 0.73 ng/ml

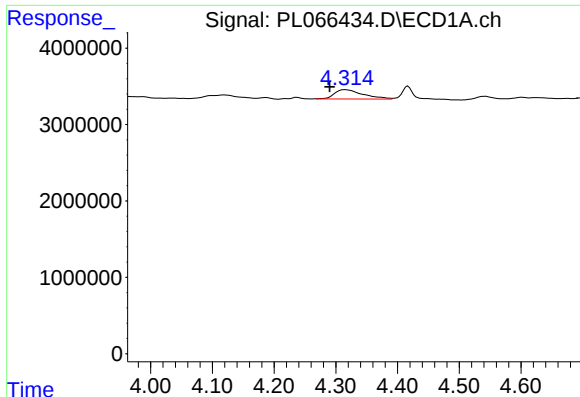

#23 Chlordane-1


R.T.: 4.315 min
Delta R.T.: 0.025 min
Response: 3952559
Conc: 30.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

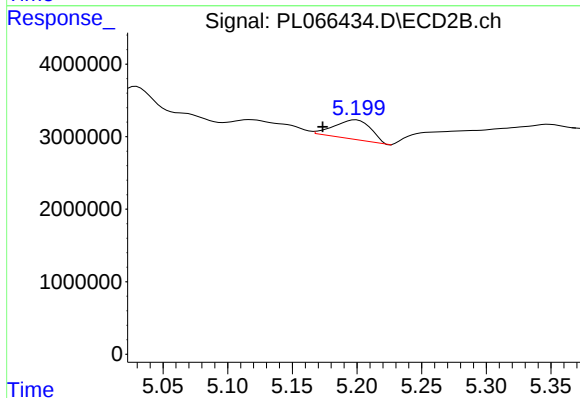


#23 Chlordane-1

R.T.: 5.199 min
Delta R.T.: 0.026 min
Response: 5254463
Conc: 32.42 ng/ml

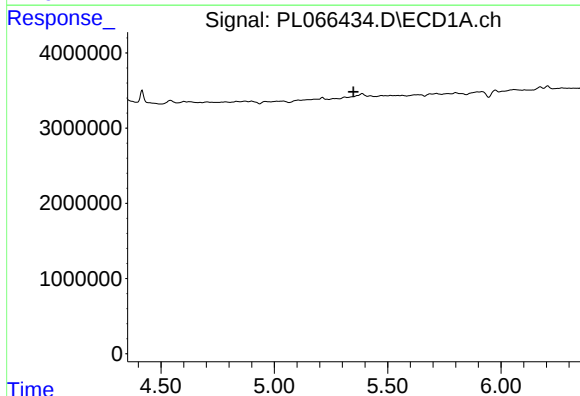


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.350 min
Response: 0
Conc: N.D.

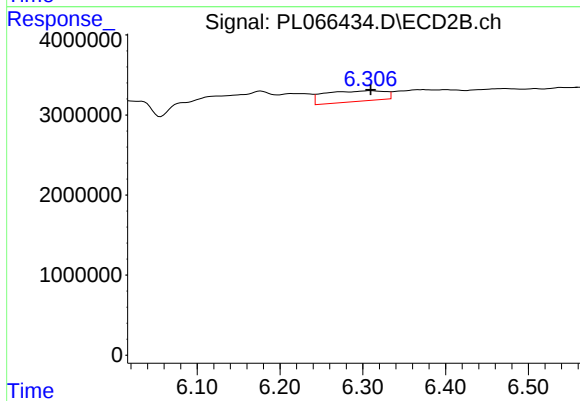

#25 Chlordane-3


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 6719166
Conc: 11.04 ng/ml

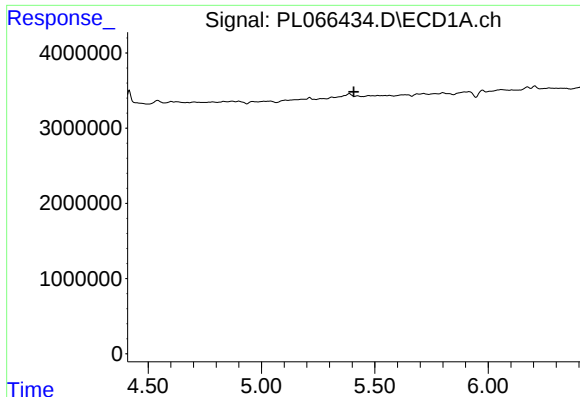

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

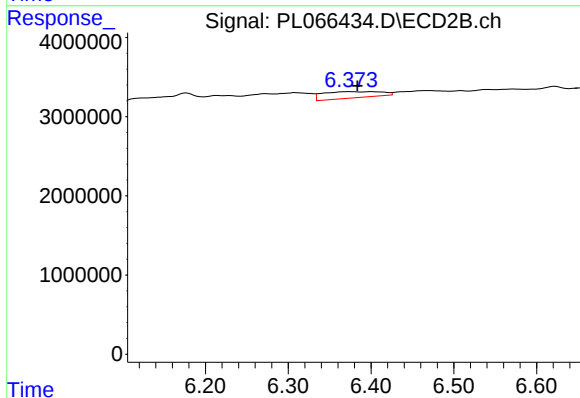


#26 Chlordane-4

R.T.: 6.401 min
Delta R.T.: 0.017 min
Response: 3852571
Conc: 5.30 ng/ml

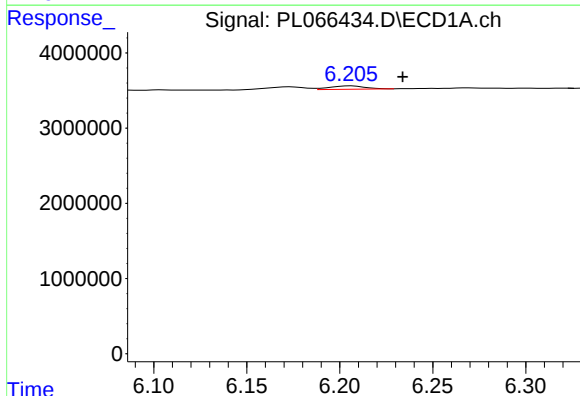


#27 Chlordane-5

R.T.: 6.206 min
Delta R.T.: -0.028 min
Response: 604082
Conc: 4.58 ng/ml

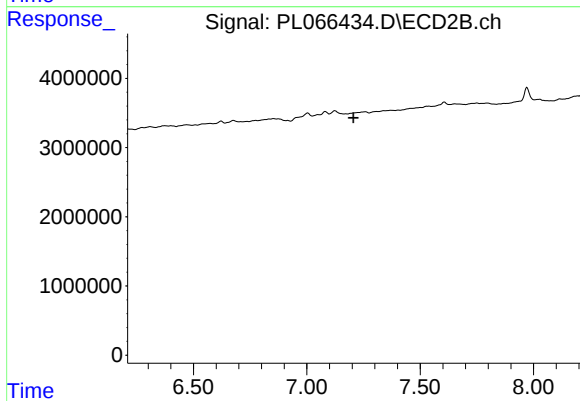

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.206 min
Response: 0
Conc: N.D.

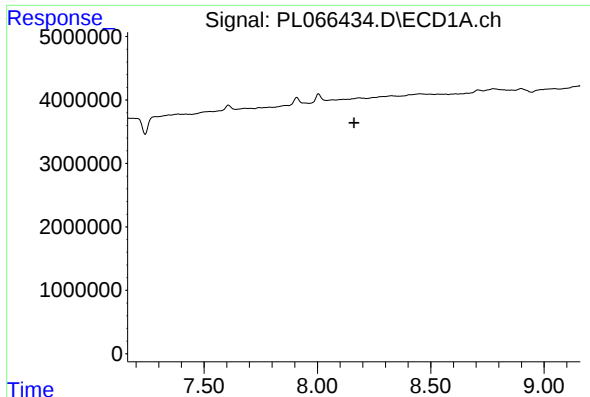

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

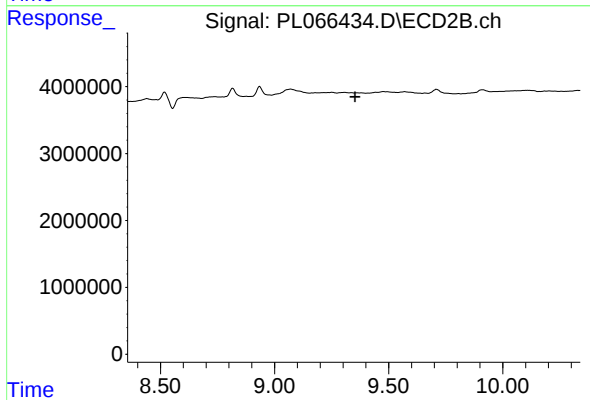

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.353 min
Response: 0
Conc: N.D.