

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 17:04
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 05:38:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 05:35:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

6) B	beta-BHC	4.403	5.033	1289435	3910603	0.636	1.462 #
11) B	alpha-Chl...	0.000	6.408f	0	4652805	N.D.	1.088 #
15) B	Endosulfa...	6.250f	0.000	894947	0	0.281	N.D. #
18) B	Endrin al...	6.413f	0.000	352074	0	0.127	N.D. #
21) B	Endrin ke...	0.000	7.973	0	1887655	N.D.	0.498 #
23)	Chlordane-1	4.292	0.000	1747166	0	13.355	N.D. #
26)	Chlordane-4	0.000	6.408f	0	4652805	N.D.	6.404 #
27)	Chlordane-5	6.250f	0.000	894947	0	6.784	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 17:04
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 05:38:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 05:35:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

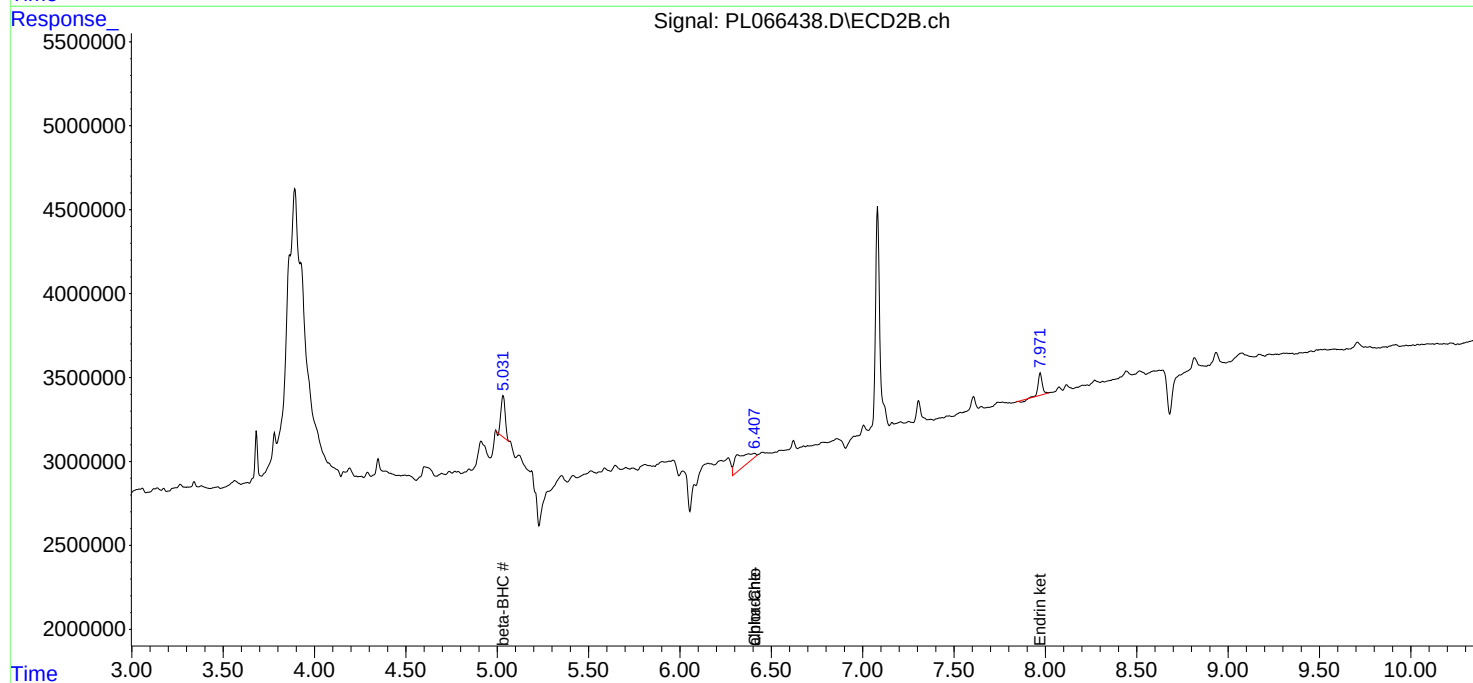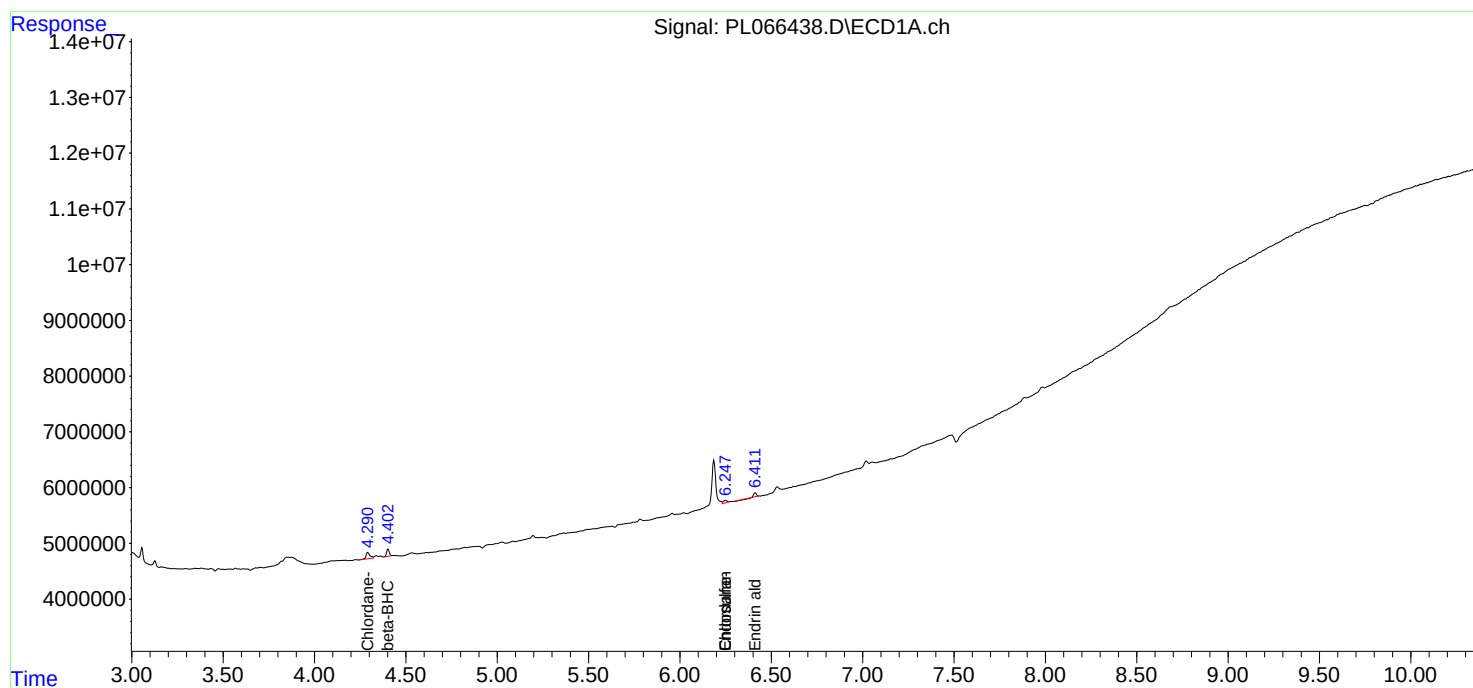


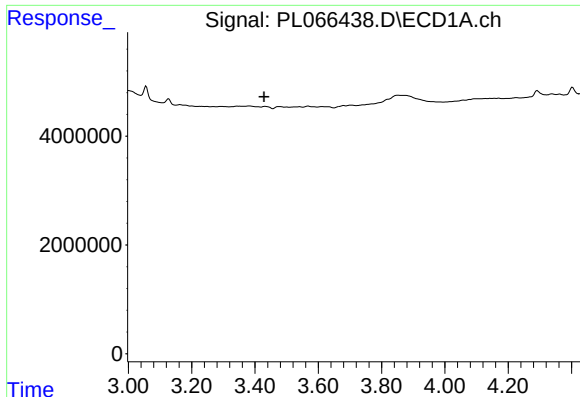

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.429 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

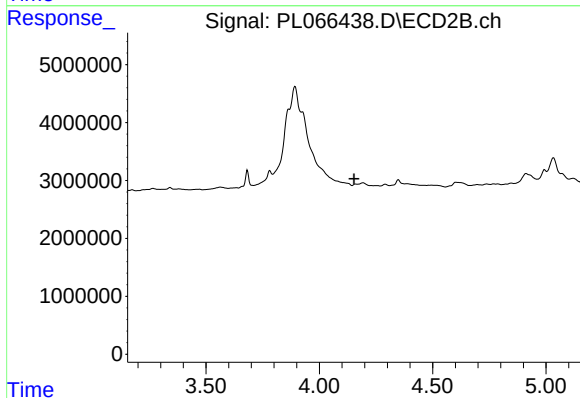


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.153 min
Response: 0
Conc: N.D.

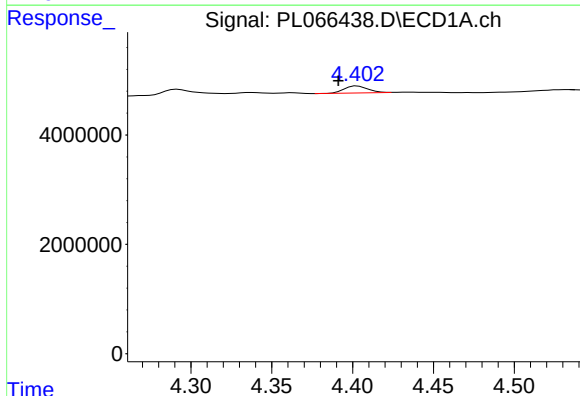


#6 beta-BHC

R.T.: 4.403 min
Delta R.T.: 0.012 min
Response: 1289435
Conc: 0.64 ng/ml

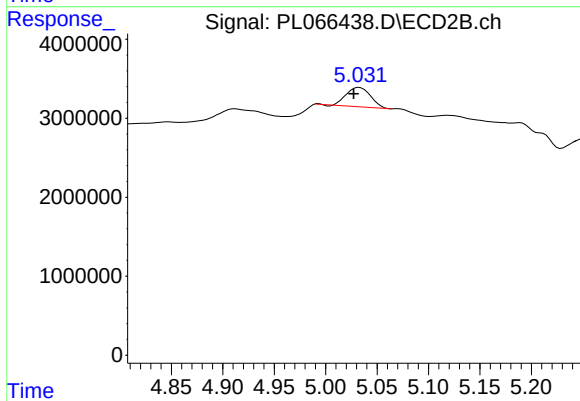

#6 beta-BHC


R.T.: 5.033 min
Delta R.T.: 0.005 min
Response: 3910603
Conc: 1.46 ng/ml

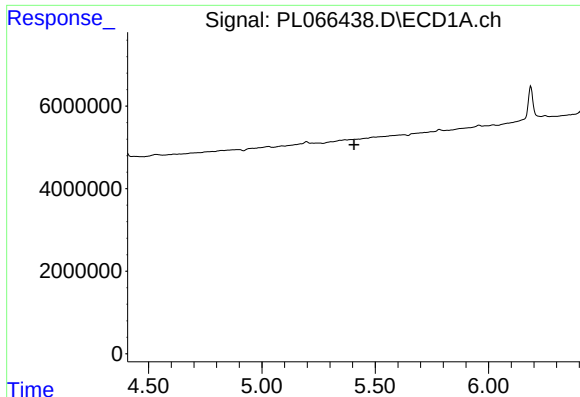

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

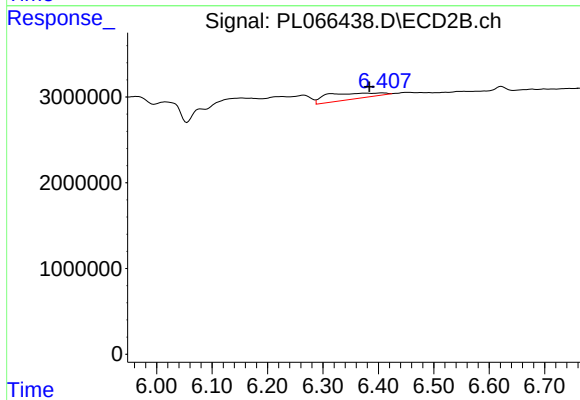


#11 alpha-Chlordane

R.T.: 6.408 min
Delta R.T.: 0.024 min
Response: 4652805
Conc: 1.09 ng/ml

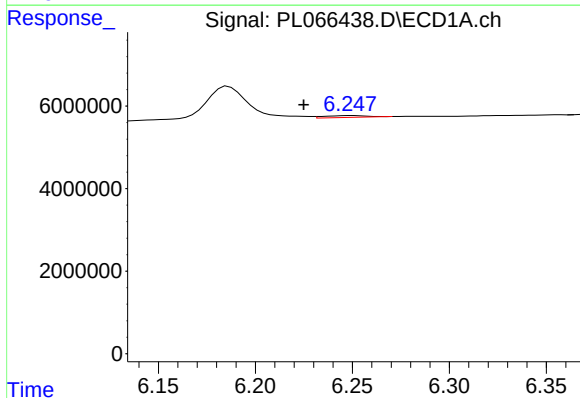


#15 Endosulfan II

R.T.: 6.250 min
Delta R.T.: 0.025 min
Response: 894947
Conc: 0.28 ng/ml

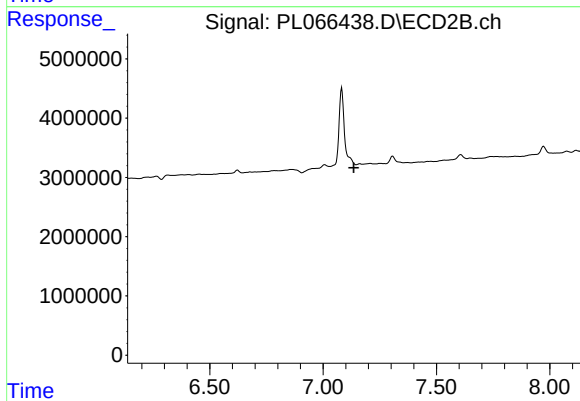

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 7.136 min
Response: 0
Conc: N.D.

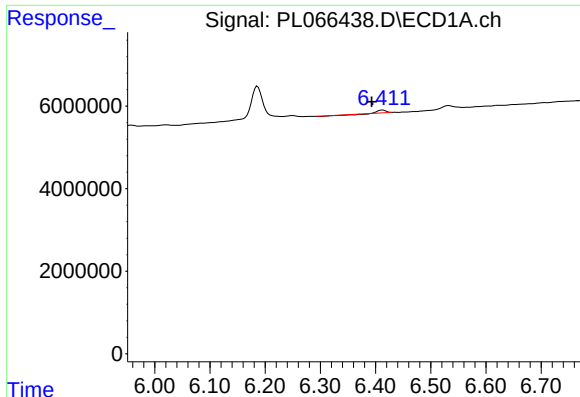

#18 Endrin aldehyde


R.T.: 6.413 min
Delta R.T.: 0.020 min
Response: 352074
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

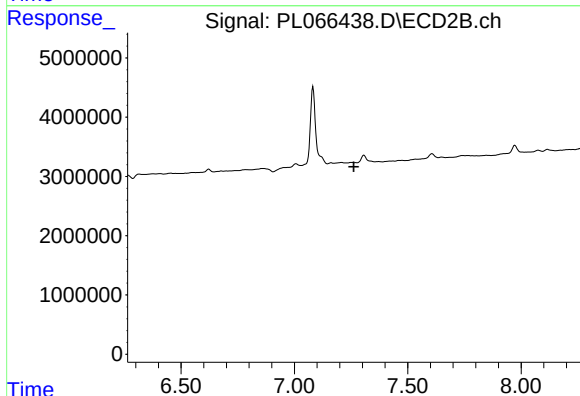


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.261 min
Response: 0
Conc: N.D.

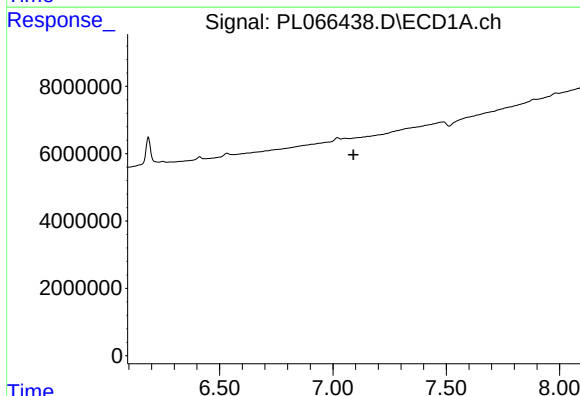


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.091 min
Response: 0
Conc: N.D.

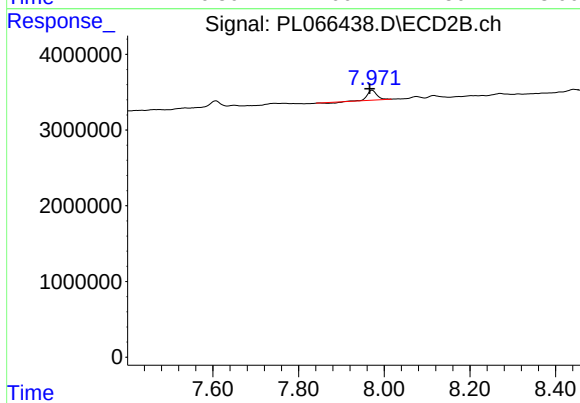

#21 Endrin ketone


R.T.: 7.973 min
Delta R.T.: 0.006 min
Response: 1887655
Conc: 0.50 ng/ml

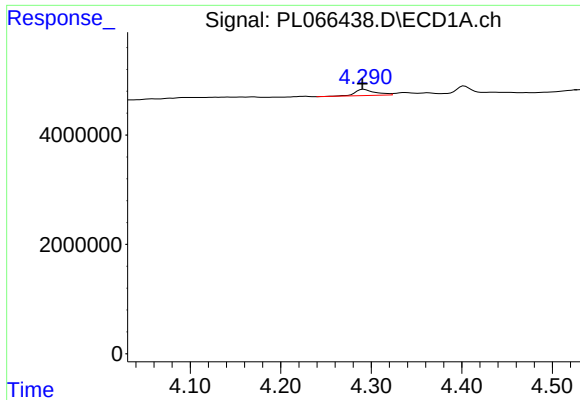

#23 Chlordane-1


R.T.: 4.292 min
Delta R.T.: 0.001 min
Response: 1747166
Conc: 13.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

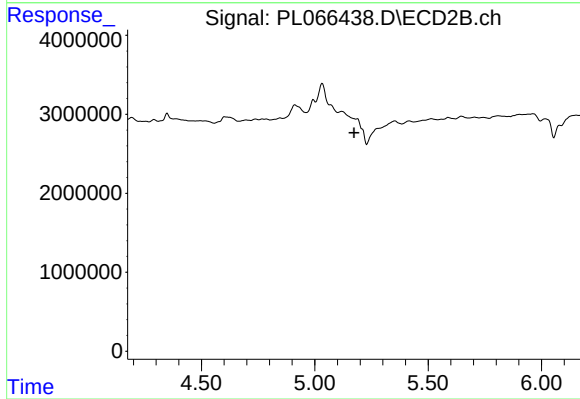


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

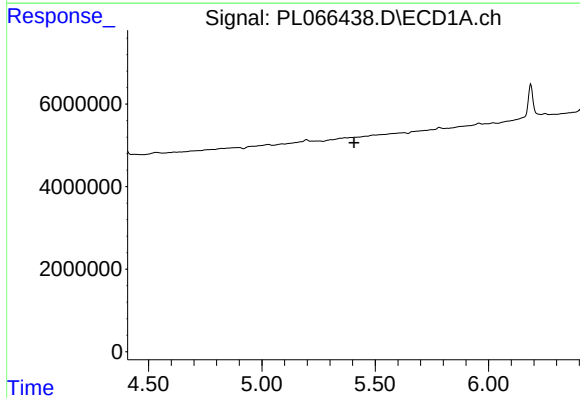


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

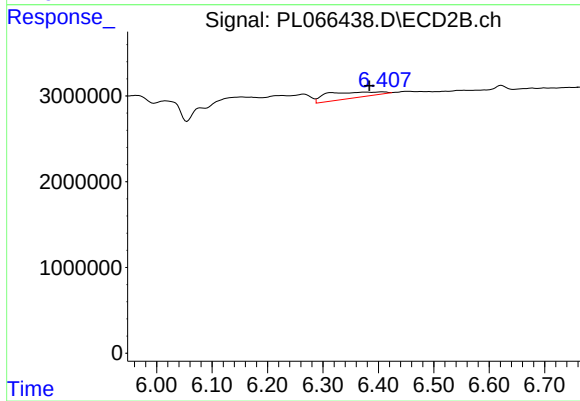

#26 Chlordane-4


R.T.: 6.408 min
Delta R.T.: 0.024 min
Response: 4652805
Conc: 6.40 ng/ml

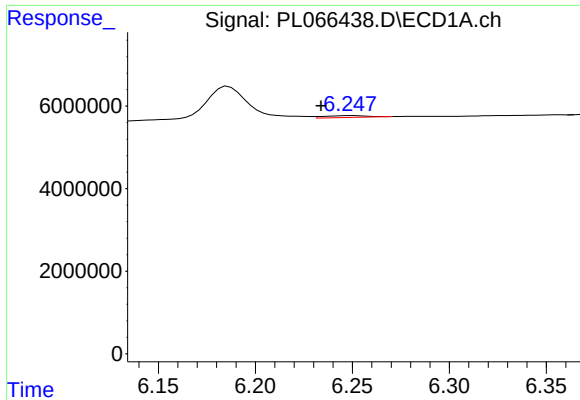

#27 Chlordane-5


R.T.: 6.250 min
Delta R.T.: 0.016 min
Response: 894947
Conc: 6.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

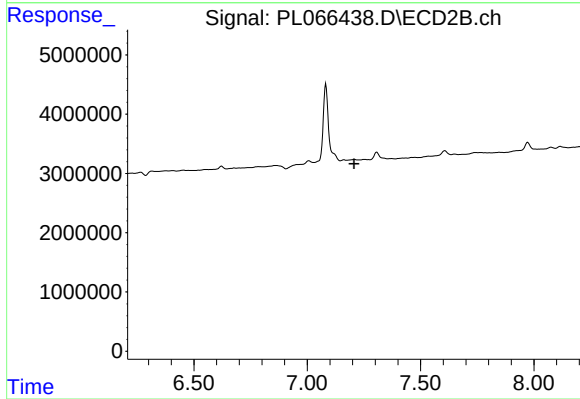


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

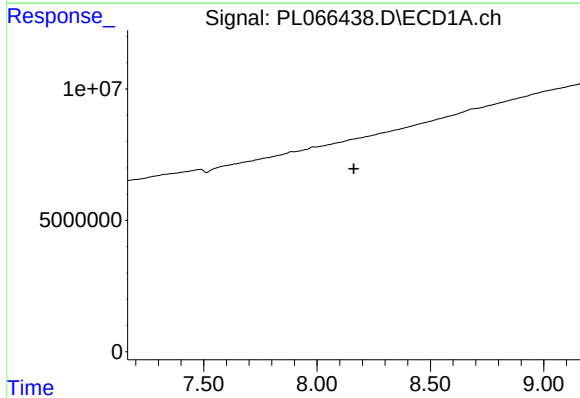

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.162 min
Response: 0
Conc: N.D.

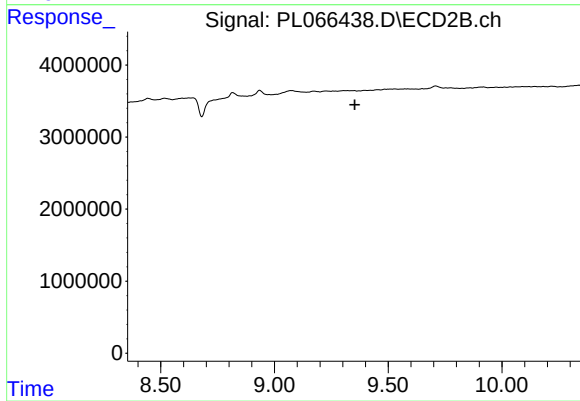

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.353 min
Response: 0
Conc: N.D.