

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 17:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 05:39:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 05:35:56 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.153	58849622	75761092	18.106	21.109
28)	SA Decachlor...	8.158	9.352	55004310	67857841	18.710	21.859
Target Compounds							
2)	A alpha-BHC	3.860	0.000	675758	0	0.135	N.D. #
6)	B beta-BHC	4.403	5.036	924932	5452750	0.457	2.038 #
10)	B gamma-Chl...	0.000	6.312	0	282823	N.D.	0.065 #
15)	B Endosulfa...	6.249f	0.000	575658	0	0.180	N.D. #
18)	B Endrin al...	6.411f	0.000	1764289	0	0.637	N.D. #
21)	B Endrin ke...	0.000	7.973	0	3261228	N.D.	0.860 #
25)	Chlordane-3	0.000	6.312	0	282823	N.D.	0.465 #
27)	Chlordane-5	6.249	0.000	575658	0	4.364	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 17:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 05:39:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 05:35:56 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

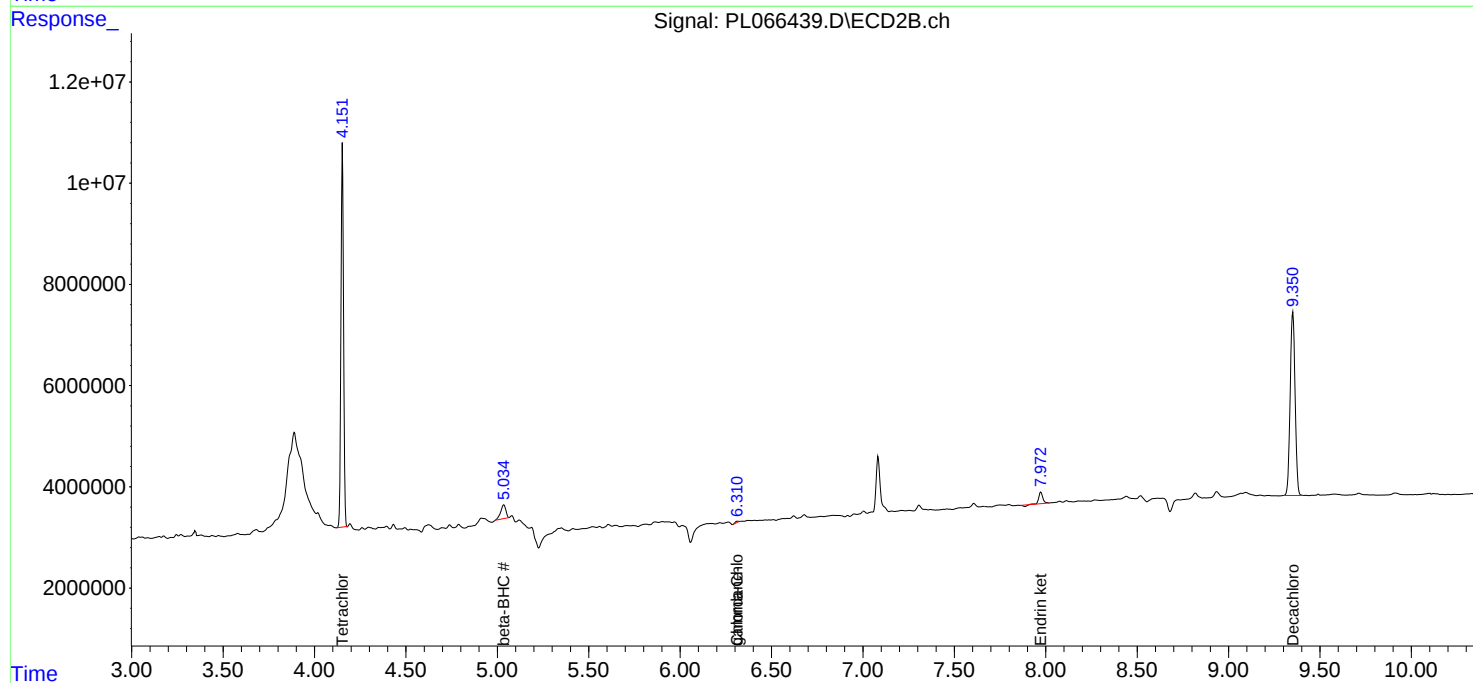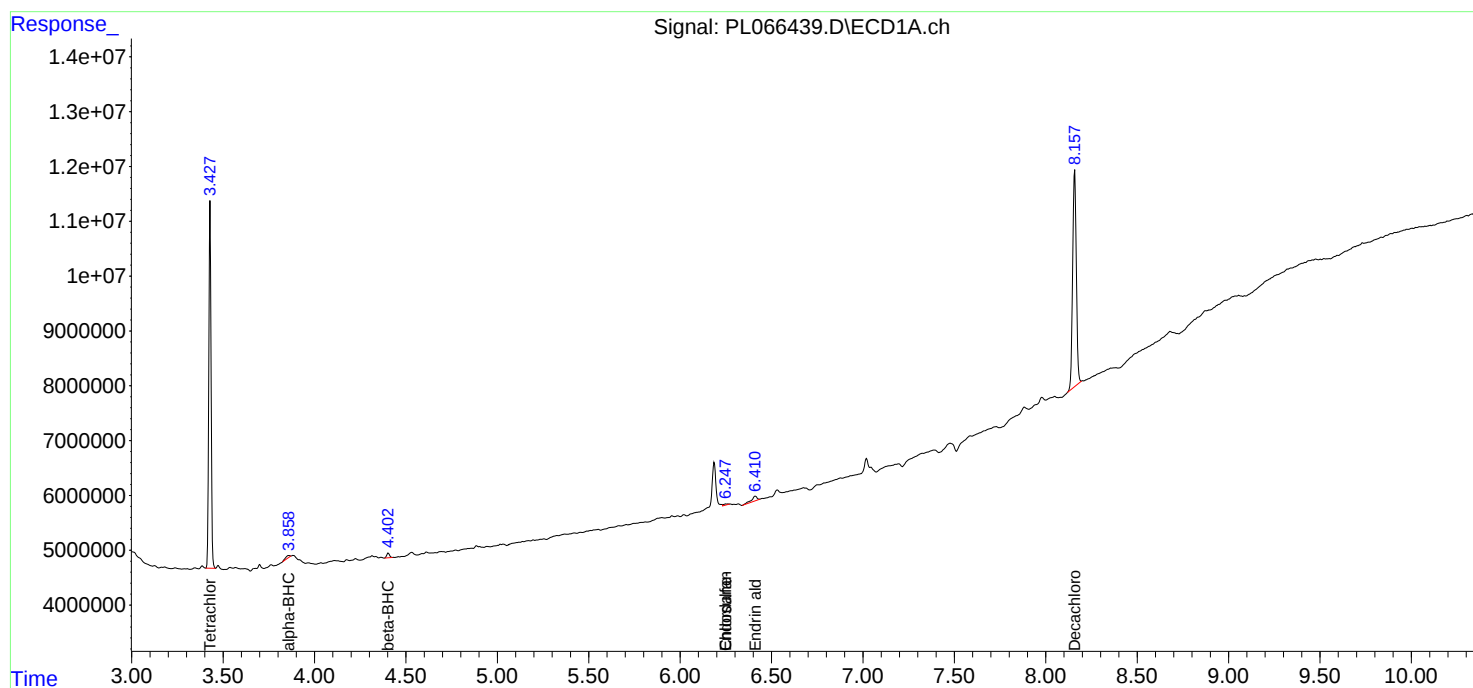


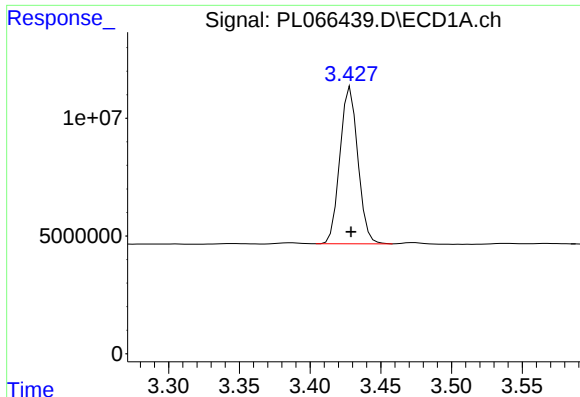

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 58849622
Conc: 18.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

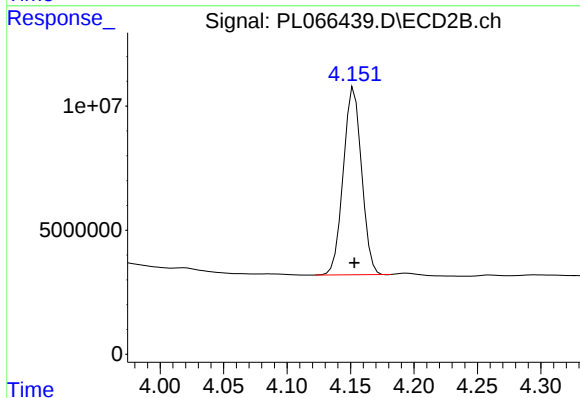


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 75761092
Conc: 21.11 ng/ml

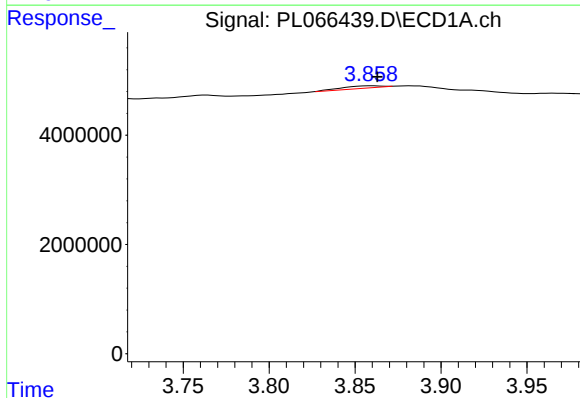


#2 alpha-BHC

R.T.: 3.860 min
Delta R.T.: -0.003 min
Response: 675758
Conc: 0.13 ng/ml

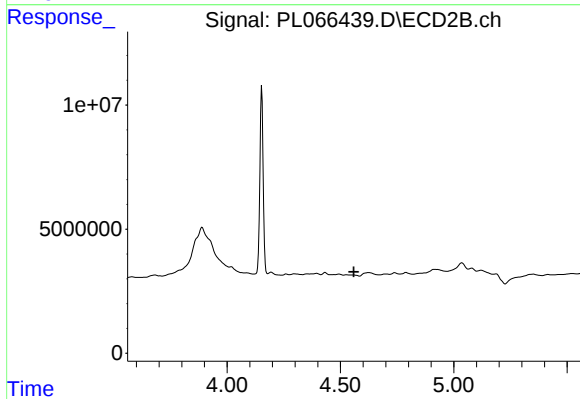

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.558 min
Response: 0
Conc: N.D.

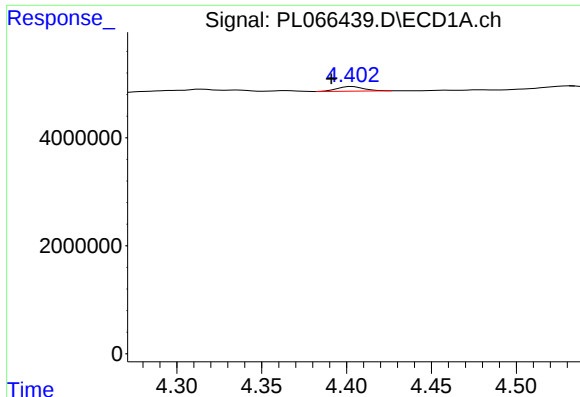

#6 beta-BHC


R.T.: 4.403 min
Delta R.T.: 0.012 min
Response: 924932
Conc: 0.46 ng/ml

Instrument :
ECD_L
ClientSampleId :

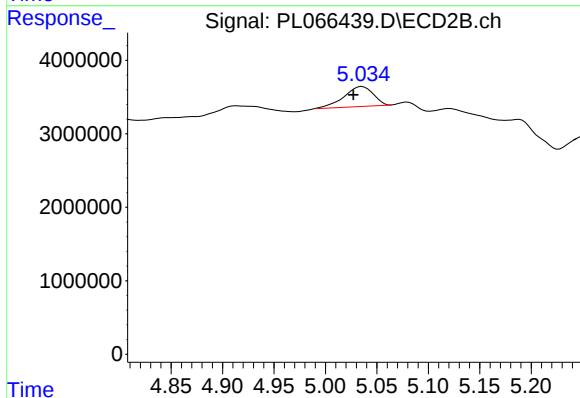


#6 beta-BHC

R.T.: 5.036 min
Delta R.T.: 0.008 min
Response: 5452750
Conc: 2.04 ng/ml

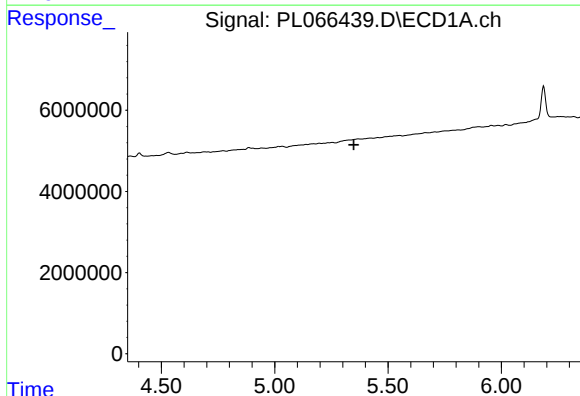


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.349 min
Response: 0
Conc: N.D.

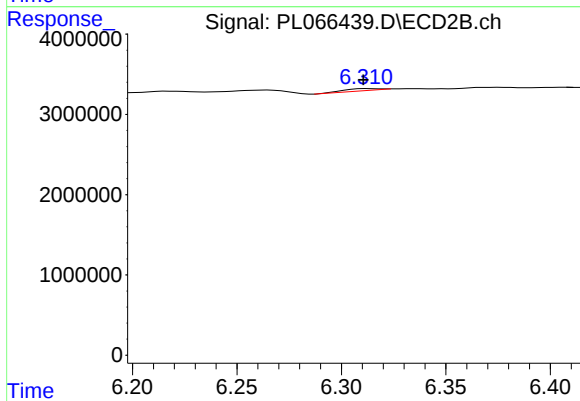

#10 gamma-Chlordane


R.T.: 6.312 min
Delta R.T.: 0.002 min
Response: 282823
Conc: 0.07 ng/ml

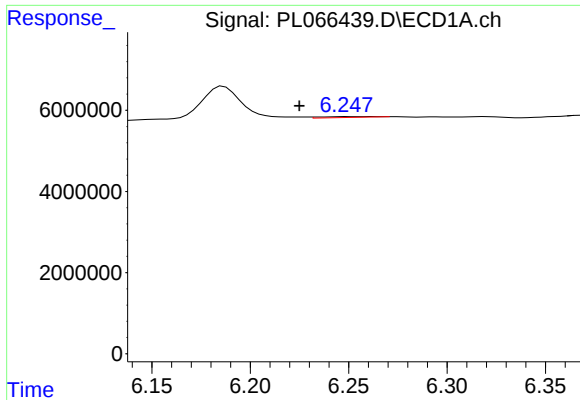

#15 Endosulfan II


R.T.: 6.249 min
Delta R.T.: 0.024 min
Response: 575658
Conc: 0.18 ng/ml

Instrument :
ECD_L
ClientSampleId :

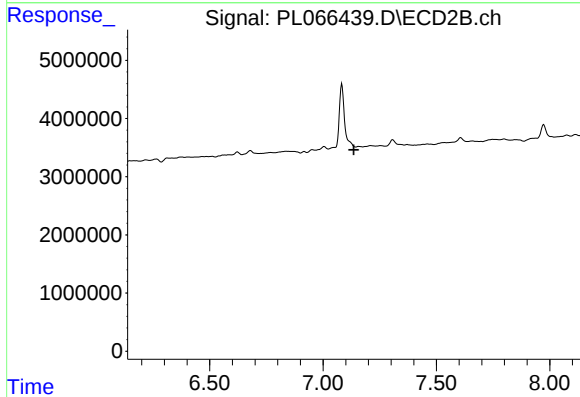


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.136 min
Response: 0
Conc: N.D.

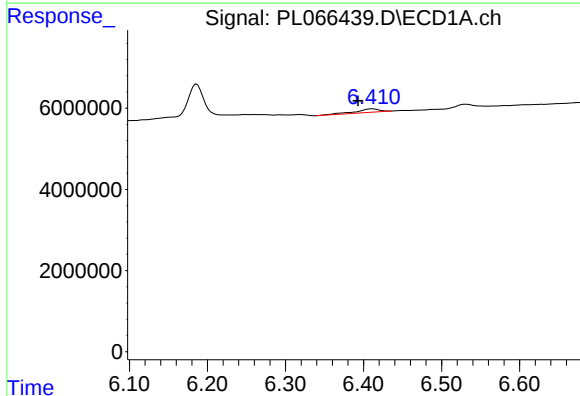


#18 Endrin aldehyde

R.T.: 6.411 min
Delta R.T.: 0.018 min
Response: 1764289
Conc: 0.64 ng/ml

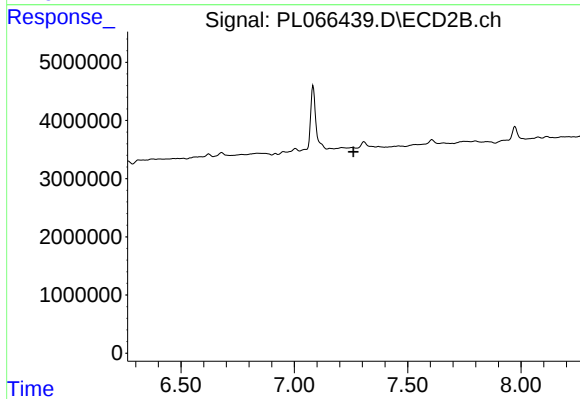

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.261 min
Response: 0
Conc: N.D.

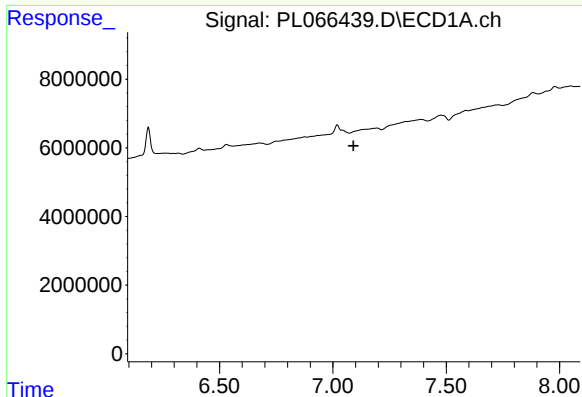

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.091 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

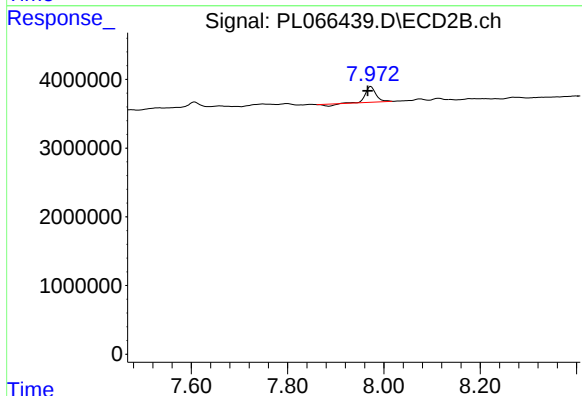


#21 Endrin ketone

R.T.: 7.973 min
Delta R.T.: 0.006 min
Response: 3261228
Conc: 0.86 ng/ml

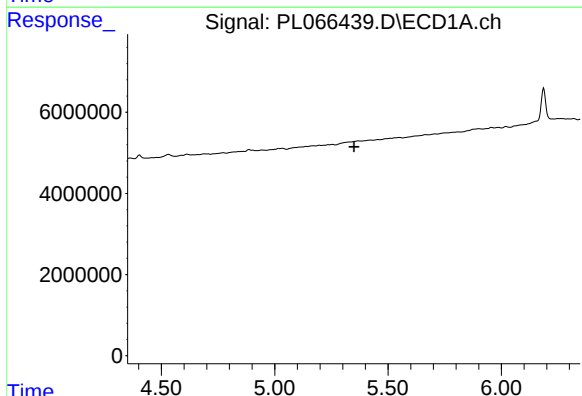


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.350 min
Response: 0
Conc: N.D.

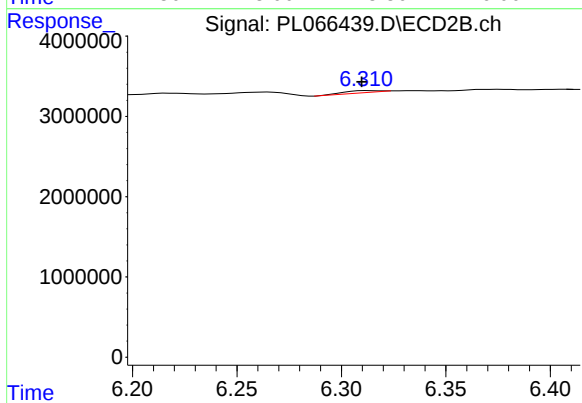

#25 Chlordane-3


R.T.: 6.312 min
Delta R.T.: 0.002 min
Response: 282823
Conc: 0.46 ng/ml

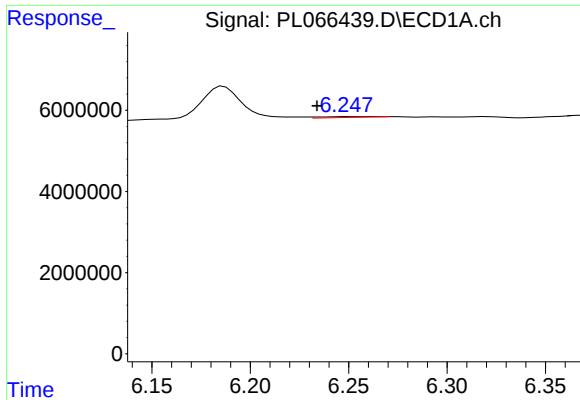

#27 Chlordane-5


R.T.: 6.249 min
Delta R.T.: 0.015 min
Response: 575658
Conc: 4.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

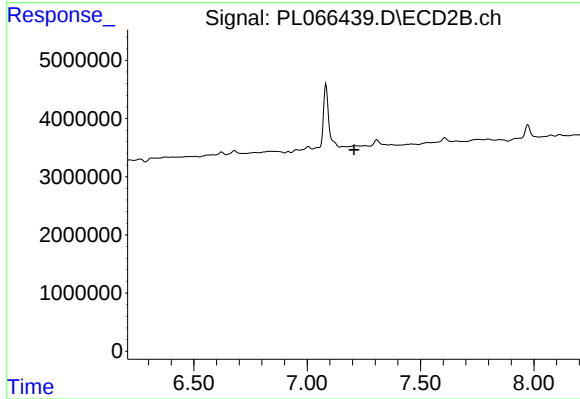


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.206 min
Response: 0
Conc: N.D.

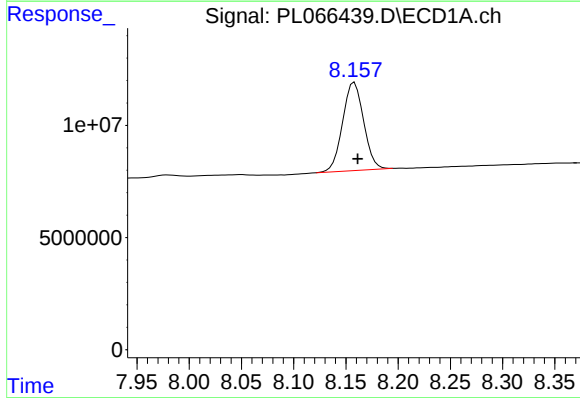

#28 Decachlorobiphenyl

R.T.: 8.158 min
Delta R.T.: -0.003 min
Response: 55004310
Conc: 18.71 ng/ml

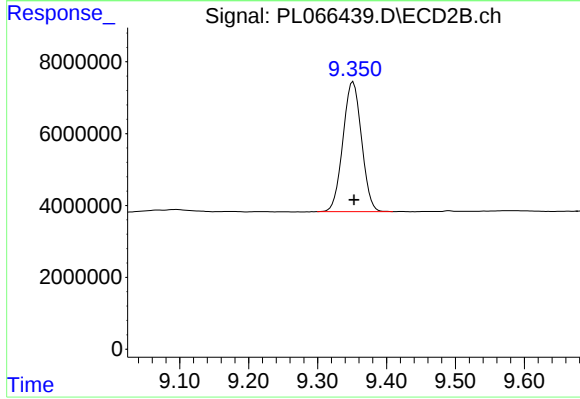

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: -0.001 min
Response: 67857841
Conc: 21.86 ng/ml