

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 21:51
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 04:14:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 04:13:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.153	194.8E6	184.5E6	52.040	51.579
28)	SA Decachlor...	8.160	9.352	142.8E6	160.1E6	47.726	51.058
Target Compounds							
23)	Chlordane-1	4.290	5.173	63599527	84900007	486.156	523.821
24)	Chlordane-2	4.787	5.651	70963852	81841991	507.495	514.675
25)	Chlordane-3	5.349	6.309	202.9E6	322.3E6	512.101	529.601
26)	Chlordane-4	5.407	6.383	170.0E6	385.0E6	509.063	529.992
27)	Chlordane-5	6.233	7.206	65293104	62628971	494.979	525.279



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 21:51
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 04:14:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 04:13:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

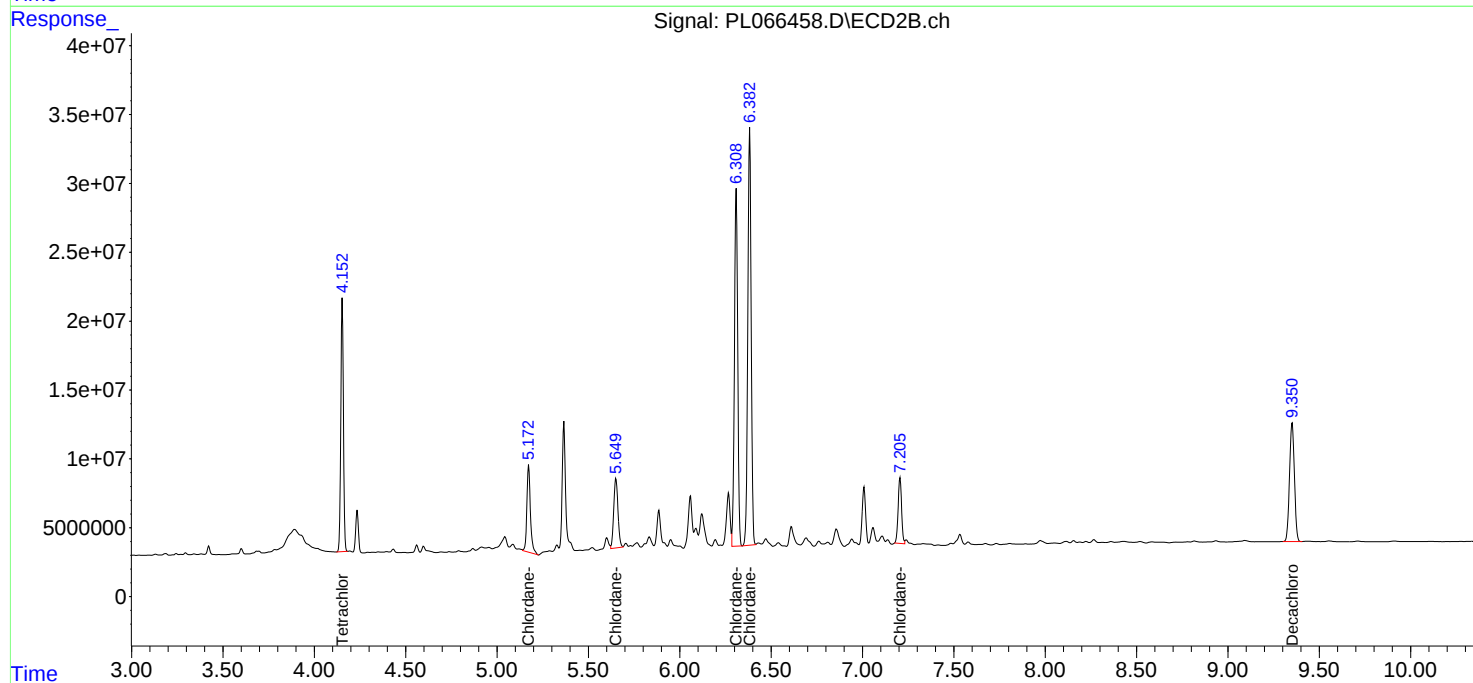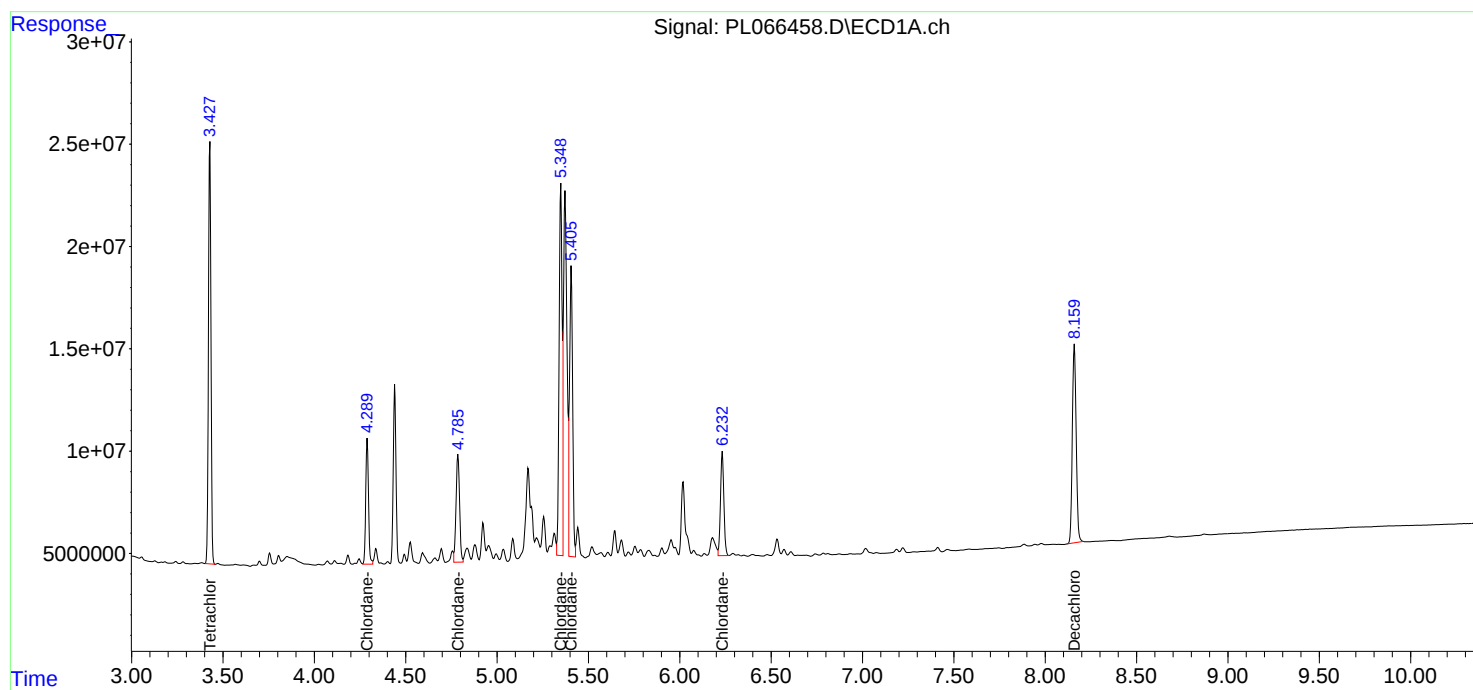


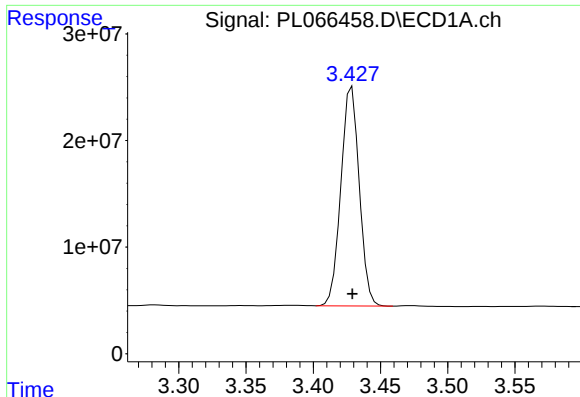

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 194786768
Conc: 52.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

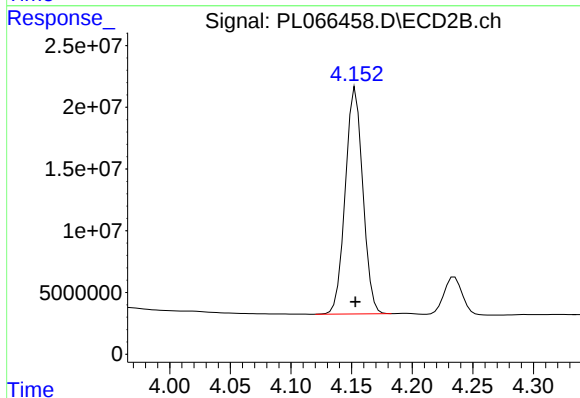


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 184542396
Conc: 51.58 ng/ml

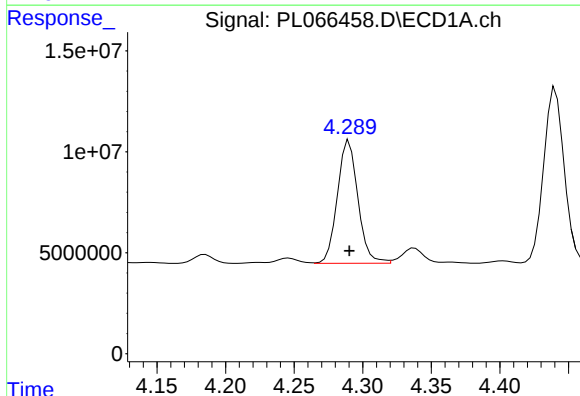


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 63599527
Conc: 486.16 ng/ml

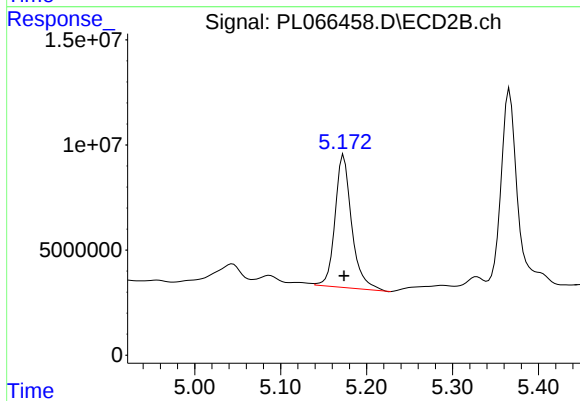

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 84900007
Conc: 523.82 ng/ml

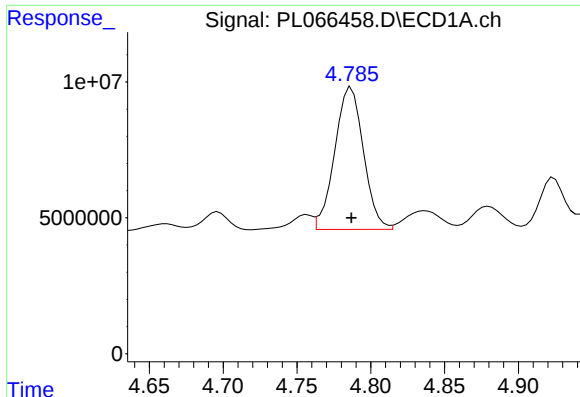

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 70963852
Conc: 507.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

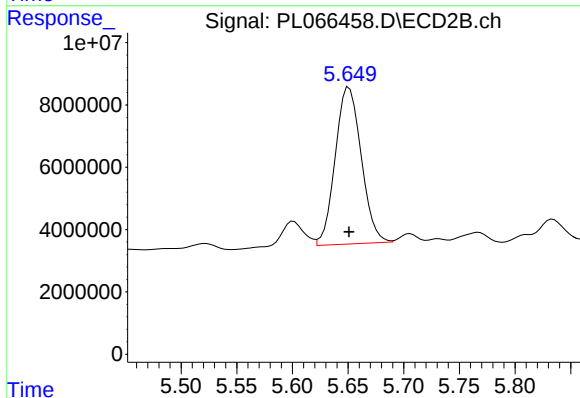


#24 Chlordane-2

R.T.: 5.651 min
Delta R.T.: 0.000 min
Response: 81841991
Conc: 514.67 ng/ml

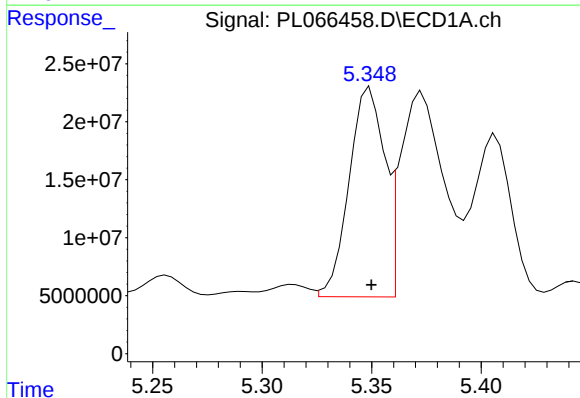


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 202854018
Conc: 512.10 ng/ml

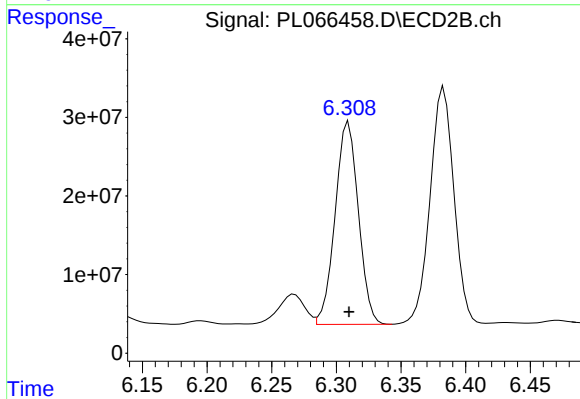

#25 Chlordane-3


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 322316878
Conc: 529.60 ng/ml

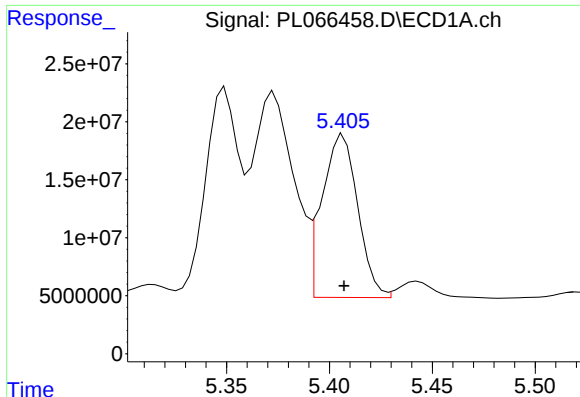

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 169953705
Conc: 509.06 ng/ml

Instrument :
ECD_L
ClientSampleId :

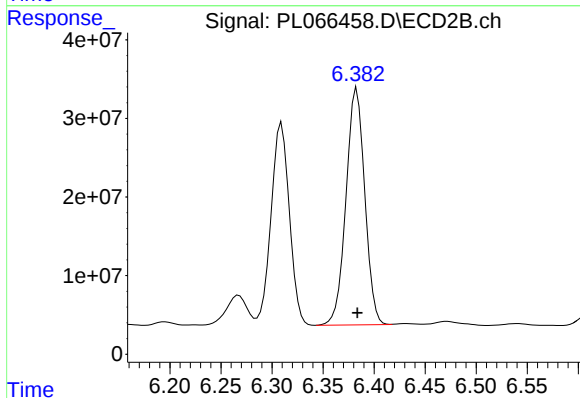


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 385039127
Conc: 529.99 ng/ml

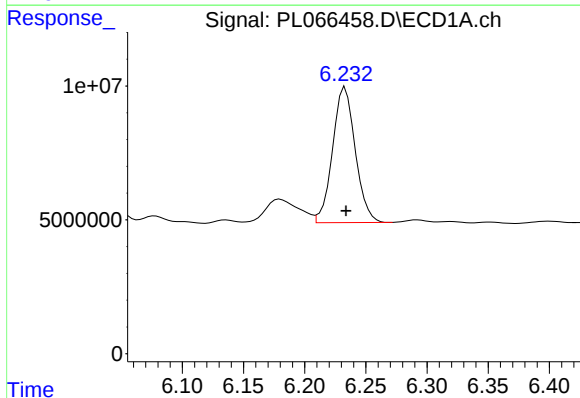


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 65293104
Conc: 494.98 ng/ml

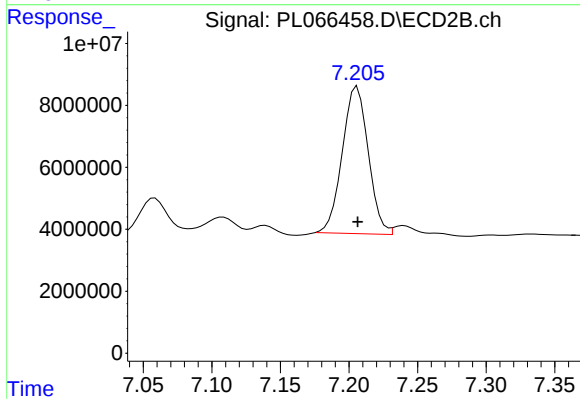

#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 62628971
Conc: 525.28 ng/ml

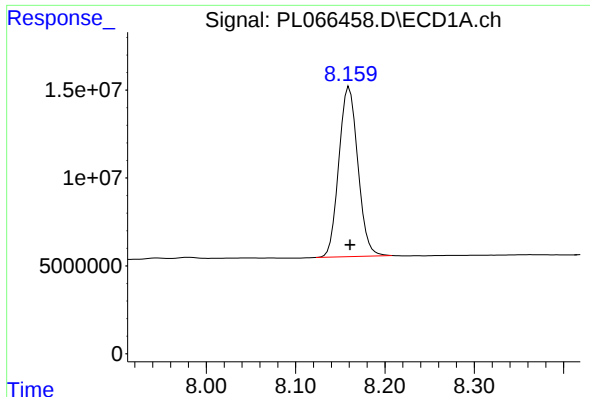

#28 Decachlorobiphenyl


R.T.: 8.160 min

Delta R.T.: -0.001 min

Response: 142840914

Conc: 47.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

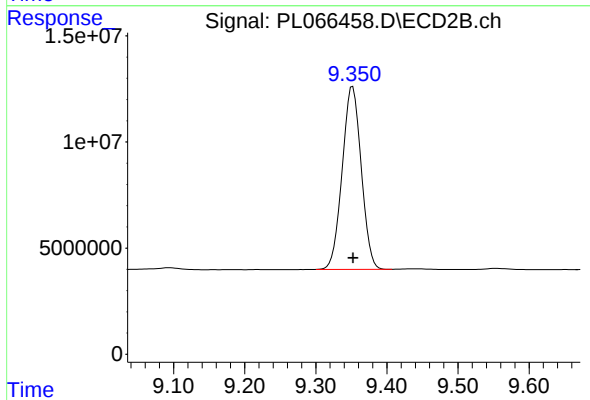

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 160110800

Conc: 51.06 ng/ml