

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 19:13
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 03:54:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 03:53:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.153	382.9E6	357.8E6	99.124	96.430
28)	SA Decachlor...	8.161	9.352	280.7E6	288.3E6	92.576	89.177
Target Compounds							
23)	Chlordane-1	4.290	5.174	120.9E6	159.7E6	939.471	964.566
24)	Chlordane-2	4.786	5.652	133.2E6	151.8E6	925.526	941.316
25)	Chlordane-3	5.349	6.310	401.9E6	627.8E6	980.725	990.967
26)	Chlordane-4	5.407	6.384	340.2E6	735.9E6	983.538	983.804
27)	Chlordane-5	6.233	7.207	129.8E6	122.4E6	960.373	983.808



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 19:13
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 03:54:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 03:53:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

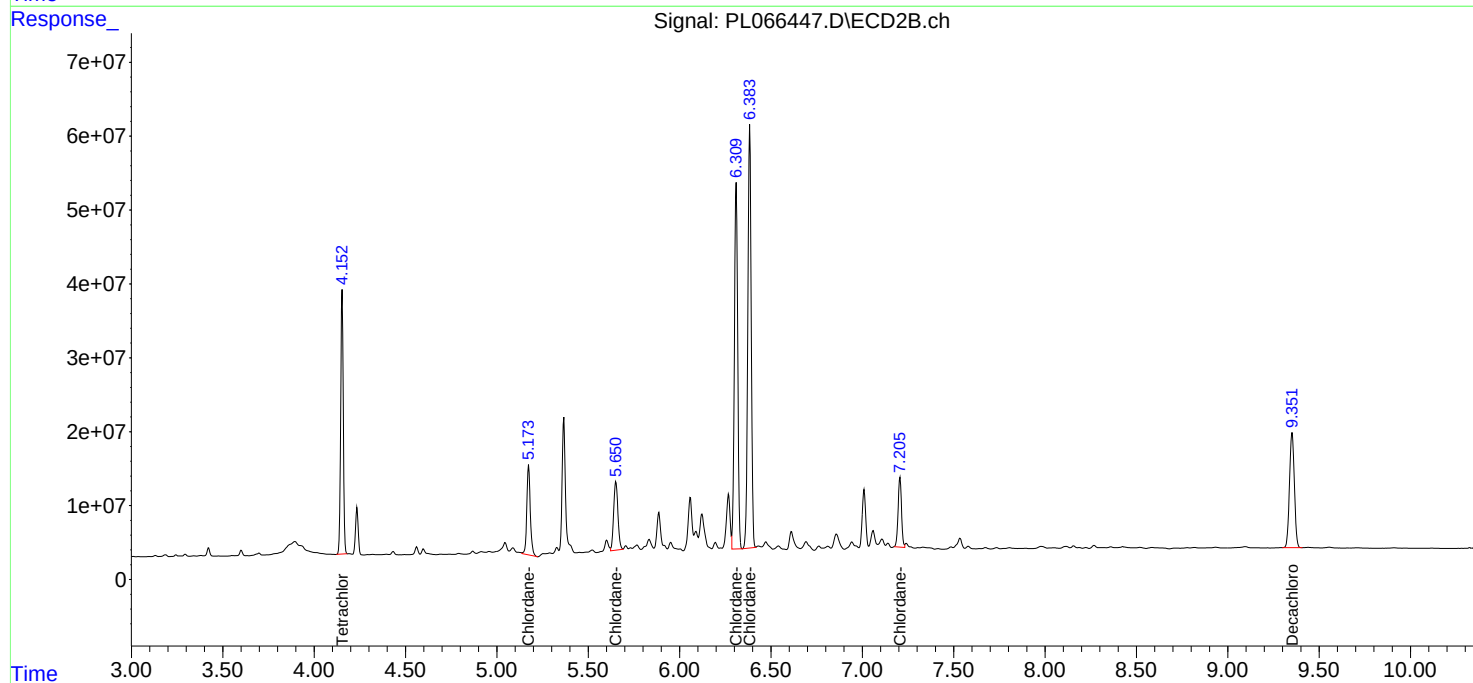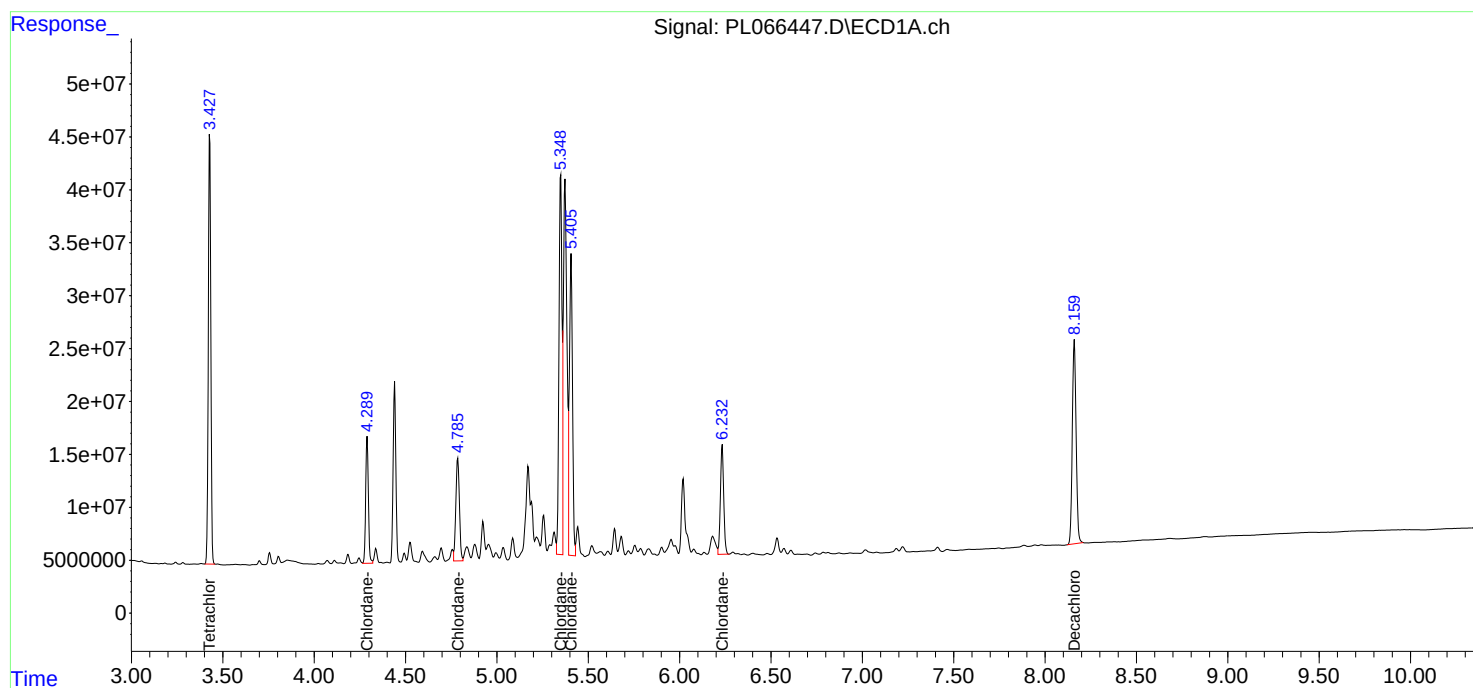


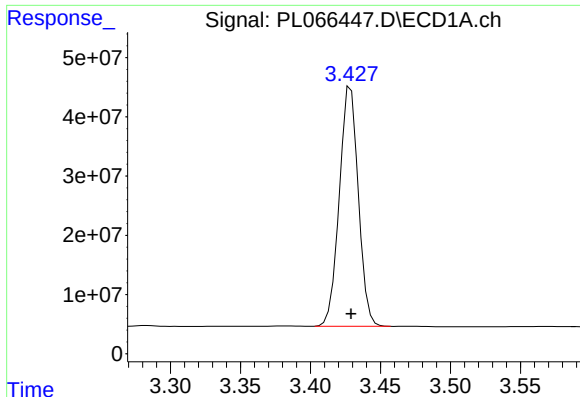

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 382881555
Conc: 99.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

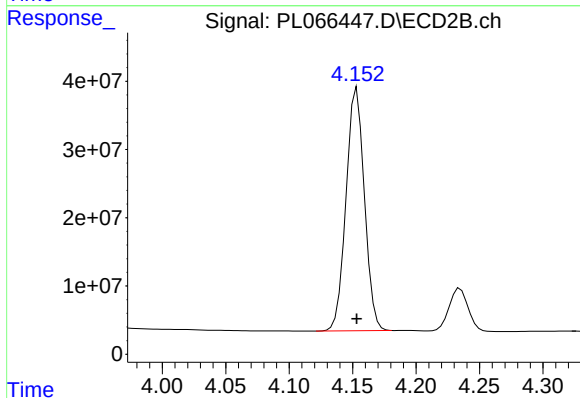


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 357782947
Conc: 96.43 ng/ml

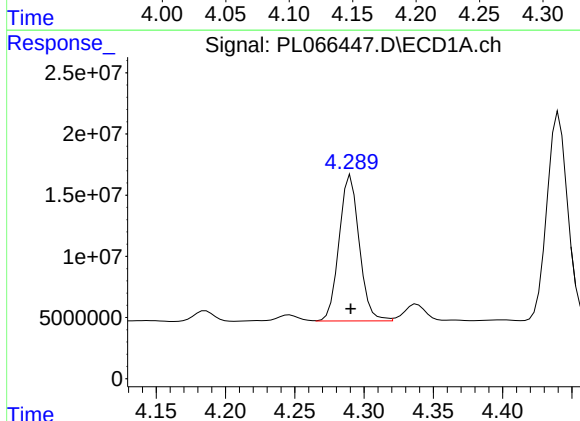


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 120929456
Conc: 939.47 ng/ml

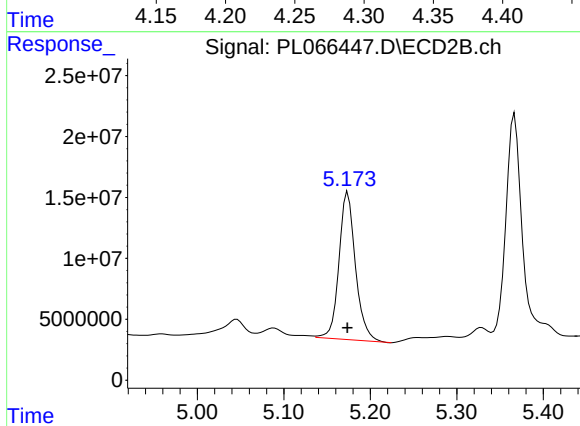

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 159680852
Conc: 964.57 ng/ml

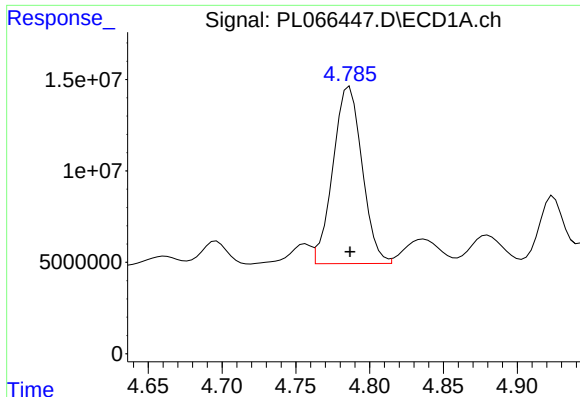

#24 Chlordane-2


R.T.: 4.786 min
Delta R.T.: 0.000 min
Response: 133189299
Conc: 925.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

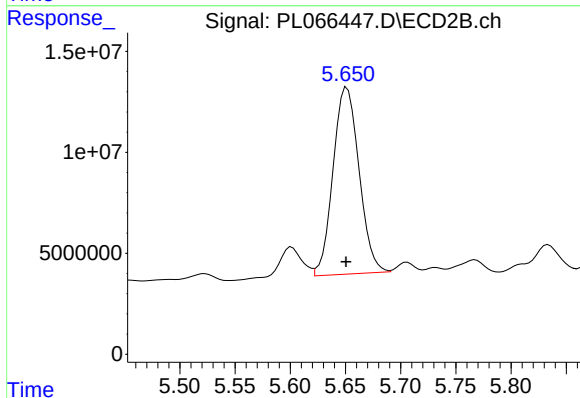


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.000 min
Response: 151762670
Conc: 941.32 ng/ml

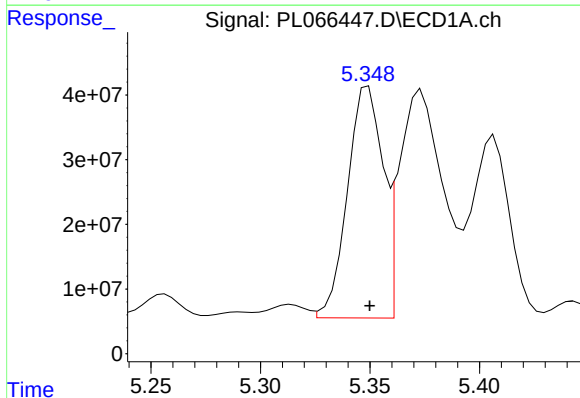


#25 Chlordane-3

R.T.: 5.349 min
Delta R.T.: 0.000 min
Response: 401932197
Conc: 980.72 ng/ml

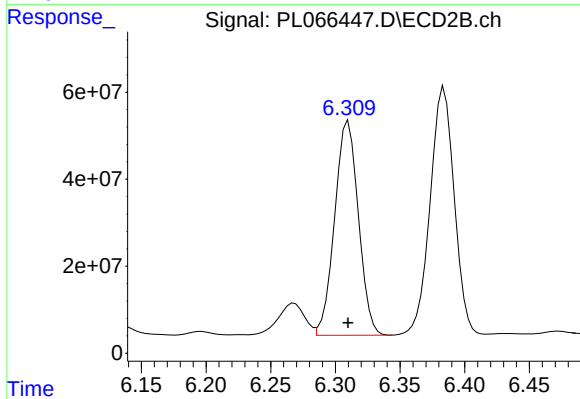

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 627769716
Conc: 990.97 ng/ml

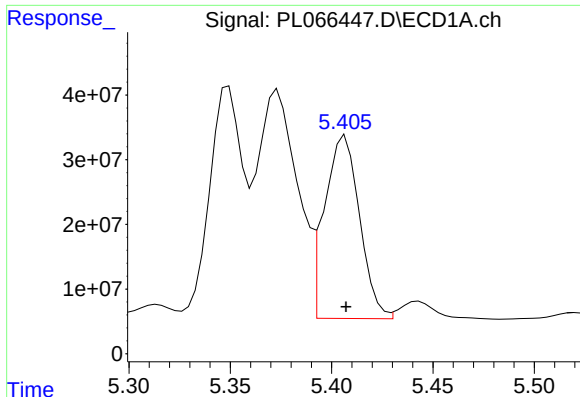

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 340248943
Conc: 983.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

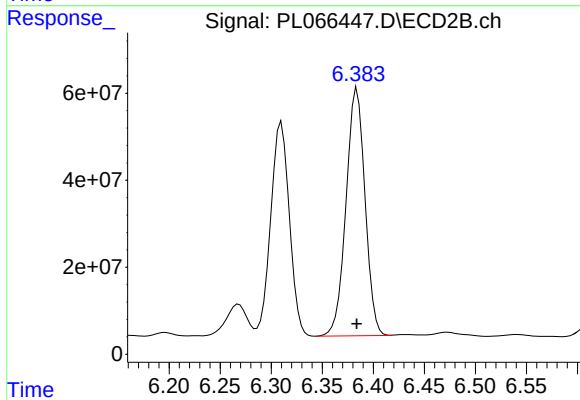


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 735942714
Conc: 983.80 ng/ml

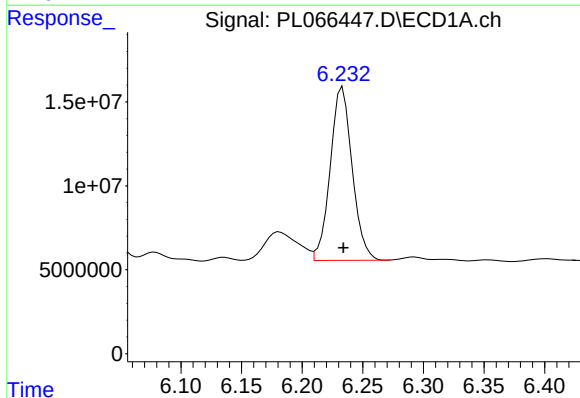


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 129776107
Conc: 960.37 ng/ml

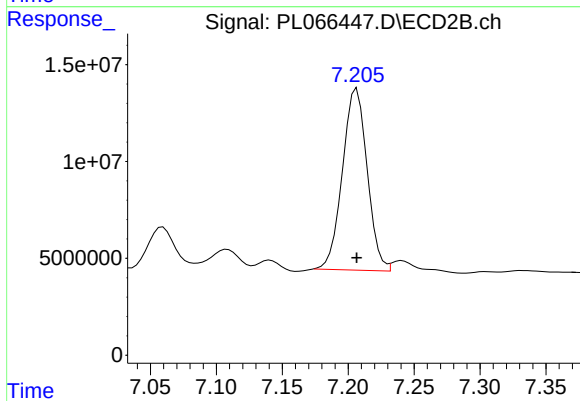

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 122399237
Conc: 983.81 ng/ml

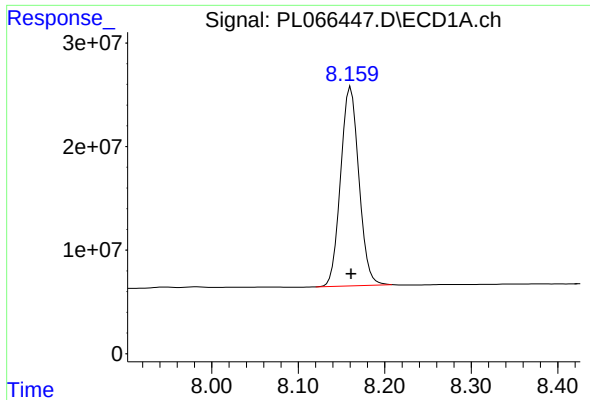

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 280736195
Conc: 92.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

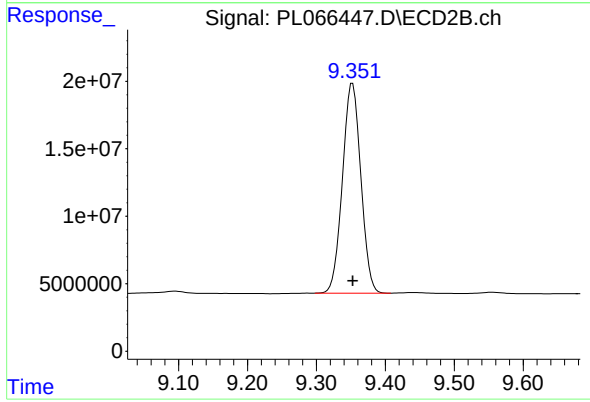

#28 Decachlorobiphenyl

R.T.: 9.352 min
Delta R.T.: 0.000 min
Response: 288261851
Conc: 89.18 ng/ml