

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 19:27
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 03:54:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 03:53:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.154	289.0E6	264.4E6	74.824	71.255
28)	SA Decachlor...	8.161	9.353	219.1E6	220.8E6	72.255	68.309
Target Compounds							
23)	Chlordane-1	4.291	5.174	92198597	114.1E6	716.268	689.107
24)	Chlordane-2	4.787	5.652	101.7E6	109.9E6	706.726	681.759
25)	Chlordane-3	5.350	6.310	304.2E6	446.0E6	742.166	704.061
26)	Chlordane-4	5.407	6.384	254.3E6	525.9E6	735.184	702.989
27)	Chlordane-5	6.234	7.207	97611176	87965044	722.345	707.036



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 19:27
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 03:54:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 03:53:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

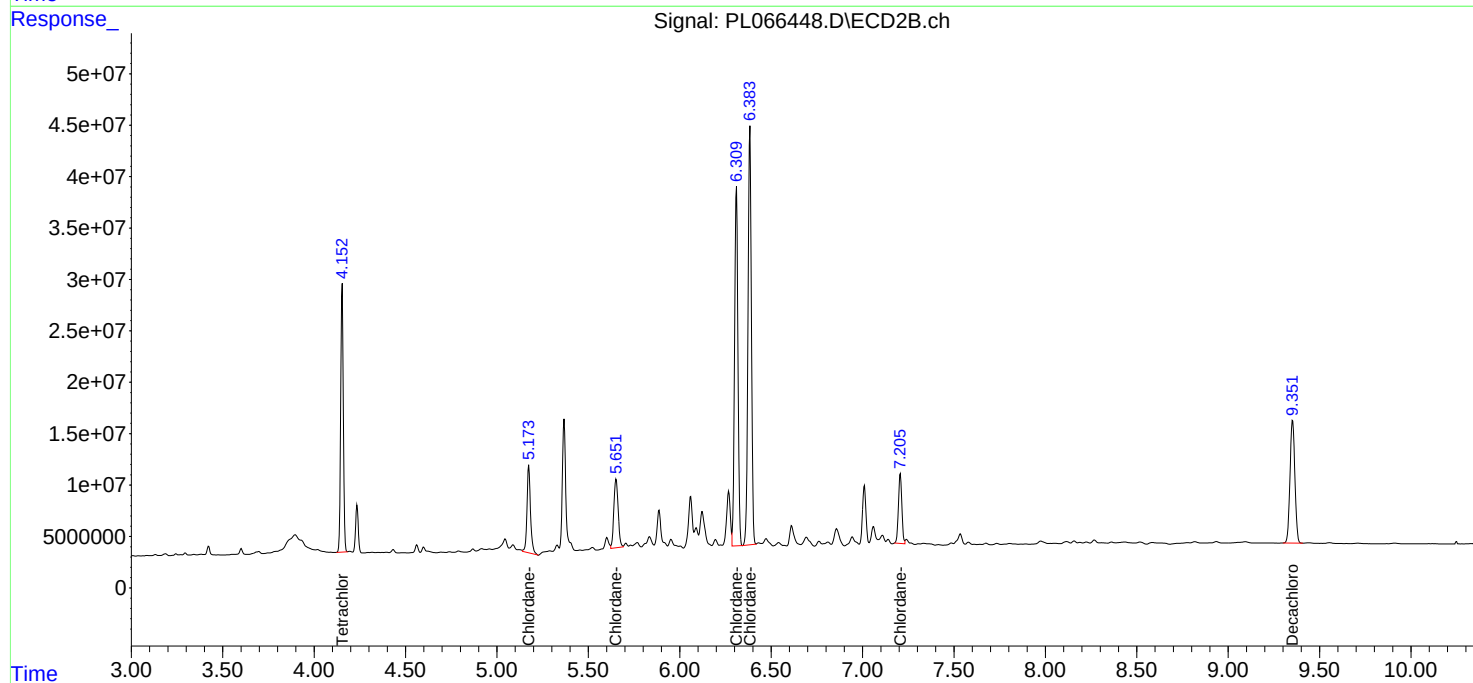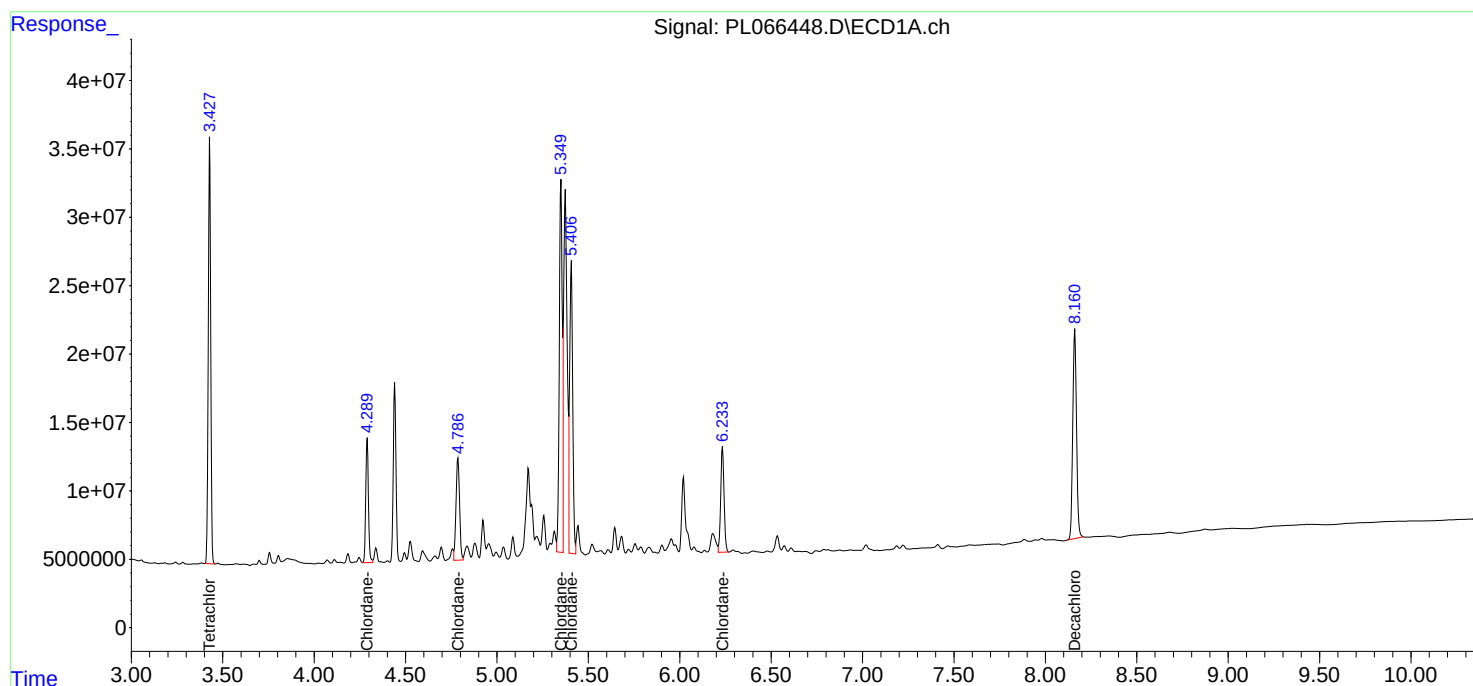


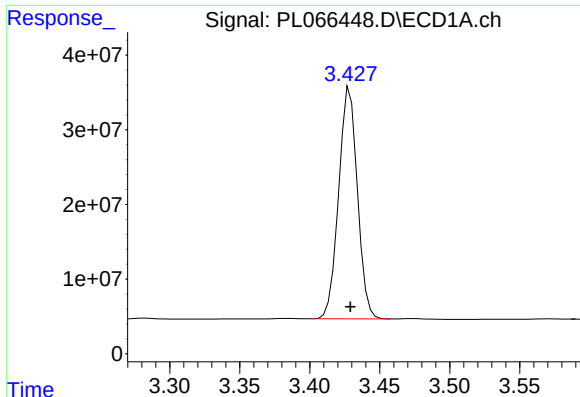

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.000 min
Response: 289019315
Conc: 74.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

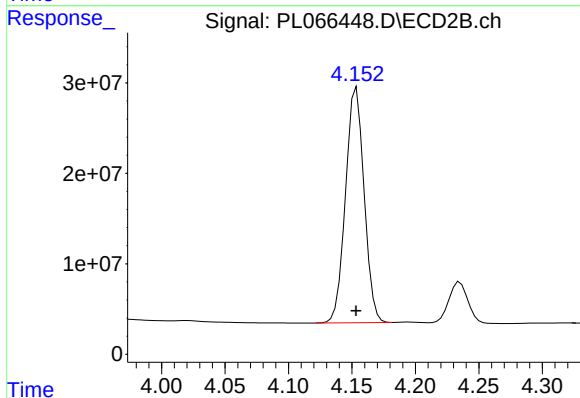


#1 Tetrachloro-m-xylene

R.T.: 4.154 min
Delta R.T.: 0.000 min
Response: 264377423
Conc: 71.26 ng/ml

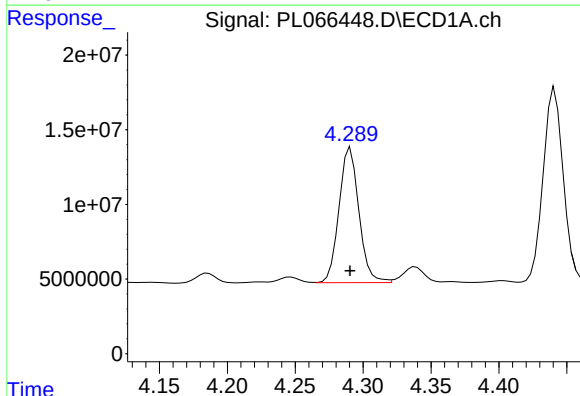


#23 Chlordane-1

R.T.: 4.291 min
Delta R.T.: 0.000 min
Response: 92198597
Conc: 716.27 ng/ml

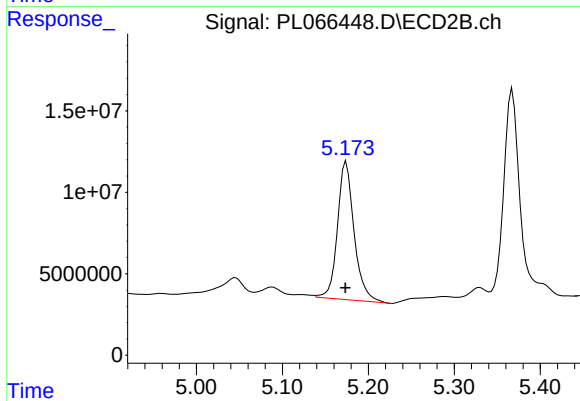

#23 Chlordane-1


R.T.: 5.174 min
Delta R.T.: 0.000 min
Response: 114079574
Conc: 689.11 ng/ml

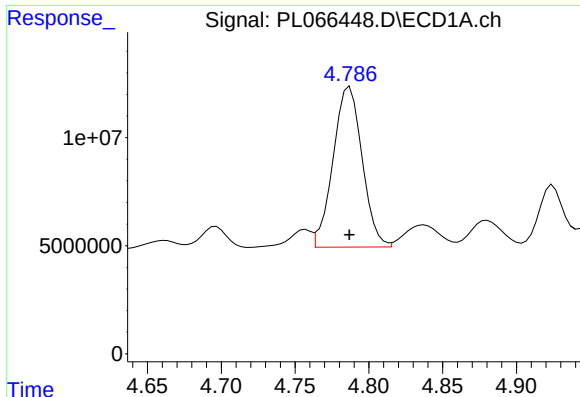

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 101702610
Conc: 706.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

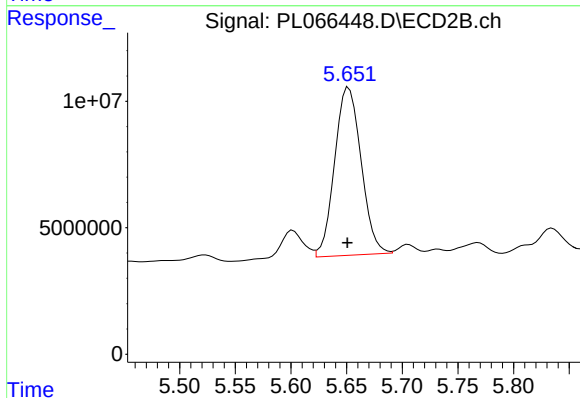


#24 Chlordane-2

R.T.: 5.652 min
Delta R.T.: 0.001 min
Response: 109915828
Conc: 681.76 ng/ml

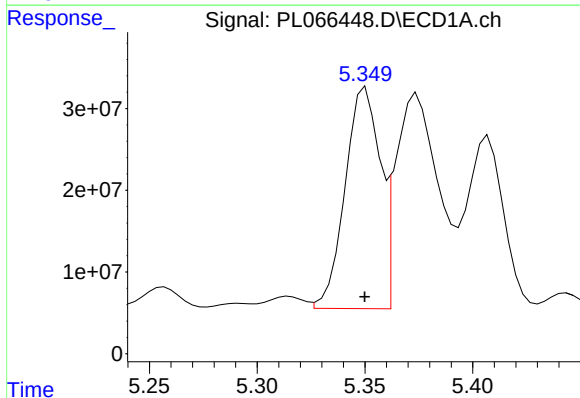


#25 Chlordane-3

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 304163353
Conc: 742.17 ng/ml

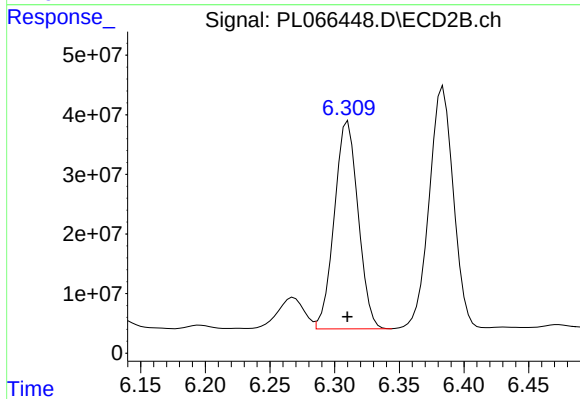

#25 Chlordane-3


R.T.: 6.310 min
Delta R.T.: 0.000 min
Response: 446017156
Conc: 704.06 ng/ml

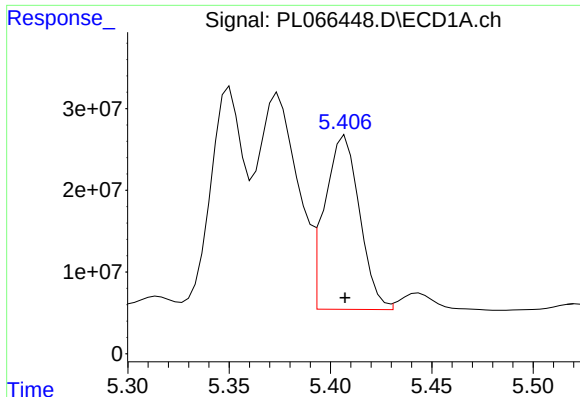

#26 Chlordane-4


R.T.: 5.407 min
Delta R.T.: 0.000 min
Response: 254332342
Conc: 735.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

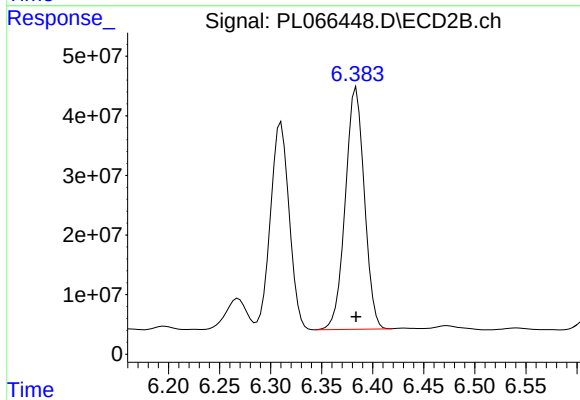


#26 Chlordane-4

R.T.: 6.384 min
Delta R.T.: 0.000 min
Response: 525876309
Conc: 702.99 ng/ml

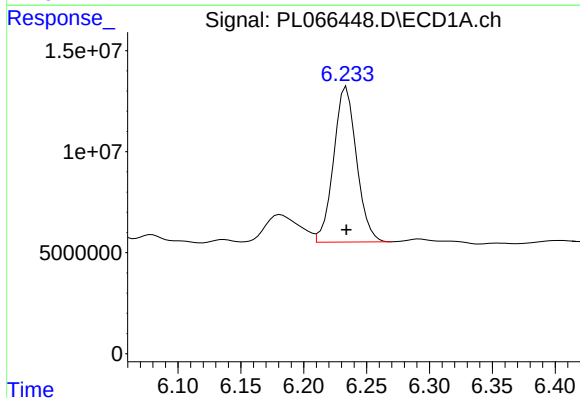


#27 Chlordane-5

R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 97611176
Conc: 722.35 ng/ml

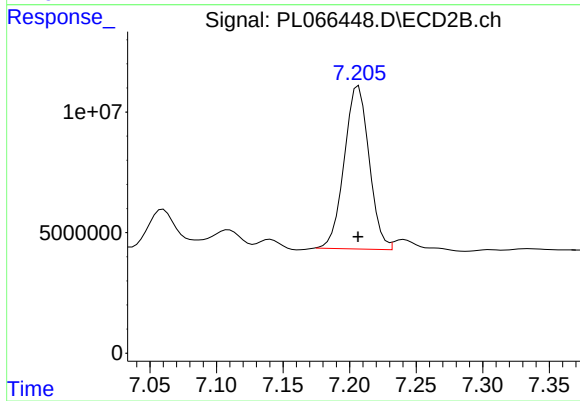

#27 Chlordane-5


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 87965044
Conc: 707.04 ng/ml

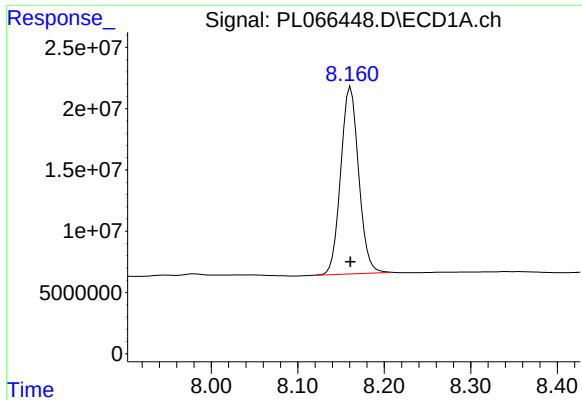

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: 0.000 min
Response: 219113268
Conc: 72.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

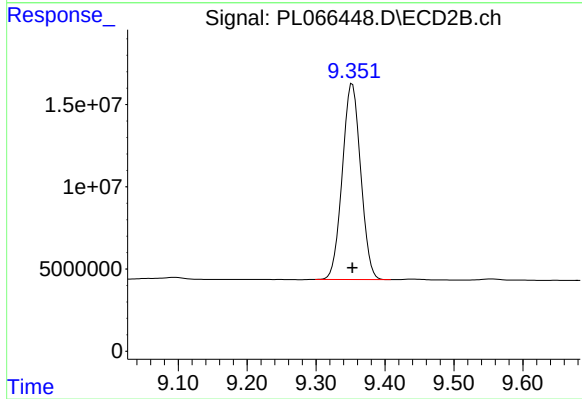

#28 Decachlorobiphenyl

R.T.: 9.353 min
Delta R.T.: 0.000 min
Response: 220804396
Conc: 68.31 ng/ml