

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
 Data File : PL066450.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2021 19:56
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 03:54:56 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
 Quant Title : GC Extractables
 QLast Update : Mon Apr 26 03:53:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.153	92345669	90361469	23.907	24.354
28)	SA Decachlor...	8.161	9.352	76935248	81851679	25.370	25.322
Target Compounds							
23)	Chlordane-1	4.290	5.173	33185735	42206241	257.812	254.950
24)	Chlordane-2	4.787	5.650	36480692	40964629	253.502	254.085
25)	Chlordane-3	5.350	6.309	98192557	150.1E6	239.592	236.957
26)	Chlordane-4	5.406	6.383	83843785	180.8E6	242.362	241.691
27)	Chlordane-5	6.233	7.206	33052010	30571046	244.592	245.721



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042321\
Data File : PL066450.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2021 19:56
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 03:54:56 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042321.M
Quant Title : GC Extractables
QLast Update : Mon Apr 26 03:53:51 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

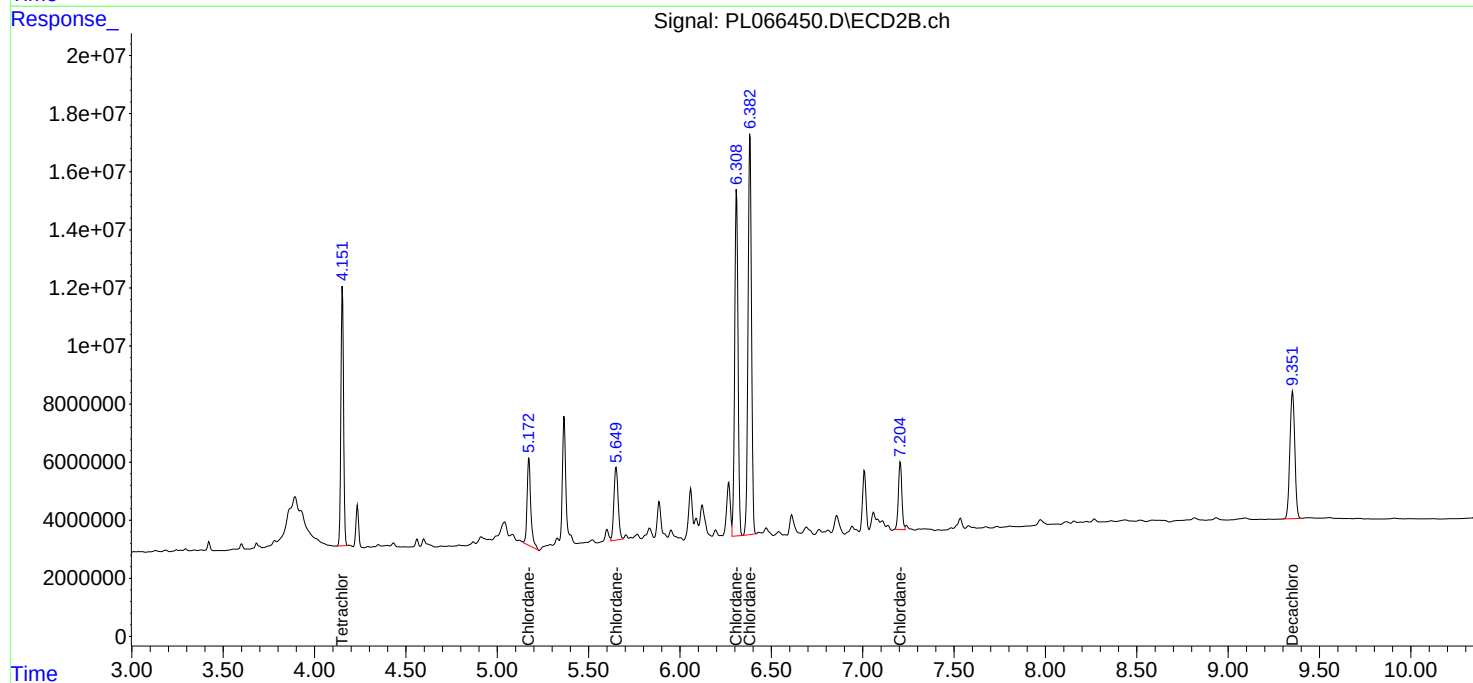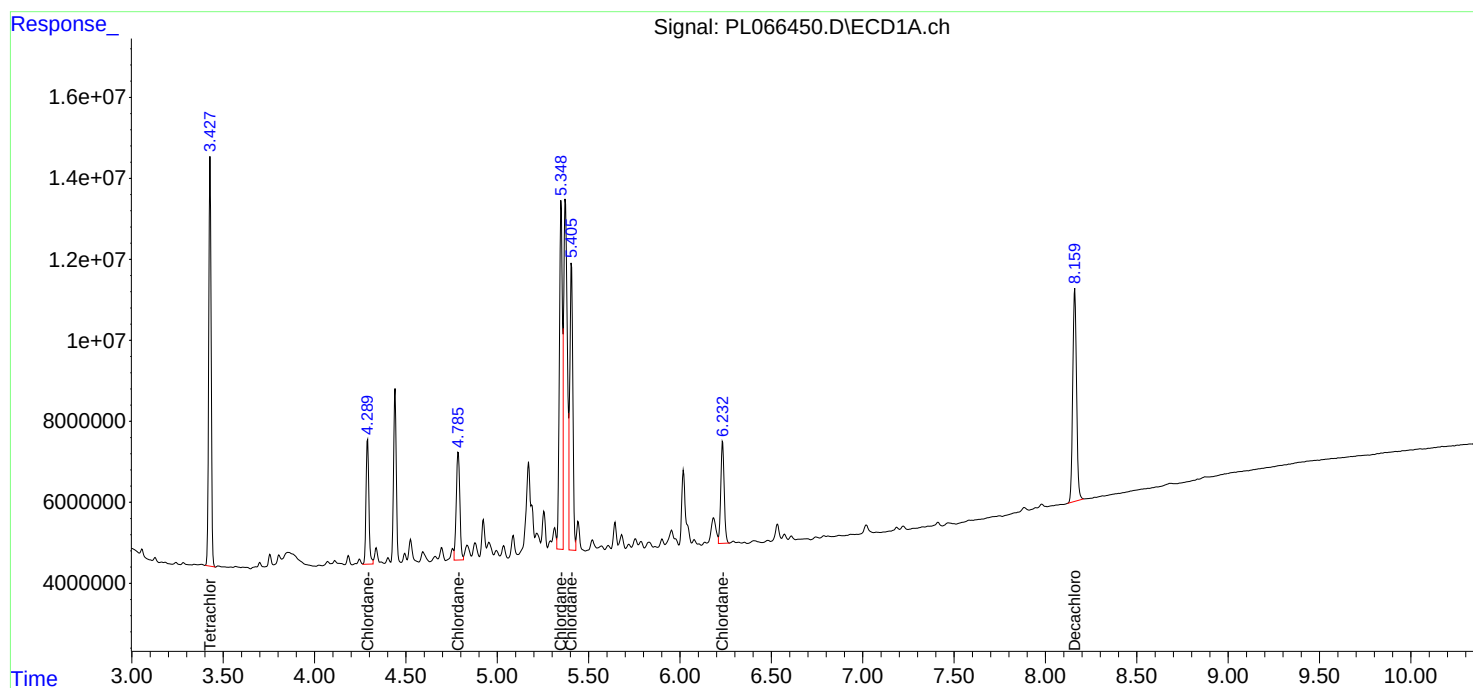


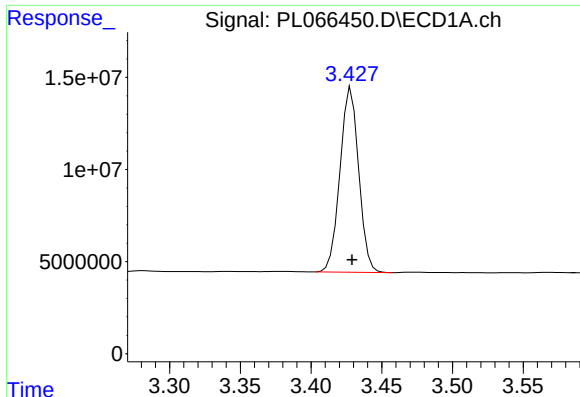

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.000 min
Response: 92345669
Conc: 23.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

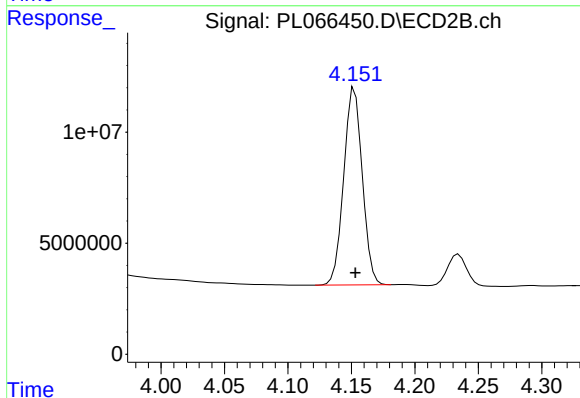


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 90361469
Conc: 24.35 ng/ml

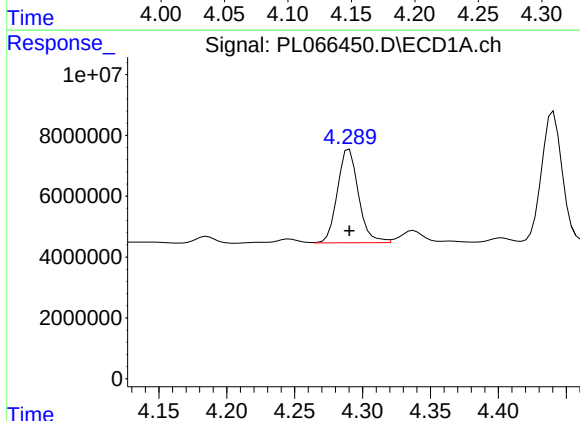


#23 Chlordane-1

R.T.: 4.290 min
Delta R.T.: 0.000 min
Response: 33185735
Conc: 257.81 ng/ml

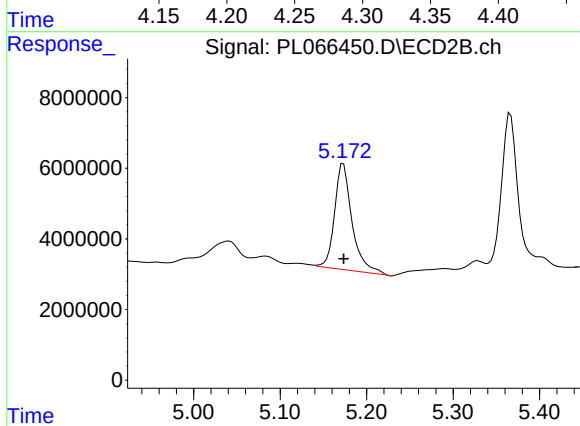

#23 Chlordane-1


R.T.: 5.173 min
Delta R.T.: 0.000 min
Response: 42206241
Conc: 254.95 ng/ml

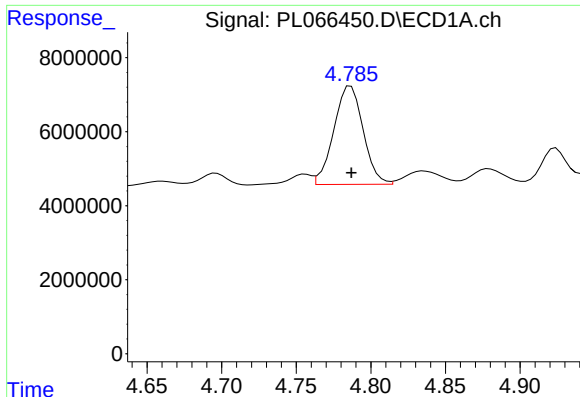

#24 Chlordane-2


R.T.: 4.787 min
Delta R.T.: 0.000 min
Response: 36480692
Conc: 253.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

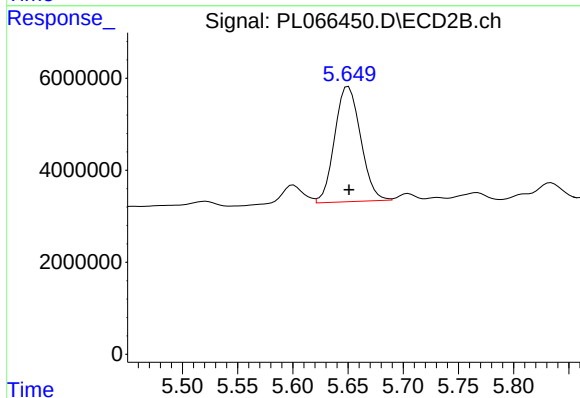


#24 Chlordane-2

R.T.: 5.650 min
Delta R.T.: 0.000 min
Response: 40964629
Conc: 254.09 ng/ml

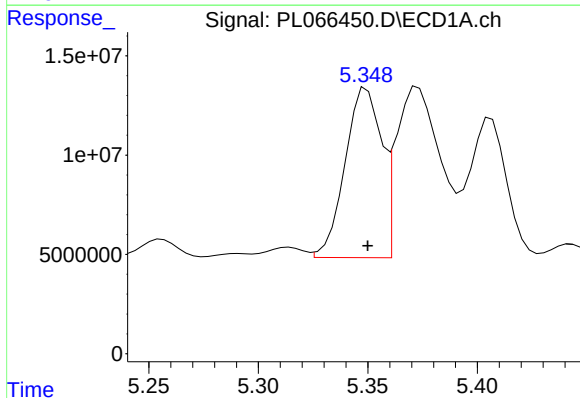


#25 Chlordane-3

R.T.: 5.350 min
Delta R.T.: 0.000 min
Response: 98192557
Conc: 239.59 ng/ml

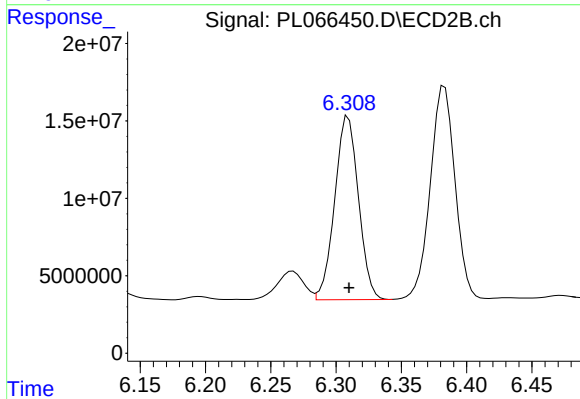

#25 Chlordane-3


R.T.: 6.309 min
Delta R.T.: 0.000 min
Response: 150110743
Conc: 236.96 ng/ml

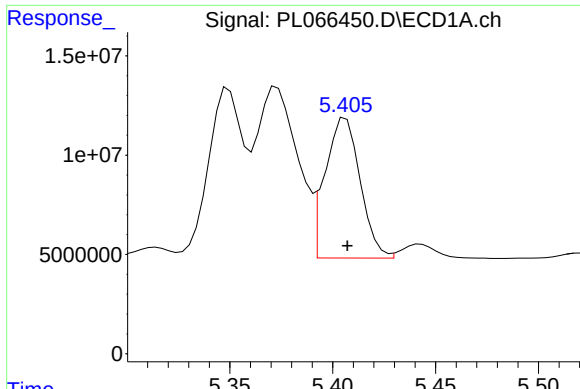

#26 Chlordane-4


R.T.: 5.406 min
Delta R.T.: 0.000 min
Response: 83843785
Conc: 242.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

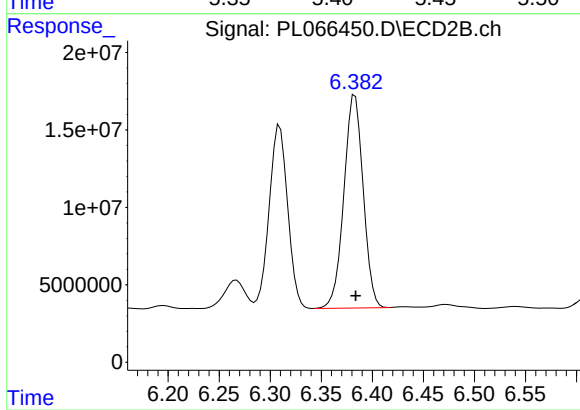


#26 Chlordane-4

R.T.: 6.383 min
Delta R.T.: 0.000 min
Response: 180799121
Conc: 241.69 ng/ml

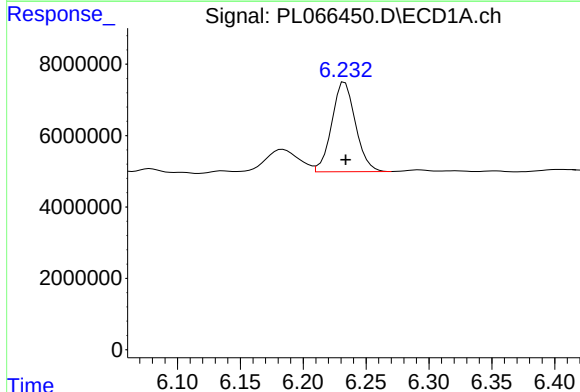


#27 Chlordane-5

R.T.: 6.233 min
Delta R.T.: 0.000 min
Response: 33052010
Conc: 244.59 ng/ml

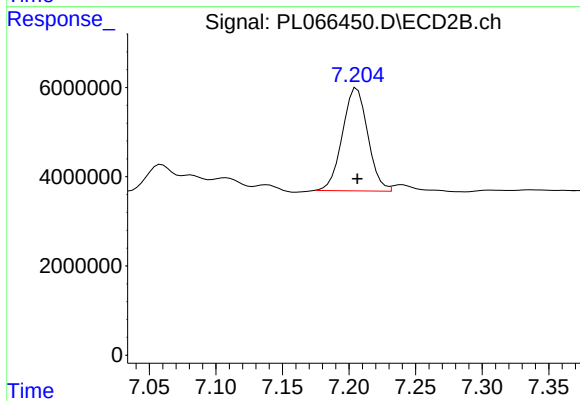

#27 Chlordane-5

R.T.: 7.206 min
Delta R.T.: 0.000 min
Response: 30571046
Conc: 245.72 ng/ml

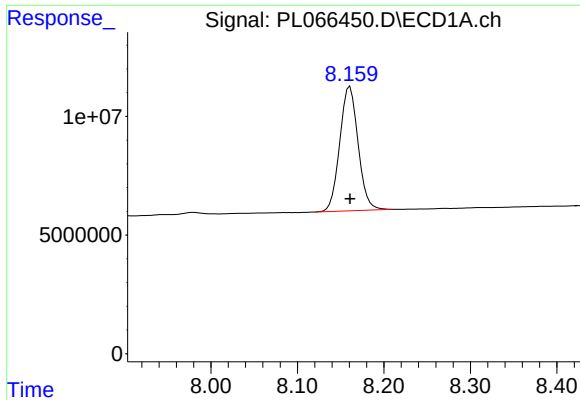

#28 Decachlorobiphenyl


R.T.: 8.161 min

Delta R.T.: 0.000 min

Response: 76935248

Conc: 25.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

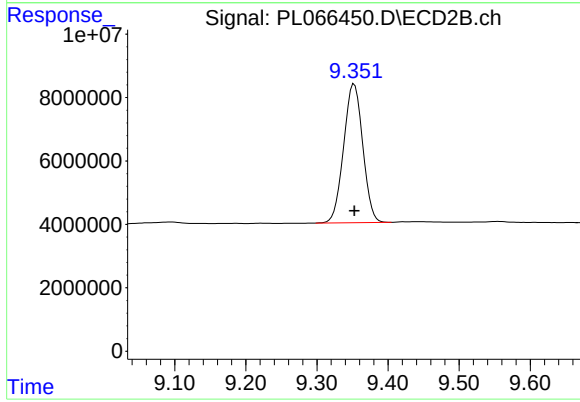

#28 Decachlorobiphenyl

R.T.: 9.352 min

Delta R.T.: 0.000 min

Response: 81851679

Conc: 25.32 ng/ml