

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
 Data File : PL095334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2025 12:40
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 13:22:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 13:22:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.595	2.906	317.2E6	394.3E6	98.972	100.386
28)	SA Decachlor...	9.123	8.090	260.2E6	296.3E6	98.087	101.036
Target Compounds							
23)	Chlordane-1	4.762	3.927	191.9E6	153.4E6	987.525	1003.641
24)	Chlordane-2	5.287	4.508	200.9E6	179.1E6	968.912	993.241
25)	Chlordane-3	5.994	5.147	778.9E6	536.1E6	998.696	1019.047
26)	Chlordane-4	6.079	5.211	935.6E6	448.3E6	994.948	1017.312
27)	Chlordane-5	6.919	6.106	150.2E6	187.8E6	1001.228	1013.839



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
Data File : PL095334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2025 12:40
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 13:22:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 13:22:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

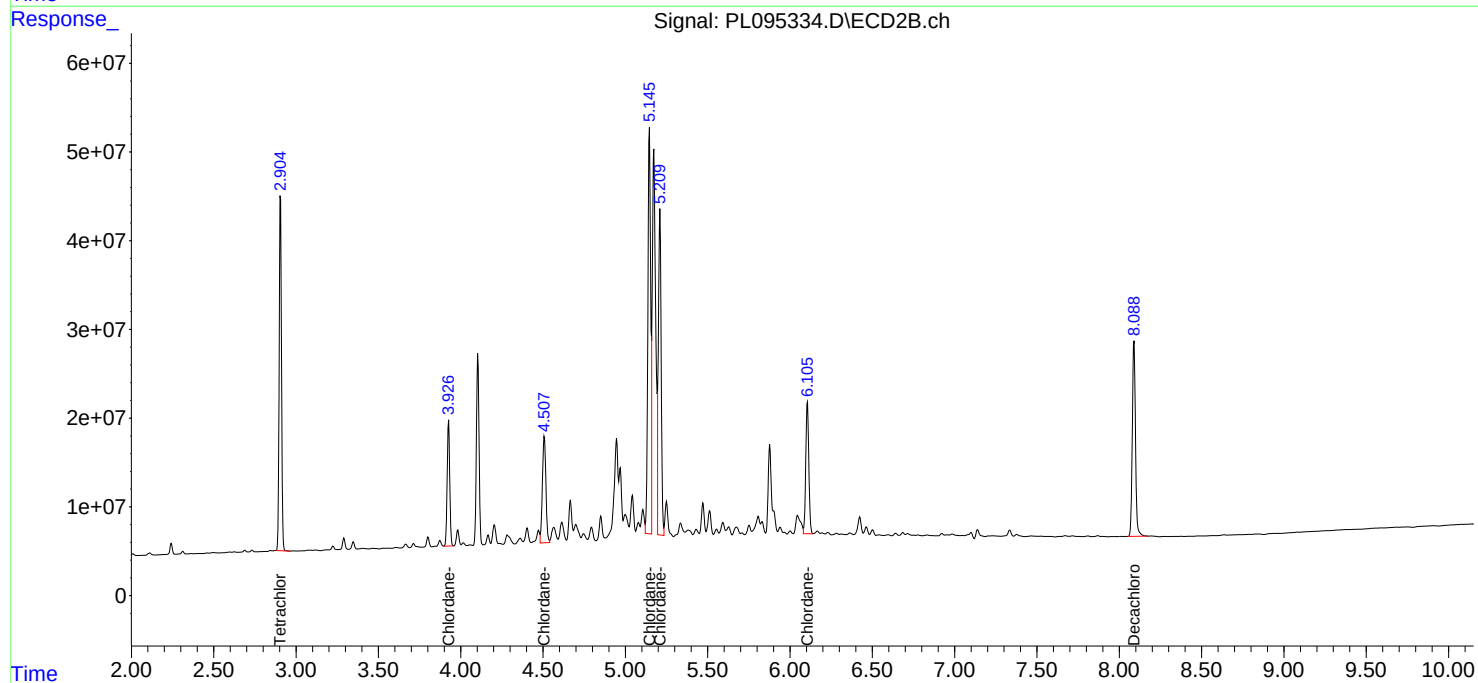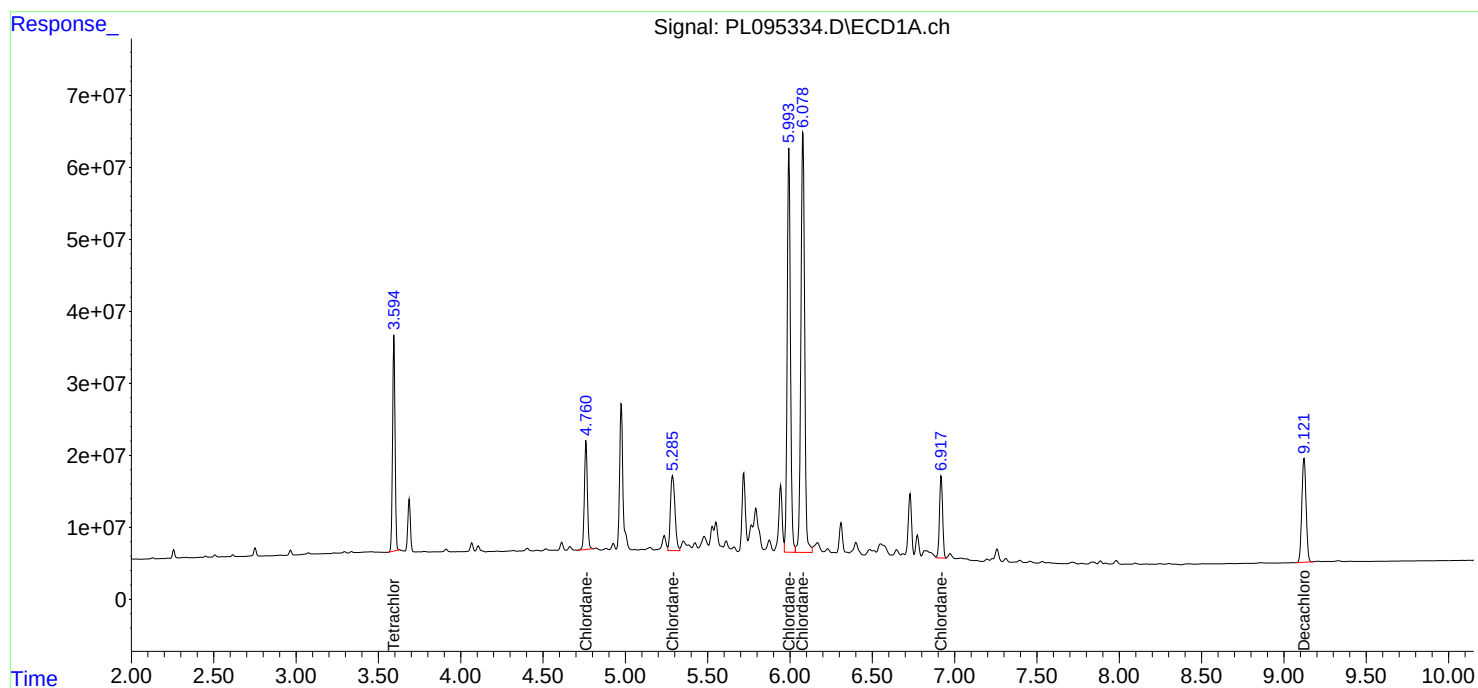


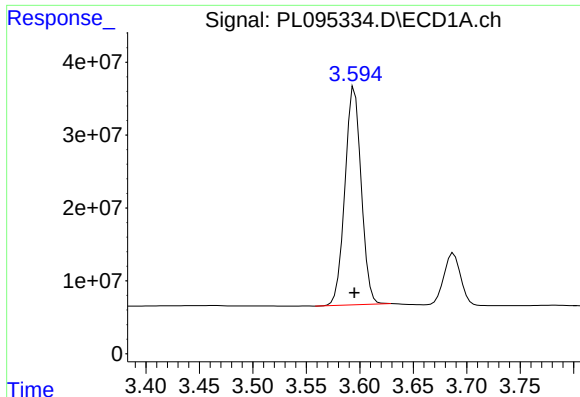

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 317191899
Conc: 98.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

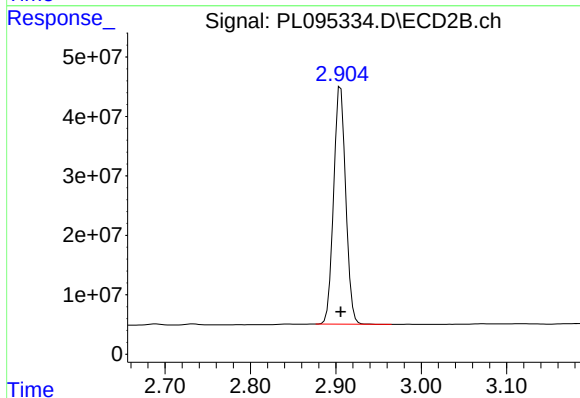


#1 Tetrachloro-m-xylene

R.T.: 2.906 min
Delta R.T.: 0.000 min
Response: 394310930
Conc: 100.39 ng/ml

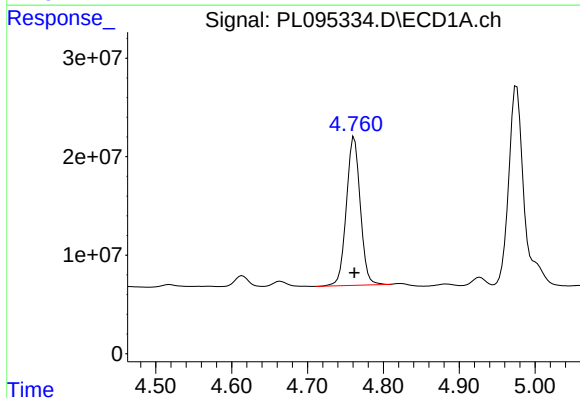


#23 Chlordane-1

R.T.: 4.762 min
Delta R.T.: 0.000 min
Response: 191875216
Conc: 987.53 ng/ml

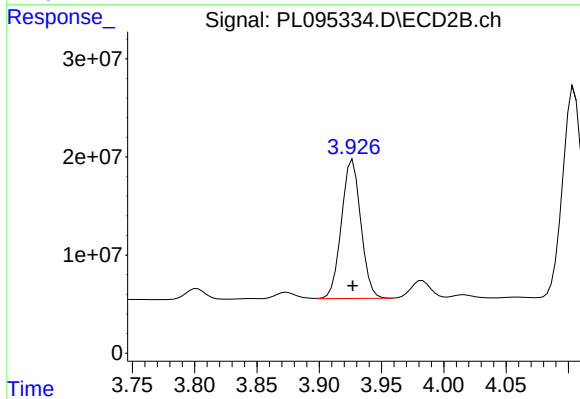

#23 Chlordane-1


R.T.: 3.927 min
Delta R.T.: 0.000 min
Response: 153431652
Conc: 1003.64 ng/ml

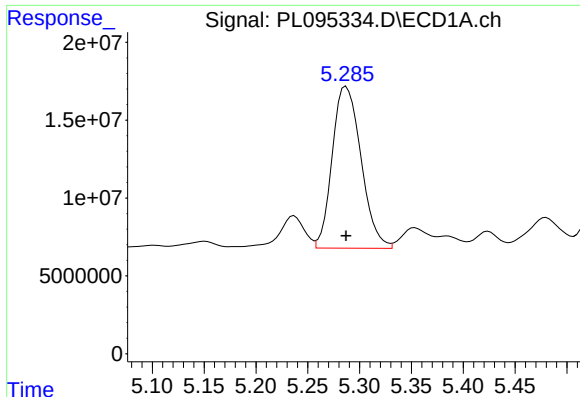

#24 Chlordane-2


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 200931615
Conc: 968.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

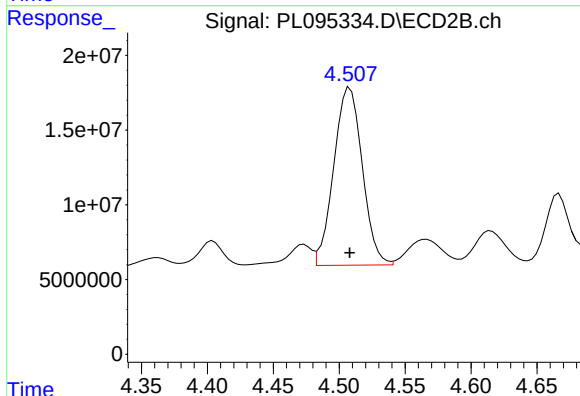


#24 Chlordane-2

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 179134846
Conc: 993.24 ng/ml

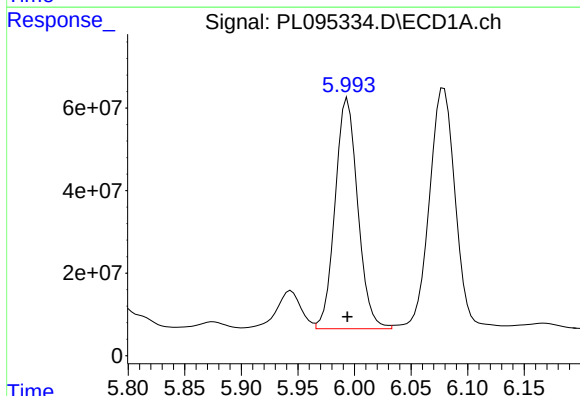


#25 Chlordane-3

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 778943770
Conc: 998.70 ng/ml

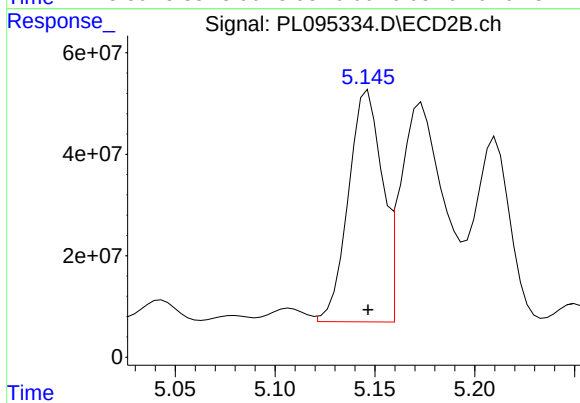

#25 Chlordane-3


R.T.: 5.147 min
Delta R.T.: 0.000 min
Response: 536109495
Conc: 1019.05 ng/ml

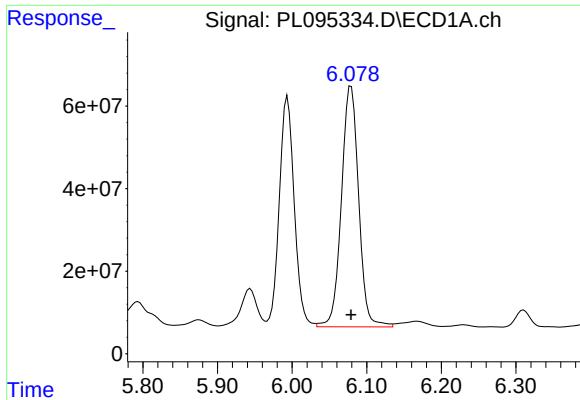

#26 Chlordane-4


R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 935591364
Conc: 994.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

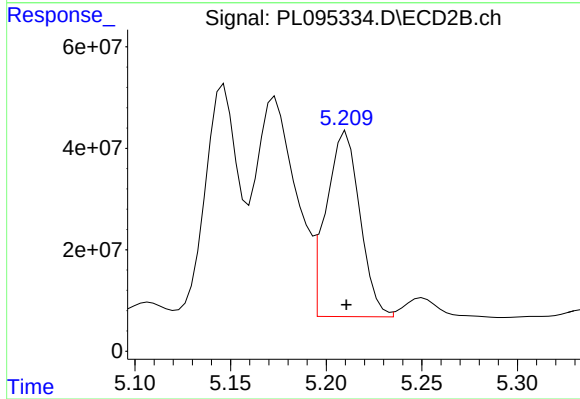


#26 Chlordane-4

R.T.: 5.211 min
Delta R.T.: 0.000 min
Response: 448316225
Conc: 1017.31 ng/ml

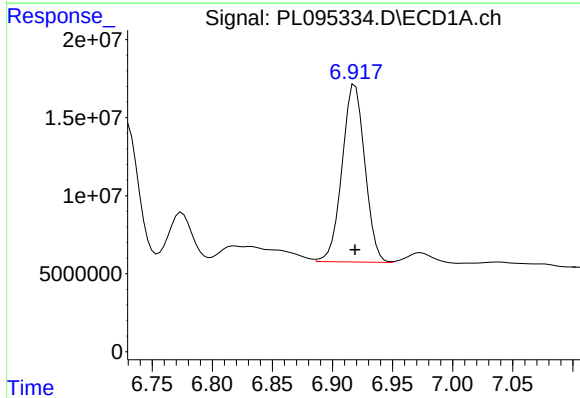


#27 Chlordane-5

R.T.: 6.919 min
Delta R.T.: 0.000 min
Response: 150170923
Conc: 1001.23 ng/ml

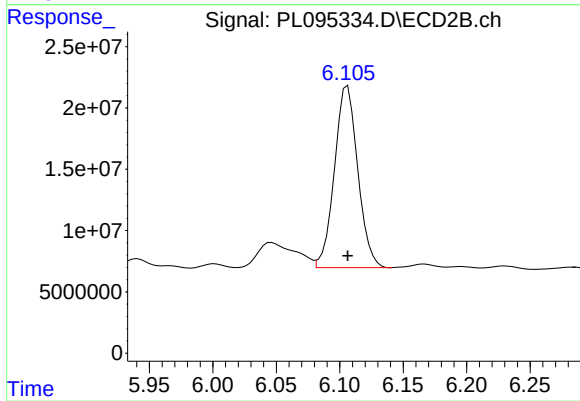

#27 Chlordane-5


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 187811711
Conc: 1013.84 ng/ml

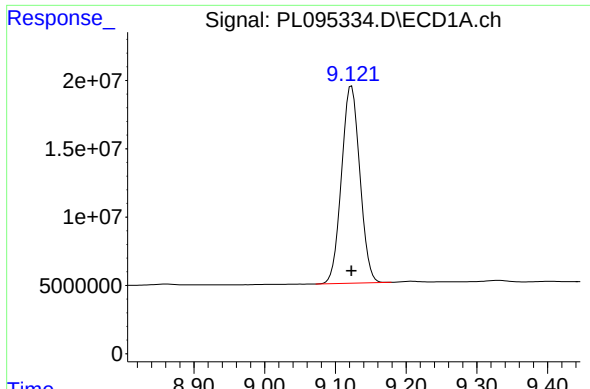

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 260194308
Conc: 98.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

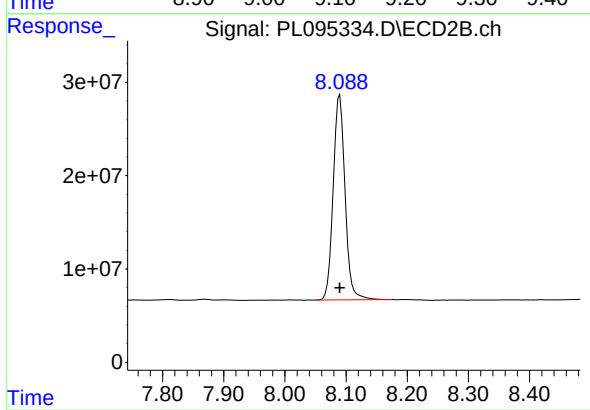

#28 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 296344198
Conc: 101.04 ng/ml