

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
 Data File : PL095337.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2025 13:21
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 13:31:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 13:31:02 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.594	2.905	81545963	97170955	25.490	24.960
28)	SA Decachlor...	9.122	8.089	69394652	73010864	25.917	25.232
Target Compounds							
23)	Chlordane-1	4.761	3.926	48796515	38144151	252.007	251.952
24)	Chlordane-2	5.287	4.507	55824186	46093184	264.134	254.096
25)	Chlordane-3	5.994	5.145	193.9E6	127.3E6	249.737	246.133
26)	Chlordane-4	6.078	5.209	237.0E6	108.0E6	252.334	248.370
27)	Chlordane-5	6.918	6.106	37757125	44928721	251.645	247.629



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
Data File : PL095337.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2025 13:21
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 13:31:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 13:31:02 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

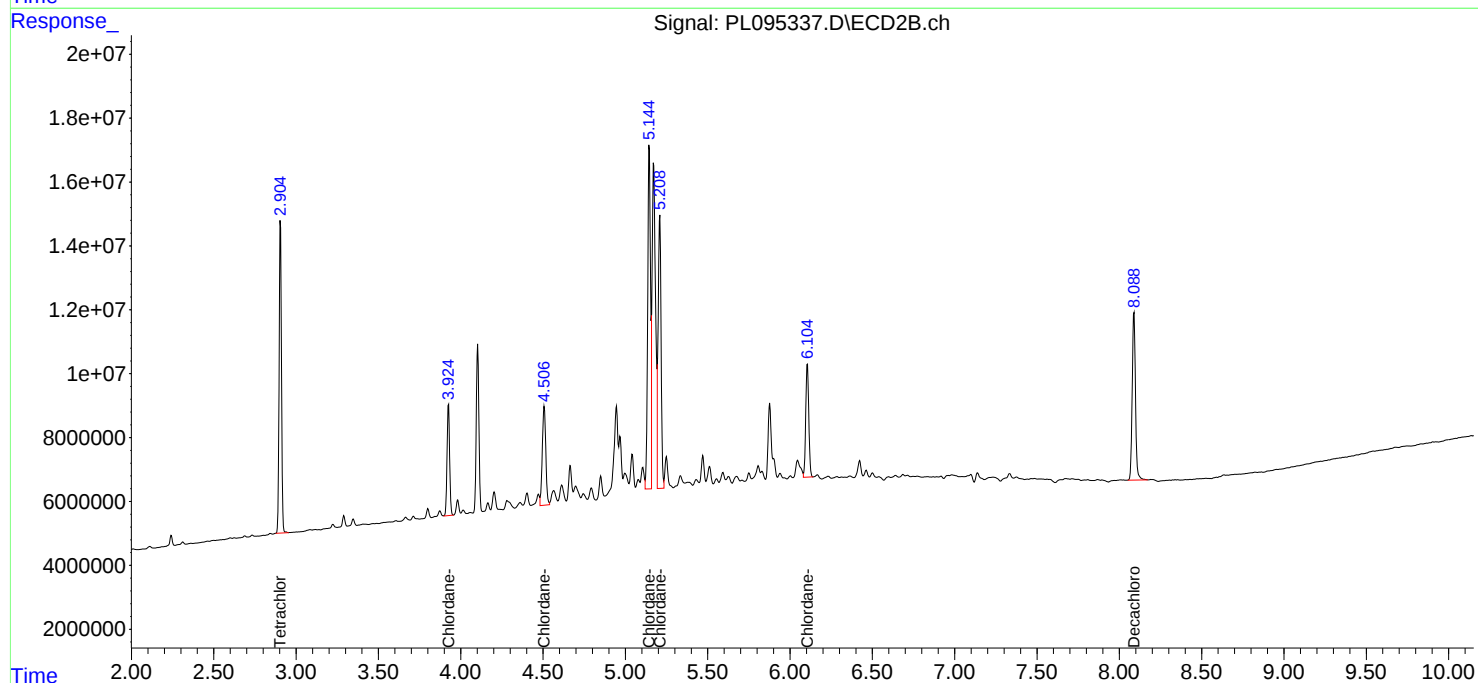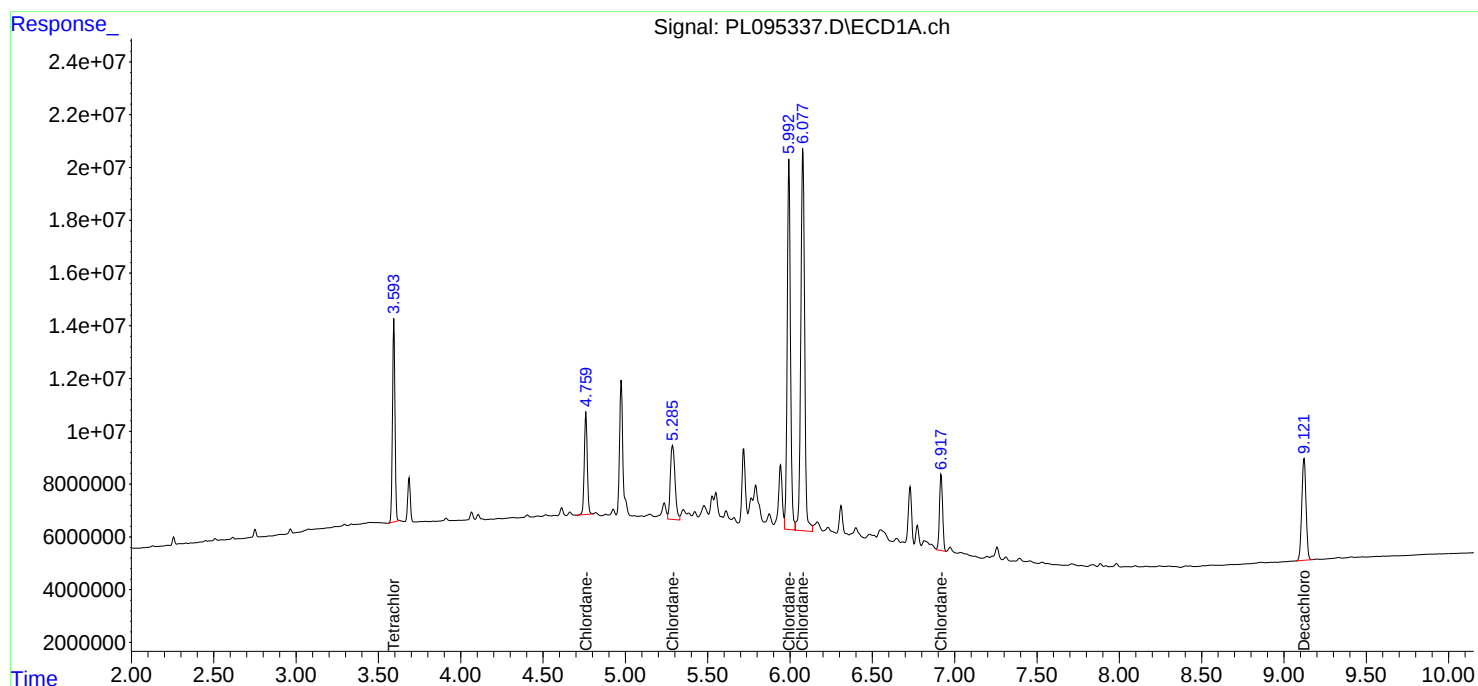


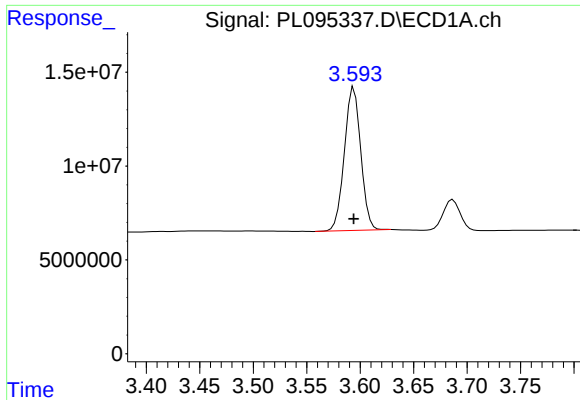

#1 Tetrachloro-m-xylene


R.T.: 3.594 min
Delta R.T.: 0.000 min
Response: 81545963
Conc: 25.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

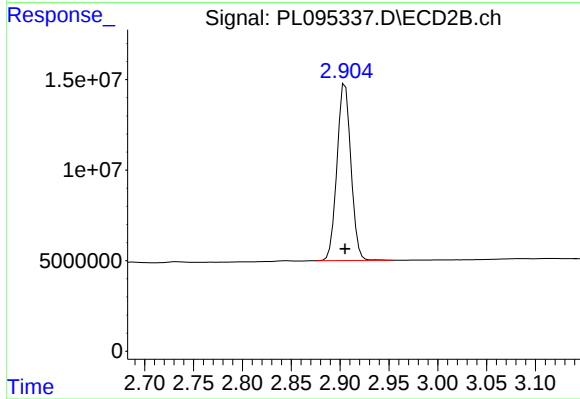


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 97170955
Conc: 24.96 ng/ml

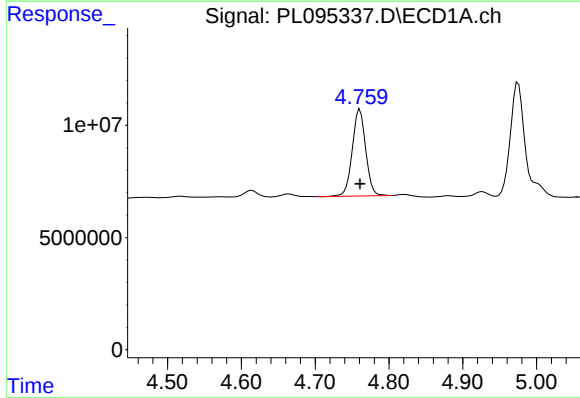


#23 Chlordane-1

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 48796515
Conc: 252.01 ng/ml

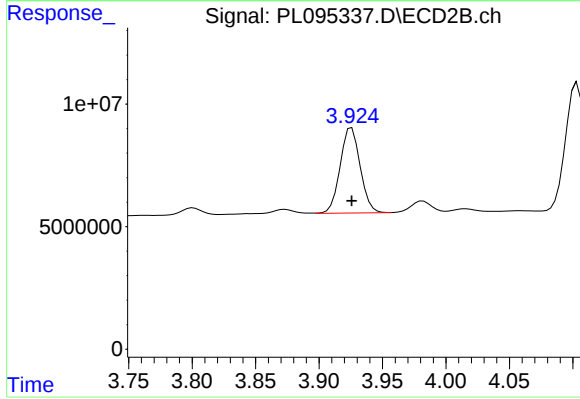

#23 Chlordane-1


R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 38144151
Conc: 251.95 ng/ml

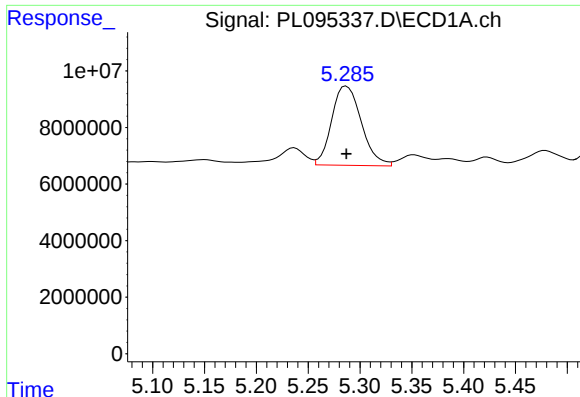

#24 Chlordane-2


R.T.: 5.287 min
Delta R.T.: 0.000 min
Response: 55824186
Conc: 264.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

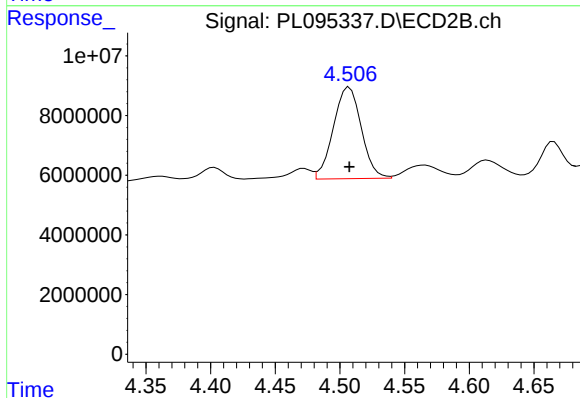


#24 Chlordane-2

R.T.: 4.507 min
Delta R.T.: 0.000 min
Response: 46093184
Conc: 254.10 ng/ml

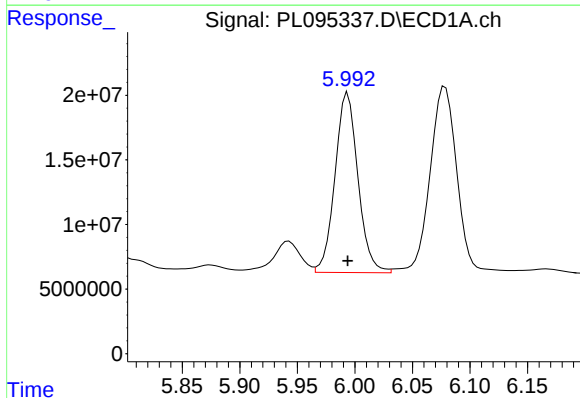


#25 Chlordane-3

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 193890242
Conc: 249.74 ng/ml

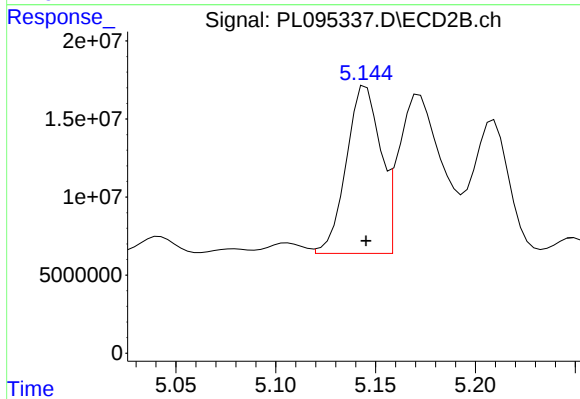

#25 Chlordane-3


R.T.: 5.145 min
Delta R.T.: 0.000 min
Response: 127328173
Conc: 246.13 ng/ml

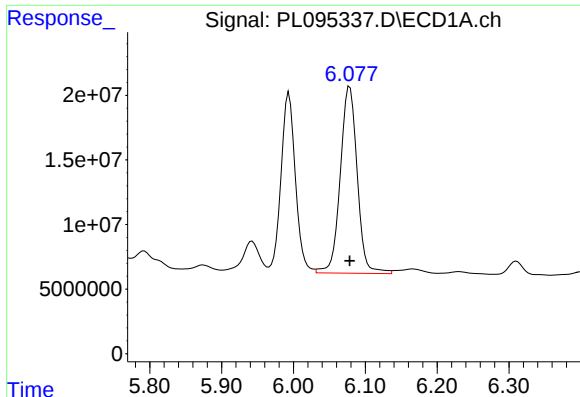

#26 Chlordane-4


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 237002077
Conc: 252.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

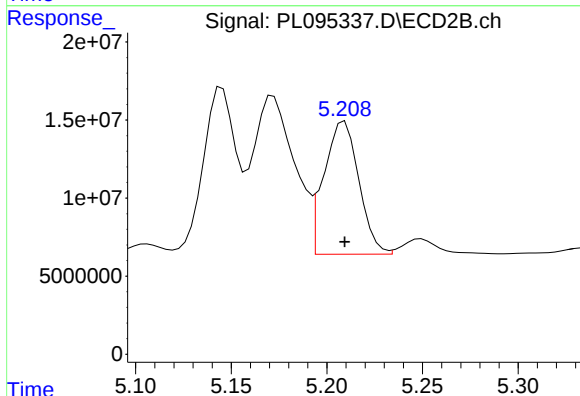


#26 Chlordane-4

R.T.: 5.209 min
Delta R.T.: 0.000 min
Response: 107994217
Conc: 248.37 ng/ml

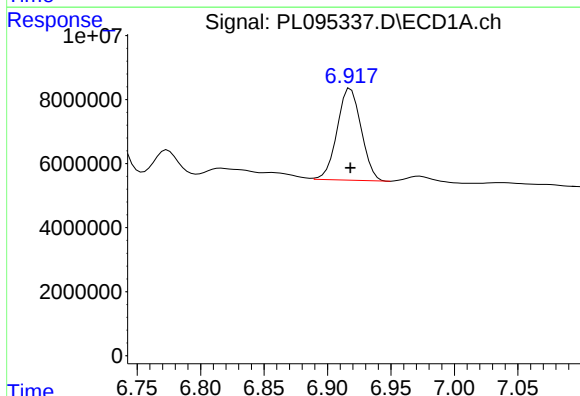


#27 Chlordane-5

R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 37757125
Conc: 251.65 ng/ml

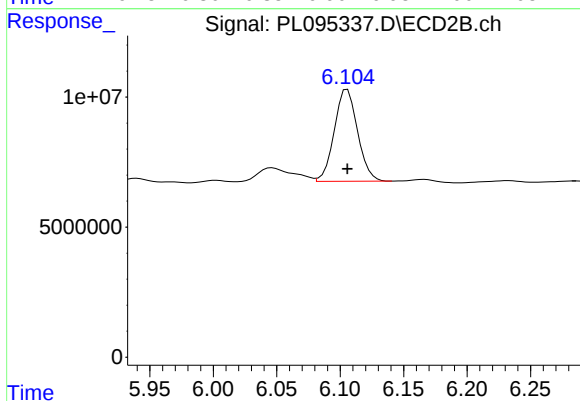

#27 Chlordane-5


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 44928721
Conc: 247.63 ng/ml

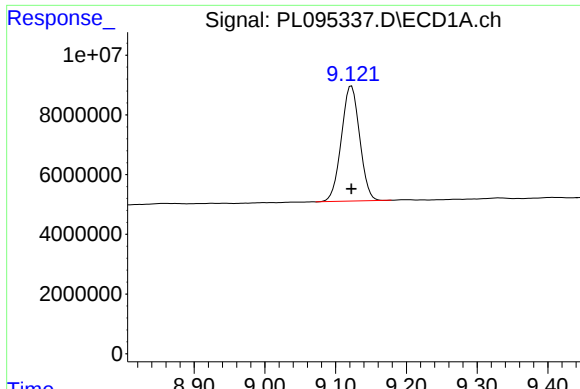

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: 0.000 min
Response: 69394652
Conc: 25.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

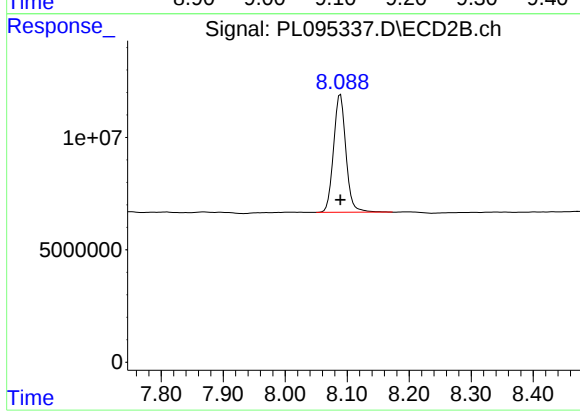

#28 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 73010864
Conc: 25.23 ng/ml