

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
 Data File : PL095335.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Apr 2025 12:53
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 23 13:24:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 13:24:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.595	2.905	234.4E6	287.2E6	73.747	73.736
28) SA Decachlor...	9.123	8.089	197.2E6	209.1E6	74.558	72.486
Target Compounds						
23) Chlordane-1	4.761	3.926	143.1E6	110.4E6	740.792	731.379
24) Chlordane-2	5.288	4.508	155.5E6	135.4E6	749.904	750.463
25) Chlordane-3	5.994	5.146	577.5E6	380.8E6	743.607	732.383
26) Chlordane-4	6.078	5.210	696.2E6	319.4E6	743.551	733.026
27) Chlordane-5	6.920	6.106	111.9E6	131.6E6	747.249	723.311



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042325\
Data File : PL095335.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Apr 2025 12:53
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 23 13:24:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 13:24:36 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

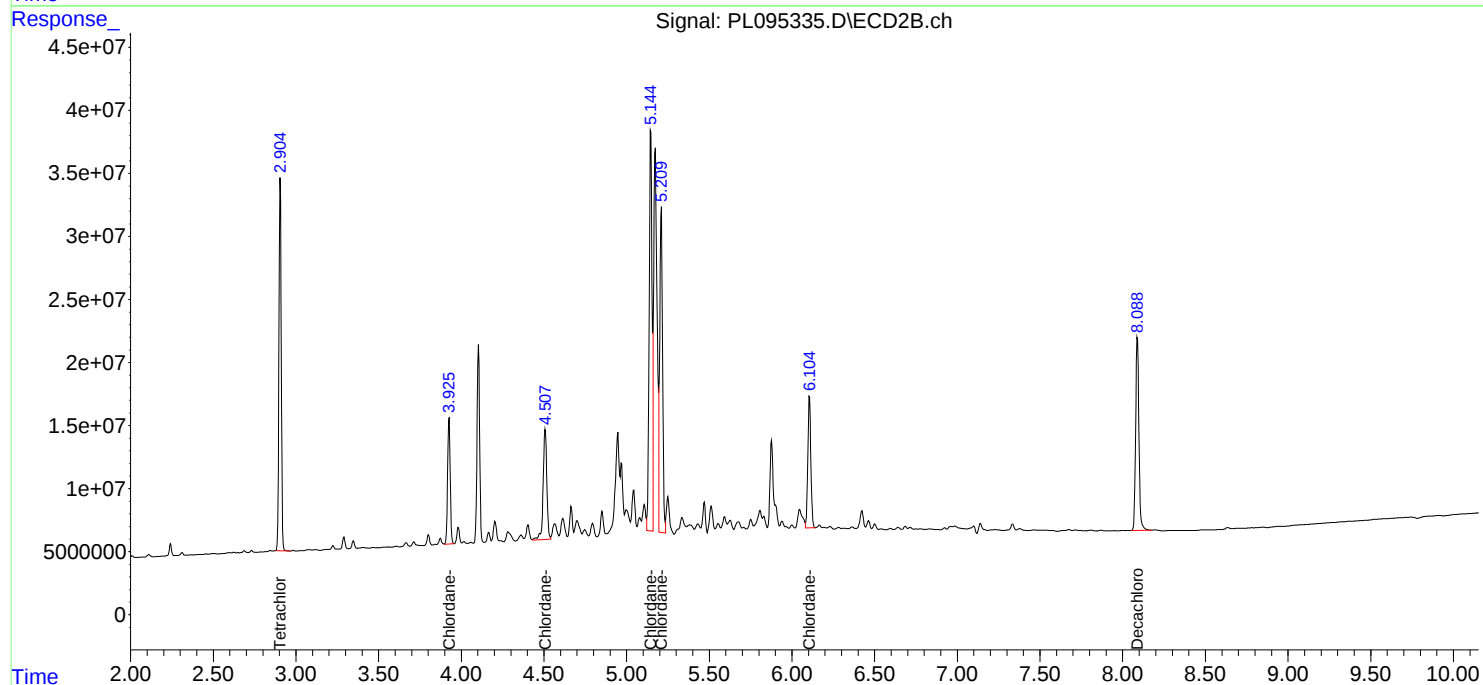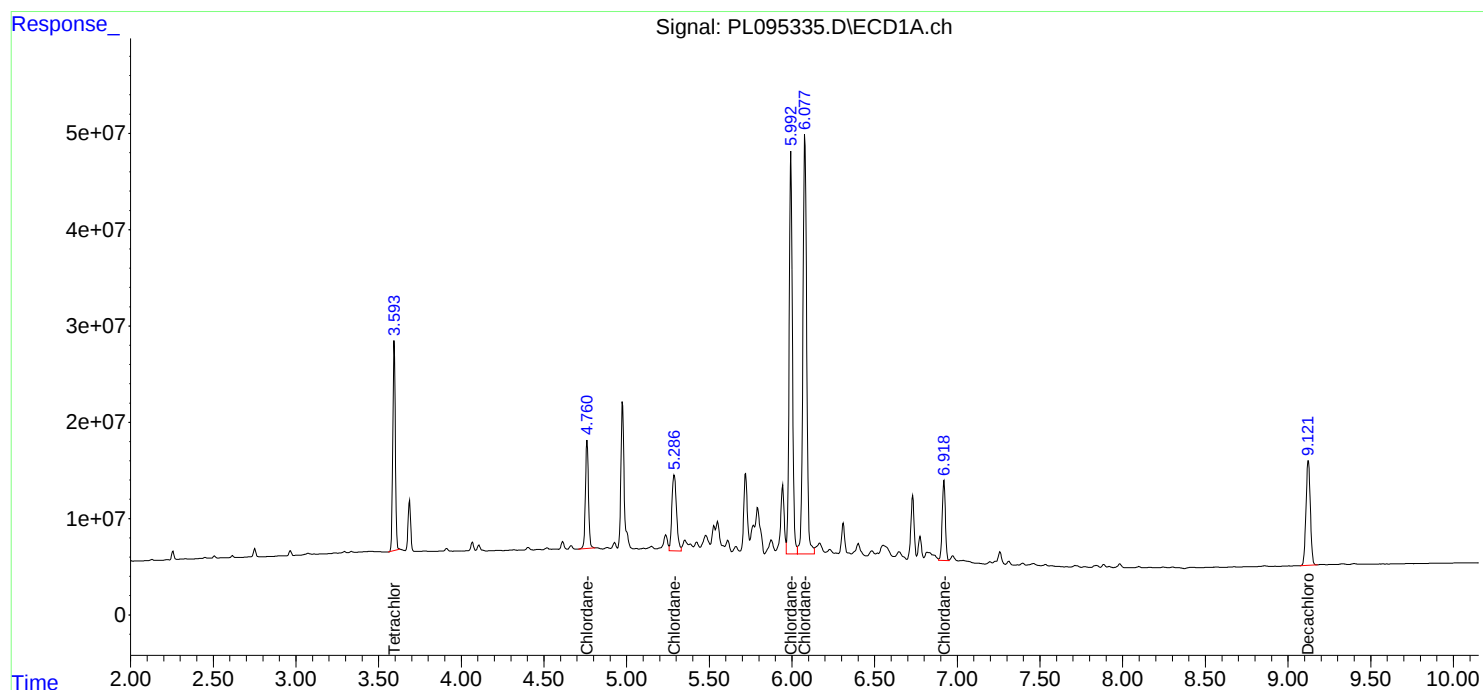


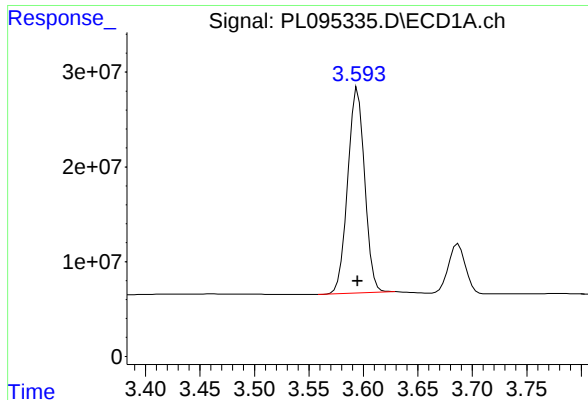

#1 Tetrachloro-m-xylene


R.T.: 3.595 min
Delta R.T.: 0.000 min
Response: 234389422
Conc: 73.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

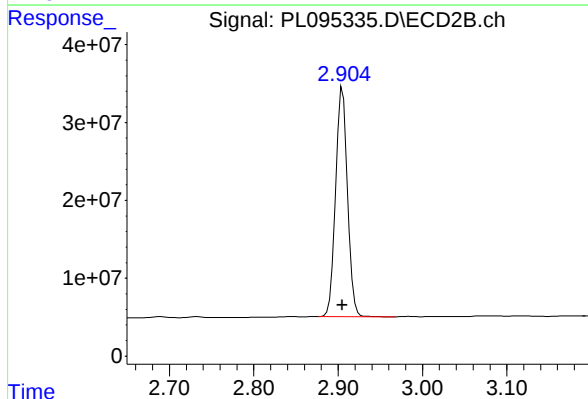


#1 Tetrachloro-m-xylene

R.T.: 2.905 min
Delta R.T.: 0.000 min
Response: 287213083
Conc: 73.74 ng/ml

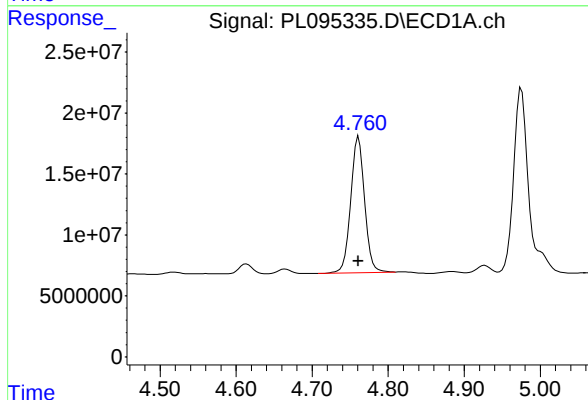


#23 Chlordane-1

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 143056930
Conc: 740.79 ng/ml

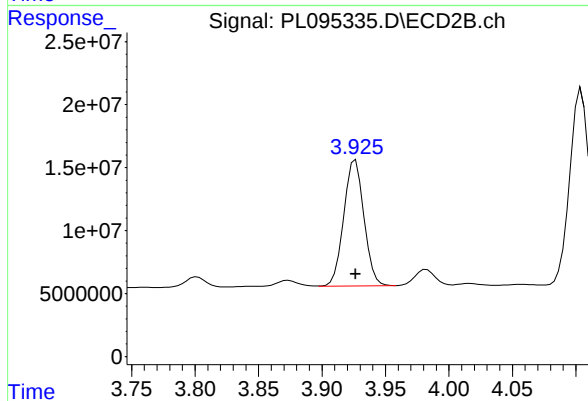

#23 Chlordane-1


R.T.: 3.926 min
Delta R.T.: 0.000 min
Response: 110438576
Conc: 731.38 ng/ml

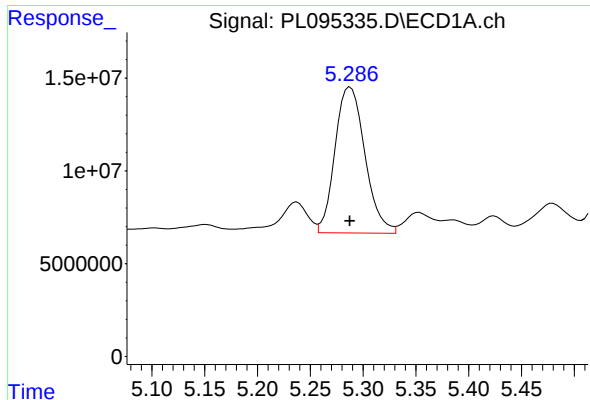

#24 Chlordane-2


R.T.: 5.288 min
Delta R.T.: 0.000 min
Response: 155504261
Conc: 749.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

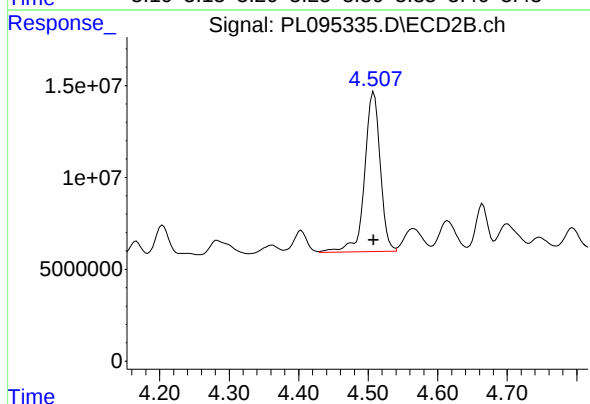


#24 Chlordane-2

R.T.: 4.508 min
Delta R.T.: 0.000 min
Response: 135390693
Conc: 750.46 ng/ml

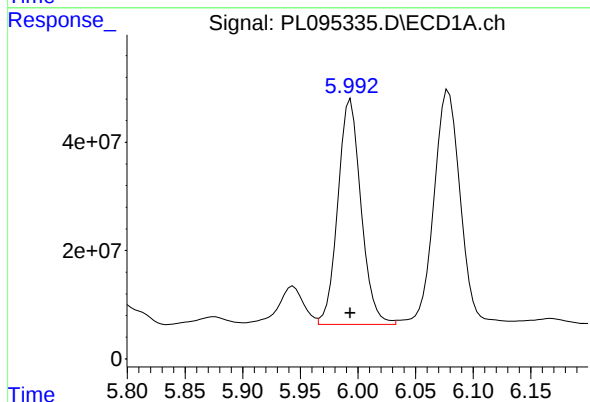


#25 Chlordane-3

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 577523775
Conc: 743.61 ng/ml

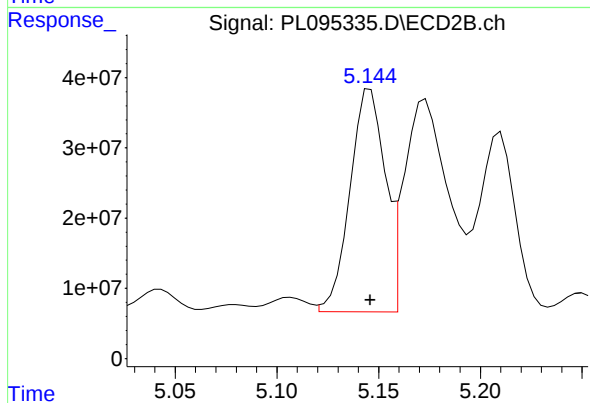

#25 Chlordane-3


R.T.: 5.146 min
Delta R.T.: 0.000 min
Response: 380826341
Conc: 732.38 ng/ml

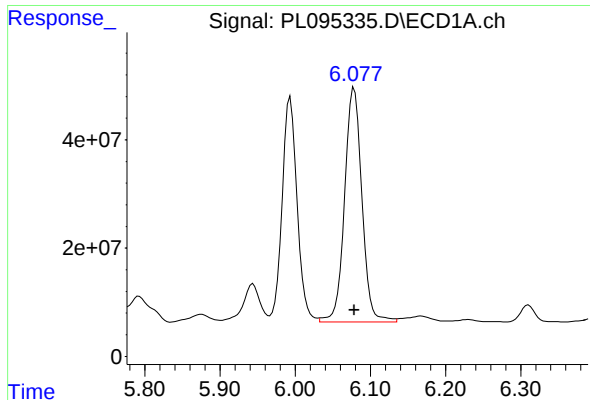

#26 Chlordane-4


R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 696198471
Conc: 743.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

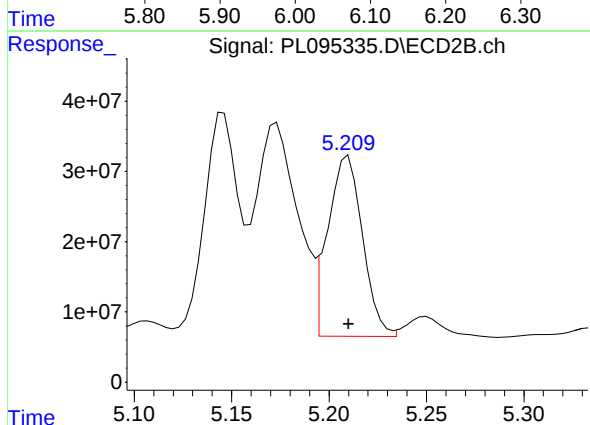


#26 Chlordane-4

R.T.: 5.210 min
Delta R.T.: 0.000 min
Response: 319420855
Conc: 733.03 ng/ml

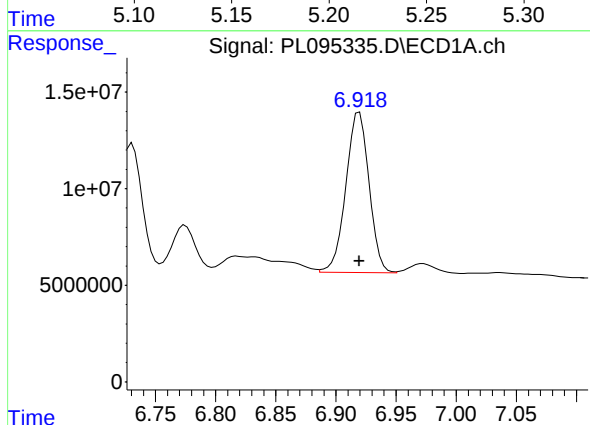


#27 Chlordane-5

R.T.: 6.920 min
Delta R.T.: 0.000 min
Response: 111872210
Conc: 747.25 ng/ml

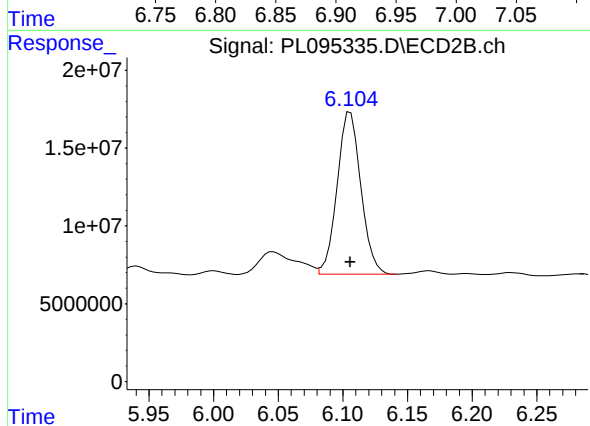

#27 Chlordane-5


R.T.: 6.106 min
Delta R.T.: 0.000 min
Response: 131649515
Conc: 723.31 ng/ml

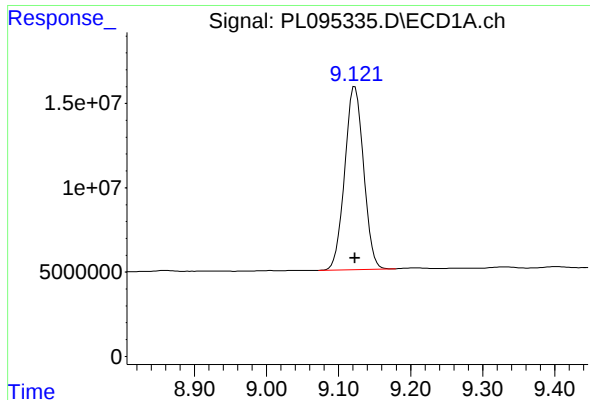

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: 0.000 min
Response: 197196909
Conc: 74.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

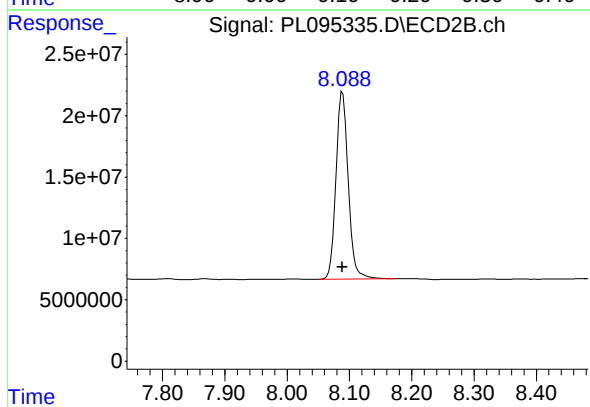

#28 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 209100289
Conc: 72.49 ng/ml