

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
 Data File : PL047709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 20:38
 Operator : AJ\SJ
 Sample : K2541-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CHRT-26835

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 02:38:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	182.5E6	48691919	19.737	20.397
28)	SA Decachlor...	8.003	8.981	207.8E6	53790575	18.559	18.844
Target Compounds							
5)	MB Aldrin	4.560	5.434	21362008	2623309	1.534	0.841 #
6)	B beta-BHC	0.000	4.807f	0	3386816	N.D.	2.351 #
7)	B delta-BHC	4.488	5.024f	20291610	-3133856	1.562	N.D. #
10)	B gamma-Chl...	0.000	6.030	0	1886315	N.D.	0.623 #
14)	MA Endrin	5.830	0.000	13413130	0	1.129	N.D. #
23)	Chlordane-1	4.169	5.024f	15346142	-3133856	35.494	N.D. #
24)	Chlordane-2	4.651	5.434	13421605	2623309	28.223	8.430 #
26)	Chlordane-4	5.356f	0.000	39355573	0	32.029	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
Data File : PL047709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 20:38
Operator : AJ\SJ
Sample : K2541-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 02:38:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

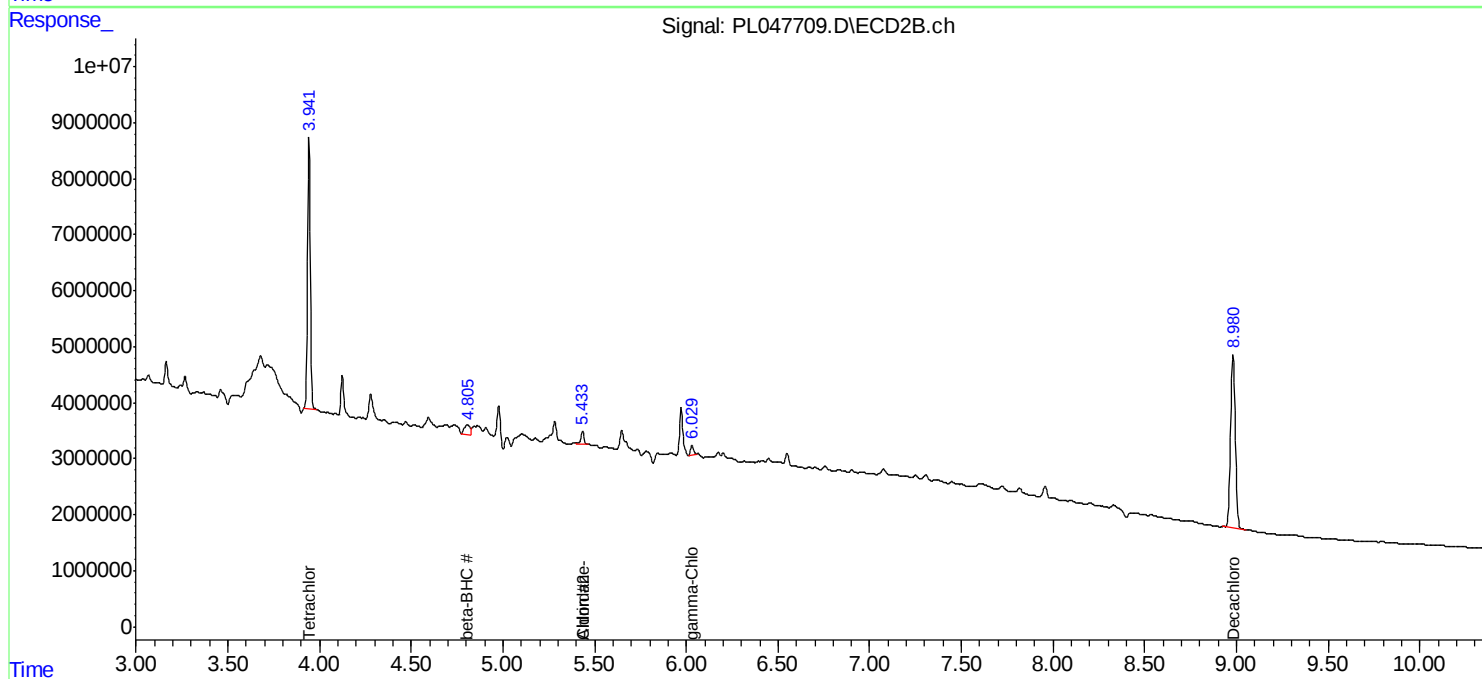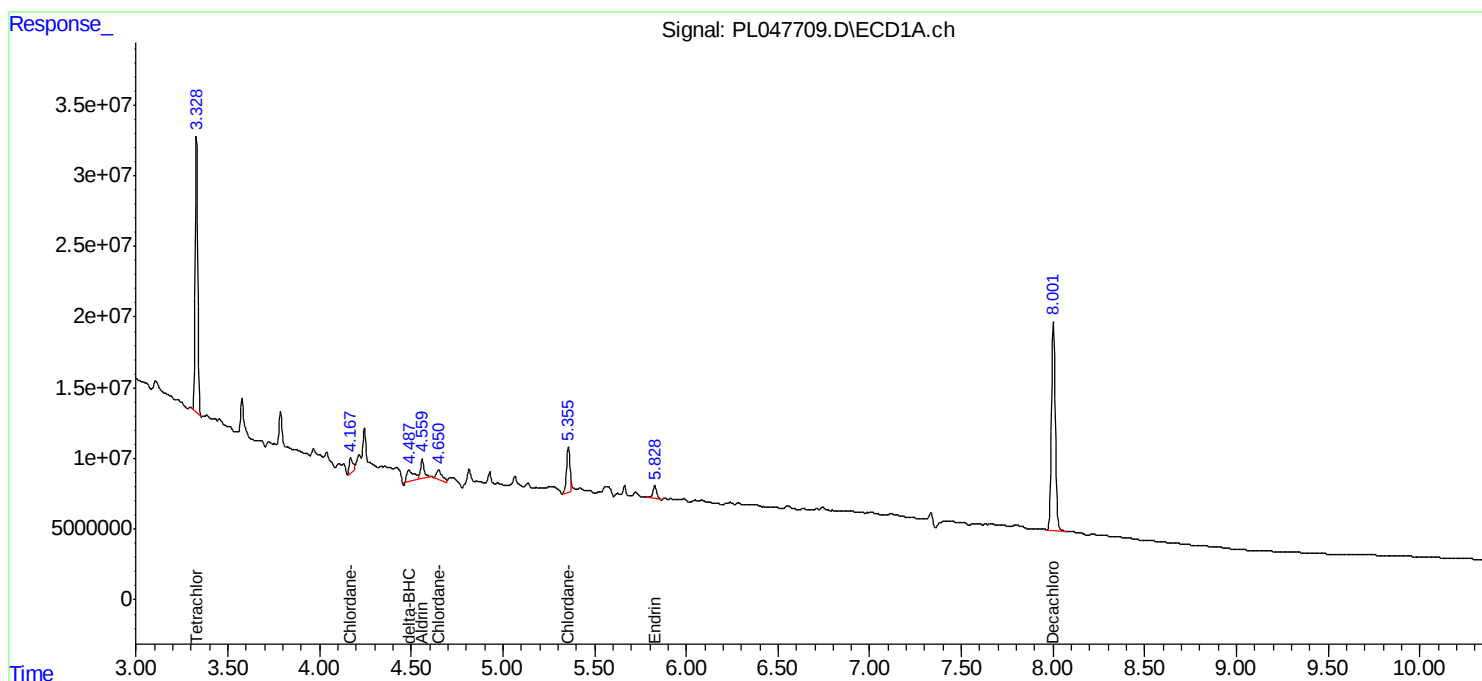


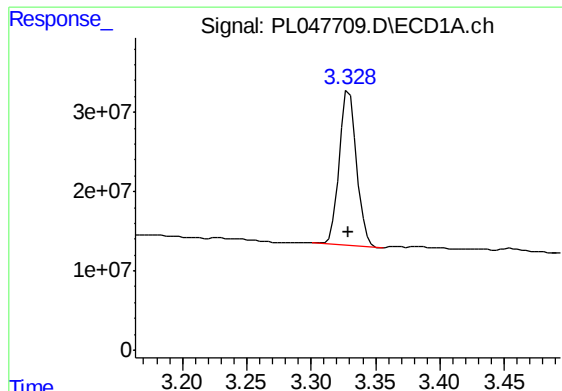

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 182535867
Conc: 19.74 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

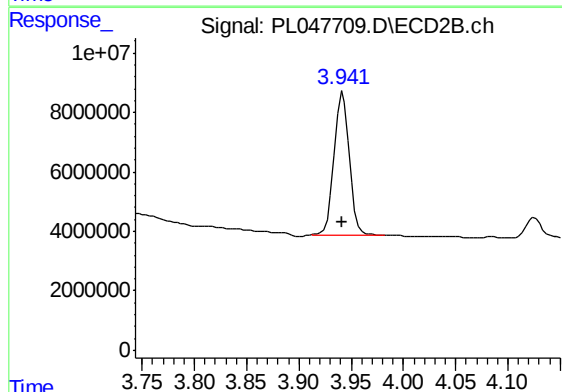


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 48691919
Conc: 20.40 ng/ml

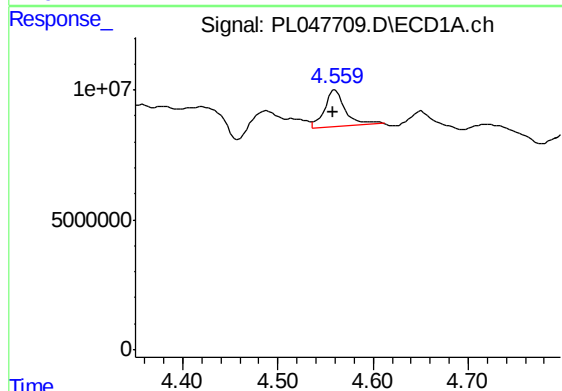


#5 Aldrin

R.T.: 4.560 min
Delta R.T.: 0.002 min
Response: 21362008
Conc: 1.53 ng/ml

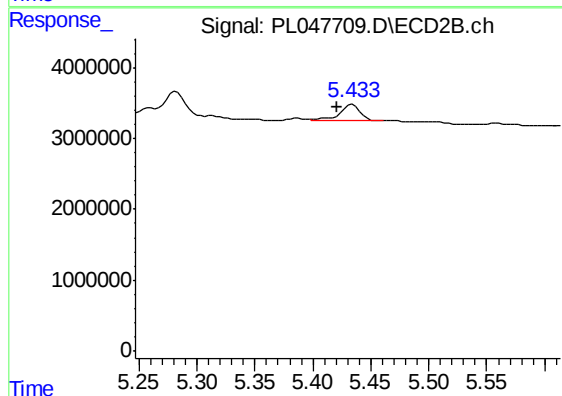

#5 Aldrin


R.T.: 5.434 min
Delta R.T.: 0.013 min
Response: 2623309
Conc: 0.84 ng/ml

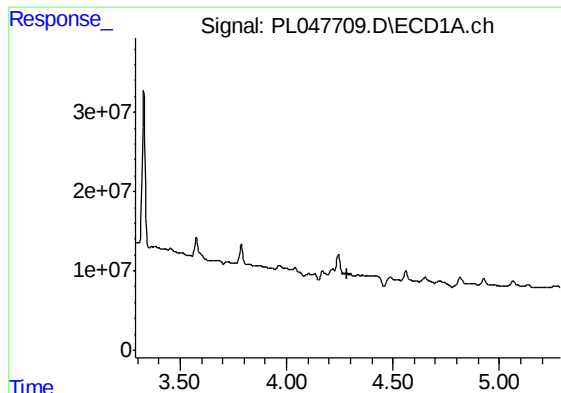

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

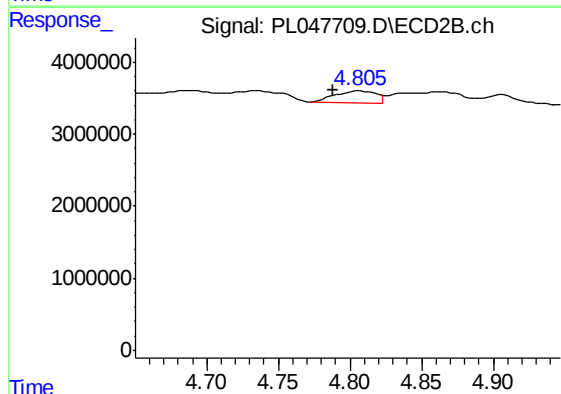


#6 beta-BHC

R.T.: 4.807 min
Delta R.T.: 0.019 min
Response: 3386816
Conc: 2.35 ng/ml

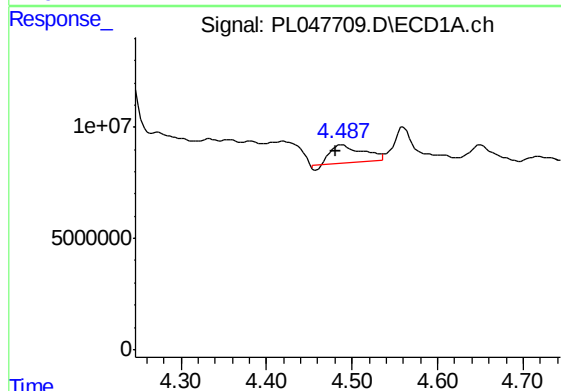


#7 delta-BHC

R.T.: 4.488 min
Delta R.T.: 0.007 min
Response: 20291610
Conc: 1.56 ng/ml

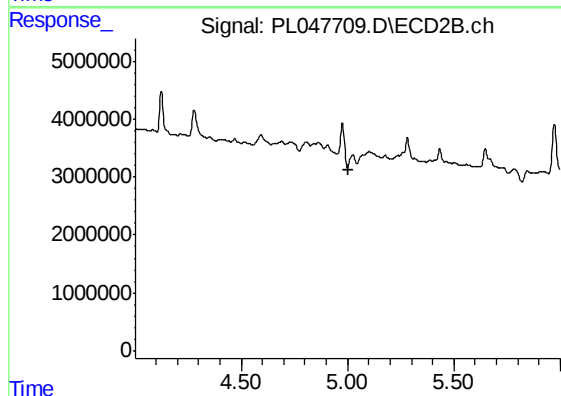

#7 delta-BHC


R.T.: 5.024 min
Delta R.T.: 0.022 min
Response: -3133856
Conc: N.D.

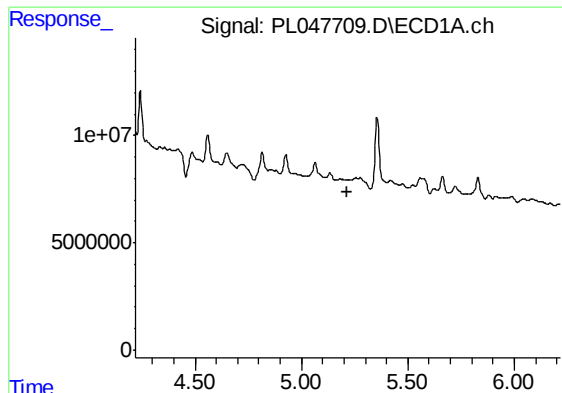

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

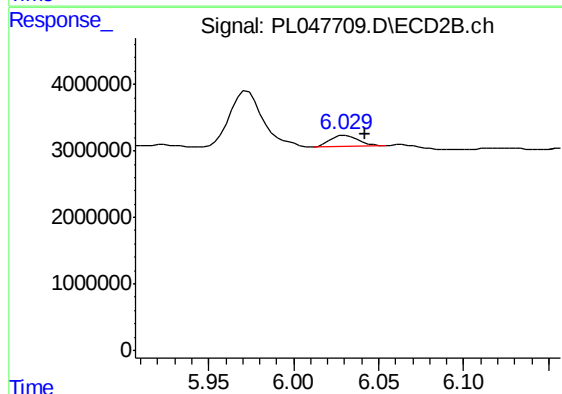


#10 gamma-Chlordane

R.T.: 6.030 min
Delta R.T.: -0.011 min
Response: 1886315
Conc: 0.62 ng/ml

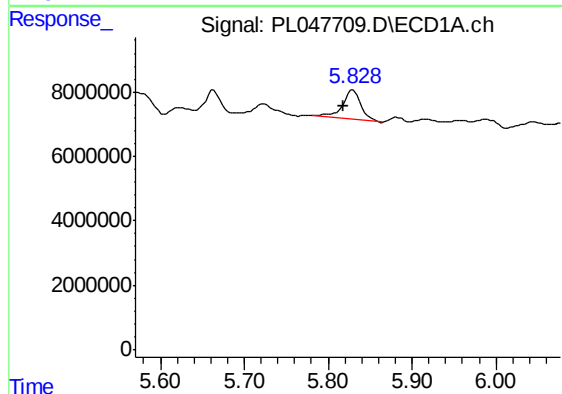


#14 Endrin

R.T.: 5.830 min
Delta R.T.: 0.011 min
Response: 13413130
Conc: 1.13 ng/ml

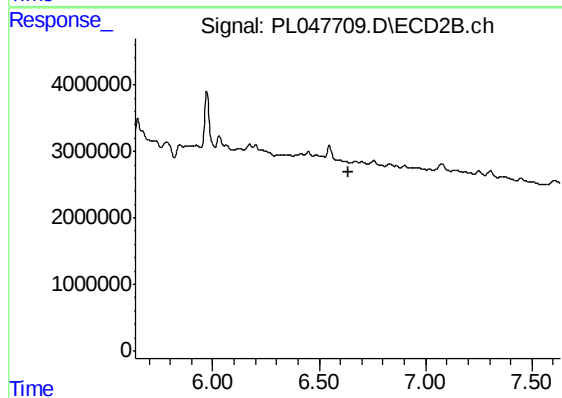

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

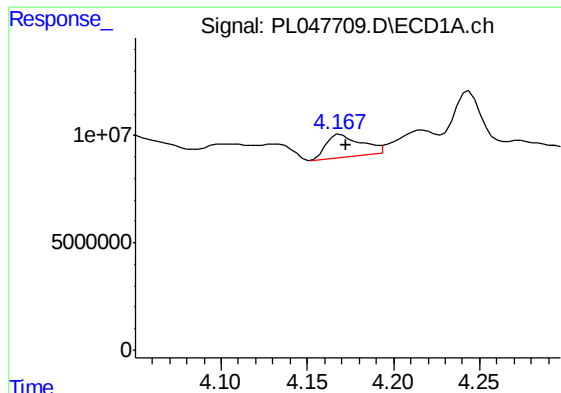

#23 Chlordane-1


R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 15346142
Conc: 35.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

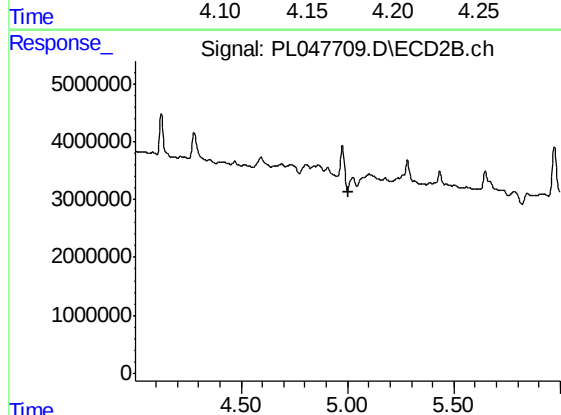


#23 Chlordane-1

R.T.: 5.024 min
Delta R.T.: 0.021 min
Response: -3133856
Conc: N.D.

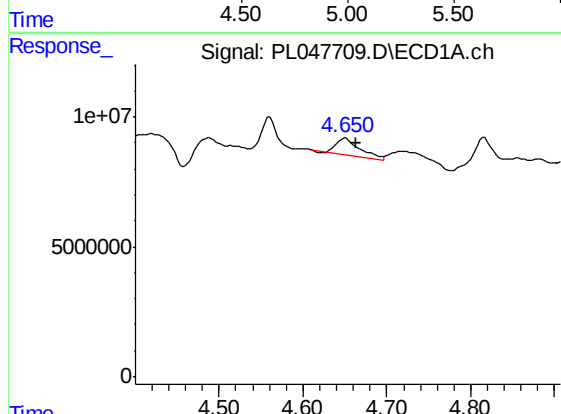


#24 Chlordane-2

R.T.: 4.651 min
Delta R.T.: -0.013 min
Response: 13421605
Conc: 28.22 ng/ml

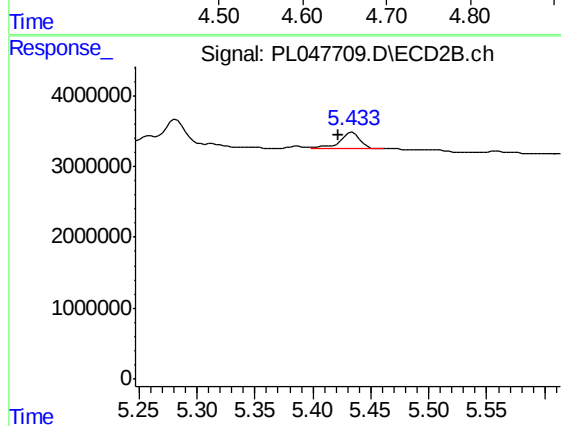

#24 Chlordane-2


R.T.: 5.434 min
Delta R.T.: 0.012 min
Response: 2623309
Conc: 8.43 ng/ml

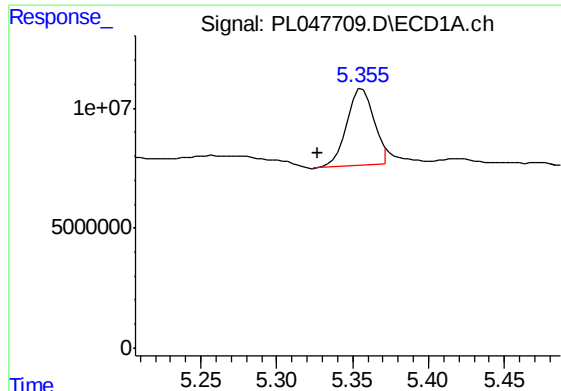

#26 Chlordane-4


R.T.: 5.356 min
Delta R.T.: 0.029 min
Response: 39355573
Conc: 32.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
CHRT-26835

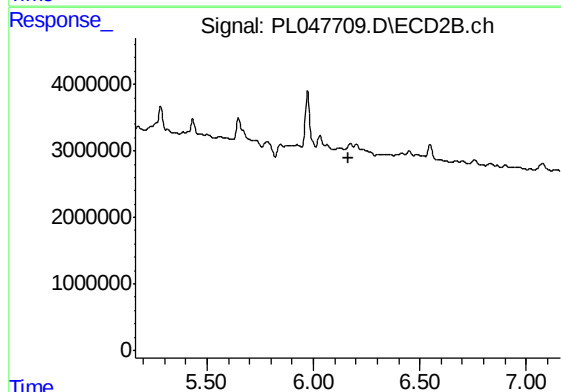


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

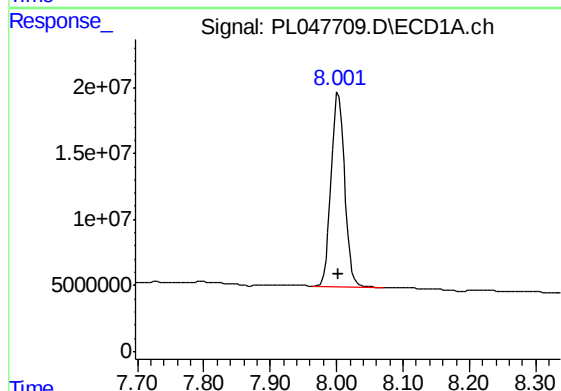

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 207752127
Conc: 18.56 ng/ml

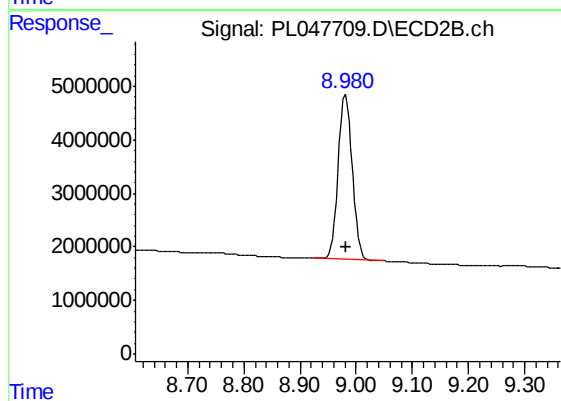

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 53790575
Conc: 18.84 ng/ml