

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
 Data File : PL047722.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 00:10
 Operator : AJ\SJ
 Sample : K2539-03 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-SF-03-006-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 02:40:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.329	3.941	13425277	3238726	1.452	1.357
28)	SA Decachlor...	8.002	8.980	21238173	6192101	1.897	2.169
Target Compounds							
10)	B gamma-Chl...	5.239f	6.040	9629659	1983045	0.723	0.655
11)	B alpha-Chl...	0.000	6.114	0	4643258	N.D.	1.535 #
12)	B 4,4'-DDE	0.000	6.271	0	1684715	N.D.	0.610 #
17)	MA 4,4'-DDT	6.184	0.000	5642576	0	0.566	N.D. #
23)	Chlordane-1	4.172	0.000	4749764	0	10.986	N.D. #
25)	Chlordane-3	0.000	6.114	0	4643258	N.D.	15.675 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
Data File : PL047722.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 00:10
Operator : AJ\SJ
Sample : K2539-03 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-006-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 02:40:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

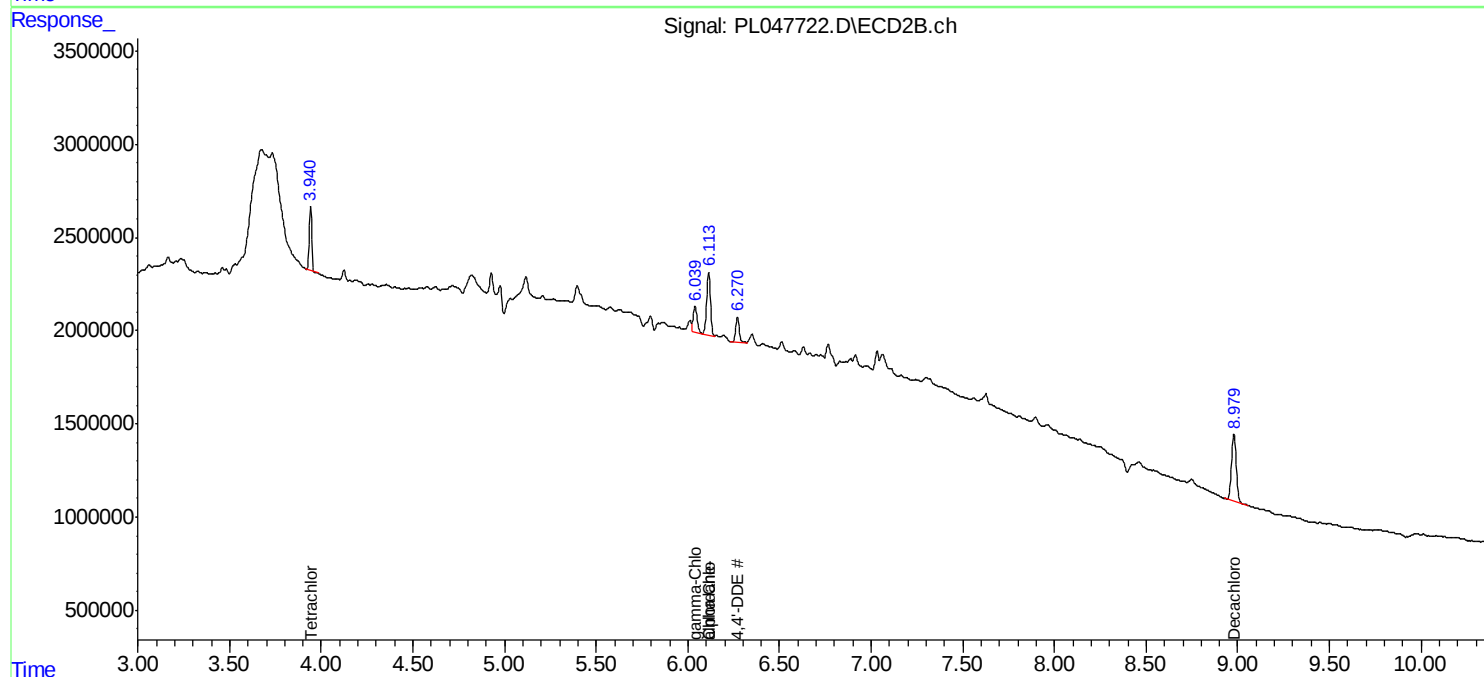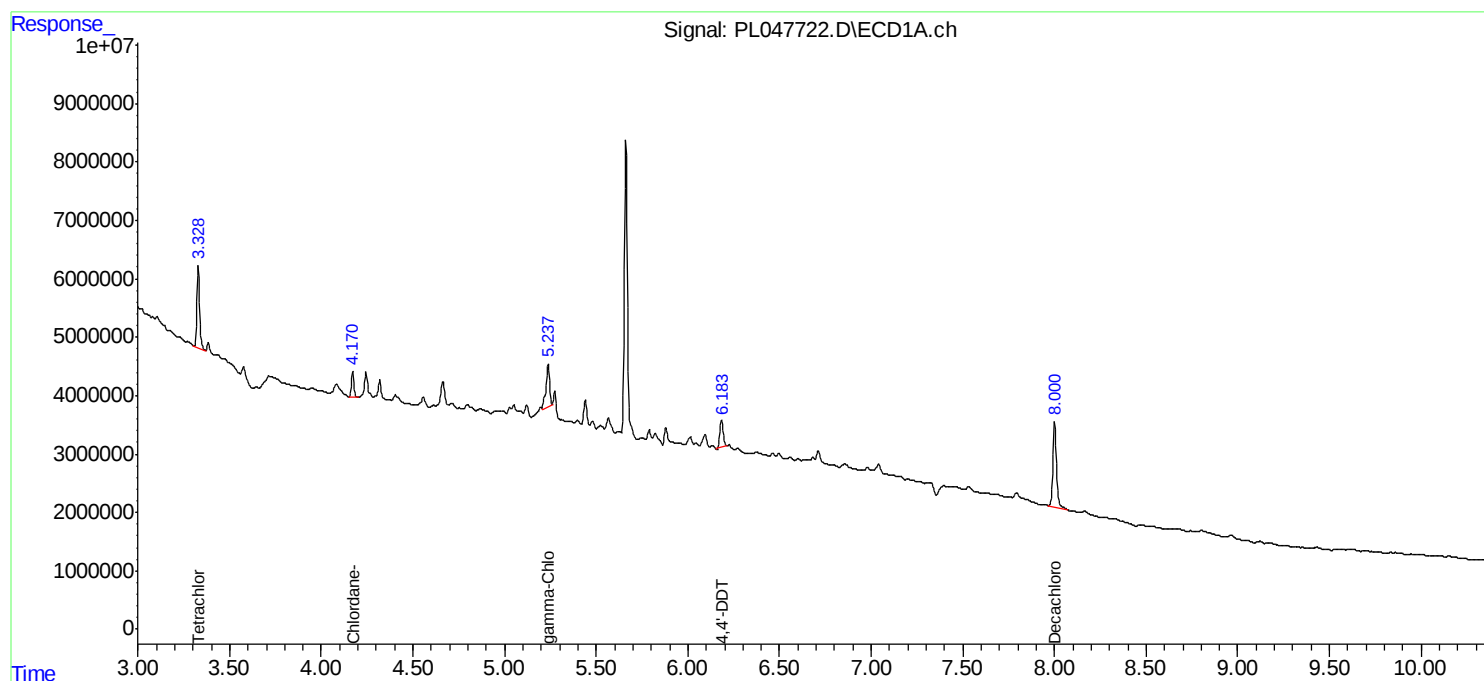


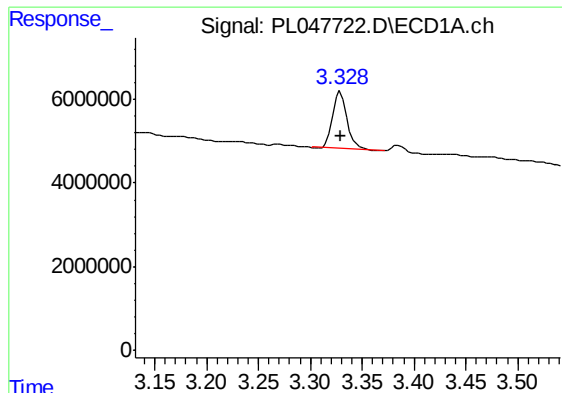

#1 Tetrachloro-m-xylene


R.T.: 3.329 min
Delta R.T.: 0.000 min
Response: 13425277
Conc: 1.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-006-B

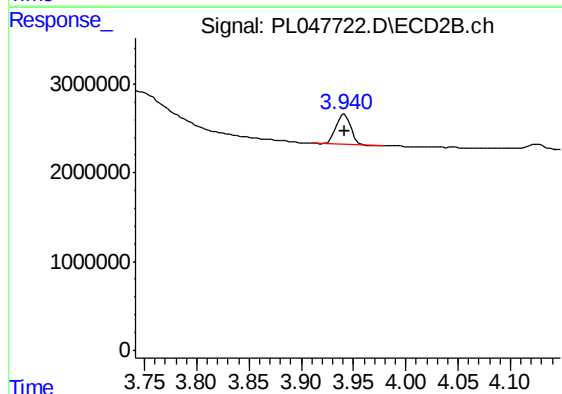


#1 Tetrachloro-m-xylene

R.T.: 3.941 min
Delta R.T.: 0.000 min
Response: 3238726
Conc: 1.36 ng/ml

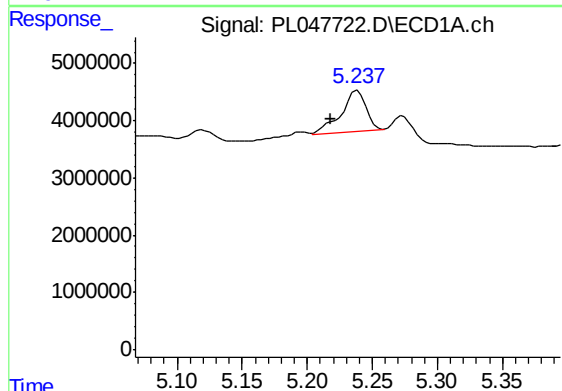


#10 gamma-Chlordane

R.T.: 5.239 min
Delta R.T.: 0.021 min
Response: 9629659
Conc: 0.72 ng/ml

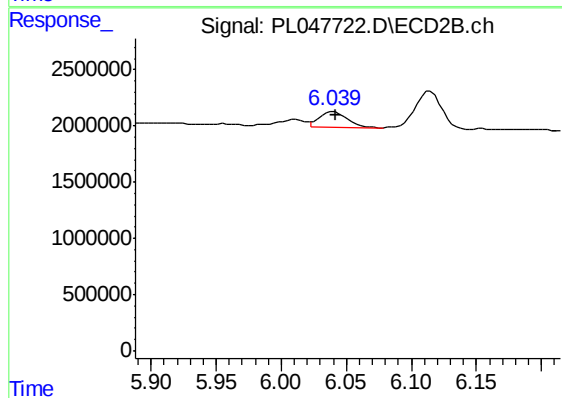

#10 gamma-Chlordane


R.T.: 6.040 min
Delta R.T.: -0.001 min
Response: 1983045
Conc: 0.66 ng/ml

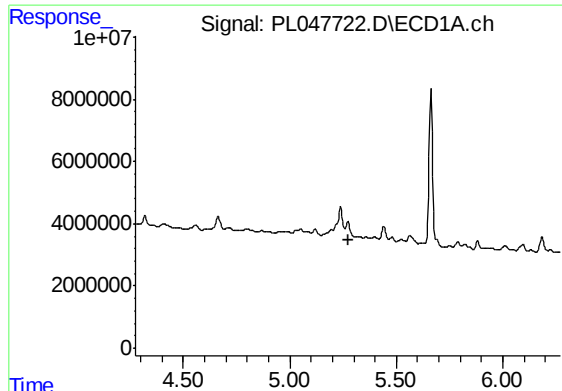

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-006-B

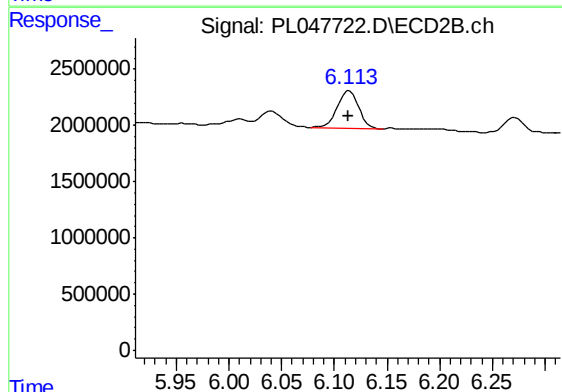


#11 alpha-Chlordane

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 4643258
Conc: 1.53 ng/ml

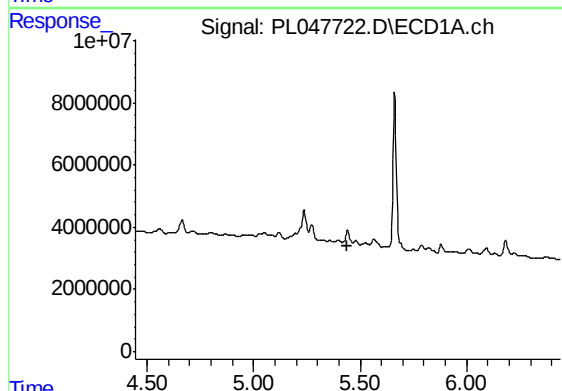


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.442 min
Response: 0
Conc: N.D.

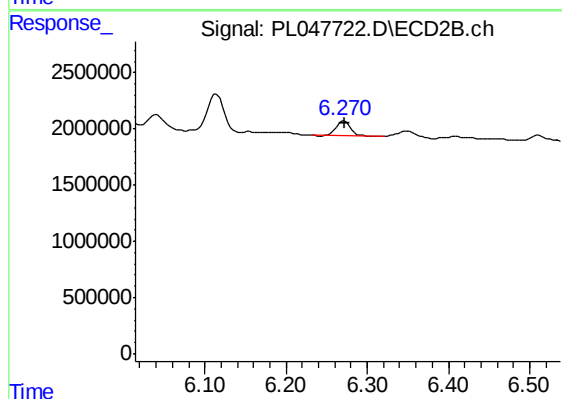

#12 4,4'-DDE


R.T.: 6.271 min
Delta R.T.: -0.002 min
Response: 1684715
Conc: 0.61 ng/ml

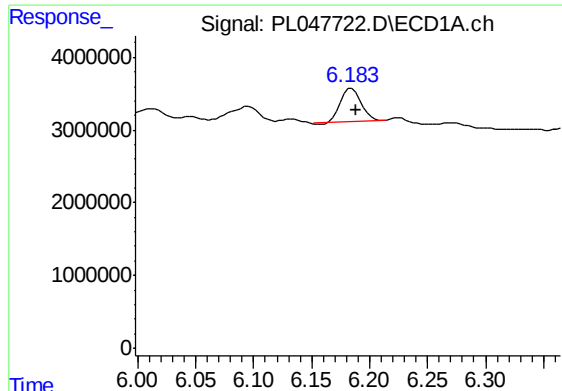

#17 4,4'-DDT


R.T.: 6.184 min
Delta R.T.: -0.004 min
Response: 5642576
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-006-B

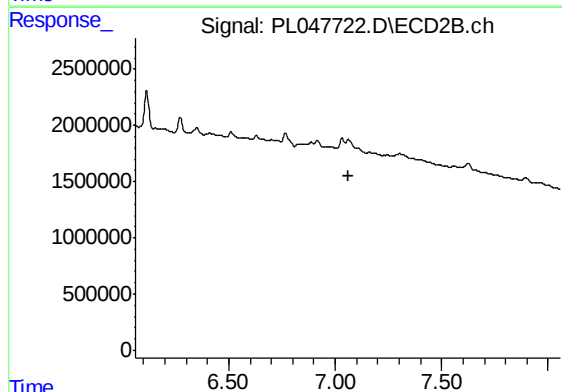


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.061 min
Response: 0
Conc: N.D.

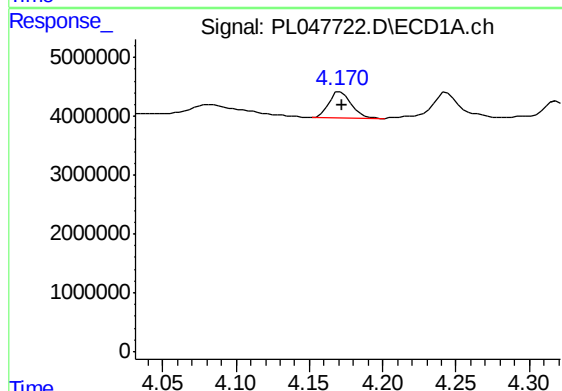


#23 Chlordane-1

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 4749764
Conc: 10.99 ng/ml

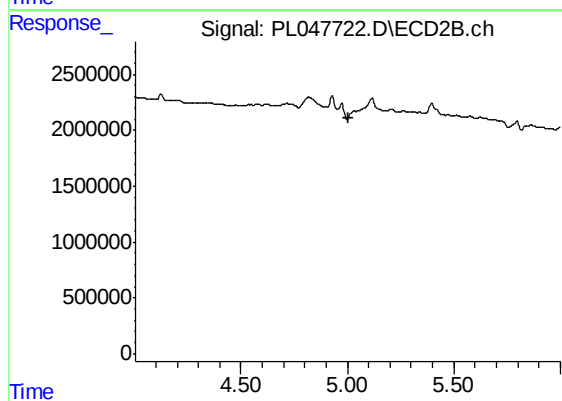

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.003 min
Response: 0
Conc: N.D.

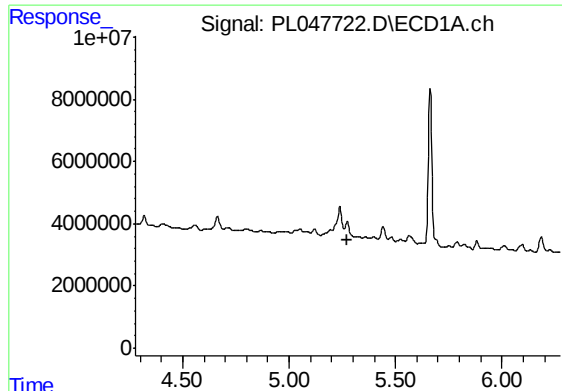

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-006-B

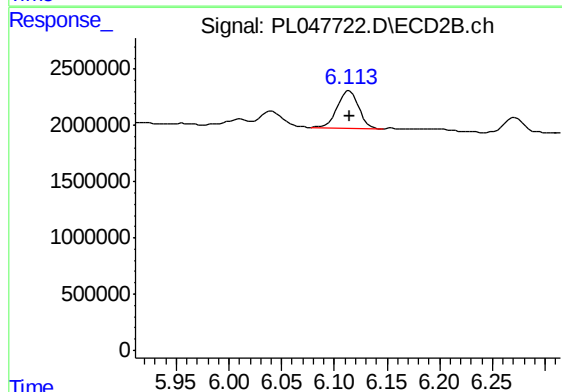


#25 Chlordane-3

R.T.: 6.114 min
Delta R.T.: 0.000 min
Response: 4643258
Conc: 15.67 ng/ml

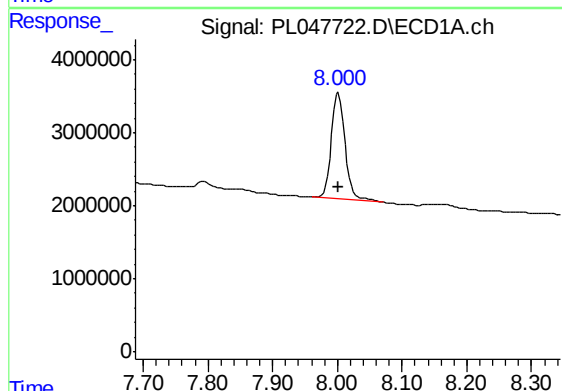

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 21238173
Conc: 1.90 ng/ml

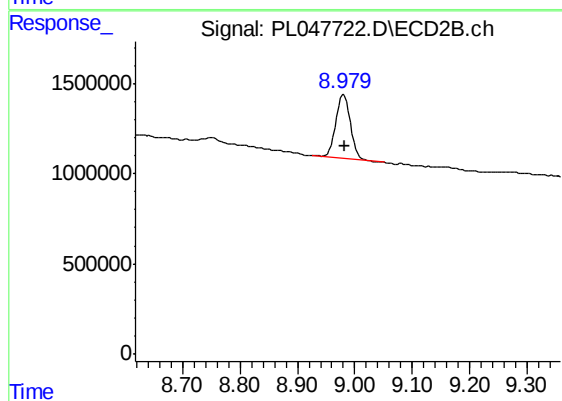

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.001 min
Response: 6192101
Conc: 2.17 ng/ml