

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
 Data File : PL047737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 04:12
 Operator : AJ\SJ
 Sample : K2200-07
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EO-02-042319-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 04:40:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	81732462	20578192	8.838	8.620
28)	SA Decachlor...	8.003	8.981	75100141	26390248	6.709	9.245 #
Target Compounds							
6)	B beta-BHC	0.000	4.811f	0	3496736	N.D.	2.427 #
10)	B gamma-Chl...	5.239f	0.000	6396904	0	0.480	N.D. #
11)	B alpha-Chl...	0.000	6.116	0	3855606	N.D.	1.274 #
12)	B 4,4'-DDE	5.443	6.271	23754133	5835698	1.910	2.113
17)	MA 4,4'-DDT	6.188	7.061	5247935	2529422	0.526	1.062 #
25)	Chlordane-3	0.000	6.116	0	3855606	N.D.	13.016 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
Data File : PL047737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 04:12
Operator : AJ\SJ
Sample : K2200-07
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EO-02-042319-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 04:40:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

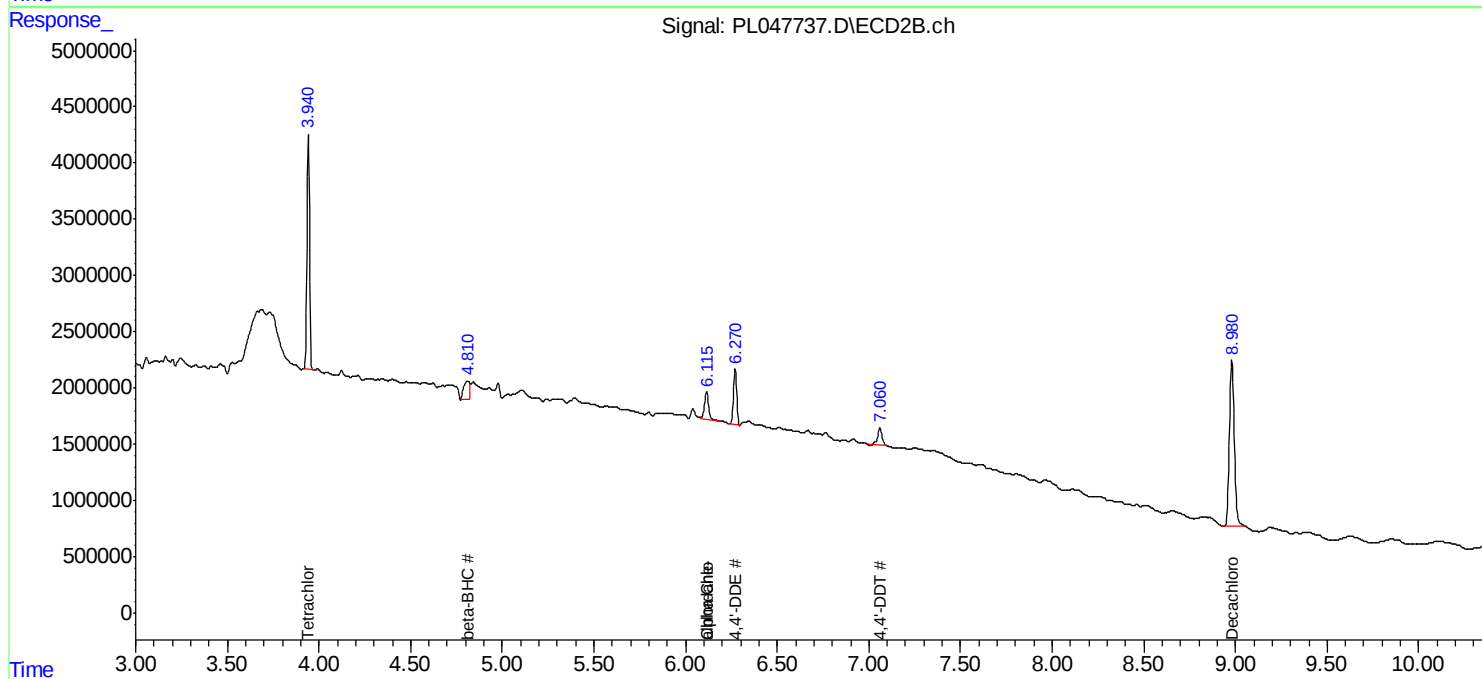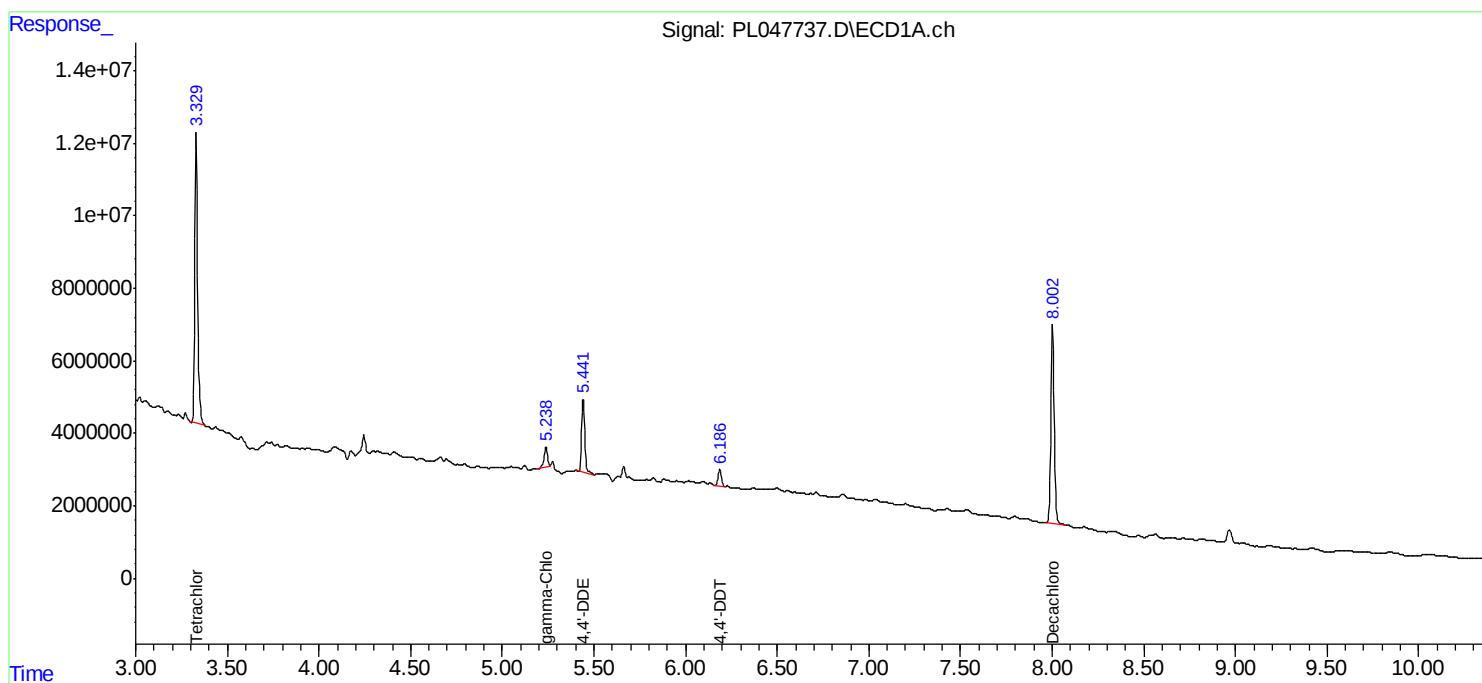


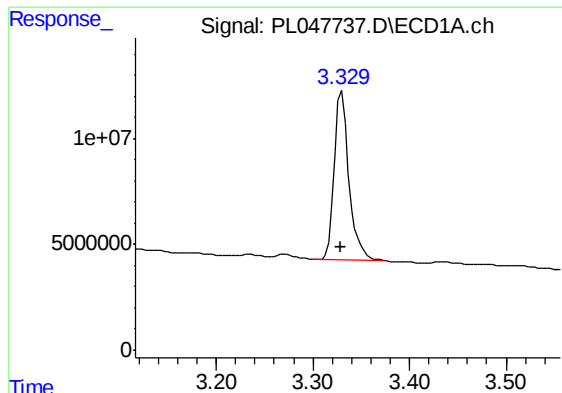

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 81732462
Conc: 8.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-042319-A

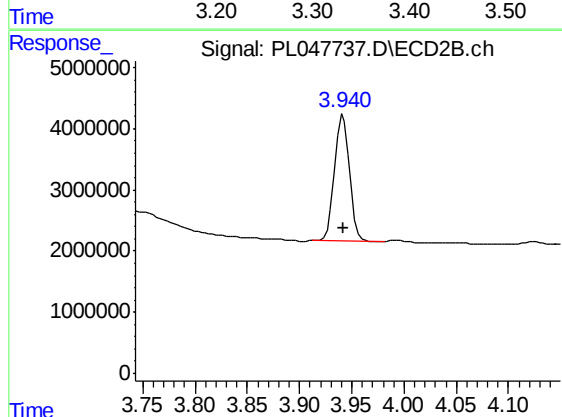


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 20578192
Conc: 8.62 ng/ml

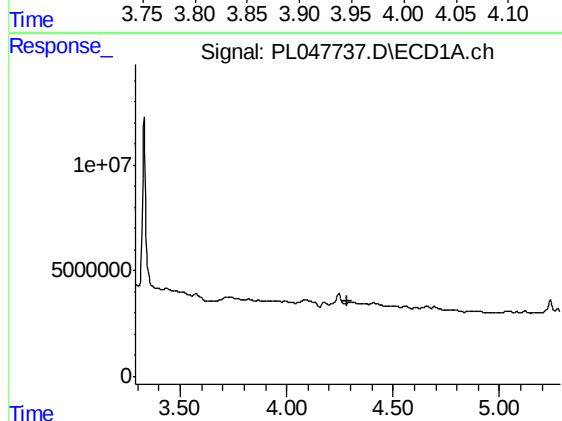


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.287 min
Response: 0
Conc: N.D.

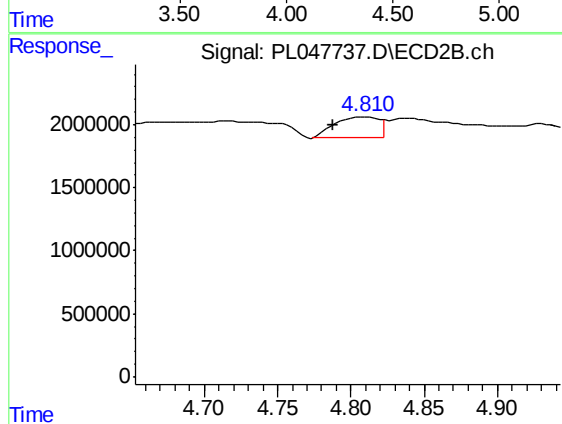

#6 beta-BHC


R.T.: 4.811 min
Delta R.T.: 0.023 min
Response: 3496736
Conc: 2.43 ng/ml

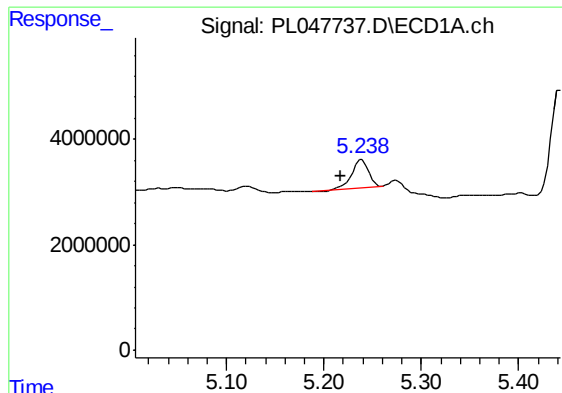

#10 gamma-Chlordane


R.T.: 5.239 min
Delta R.T.: 0.021 min
Response: 6396904
Conc: 0.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-042319-A

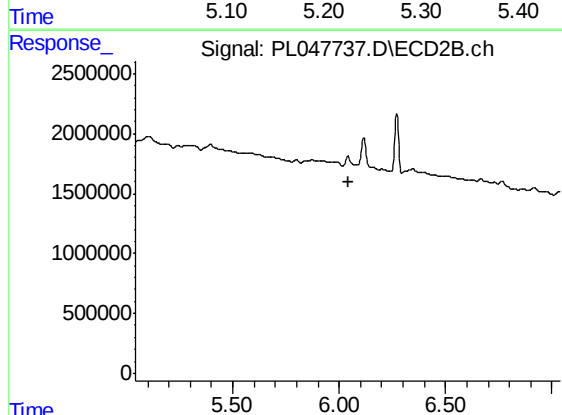


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.042 min
Response: 0
Conc: N.D.

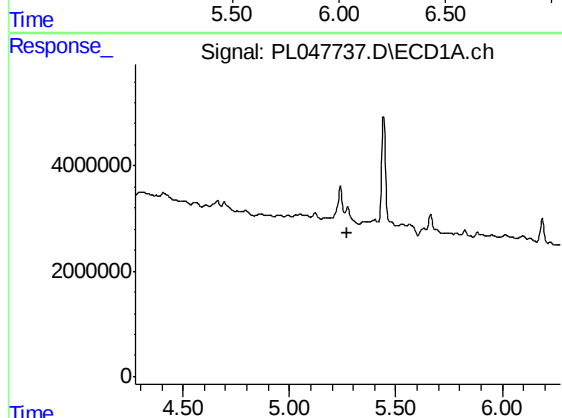


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.274 min
Response: 0
Conc: N.D.

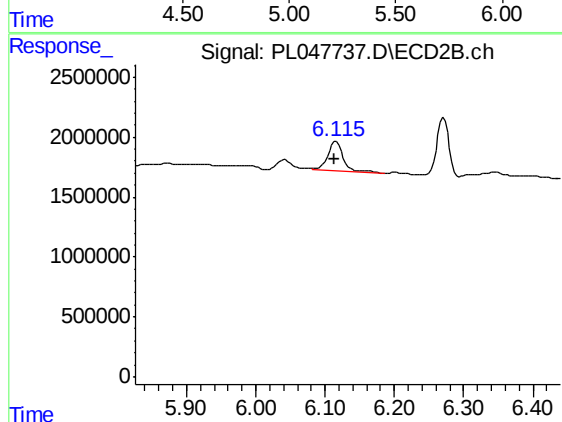

#11 alpha-Chlordane


R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 3855606
Conc: 1.27 ng/ml

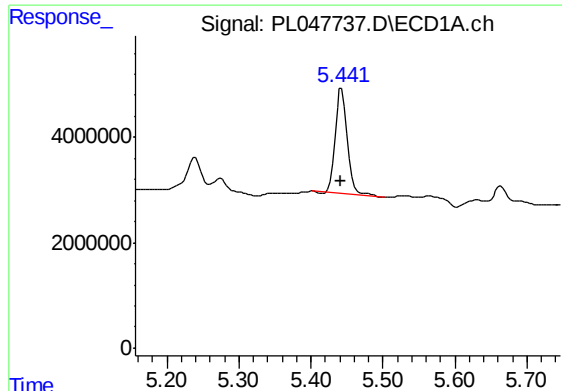

#12 4,4'-DDE


R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 23754133
Conc: 1.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
EO-02-042319-A

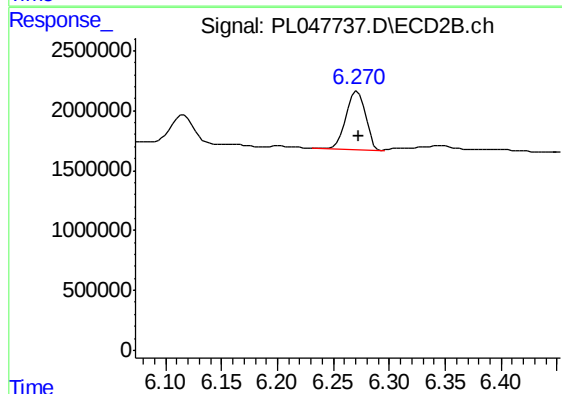


#12 4,4'-DDE

R.T.: 6.271 min
Delta R.T.: -0.002 min
Response: 5835698
Conc: 2.11 ng/ml

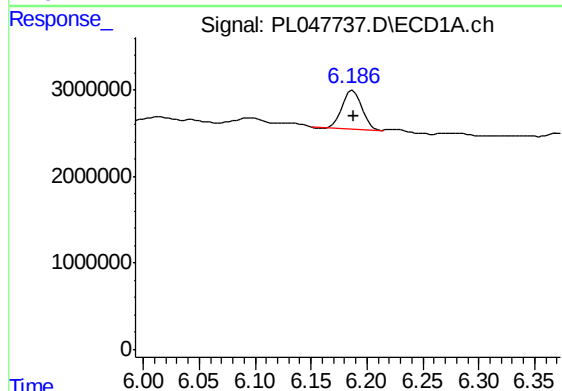


#17 4,4'-DDT

R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 5247935
Conc: 0.53 ng/ml

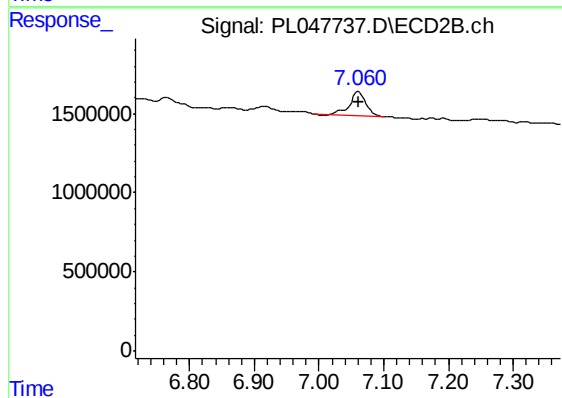

#17 4,4'-DDT


R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 2529422
Conc: 1.06 ng/ml

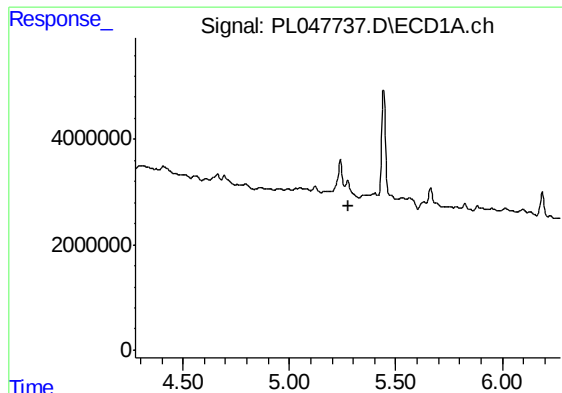

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EO-02-042319-A

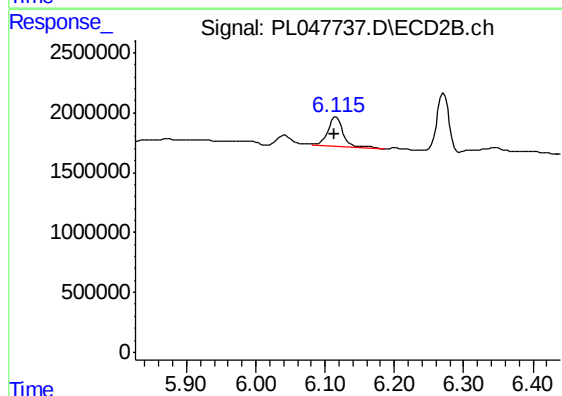


#25 Chlordane-3

R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 3855606
Conc: 13.02 ng/ml

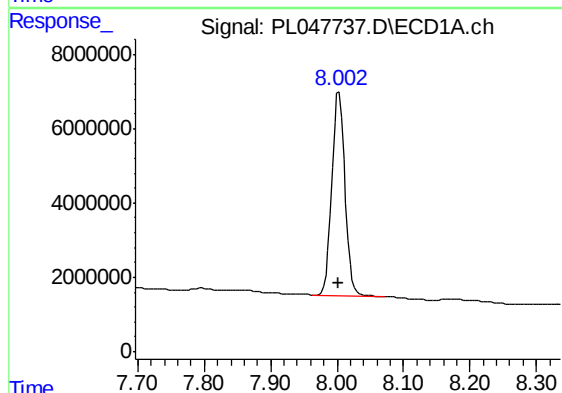

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.001 min
Response: 75100141
Conc: 6.71 ng/ml

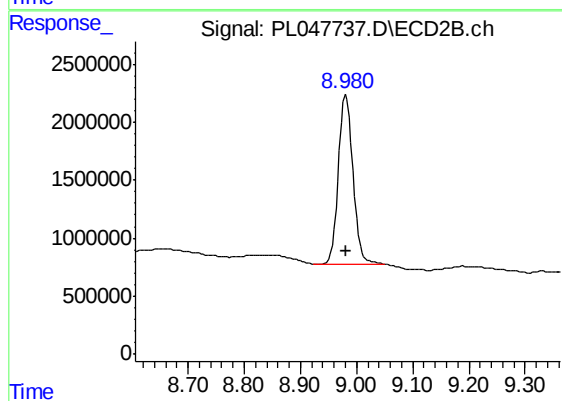

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 26390248
Conc: 9.24 ng/ml