

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
 Data File : PL047695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2019 16:46
 Operator : AJ\SJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:45:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:45:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	476.8E6	113.8E6	50.000	50.000
28)	SA Decachlor...	8.002	8.982	540.6E6	134.0E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.172	4.930	216.2E6	55959469	500.000	500.000
24)	Chlordane-2	4.663	5.397	237.8E6	59811589	500.000	500.000
25)	Chlordane-3	5.220	6.042	789.8E6	202.7E6	500.000	500.000
26)	Chlordane-4	5.275	6.115	712.1E6	242.0E6	500.000	500.000
27)	Chlordane-5	6.098	6.917	212.0E6	48409202	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042419\
Data File : PL047695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2019 16:46
Operator : AJ\SJ
Sample : PCHLORICC500
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:45:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:45:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

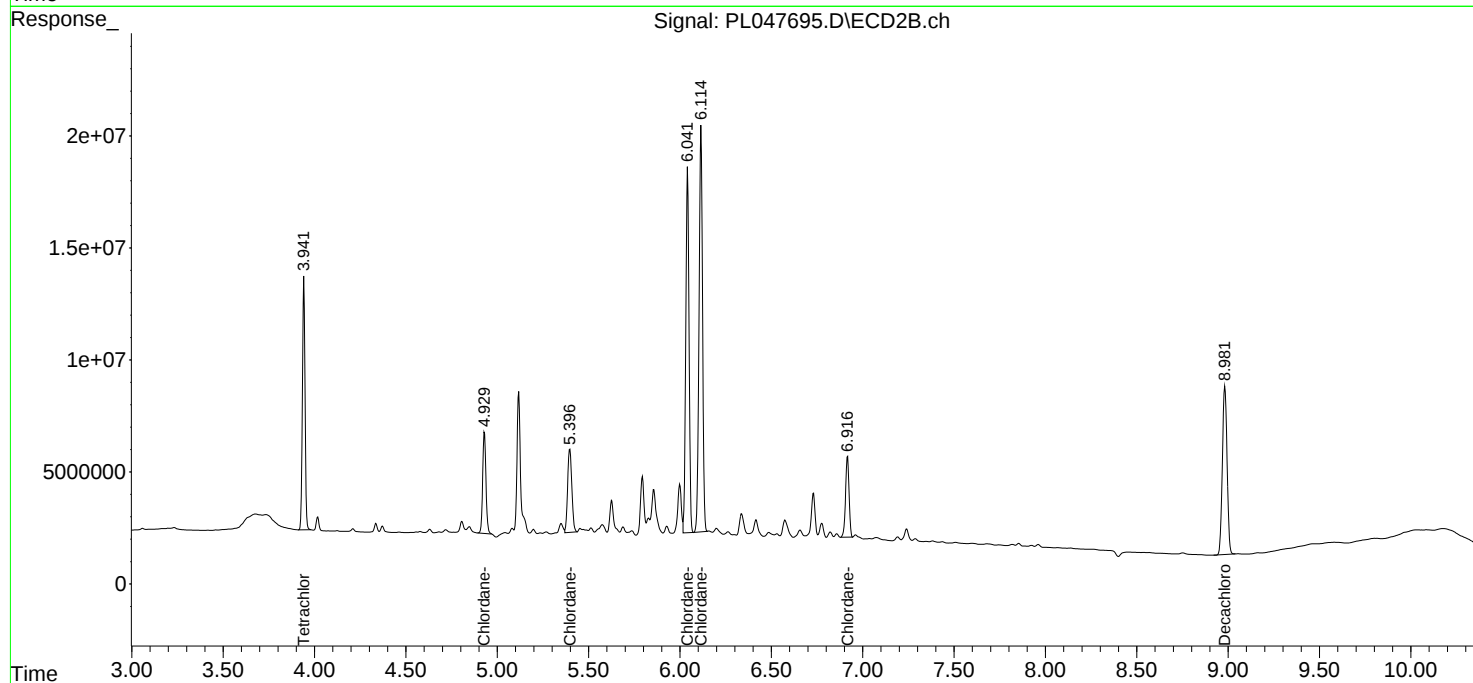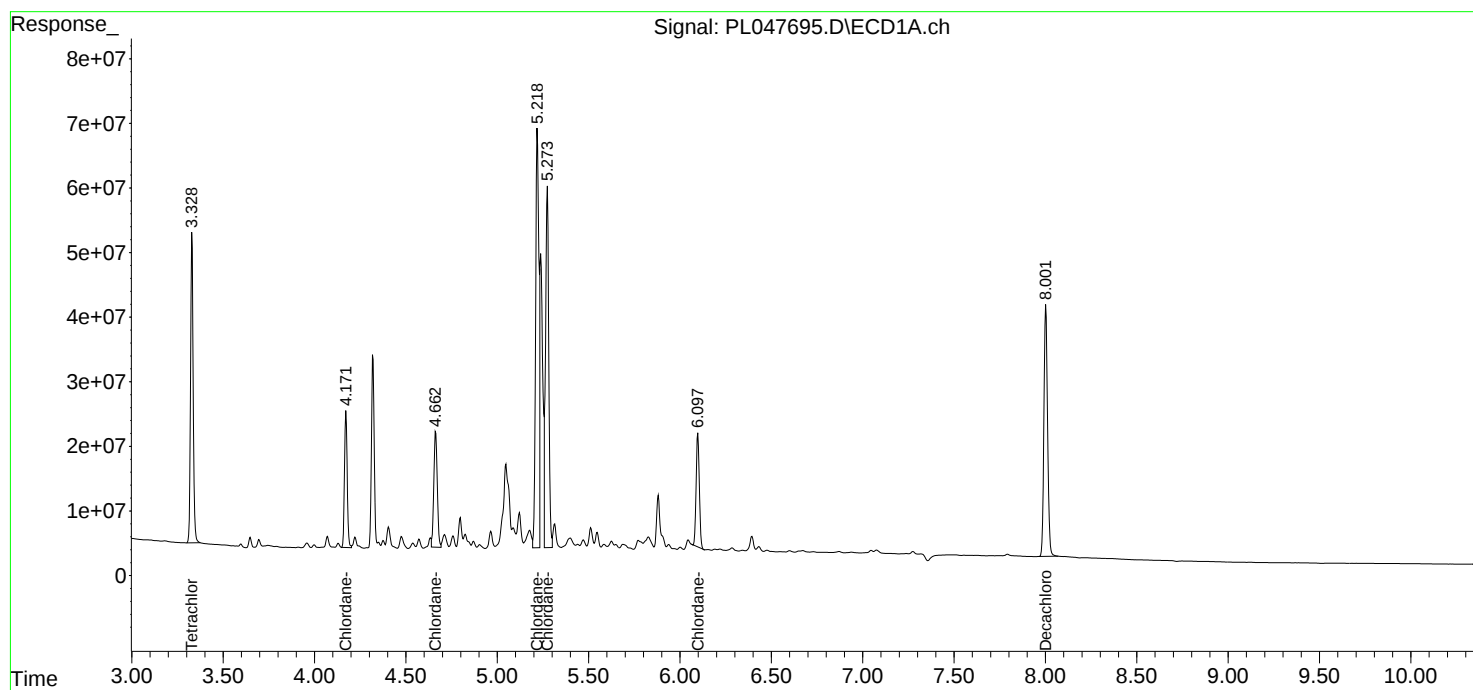


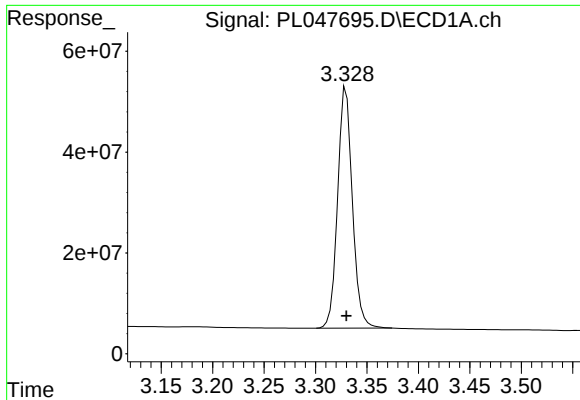

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 476849654
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

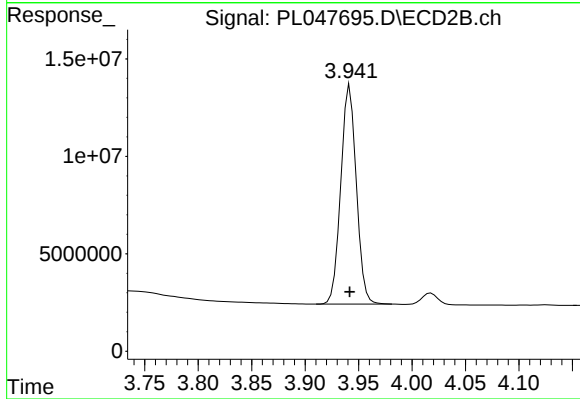


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 113752621
Conc: 50.00 ng/ml

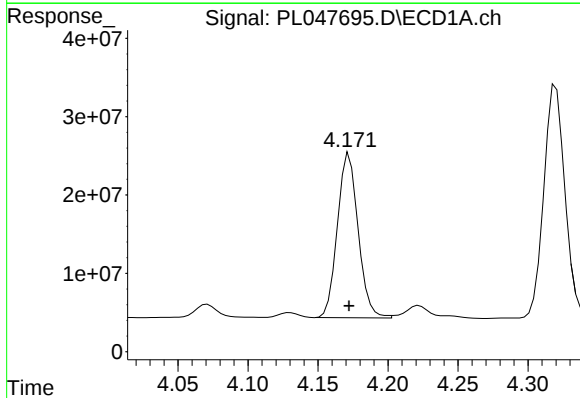


#23 Chlordane-1

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 216177065
Conc: 500.00 ng/ml

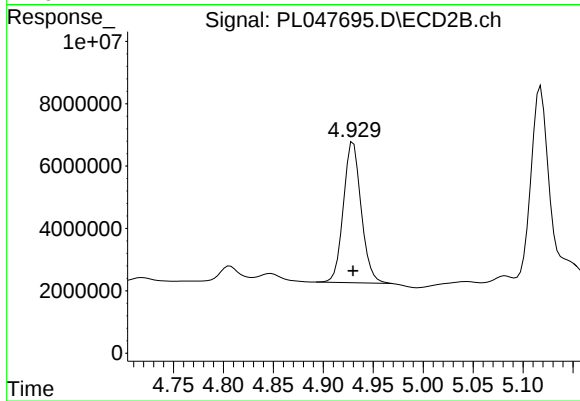

#23 Chlordane-1


R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 55959469
Conc: 500.00 ng/ml

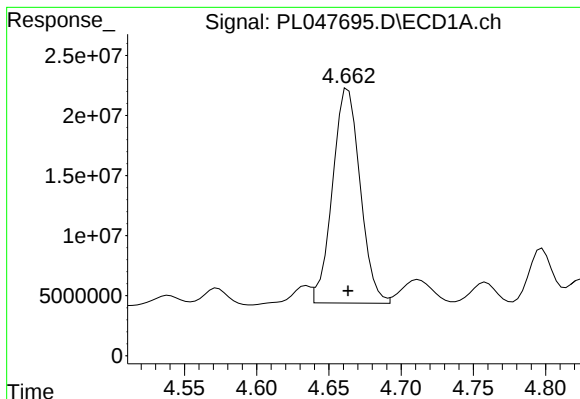

#24 Chlordane-2


R.T.: 4.663 min
Delta R.T.: 0.000 min
Response: 237776868
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

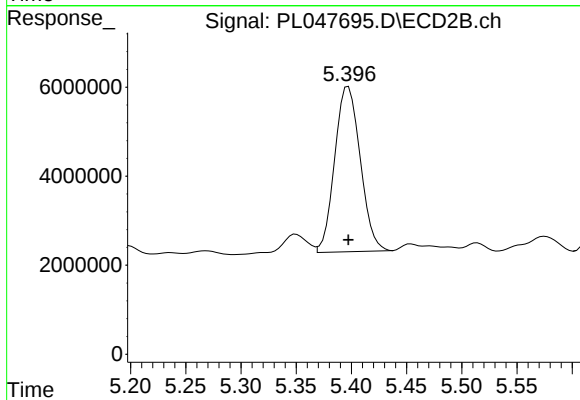


#24 Chlordane-2

R.T.: 5.397 min
Delta R.T.: 0.000 min
Response: 59811589
Conc: 500.00 ng/ml

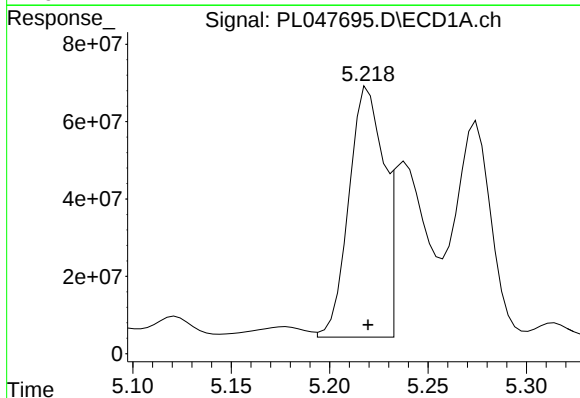


#25 Chlordane-3

R.T.: 5.220 min
Delta R.T.: 0.000 min
Response: 789807639
Conc: 500.00 ng/ml

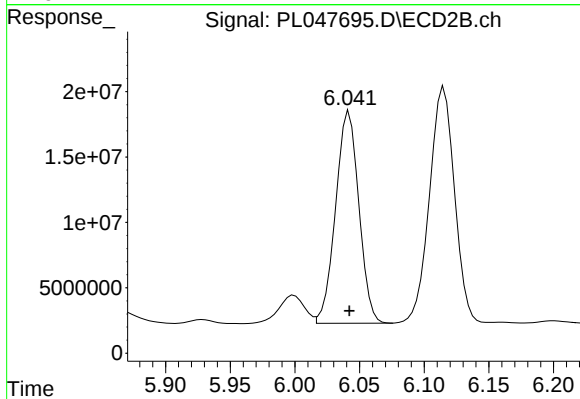

#25 Chlordane-3


R.T.: 6.042 min
Delta R.T.: 0.000 min
Response: 202685319
Conc: 500.00 ng/ml

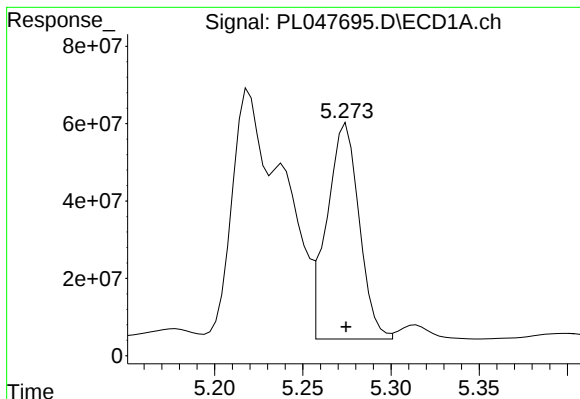

#26 Chlordane-4


R.T.: 5.275 min
Delta R.T.: 0.000 min
Response: 712106773
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

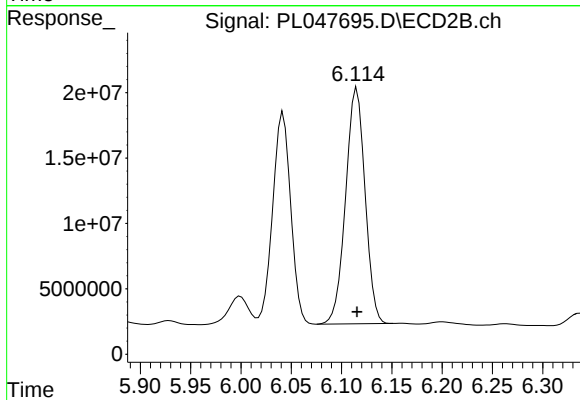


#26 Chlordane-4

R.T.: 6.115 min
Delta R.T.: 0.000 min
Response: 241967935
Conc: 500.00 ng/ml

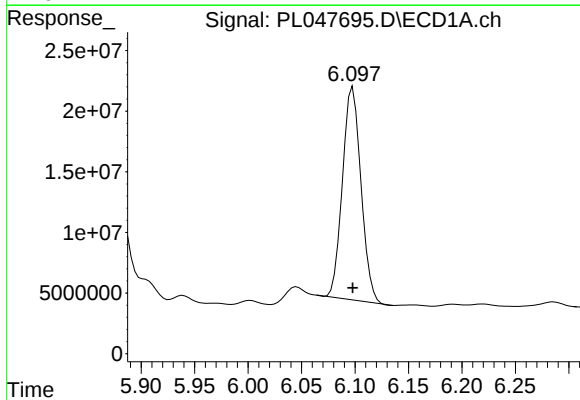


#27 Chlordane-5

R.T.: 6.098 min
Delta R.T.: 0.000 min
Response: 211987201
Conc: 500.00 ng/ml

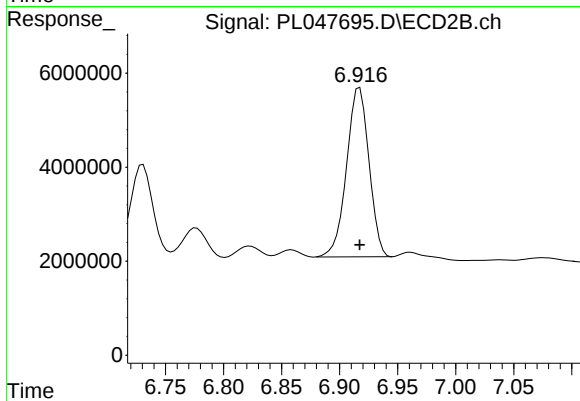

#27 Chlordane-5


R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 48409202
Conc: 500.00 ng/ml

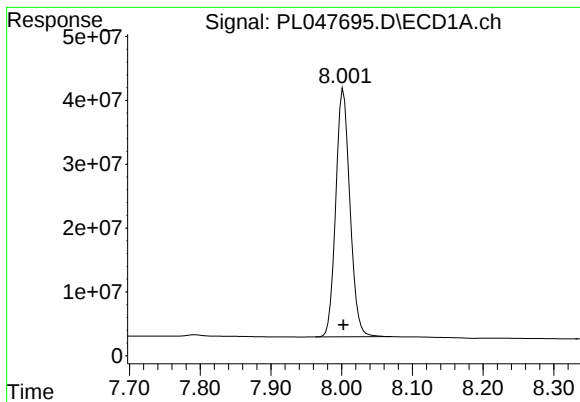

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 540620592
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

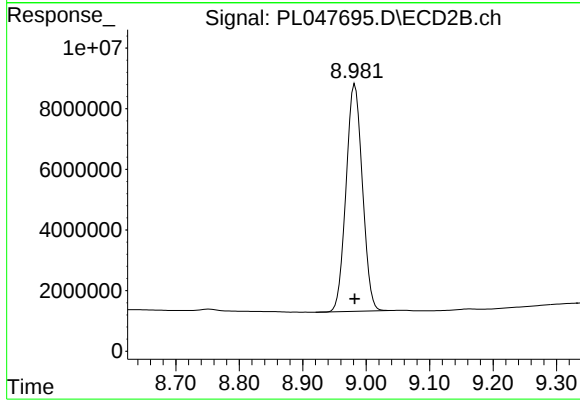

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 134037840
Conc: 50.00 ng/ml