

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042420\
 Data File : PL058377.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2020 18:37
 Operator : AJ\MA
 Sample : L2399-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SP1-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.456	3.955	203.6E6	46320069	20.199	21.344
28)	SA Decachlor...	8.202	8.976	198.6E6	42104469	19.265	18.849
Target Compounds							
4)	MA Heptachlor	4.463f	5.136	1063152	793404	0.066	0.236 #
7)	B delta-BHC	0.000	4.987f	0	4739334	N.D.	3.844 #
15)	B Endosulfa...	0.000	6.867	0	586937	N.D.	0.226 #
23)	Chlordane-1	4.324	0.000	3160364	0	8.545	N.D. #
24)	Chlordane-2	4.804f	0.000	9952514	0	24.652	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042420\
Data File : PL058377.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2020 18:37
Operator : AJ\MA
Sample : L2399-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SP1-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:57:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

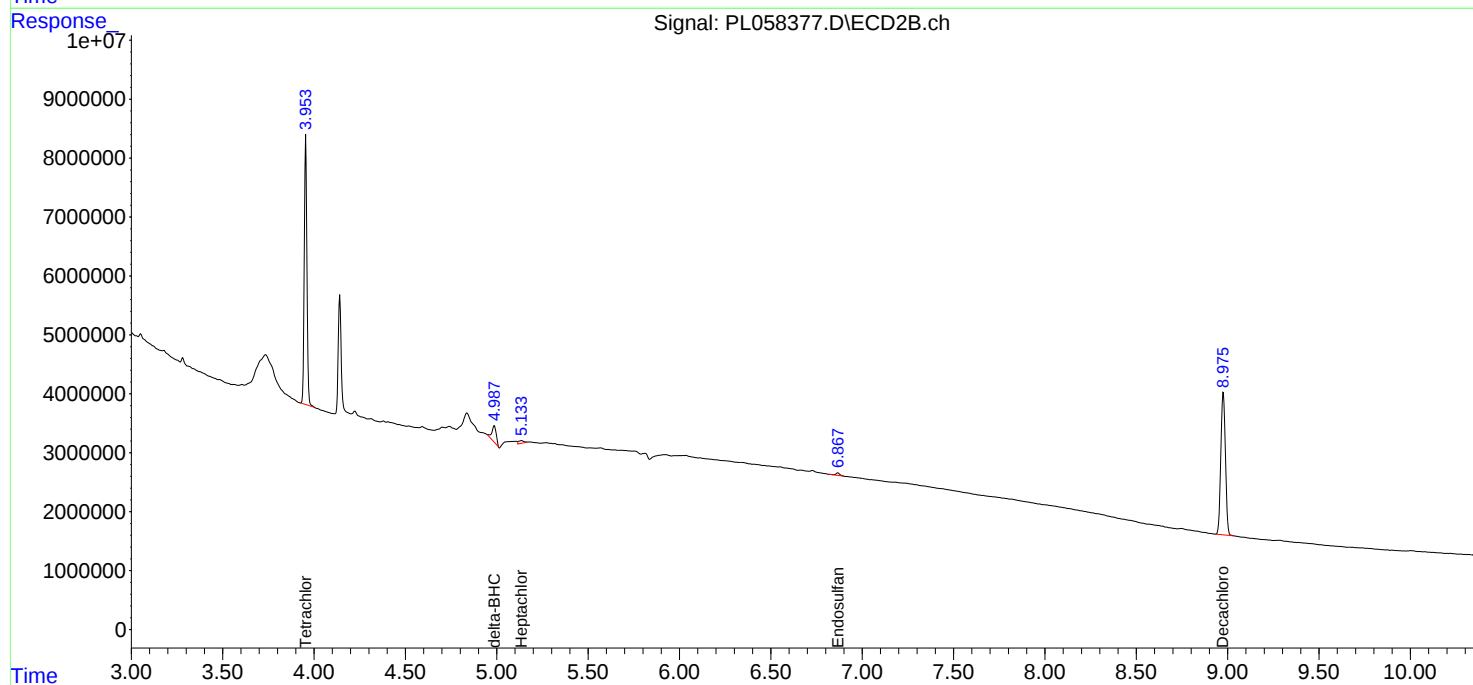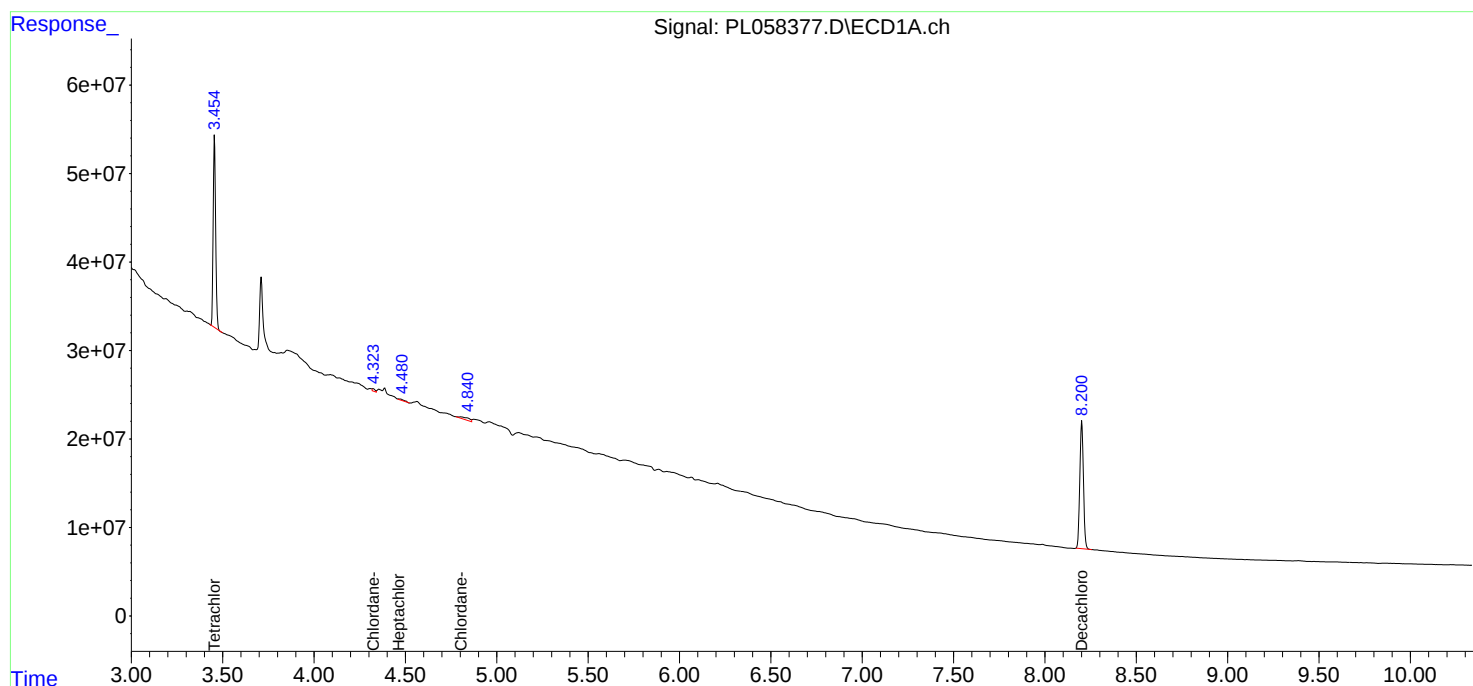


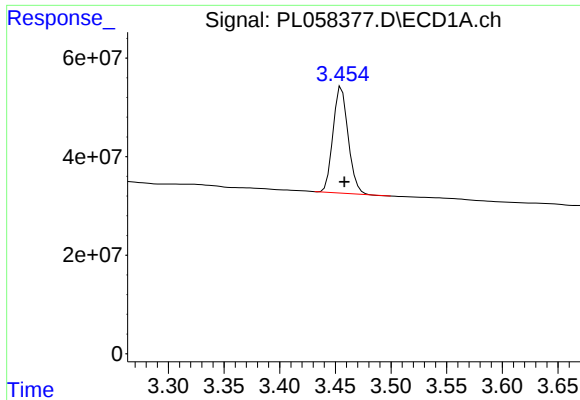

#1 Tetrachloro-m-xylene


R.T.: 3.456 min
Delta R.T.: -0.002 min
Response: 203628400
Conc: 20.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP1-A

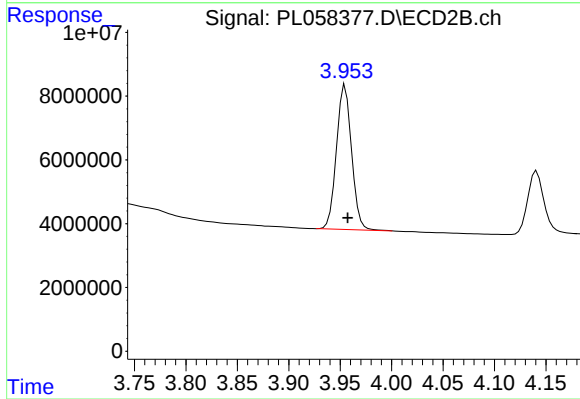


#1 Tetrachloro-m-xylene

R.T.: 3.955 min
Delta R.T.: -0.002 min
Response: 46320069
Conc: 21.34 ng/ml

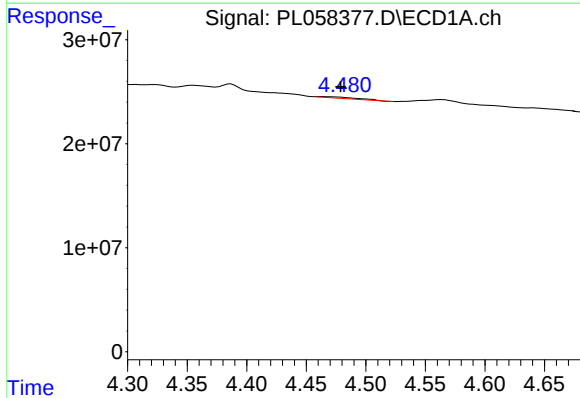


#4 Heptachlor

R.T.: 4.463 min
Delta R.T.: -0.015 min
Response: 1063152
Conc: 0.07 ng/ml

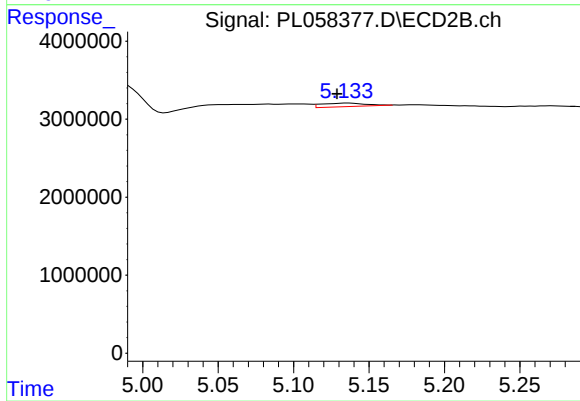

#4 Heptachlor


R.T.: 5.136 min
Delta R.T.: 0.007 min
Response: 793404
Conc: 0.24 ng/ml

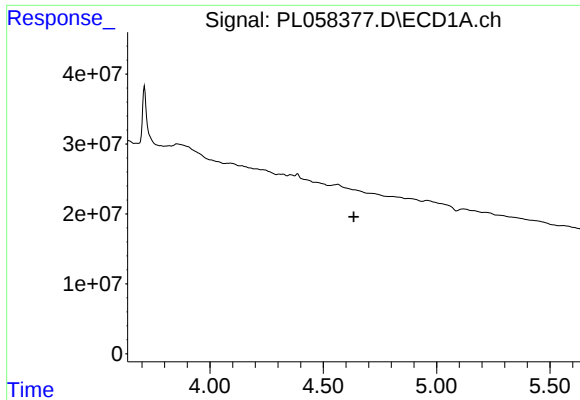

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.634 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
SP1-A

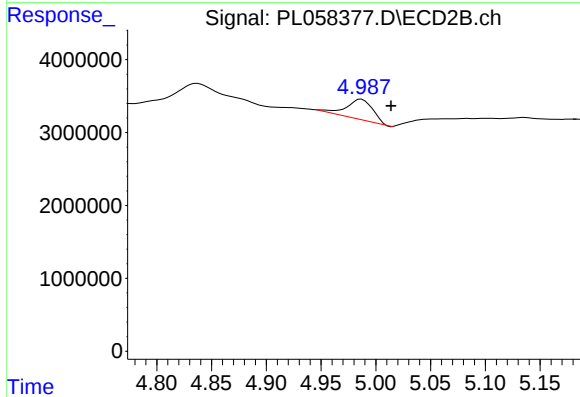


#7 delta-BHC

R.T.: 4.987 min
Delta R.T.: -0.027 min
Response: 4739334
Conc: 3.84 ng/ml

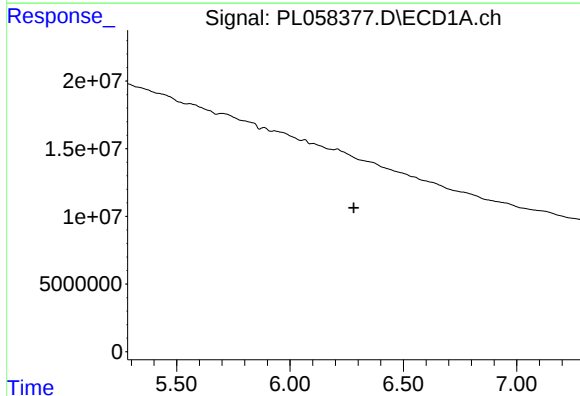


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

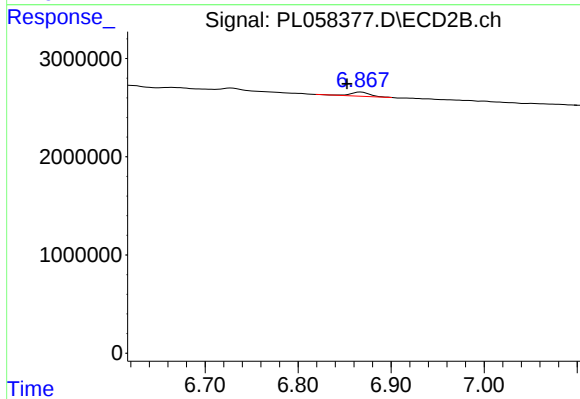

#15 Endosulfan II


R.T.: 6.867 min
Delta R.T.: 0.015 min
Response: 586937
Conc: 0.23 ng/ml

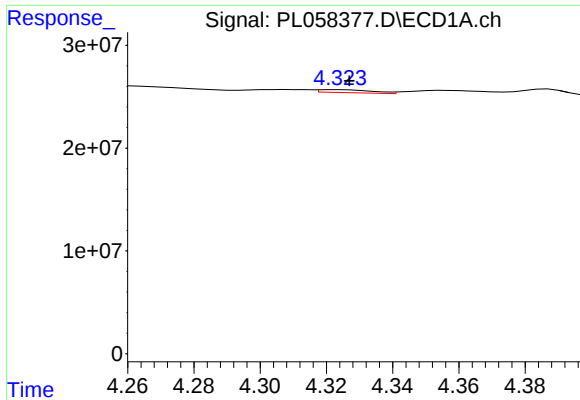

#23 Chlordane-1


R.T.: 4.324 min
Delta R.T.: -0.003 min
Response: 3160364
Conc: 8.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP1-A

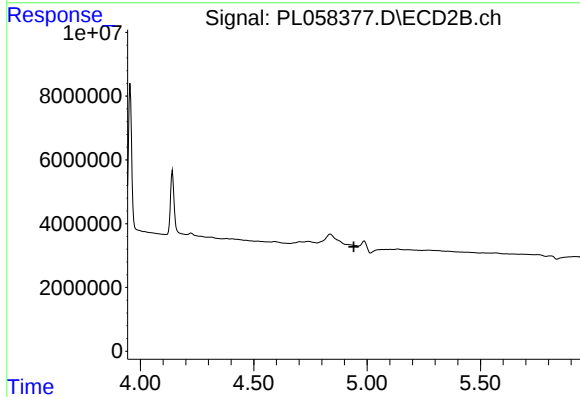


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

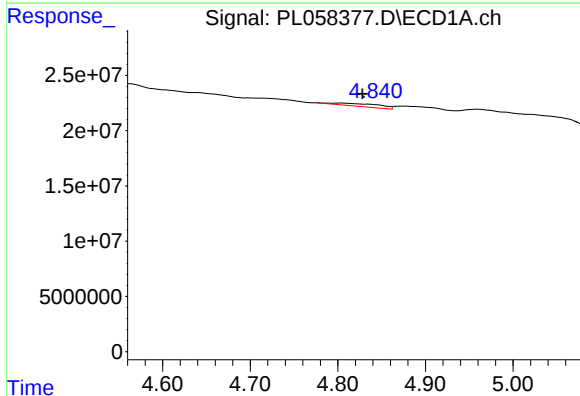


#24 Chlordane-2

R.T.: 4.804 min
Delta R.T.: -0.024 min
Response: 9952514
Conc: 24.65 ng/ml

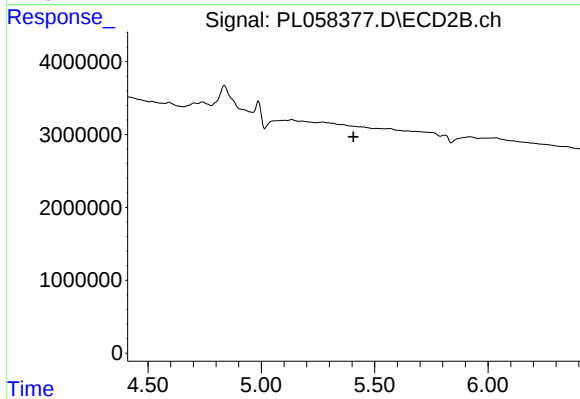

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.407 min
Response: 0
Conc: N.D.

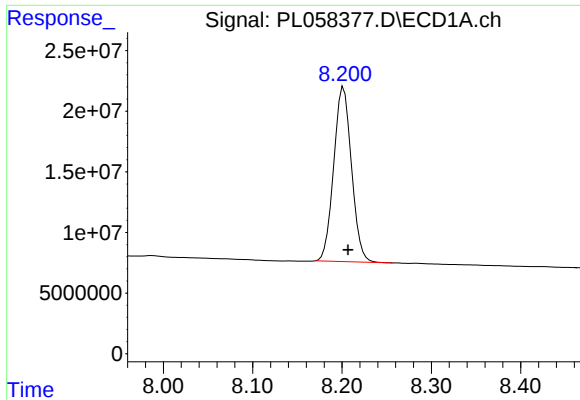

#28 Decachlorobiphenyl

R.T.: 8.202 min
Delta R.T.: -0.005 min
Response: 198590984
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
SP1-A

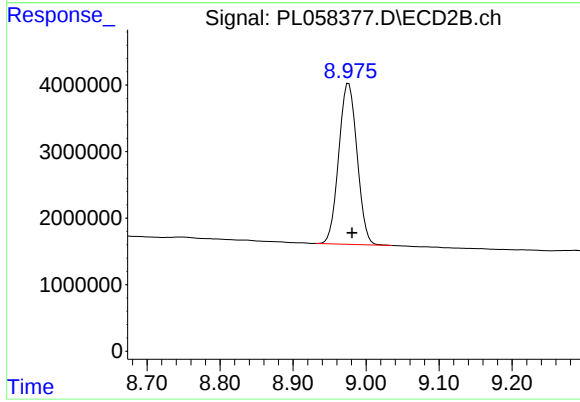

#28 Decachlorobiphenyl

R.T.: 8.976 min
Delta R.T.: -0.005 min
Response: 42104469
Conc: 18.85 ng/ml