

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042420\
 Data File : PL058376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2020 18:23
 Operator : AJ\MA
 Sample : L2397-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-1-COMP

Manual Integrations
 APPROVED

mohammad
 4/27/2020 11:31:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 00:57:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
 Quant Title : GC Extractables
 QLast Update : Sat Apr 04 06:41:11 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.454	3.955	229.9E6	49781278	22.808m	22.939
28)	SA Decachlor...	8.202	8.976	209.2E6	44439776	20.296	19.894

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042420\
Data File : PL058376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2020 18:23
Operator : AJ\MA
Sample : L2397-06
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-1-COMP


Manual Integrations
APPROVED

mohammad
4/27/2020 11:31:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 00:57:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040320.M
Quant Title : GC Extractables
QLast Update : Sat Apr 04 06:41:11 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

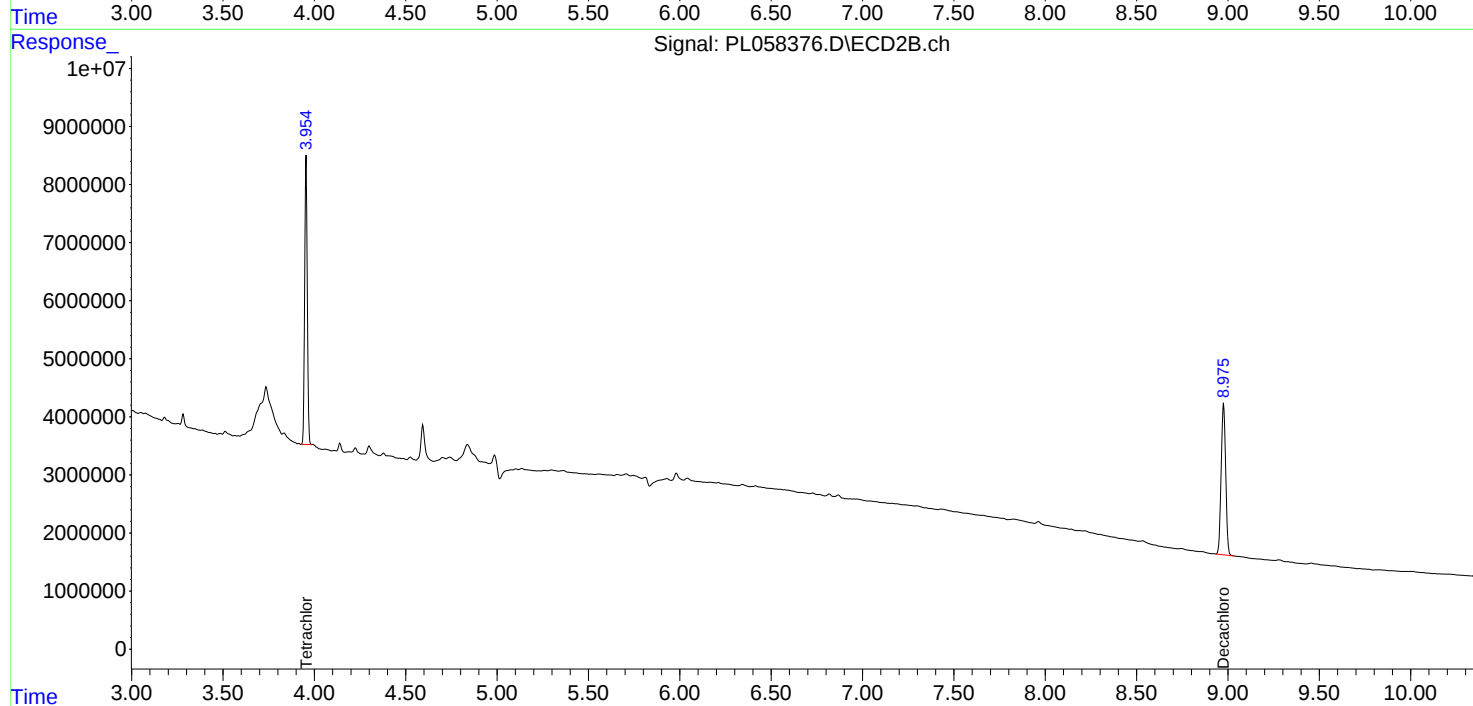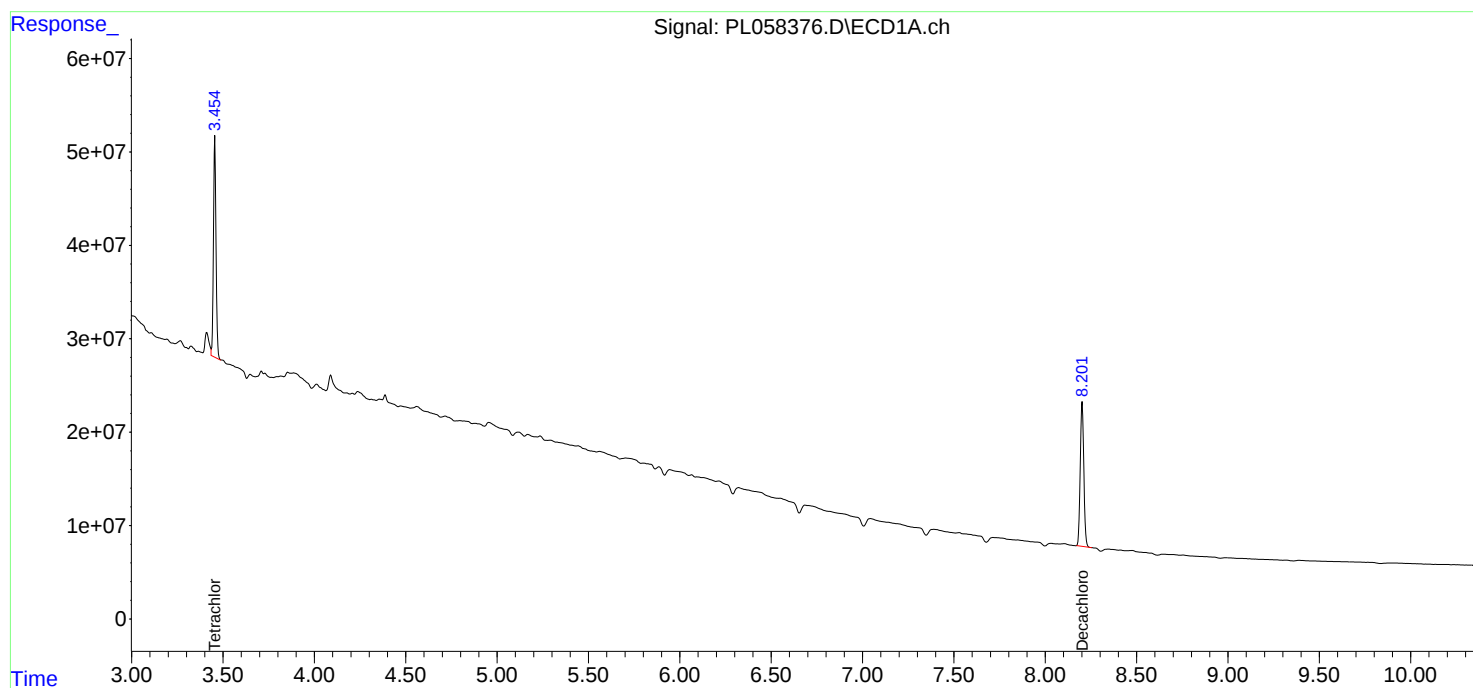

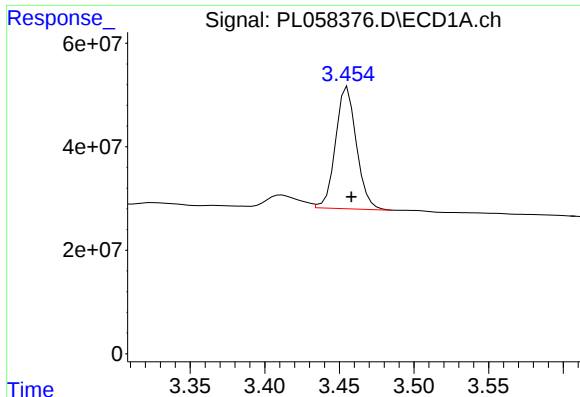

#1 Tetrachloro-m-xylene

R.T.: 3.454 min

Delta R.T.: -0.004 min


Response: 229928931

Conc: 22.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
TP-1-COMP

Manual Integrations
APPROVED

mohammad
4/27/2020 11:31:50 AM

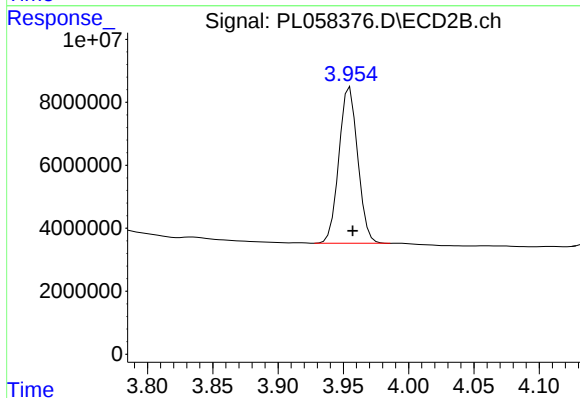


#1 Tetrachloro-m-xylene

R.T.: 3.955 min

Delta R.T.: -0.002 min

Response: 49781278

Conc: 22.94 ng/ml

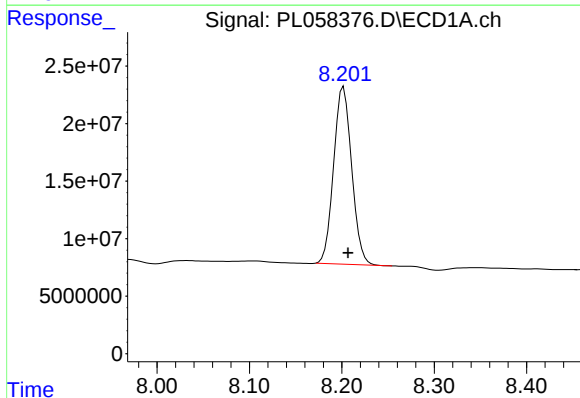


#28 Decachlorobiphenyl

R.T.: 8.202 min

Delta R.T.: -0.005 min

Response: 209217475

Conc: 20.30 ng/ml

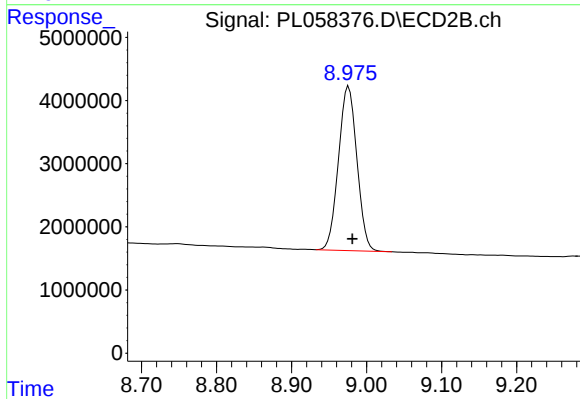

#28 Decachlorobiphenyl

R.T.: 8.976 min

Delta R.T.: -0.005 min

Response: 44439776

Conc: 19.89 ng/ml