

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
 Data File : PL082277.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2023 10:32
 Operator : AR\AJ
 Sample : 02427-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 20230351-COMP-29

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/25/2023
 Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 22:22:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.323	2.649	24163271	20250399	9.046m	8.741
28) SA Decachlor...	8.747	7.763	22377544	21431104	11.722	9.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
Data File : PL082277.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2023 10:32
Operator : AR\AJ
Sample : 02427-10
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
20230351-COMP-29


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/25/2023
Supervised By : Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 22:22:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

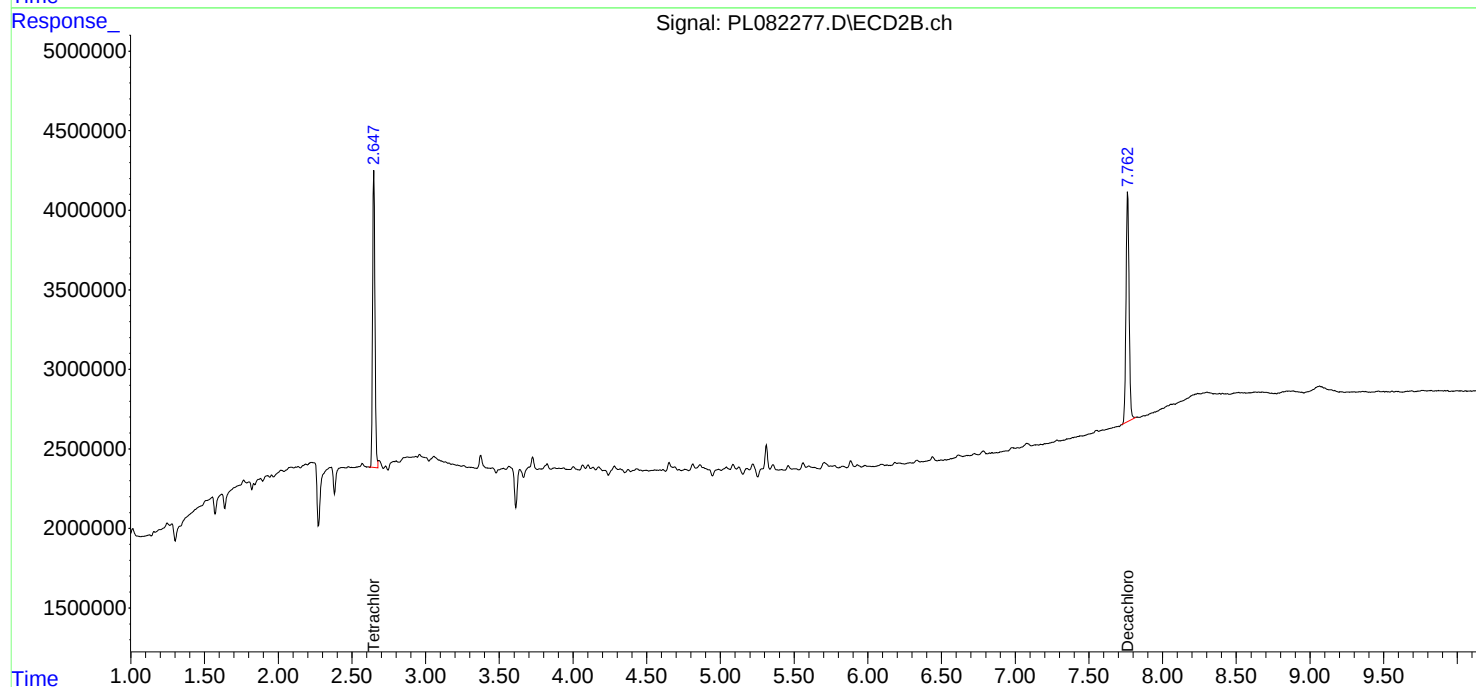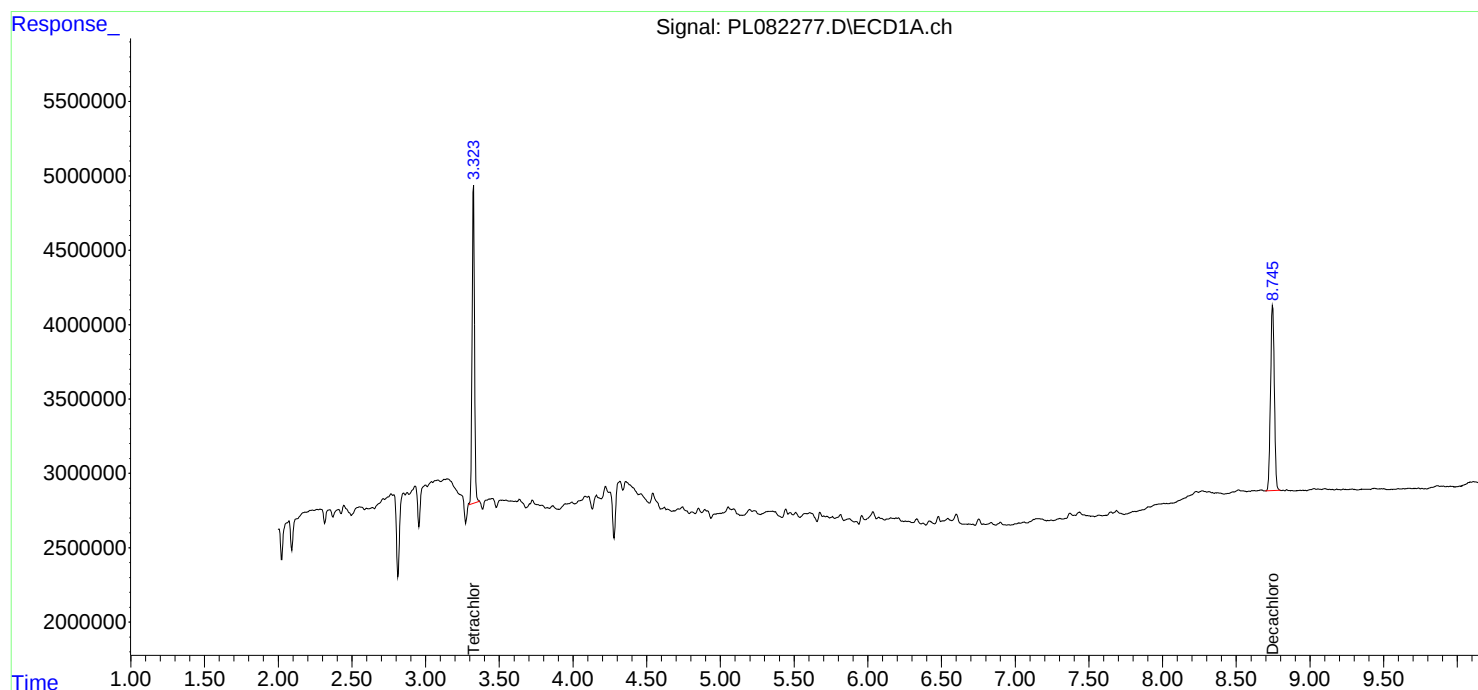

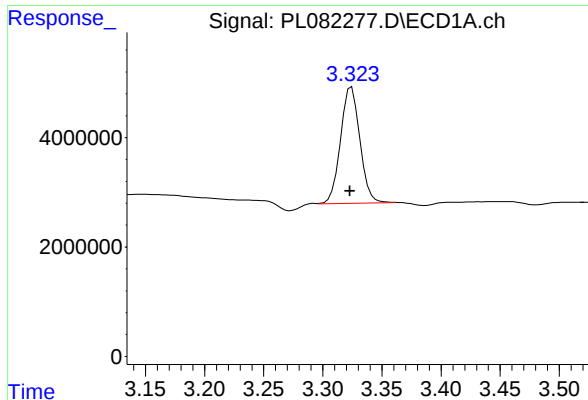


#1 Tetrachloro-m-xylene

R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 24163271
Conc: 9.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
20230351-COMP-29


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

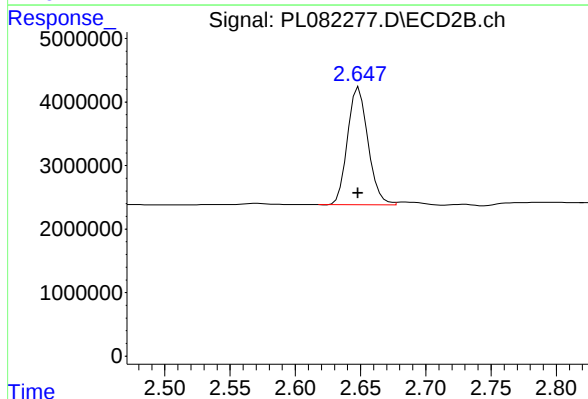


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 20250399
Conc: 8.74 ng/ml

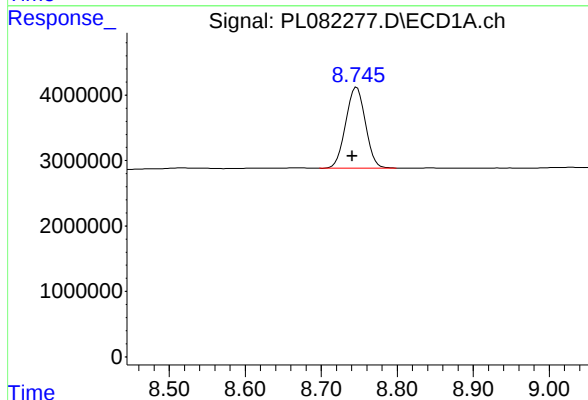

#28 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: 0.006 min
Response: 22377544
Conc: 11.72 ng/ml

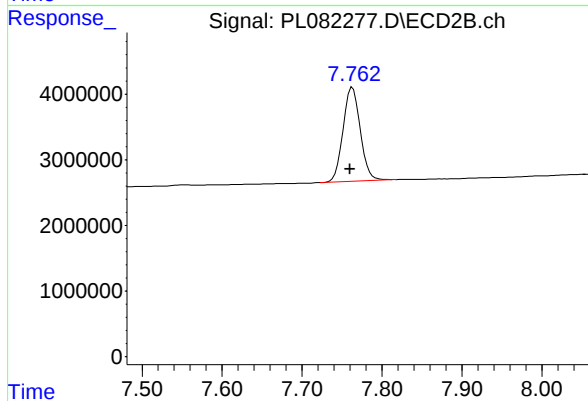

#28 Decachlorobiphenyl

R.T.: 7.763 min
Delta R.T.: 0.003 min
Response: 21431104
Conc: 9.39 ng/ml