

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
 Data File : PL082304.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2023 17:14
 Operator : AR\AJ
 Sample : 02423-12
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPE-1WC-23-04-18

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 22:41:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	2.649	49573746	39802769	18.559	17.181
28) SA Decachlor...	8.747	7.763	32289097	34121964	16.913	14.949

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
Data File : PL082304.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2023 17:14
Operator : AR\AJ
Sample : 02423-12
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPE-1WC-23-04-18

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 22:41:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

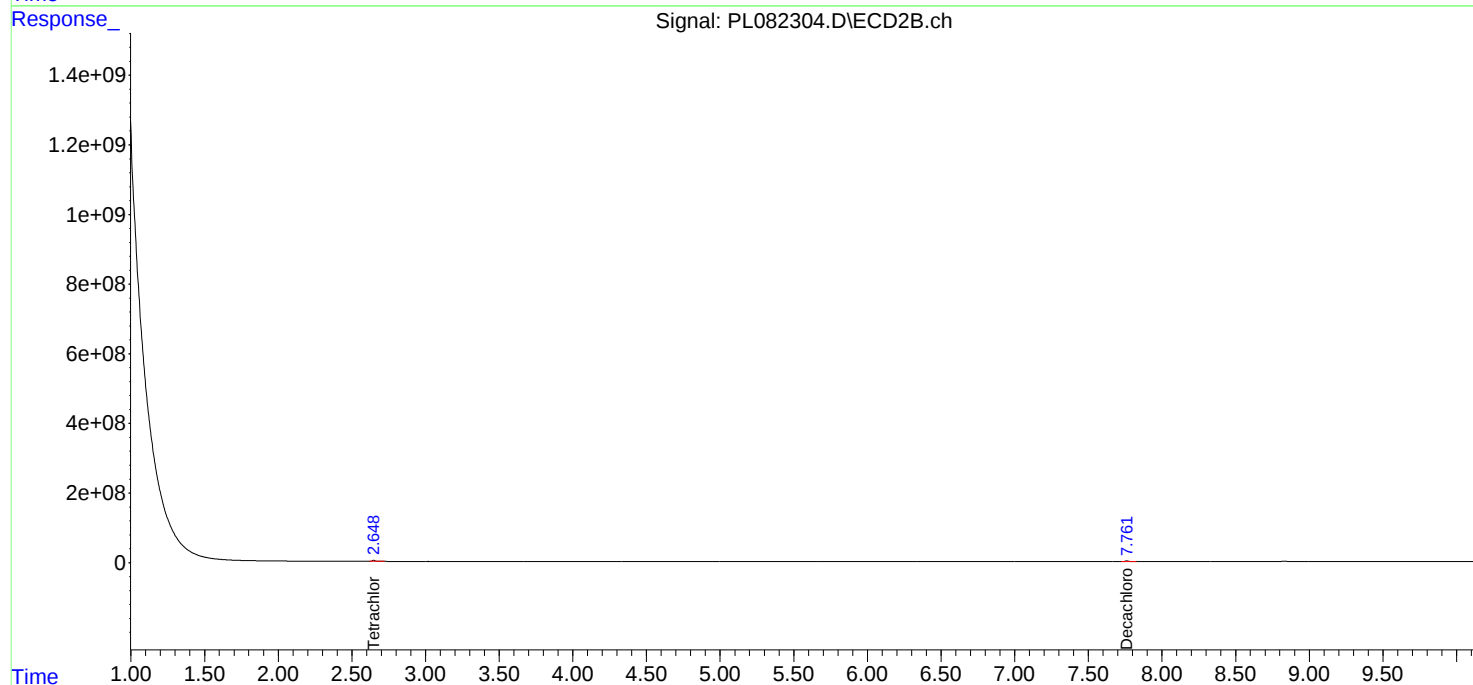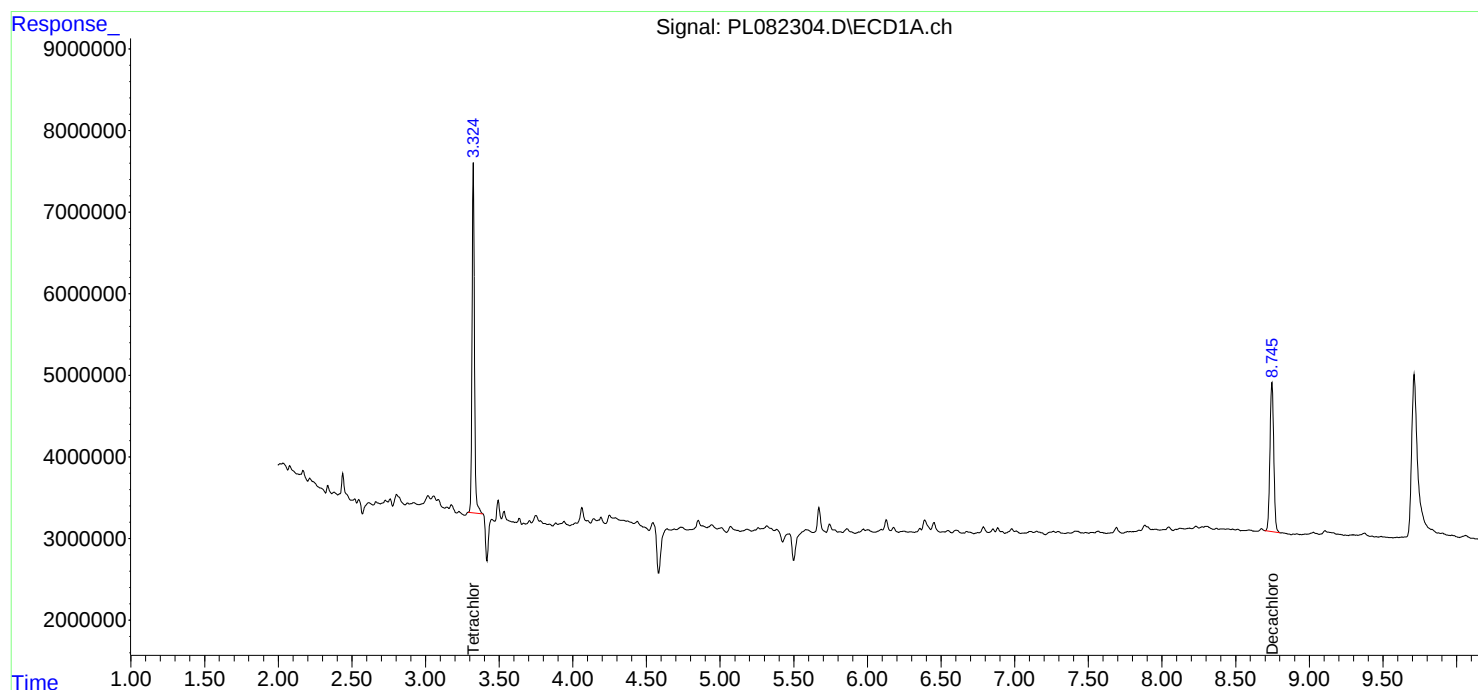


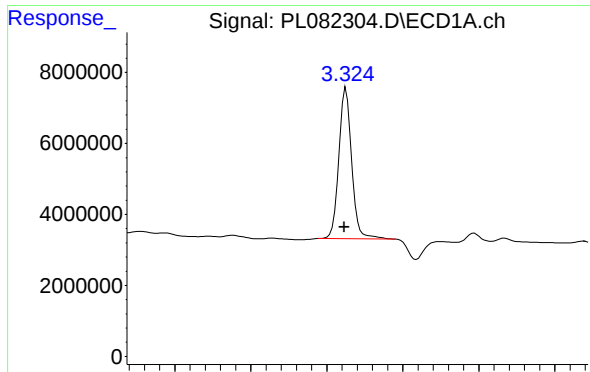

#1 Tetrachloro-m-xylene


R.T.: 3.325 min
Delta R.T.: 0.002 min
Response: 49573746
Conc: 18.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPE-1WC-23-04-18

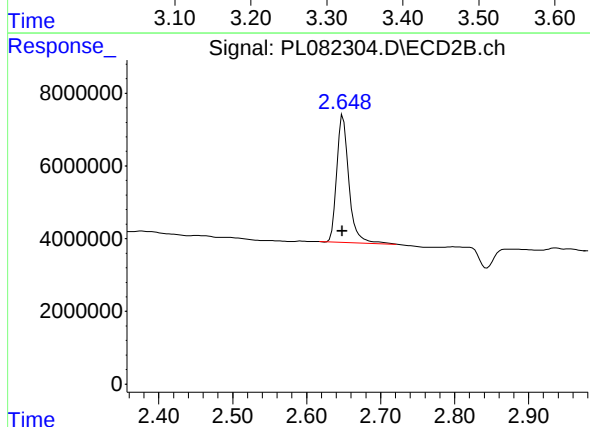


#1 Tetrachloro-m-xylene

R.T.: 2.649 min
Delta R.T.: 0.000 min
Response: 39802769
Conc: 17.18 ng/ml

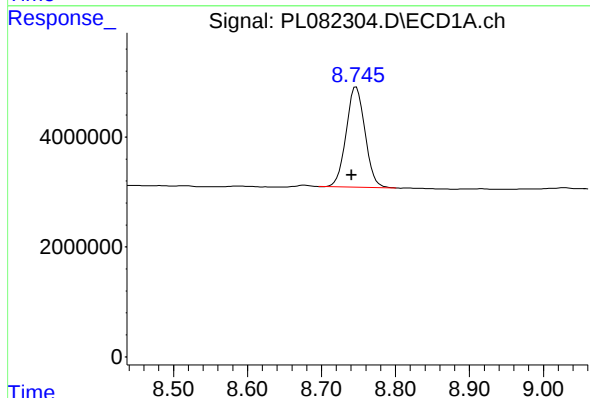

#28 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: 0.006 min
Response: 32289097
Conc: 16.91 ng/ml

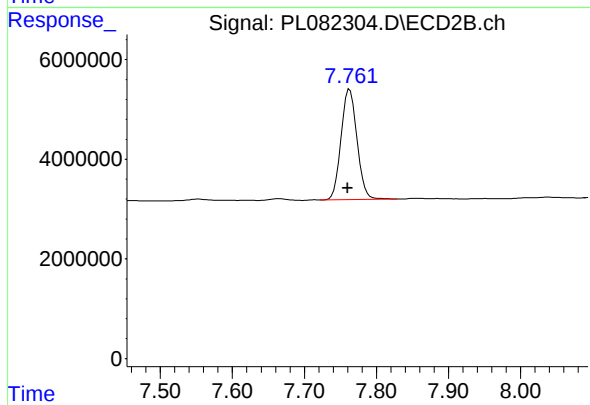

#28 Decachlorobiphenyl

R.T.: 7.763 min
Delta R.T.: 0.003 min
Response: 34121964
Conc: 14.95 ng/ml