

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
 Data File : PL082305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2023 17:28
 Operator : AR\AJ
 Sample : 02423-16
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPE-2WC-23-04-18

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 04/25/2023
 Supervised By :Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 24 22:41:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
 Quant Title : GC Extractables
 QLast Update : Fri Apr 21 03:12:31 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.325	2.650	46368677	37675416	17.359	16.262
28) SA Decachlor...	8.747	7.764	29720507	30266198	15.568m	13.260

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042423\
Data File : PL082305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2023 17:28
Operator : AR\AJ
Sample : 02423-16
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SPE-2WC-23-04-18


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 04/25/2023
Supervised By : Ankita Jodhani 04/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 24 22:41:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042023.M
Quant Title : GC Extractables
QLast Update : Fri Apr 21 03:12:31 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

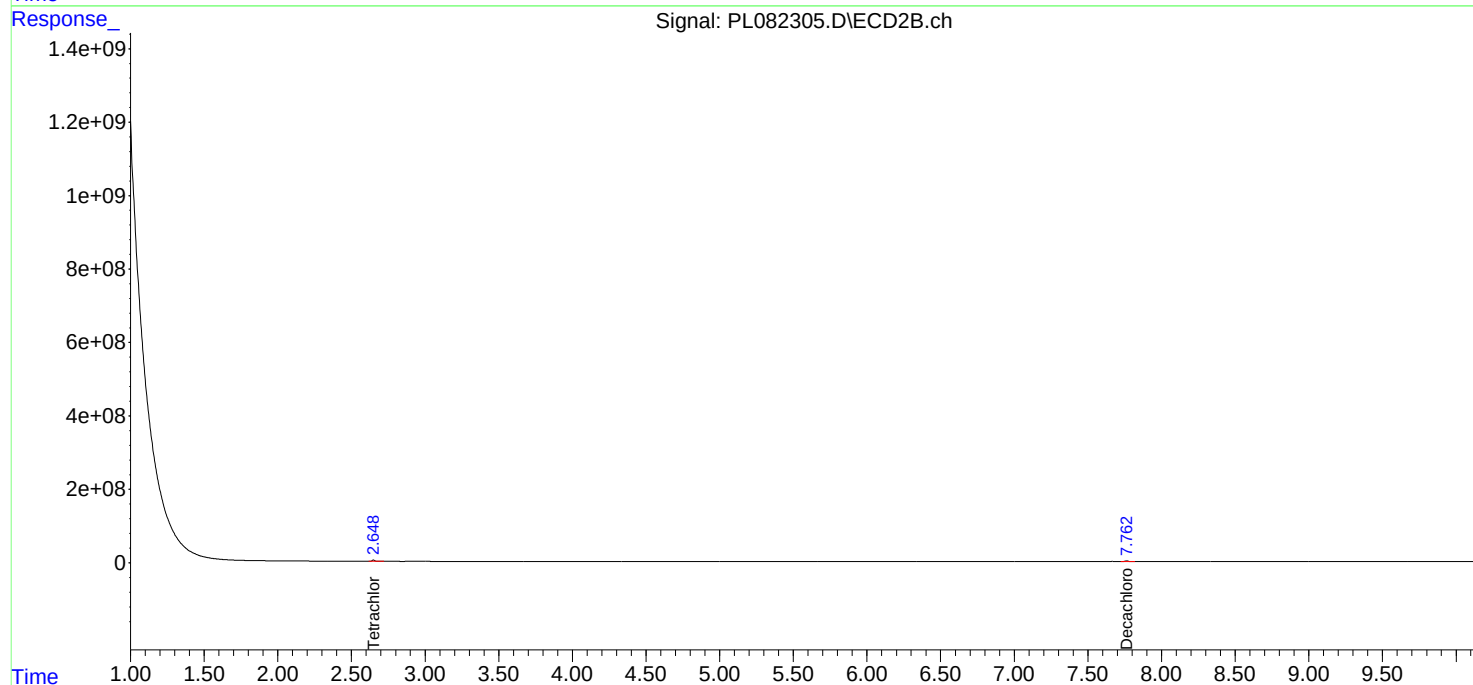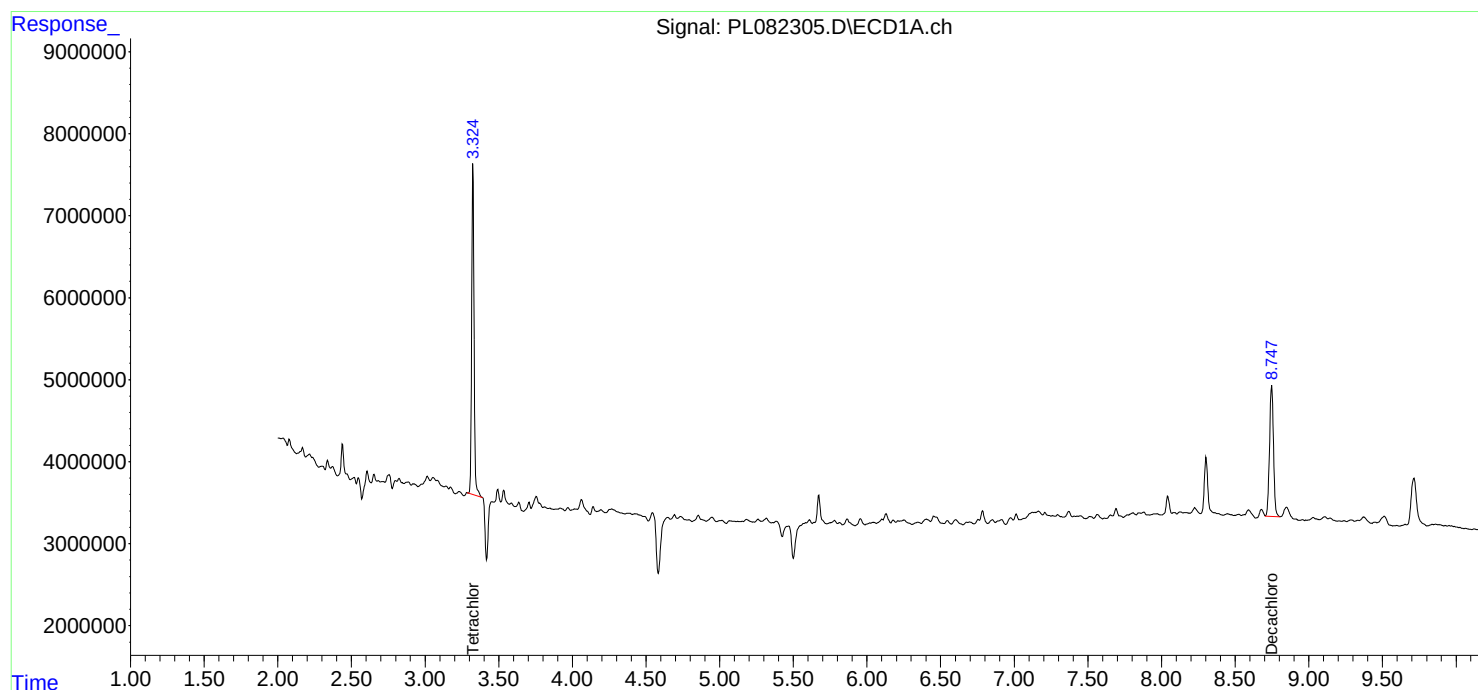

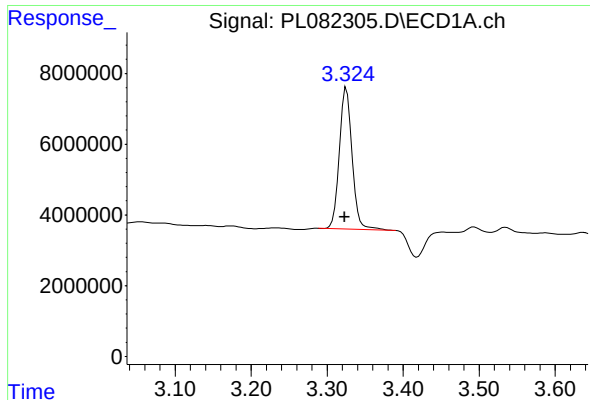


#1 Tetrachloro-m-xylene

R.T.: 3.325 min
Delta R.T.: 0.002 min
Response: 46368677
Conc: 17.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPE-2WC-23-04-18


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 04/25/2023
Supervised By :Ankita Jodhani 04/25/2023

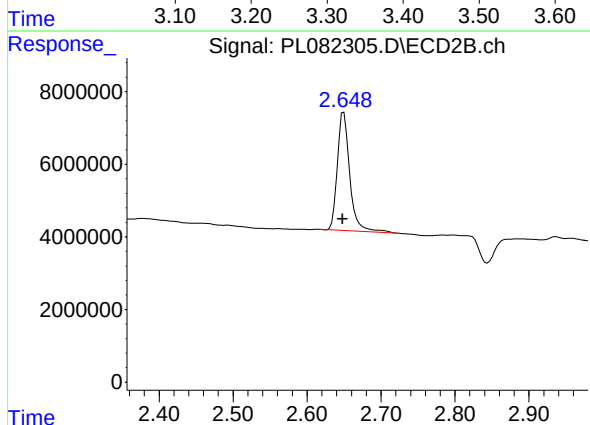


#1 Tetrachloro-m-xylene

R.T.: 2.650 min
Delta R.T.: 0.001 min
Response: 37675416
Conc: 16.26 ng/ml

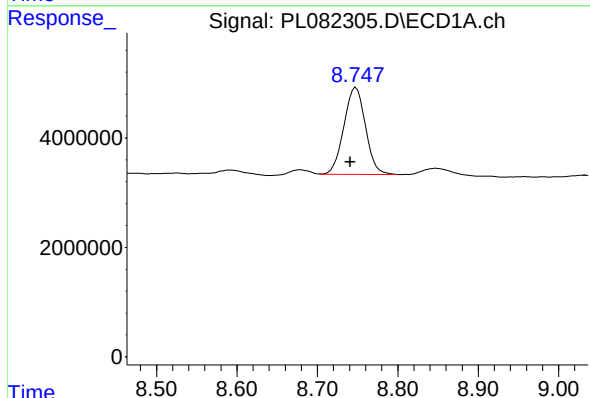

#28 Decachlorobiphenyl

R.T.: 8.747 min
Delta R.T.: 0.006 min
Response: 29720507
Conc: 15.57 ng/ml m

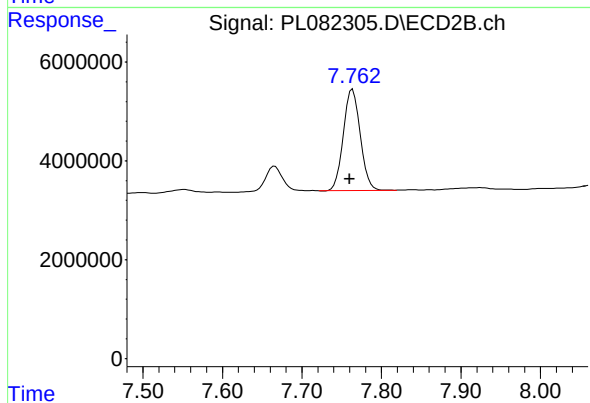

#28 Decachlorobiphenyl

R.T.: 7.764 min
Delta R.T.: 0.004 min
Response: 30266198
Conc: 13.26 ng/ml