

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042425\
 Data File : PL095360.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Apr 2025 09:08
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 25 01:42:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 23 16:23:18 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
8) B	Heptachlo...	5.739	0.000	66760683	0	16.669	N.D. #
10) B	gamma-Chl...	5.969f	0.000	73970519	0	18.133	N.D. #
13) MA	Dieldrin	0.000	5.559f	0	23991509	N.D.	5.899 #
14) MA	Endrin	0.000	5.812	0	4298696	N.D.	1.181 #
16) A	4,4'-DDD	6.749	0.000	75531574	0	26.681	N.D. #
25)	Chlordane-3	5.969f	0.000	73970519	0	94.965	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042425\
Data File : PL095360.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Apr 2025 09:08
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 25 01:42:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042325.M
Quant Title : GC Extractables
QLast Update : Wed Apr 23 16:23:18 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

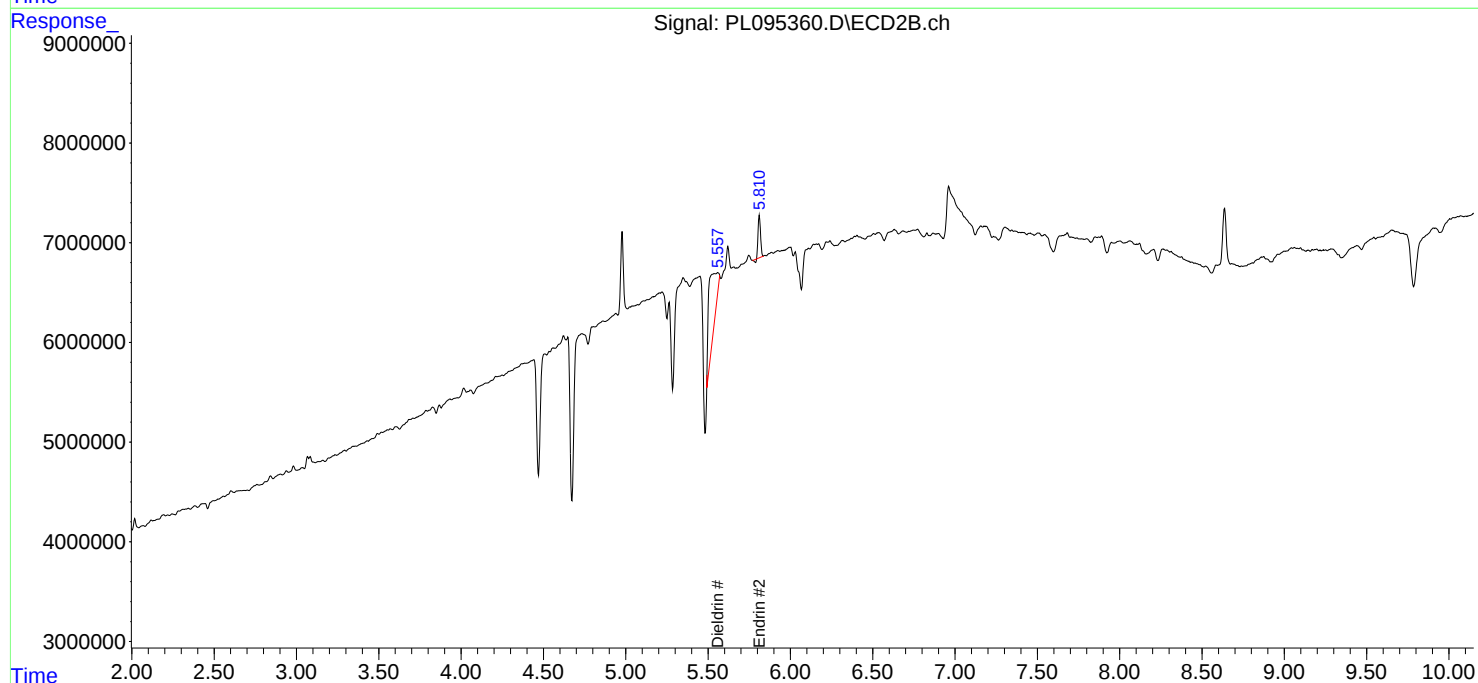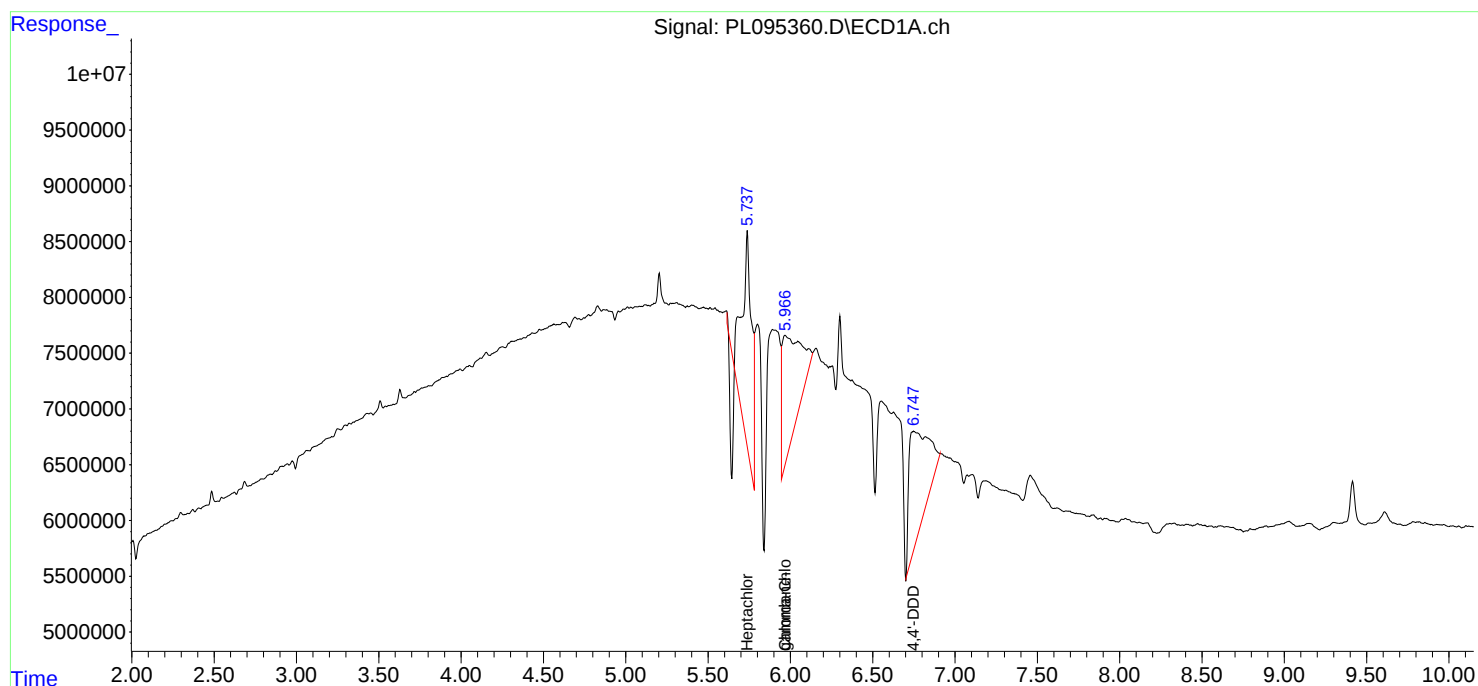


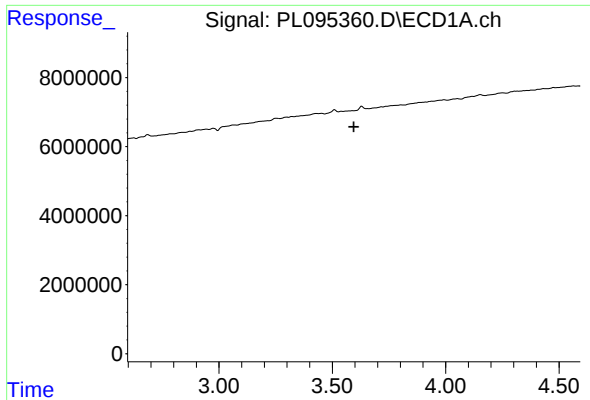

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

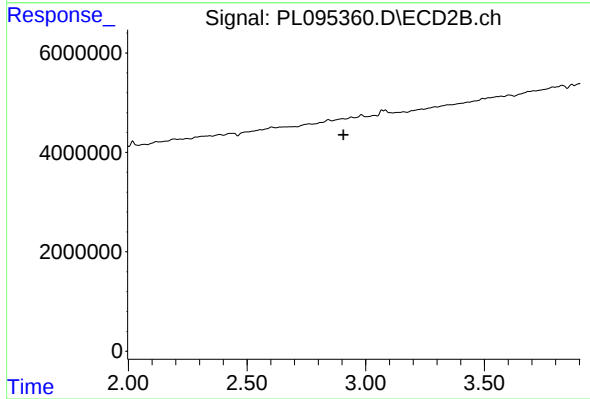


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.906 min
Response: 0
Conc: N.D.

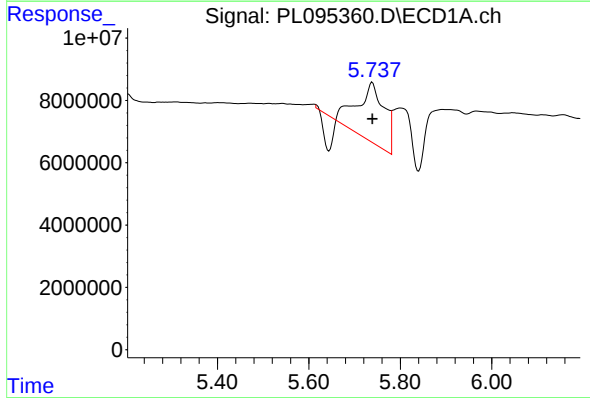


#8 Heptachlor epoxide

R.T.: 5.739 min
Delta R.T.: 0.000 min
Response: 66760683
Conc: 16.67 ng/ml

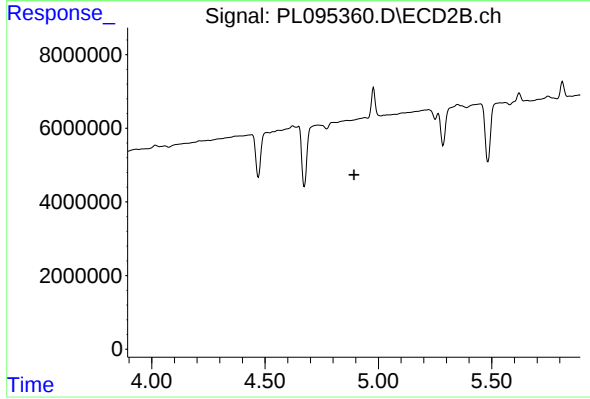

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.893 min
Response: 0
Conc: N.D.

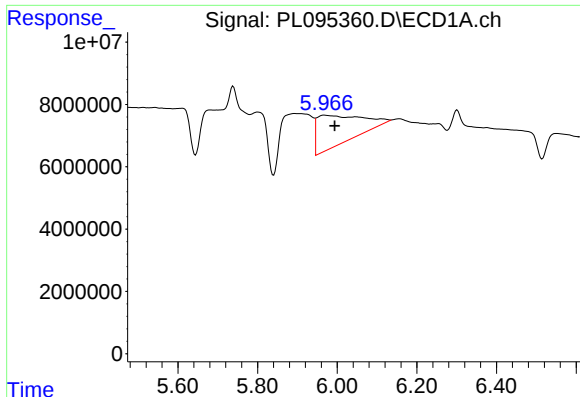

#10 gamma-Chlordane


R.T.: 5.969 min
Delta R.T.: -0.025 min
Response: 73970519
Conc: 18.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

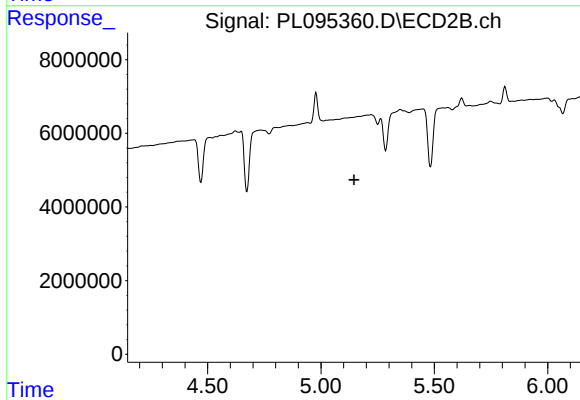


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

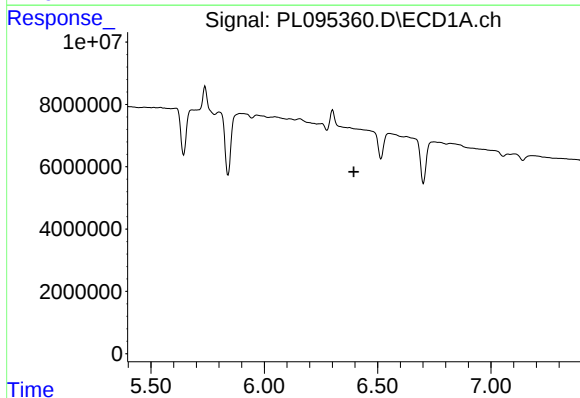


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

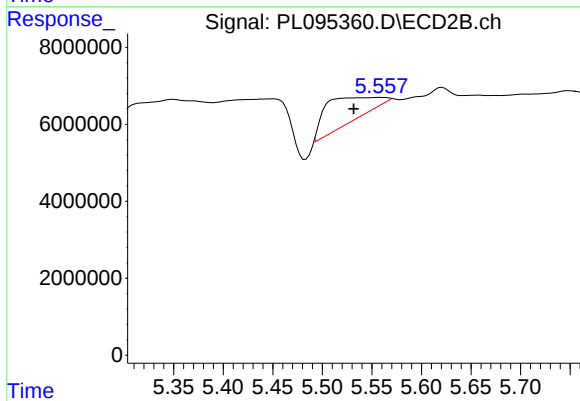

#13 Dieldrin


R.T.: 5.559 min
Delta R.T.: 0.028 min
Response: 23991509
Conc: 5.90 ng/ml

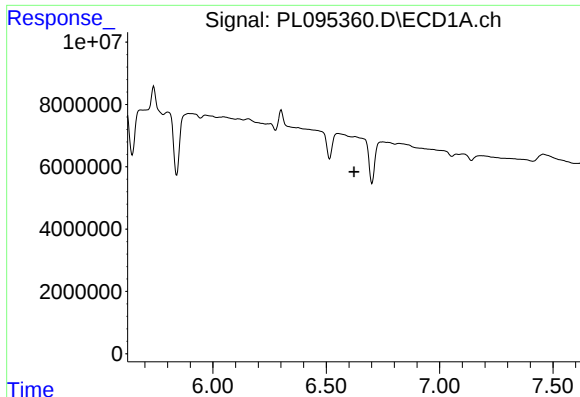

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.623 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

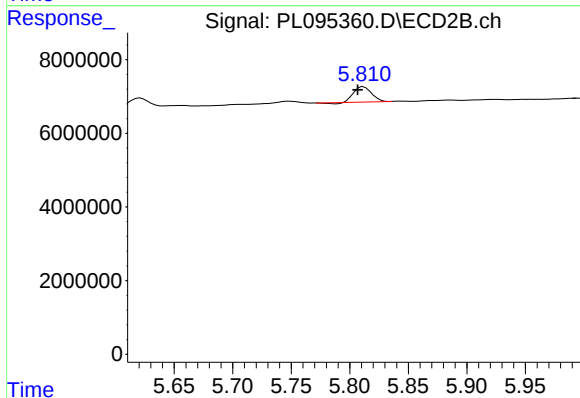


#14 Endrin

R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 4298696
Conc: 1.18 ng/ml

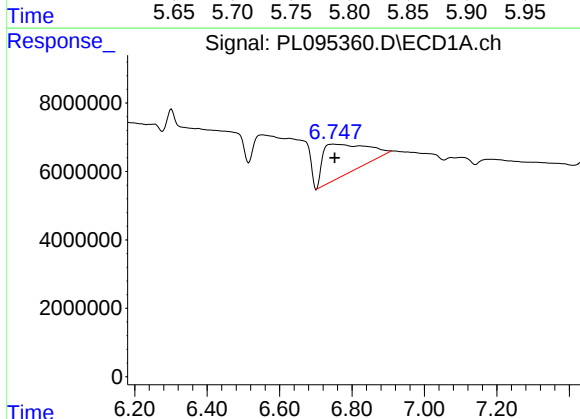


#16 4,4'-DDD

R.T.: 6.749 min
Delta R.T.: -0.004 min
Response: 75531574
Conc: 26.68 ng/ml

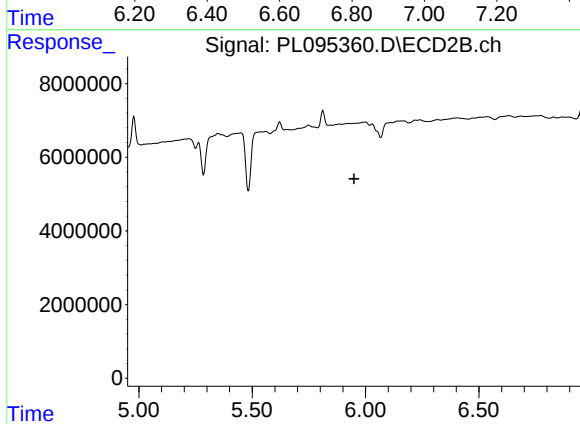

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

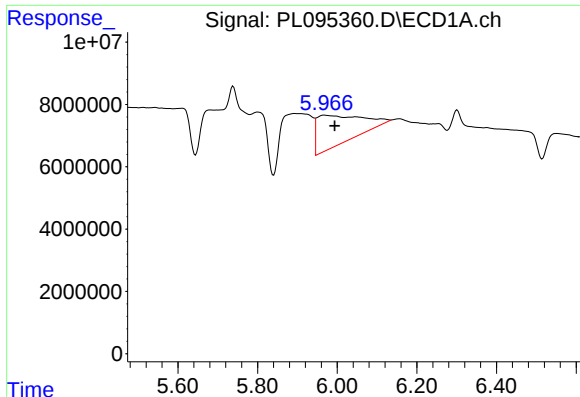

#25 Chlordane-3


R.T.: 5.969 min
Delta R.T.: -0.025 min
Response: 73970519
Conc: 94.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

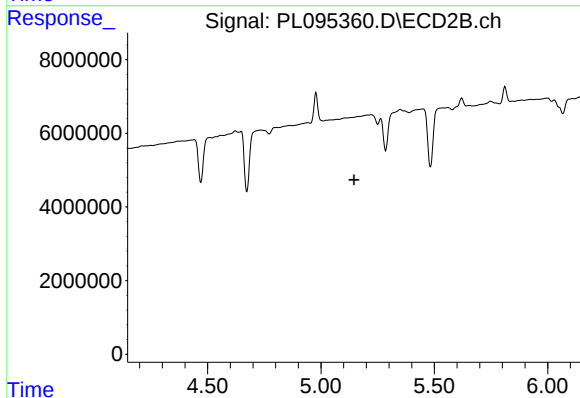


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.147 min
Response: 0
Conc: N.D.

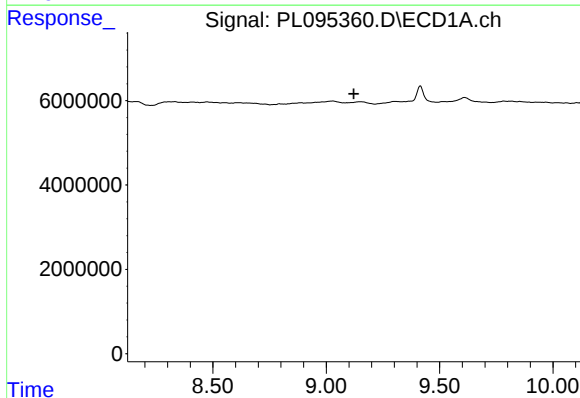

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.122 min
Response: 0
Conc: N.D.

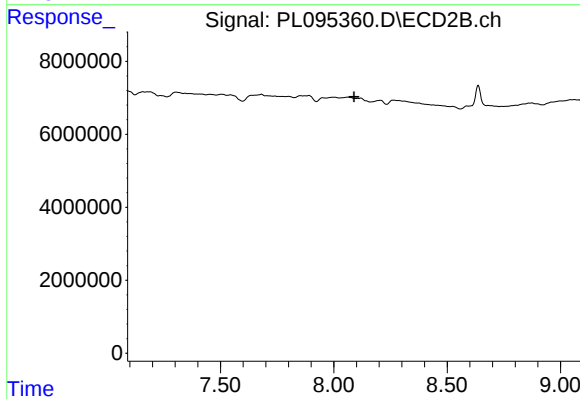

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.089 min
Response: 0
Conc: N.D.