

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 16:19
 Operator : AJ\SJ
 Sample : K2533-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:46:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	173.9E6	43274351	18.807	18.127
28)	SA Decachlor...	8.002	8.982	99119536	29376112	8.854	10.291
Target Compounds							
10)	B gamma-Chl...	5.239f	6.034	41008094	7003907	3.080	2.314
11)	B alpha-Chl...	0.000	6.116	0	8287697	N.D.	2.739 #
12)	B 4,4'-DDE	5.442	6.273	33895731	8763917	2.725	3.174
13)	MA Dieldrin	5.564	6.419	23488465	1252075	1.809	0.428 #
14)	MA Endrin	5.828	0.000	9670985	0	0.814	N.D. #
15)	B Endosulfa...	6.111f	6.866f	9143942	1504496	0.817	0.573 #
17)	MA 4,4'-DDT	6.187	7.061	24182060	7125910	2.426	2.991
19)	B Endosulfa...	6.458	7.195	6930267	2313696	0.622	0.845 #
25)	Chlordane-3	0.000	6.116	0	8287697	N.D.	27.978 #
27)	Chlordane-5	6.111	0.000	9143942	0	21.567	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 16:19
Operator : AJ\SJ
Sample : K2533-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:46:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

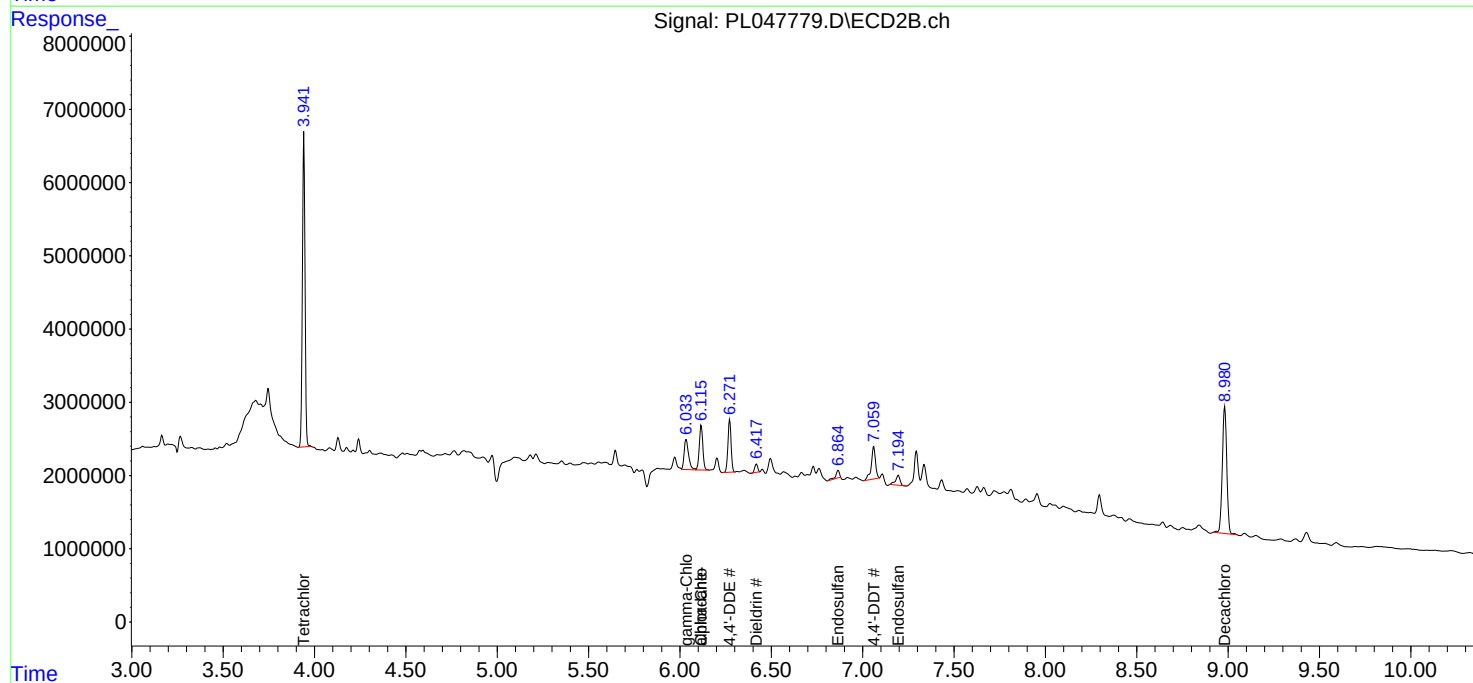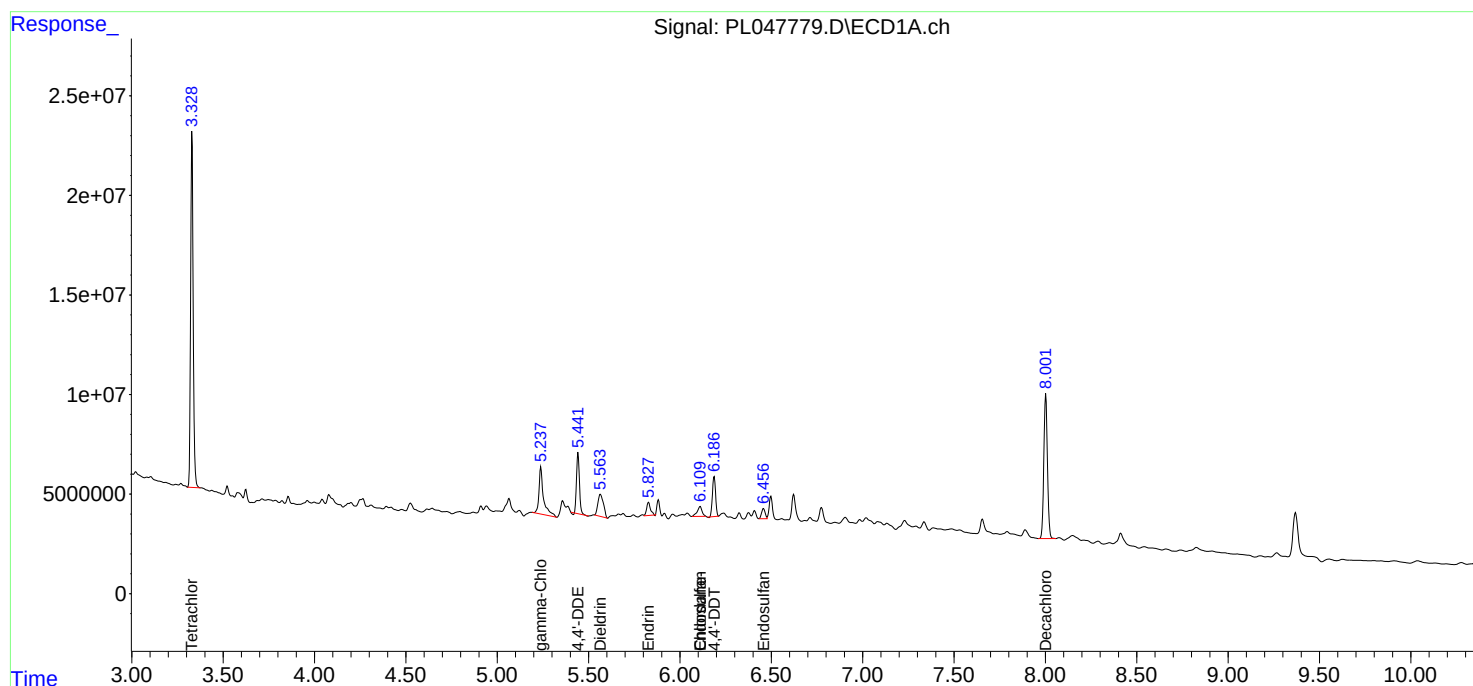


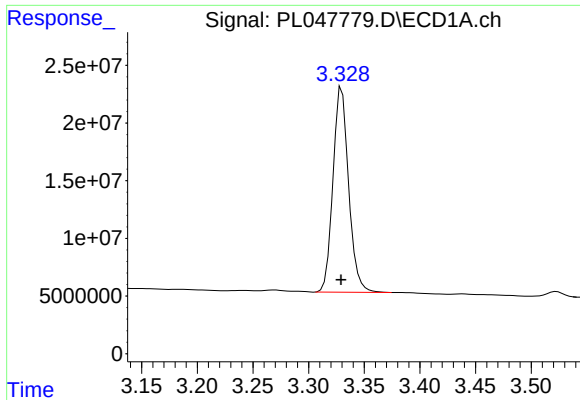

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 173928952
Conc: 18.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

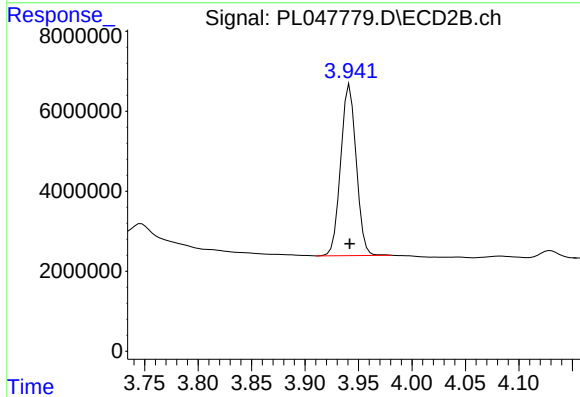


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 43274351
Conc: 18.13 ng/ml

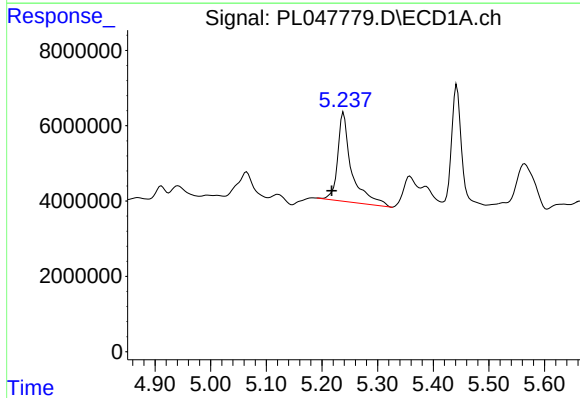


#10 gamma-Chlordane

R.T.: 5.239 min
Delta R.T.: 0.021 min
Response: 41008094
Conc: 3.08 ng/ml

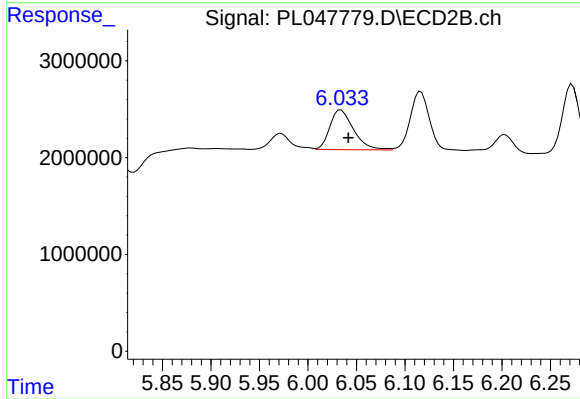

#10 gamma-Chlordane


R.T.: 6.034 min
Delta R.T.: -0.008 min
Response: 7003907
Conc: 2.31 ng/ml

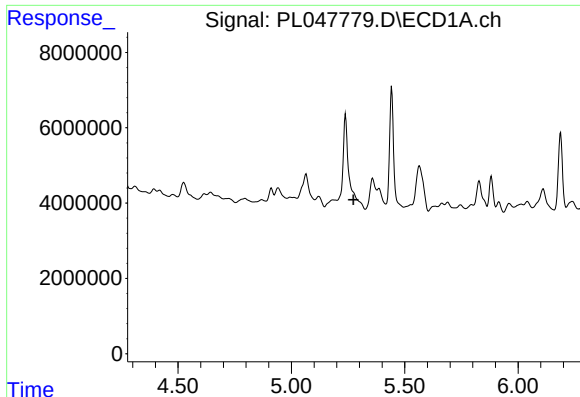

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

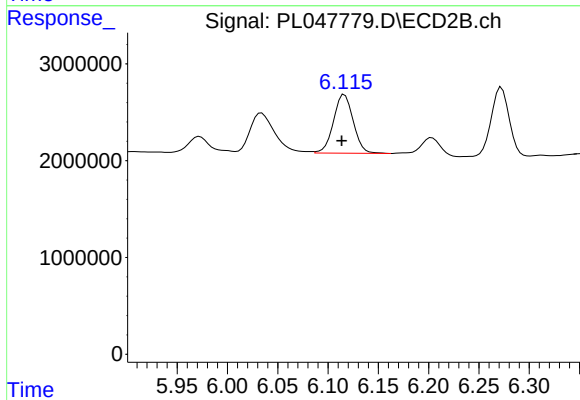


#11 alpha-Chlordane

R.T.: 6.116 min
Delta R.T.: 0.003 min
Response: 8287697
Conc: 2.74 ng/ml

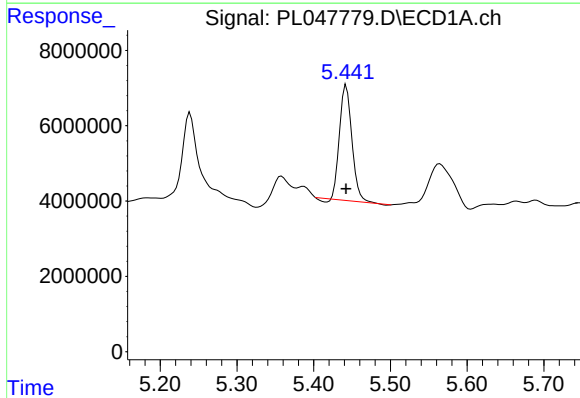


#12 4,4'-DDE

R.T.: 5.442 min
Delta R.T.: 0.000 min
Response: 33895731
Conc: 2.72 ng/ml

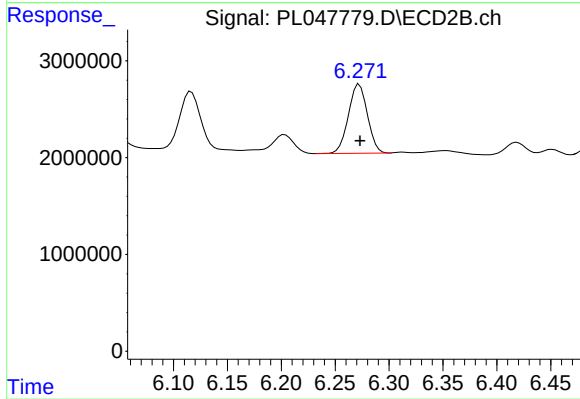

#12 4,4'-DDE


R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 8763917
Conc: 3.17 ng/ml

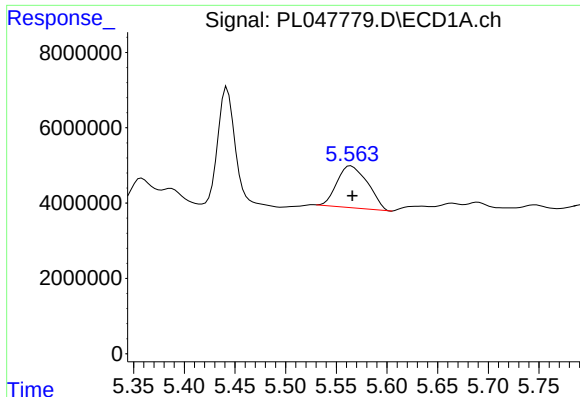

#13 Dieldrin


R.T.: 5.564 min
Delta R.T.: -0.001 min
Response: 23488465
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

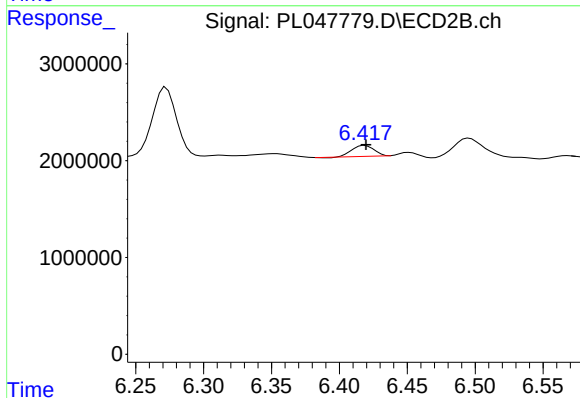


#13 Dieldrin

R.T.: 6.419 min
Delta R.T.: -0.001 min
Response: 1252075
Conc: 0.43 ng/ml

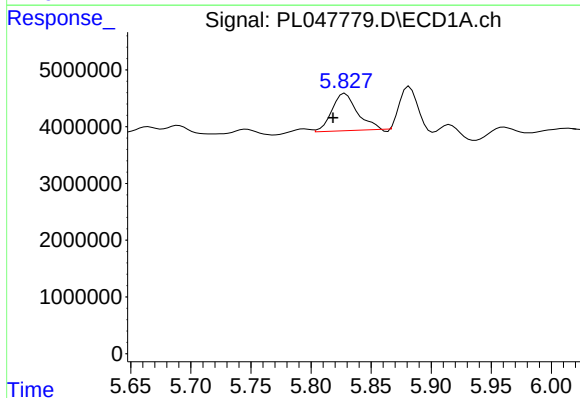


#14 Endrin

R.T.: 5.828 min
Delta R.T.: 0.010 min
Response: 9670985
Conc: 0.81 ng/ml

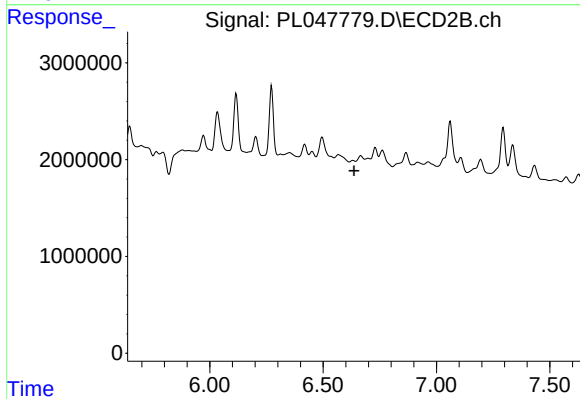

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.637 min
Response: 0
Conc: N.D.

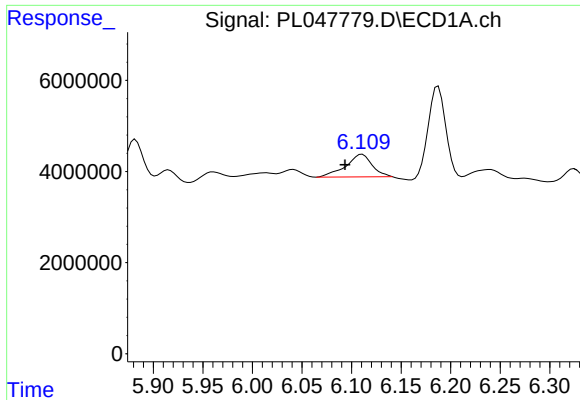

#15 Endosulfan II


R.T.: 6.111 min
Delta R.T.: 0.017 min
Response: 9143942
Conc: 0.82 ng/ml

Instrument :
ECD_L
ClientSampleId :

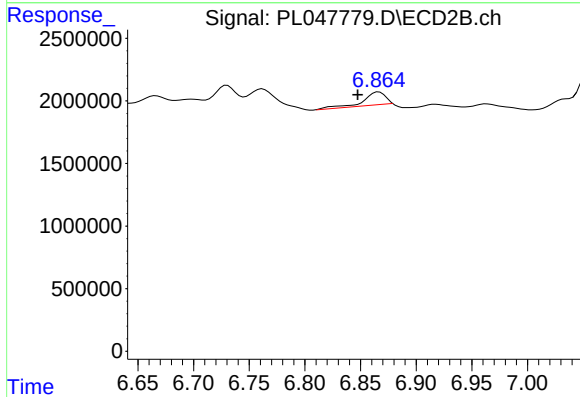


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.019 min
Response: 1504496
Conc: 0.57 ng/ml

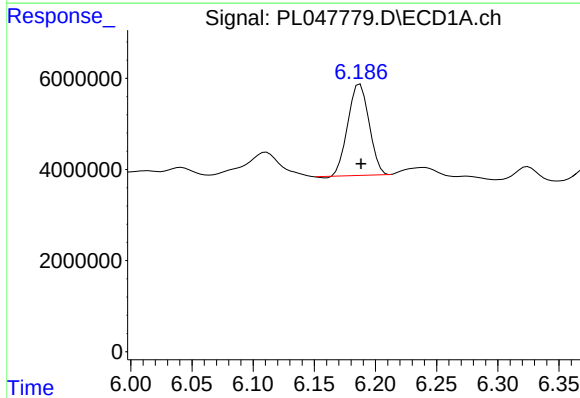


#17 4,4'-DDT

R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 24182060
Conc: 2.43 ng/ml

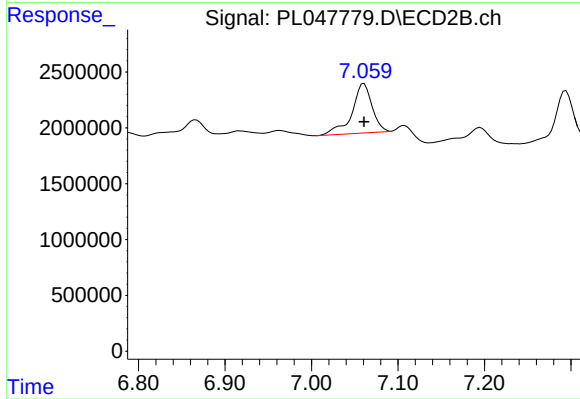

#17 4,4'-DDT


R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 7125910
Conc: 2.99 ng/ml

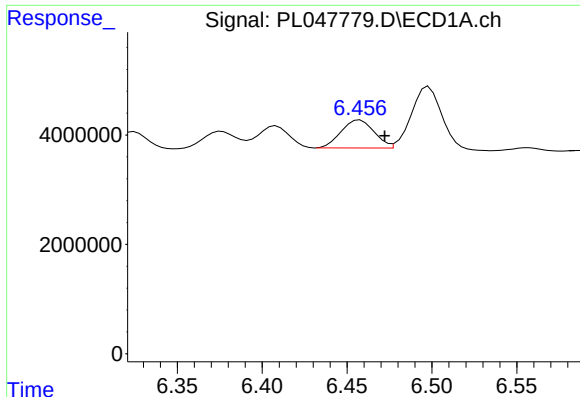

#19 Endosulfan Sulfate


R.T.: 6.458 min
Delta R.T.: -0.015 min
Response: 6930267
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

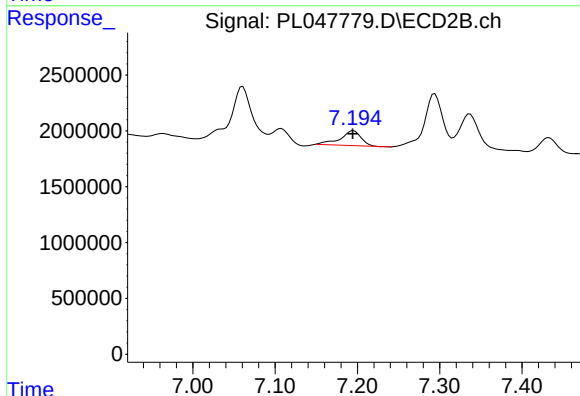


#19 Endosulfan Sulfate

R.T.: 7.195 min
Delta R.T.: 0.000 min
Response: 2313696
Conc: 0.84 ng/ml

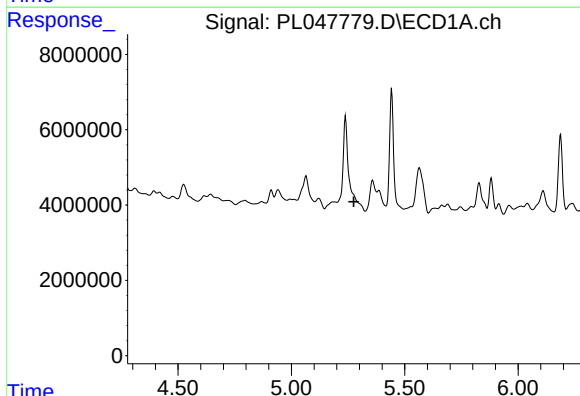


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.276 min
Response: 0
Conc: N.D.

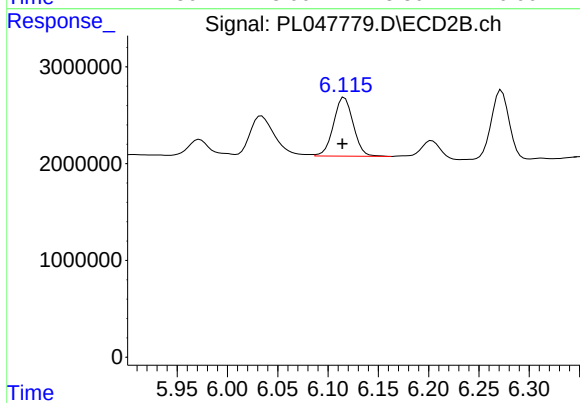

#25 Chlordane-3


R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 8287697
Conc: 27.98 ng/ml

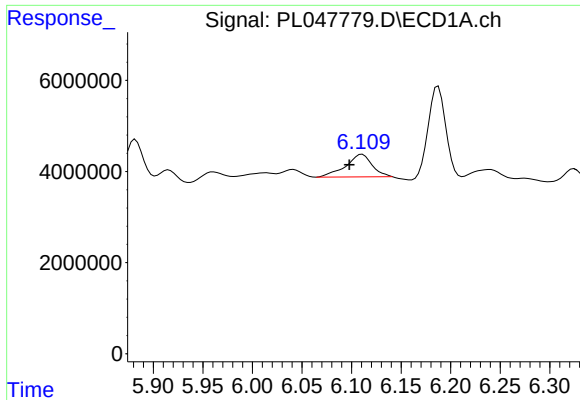

#27 Chlordane-5


R.T.: 6.111 min
Delta R.T.: 0.013 min
Response: 9143942
Conc: 21.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

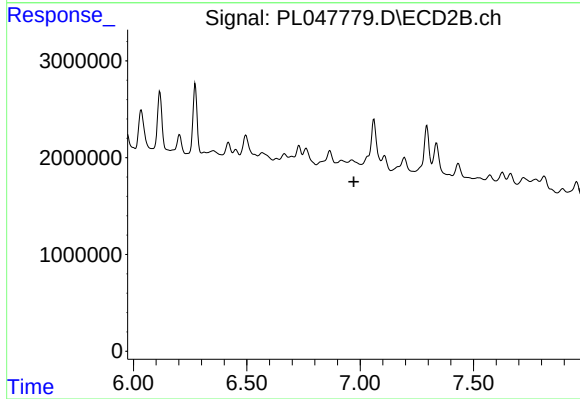


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.972 min
Response: 0
Conc: N.D.

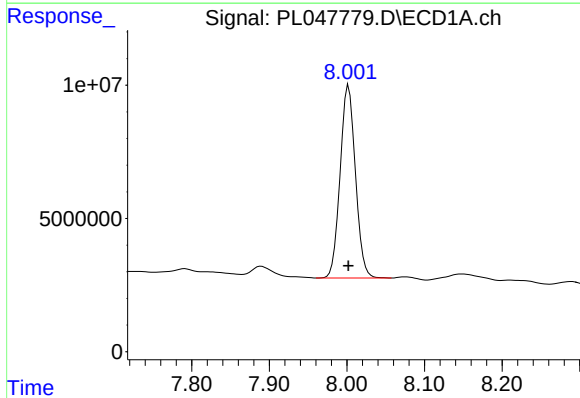

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 99119536
Conc: 8.85 ng/ml

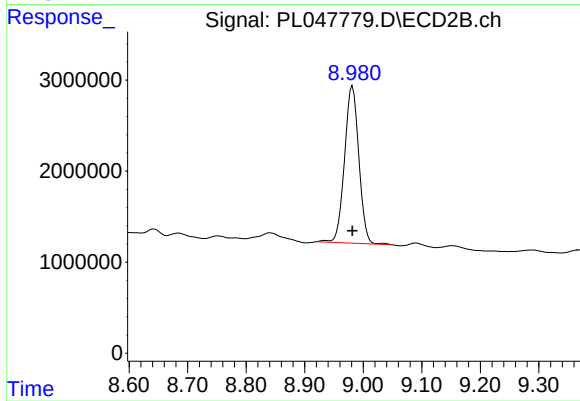

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 29376112
Conc: 10.29 ng/ml