

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047800.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2019 21:35
 Operator : AJ\SJ
 Sample : K2568-03
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:50:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	137.6E6	35717171	14.882	14.962
28)	SA Decachlor...	8.002	8.981	156.1E6	40656590	13.948	14.243
Target Compounds							
10)	B gamma-Chl...	5.240f	0.000	6634849	0	0.498	N.D. #
11)	B alpha-Chl...	0.000	6.116	0	2273310	N.D.	0.751 #
12)	B 4,4'-DDE	5.443	6.273	163.9E6	36150135	13.175	13.091
14)	MA Endrin	5.825	6.666f	6208691	1315017	0.522	0.515
16)	A 4,4'-DDD	0.000	6.767	0	3306424	N.D.	1.473 #
17)	MA 4,4'-DDT	6.187	7.060	64748665	18571320	6.494	7.796
20)	A Methoxychlor	6.712f	0.000	7877842	0	1.481	N.D. #
25)	Chlordane-3	0.000	6.116	0	2273310	N.D.	7.674 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047800.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2019 21:35
Operator : AJ\SJ
Sample : K2568-03
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:50:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

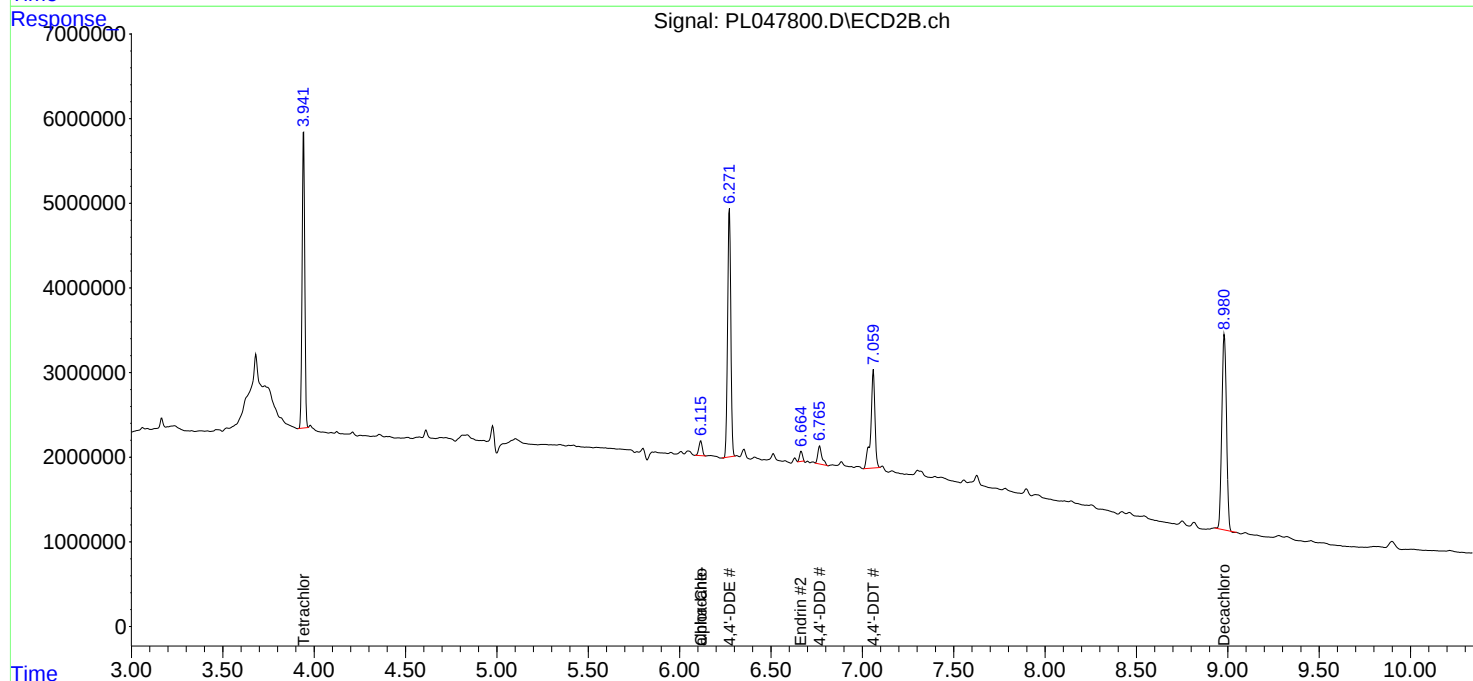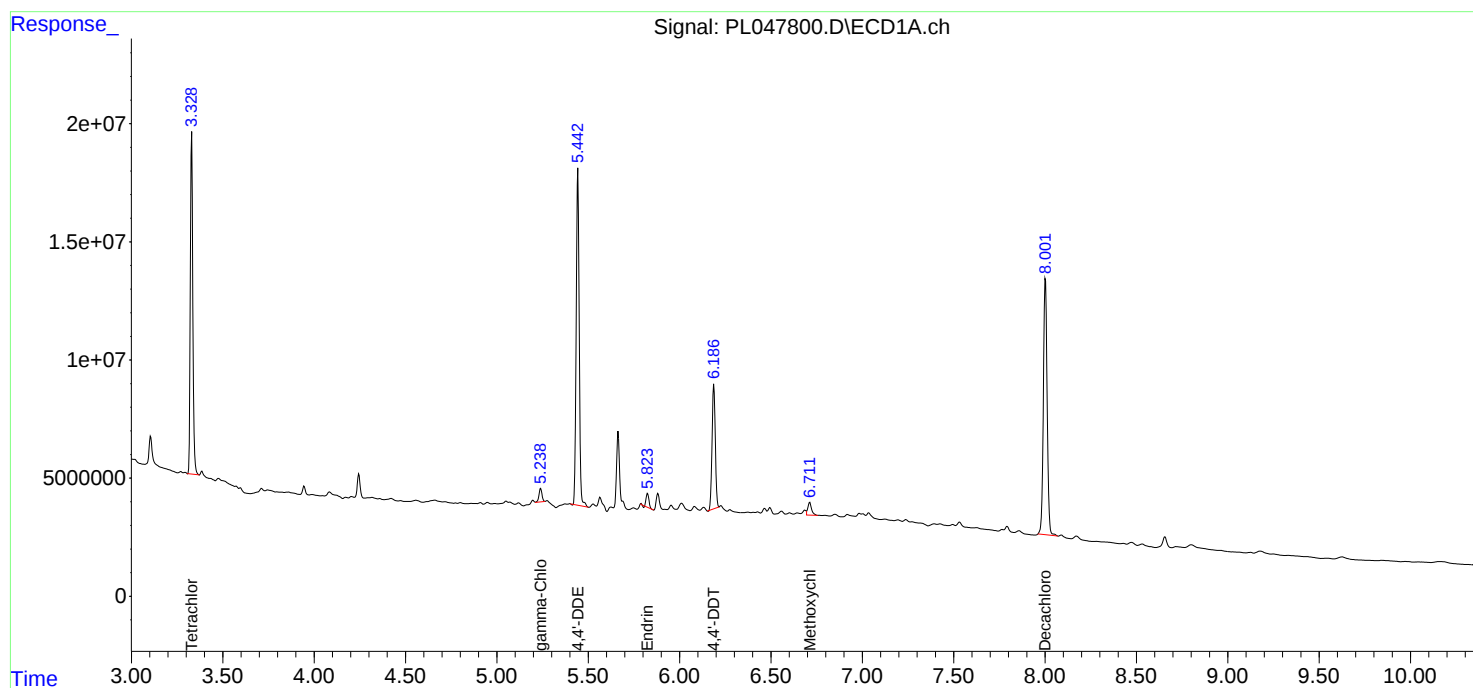


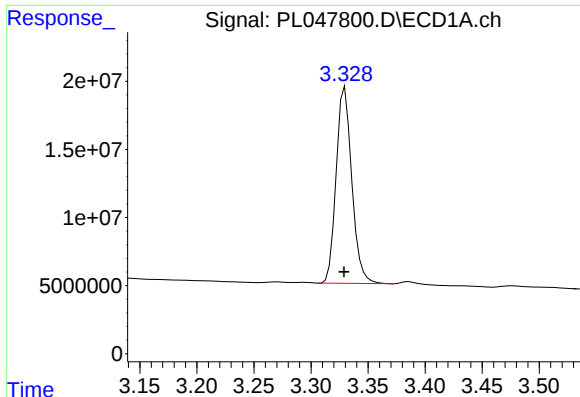

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 137631186
Conc: 14.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

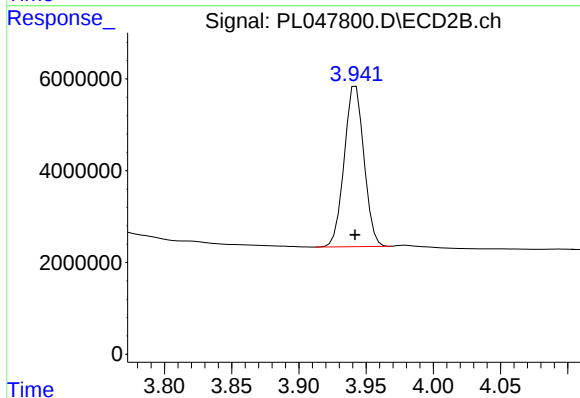


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 35717171
Conc: 14.96 ng/ml

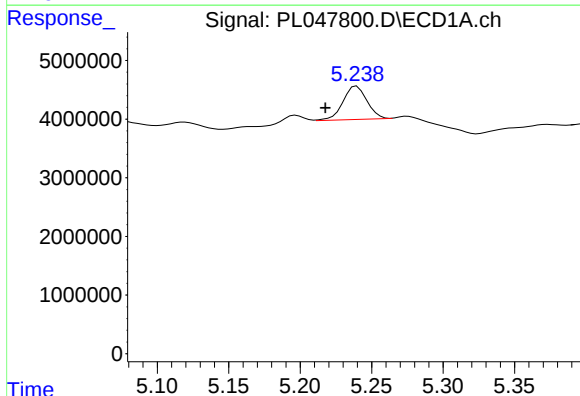


#10 gamma-Chlordane

R.T.: 5.240 min
Delta R.T.: 0.022 min
Response: 6634849
Conc: 0.50 ng/ml

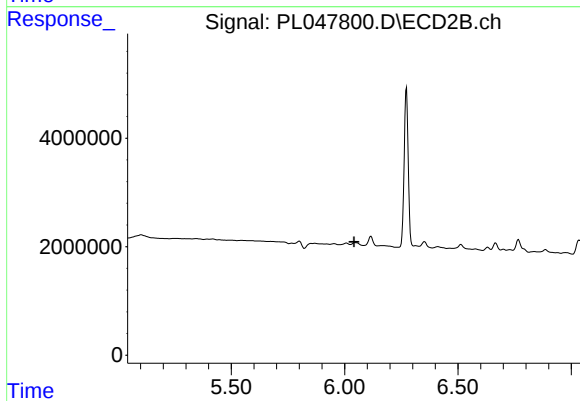

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.042 min
Response: 0
Conc: N.D.

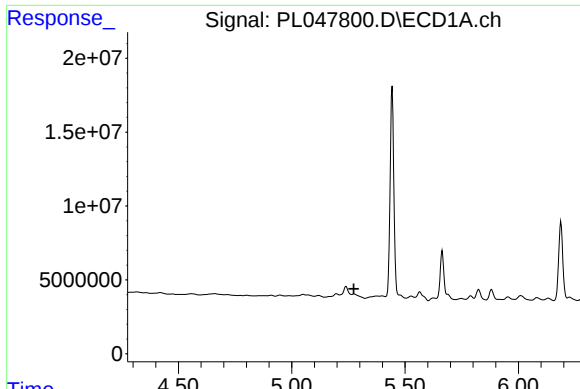

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

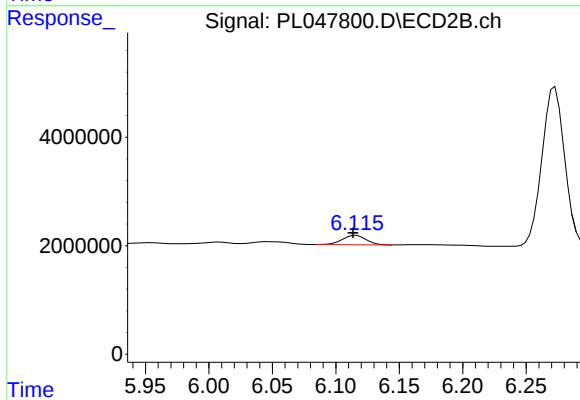


#11 alpha-Chlordane

R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 2273310
Conc: 0.75 ng/ml

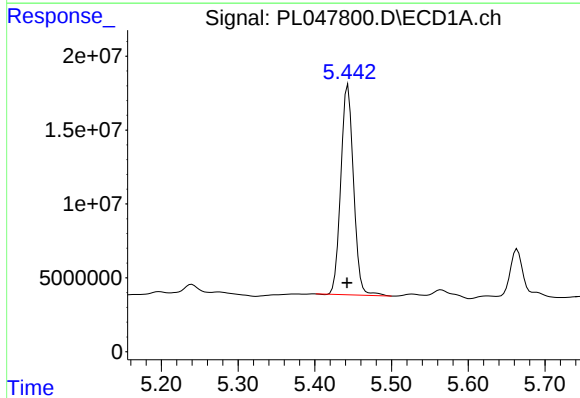


#12 4,4'-DDE

R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 163883964
Conc: 13.18 ng/ml

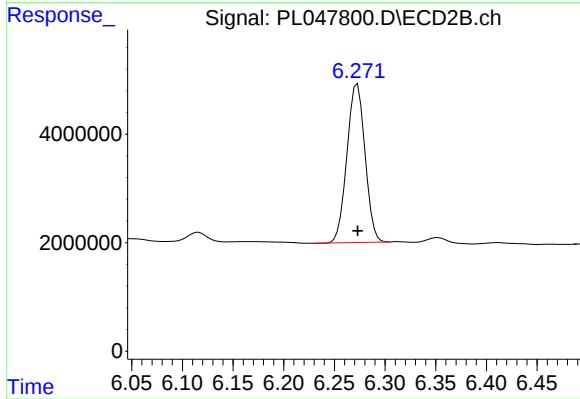

#12 4,4'-DDE


R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 36150135
Conc: 13.09 ng/ml

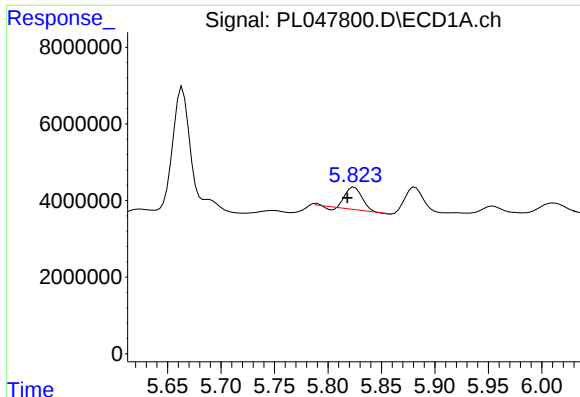

#14 Endrin


R.T.: 5.825 min
Delta R.T.: 0.006 min
Response: 6208691
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

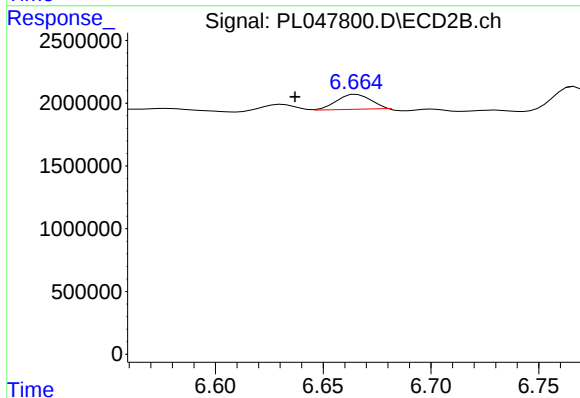


#14 Endrin

R.T.: 6.666 min
Delta R.T.: 0.029 min
Response: 1315017
Conc: 0.51 ng/ml

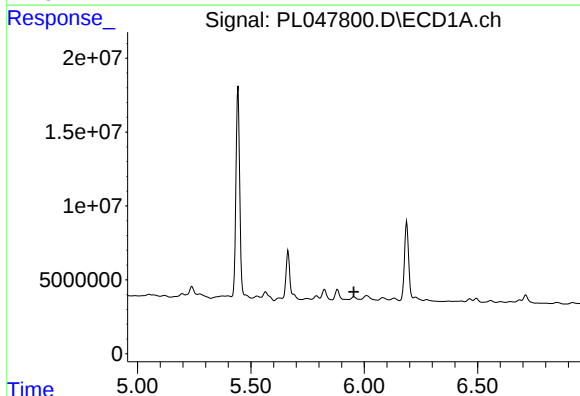


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

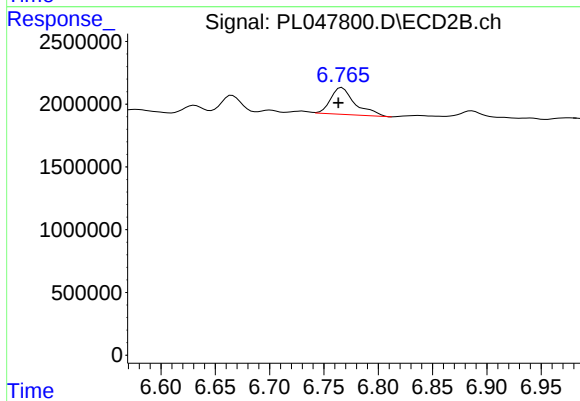

#16 4,4'-DDD


R.T.: 6.767 min
Delta R.T.: 0.003 min
Response: 3306424
Conc: 1.47 ng/ml

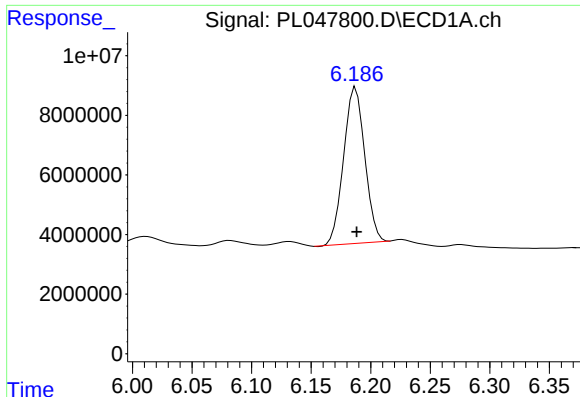

#17 4,4'-DDT


R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 64748665
Conc: 6.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

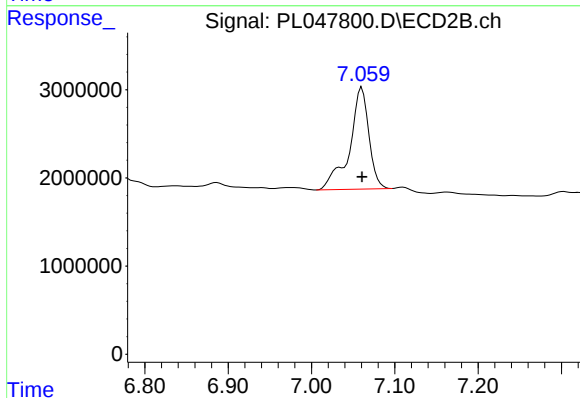


#17 4,4'-DDT

R.T.: 7.060 min
Delta R.T.: 0.000 min
Response: 18571320
Conc: 7.80 ng/ml

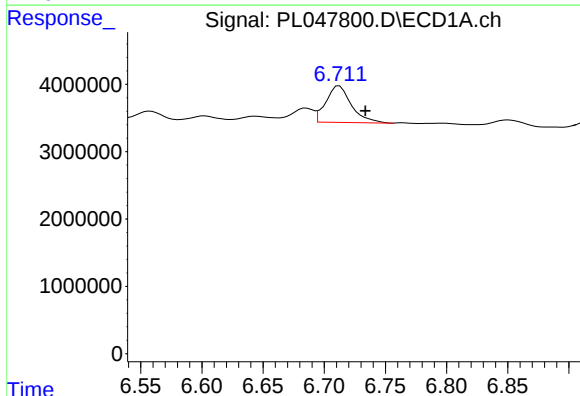


#20 Methoxychlor

R.T.: 6.712 min
Delta R.T.: -0.021 min
Response: 7877842
Conc: 1.48 ng/ml

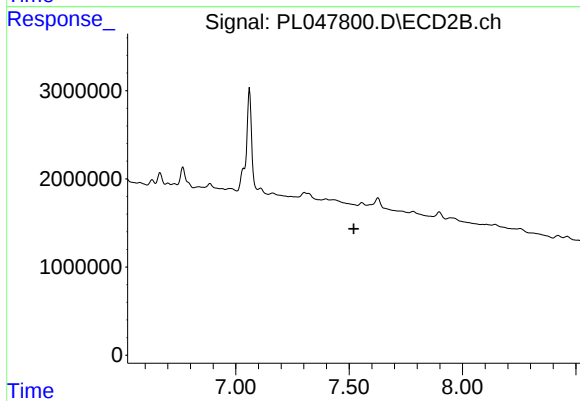

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.521 min
Response: 0
Conc: N.D.

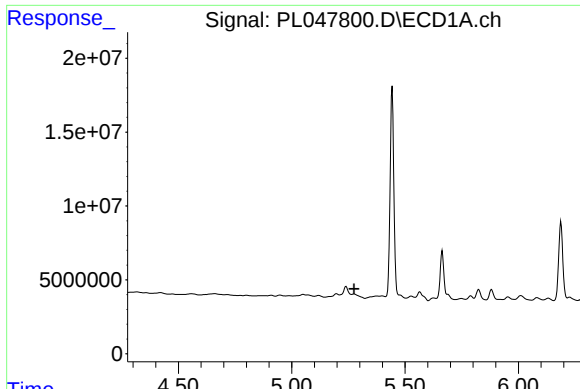

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

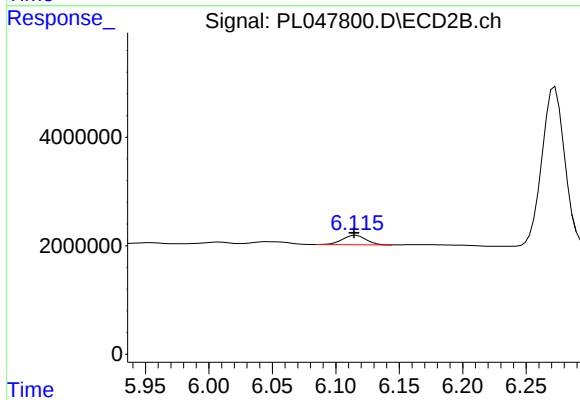


#25 Chlordane-3

R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 2273310
Conc: 7.67 ng/ml

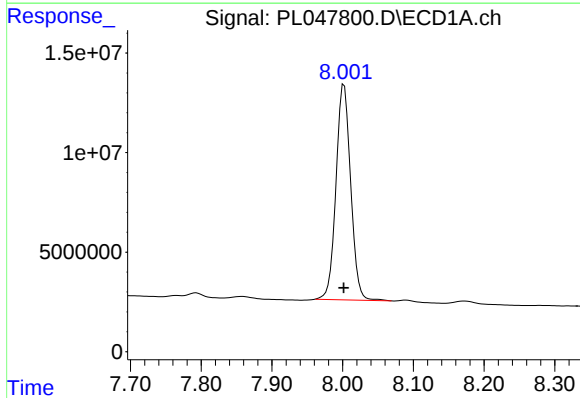

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 156139960
Conc: 13.95 ng/ml

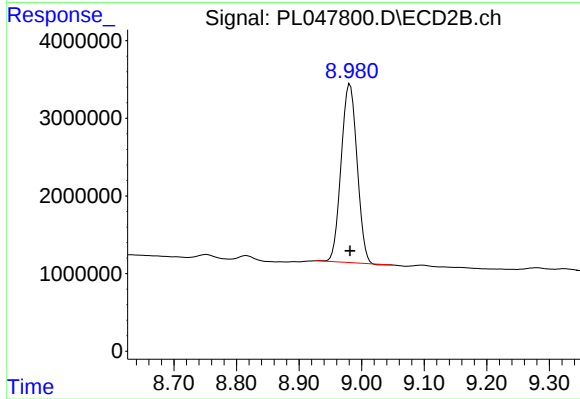

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: 0.000 min
Response: 40656590
Conc: 14.24 ng/ml