

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047817.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 02:37
 Operator : AJ\SJ
 Sample : K2553-04
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:53:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	201.9E6	49787616	21.827	20.856
28)	SA Decachlor...	8.002	8.982	169.7E6	47745816	15.157	16.726
Target Compounds							
3)	MA gamma-BHC...	4.043	0.000	4468752	0	0.337	N.D. #
6)	B beta-BHC	0.000	4.814f	0	2768683	N.D.	1.922 #
10)	B gamma-Chl...	0.000	6.031	0	6857904	N.D.	2.266 #
13)	MA Dieldrin	5.557	0.000	27380361	0	2.109	N.D. #
15)	B Endosulfa...	0.000	6.867f	0	1813905	N.D.	0.691 #
23)	Chlordane-1	4.184	5.031f	7765613	-2023898	17.961	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047817.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 02:37
Operator : AJ\SJ
Sample : K2553-04
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:53:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

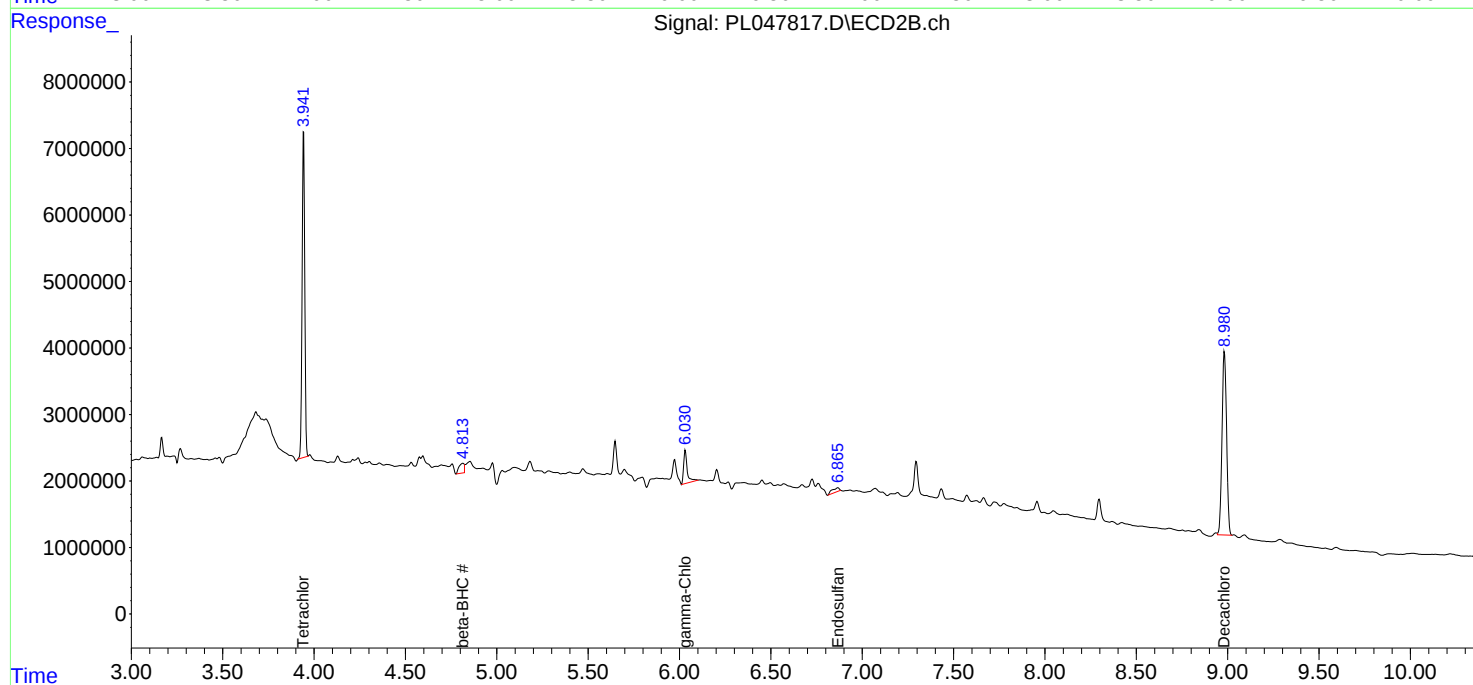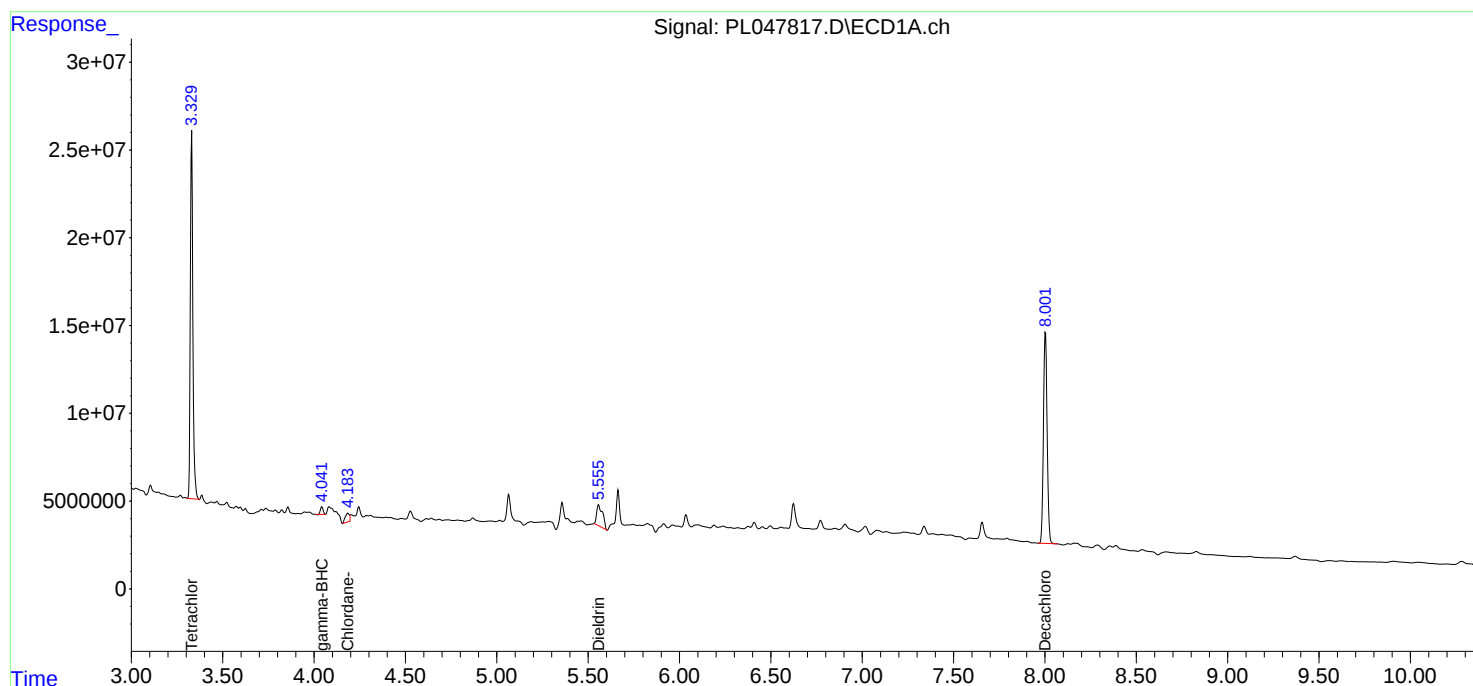


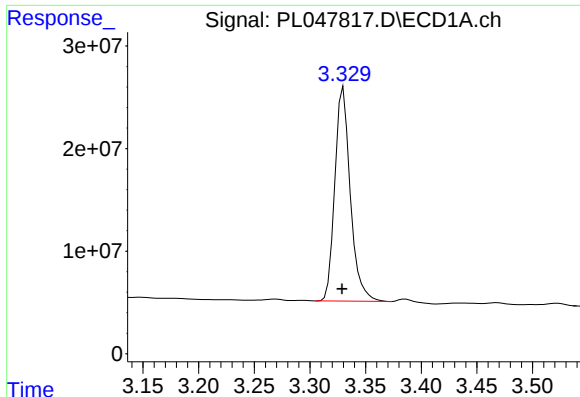

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 201858557
Conc: 21.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

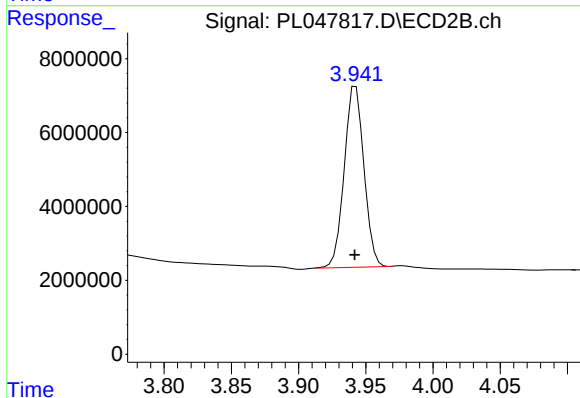


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 49787616
Conc: 20.86 ng/ml

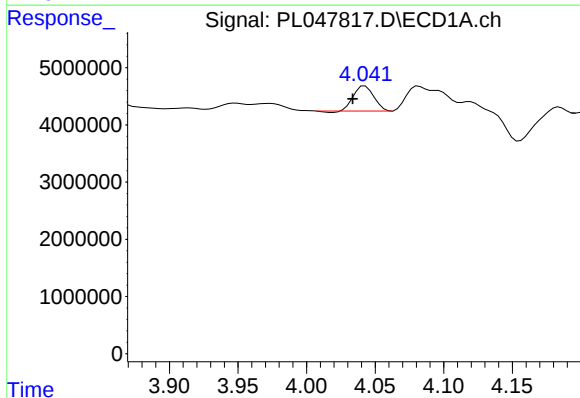


#3 gamma-BHC (Lindane)

R.T.: 4.043 min
Delta R.T.: 0.009 min
Response: 4468752
Conc: 0.34 ng/ml

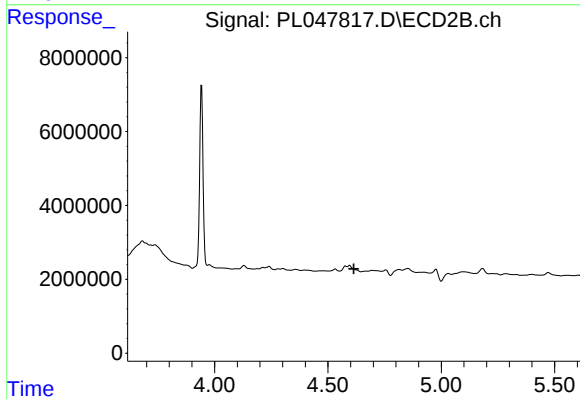

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.614 min
Response: 0
Conc: N.D.

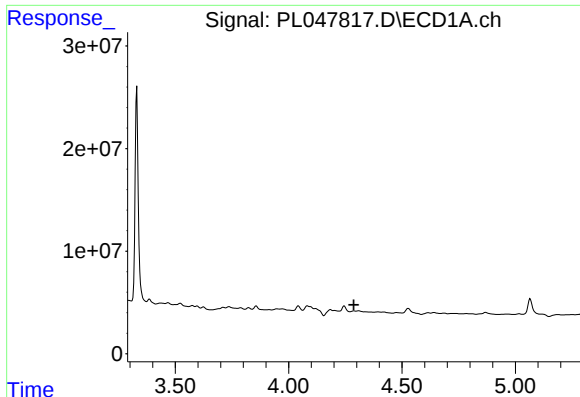

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

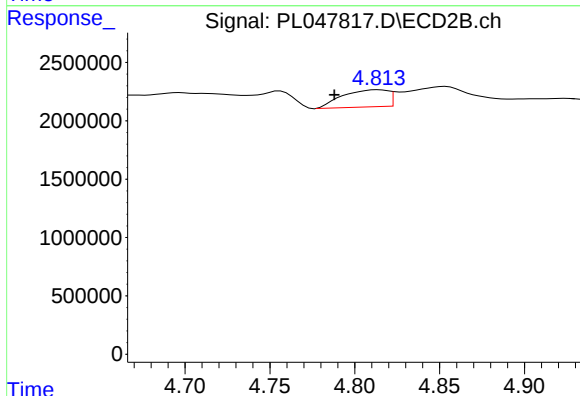


#6 beta-BHC

R.T.: 4.814 min
Delta R.T.: 0.026 min
Response: 2768683
Conc: 1.92 ng/ml

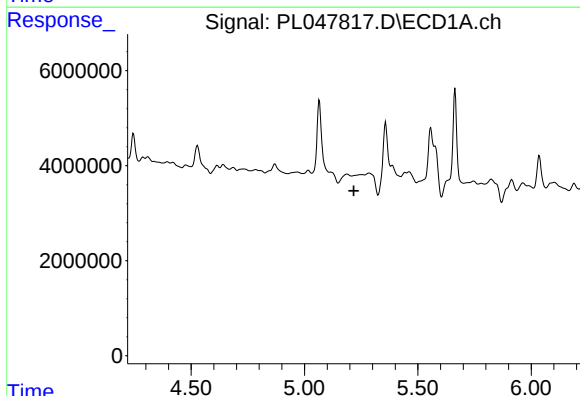


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

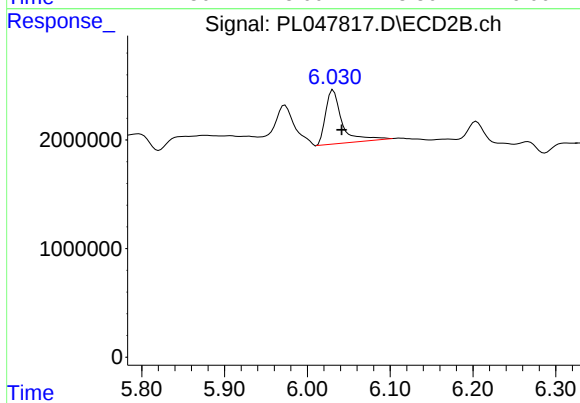

#10 gamma-Chlordane


R.T.: 6.031 min
Delta R.T.: -0.011 min
Response: 6857904
Conc: 2.27 ng/ml

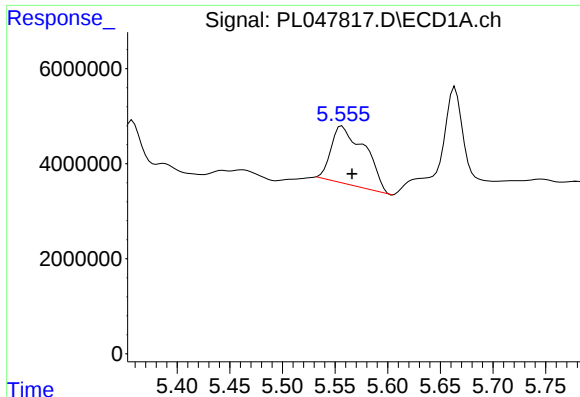

#13 Dieldrin


R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 27380361
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

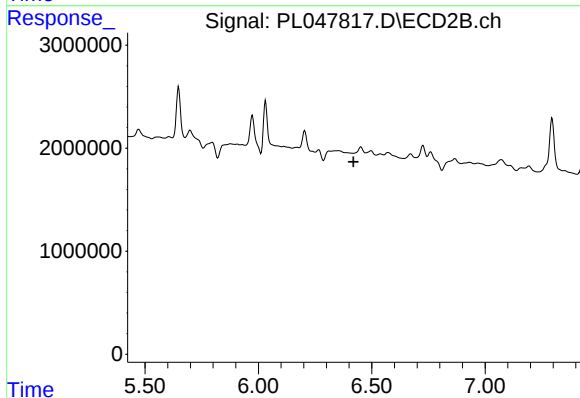


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.420 min
Response: 0
Conc: N.D.

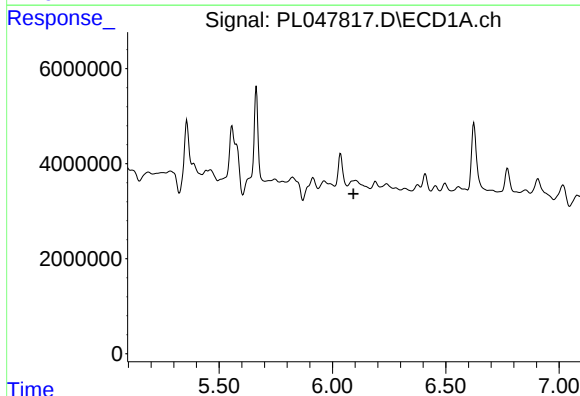


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

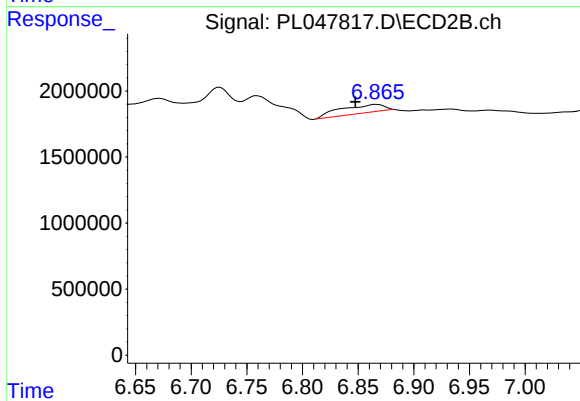

#15 Endosulfan II


R.T.: 6.867 min
Delta R.T.: 0.019 min
Response: 1813905
Conc: 0.69 ng/ml

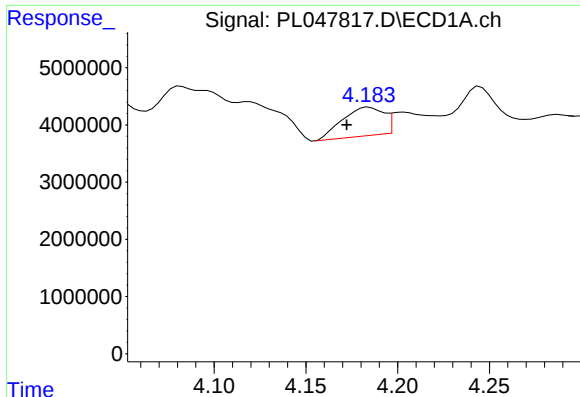

#23 Chlordane-1


R.T.: 4.184 min
Delta R.T.: 0.012 min
Response: 7765613
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

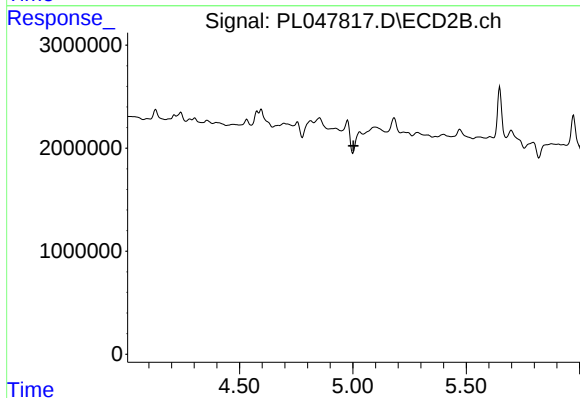


#23 Chlordane-1

R.T.: 5.031 min
Delta R.T.: 0.028 min
Response: -2023898
Conc: N.D.

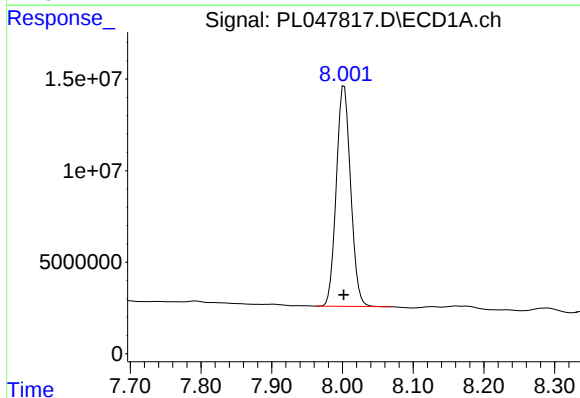

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 169672300
Conc: 15.16 ng/ml

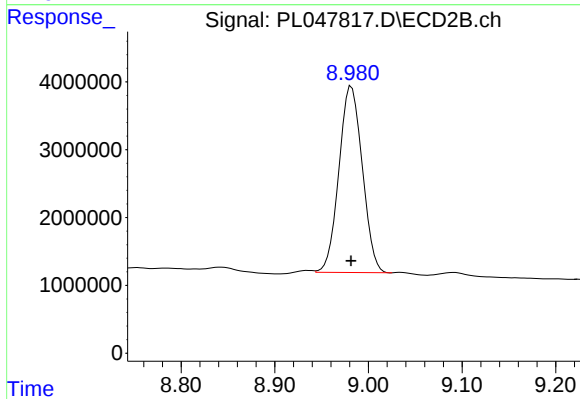

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 47745816
Conc: 16.73 ng/ml