

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 03:52
 Operator : AJ\SJ
 Sample : K2568-10
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:54:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	142.3E6	36421735	15.387	15.257
28)	SA Decachlor...	8.003	8.982	139.6E6	37409185	12.472	13.105
Target Compounds							
10)	B gamma-Chl...	5.239f	0.000	6119424	0	0.460	N.D. #
11)	B alpha-Chl...	0.000	6.116	0	2343890	N.D.	0.775 #
12)	B 4,4'-DDE	5.443	6.274	404.7E6	87367251	32.535	31.639
14)	MA Endrin	5.824	0.000	9186726	0	0.773	N.D. #
16)	A 4,4'-DDD	0.000	6.767	0	2978396	N.D.	1.327 #
17)	MA 4,4'-DDT	6.189	7.061	129.5E6	34628990	12.990	14.537
20)	A Methoxychlor	6.714f	0.000	8975042	0	1.687	N.D. #
25)	Chlordane-3	0.000	6.116	0	2343890	N.D.	7.913 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 03:52
Operator : AJ\SJ
Sample : K2568-10
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:54:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

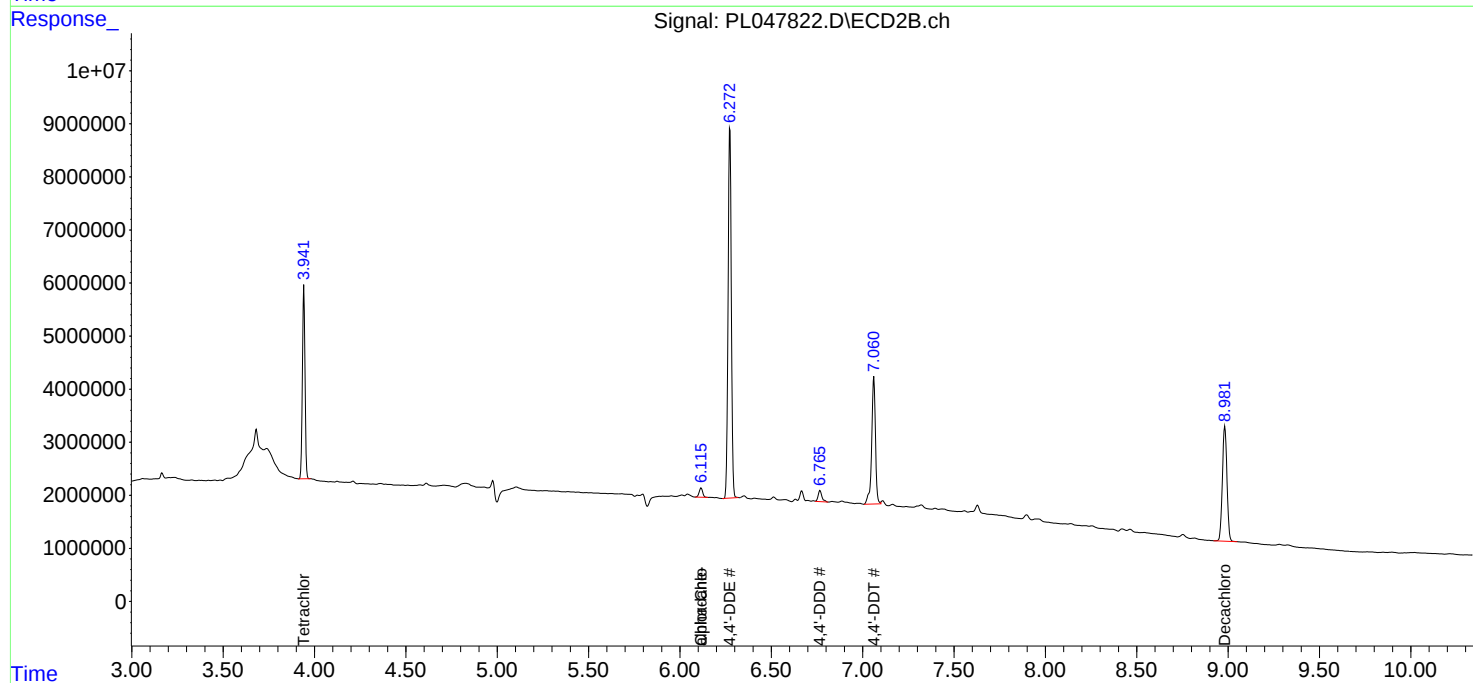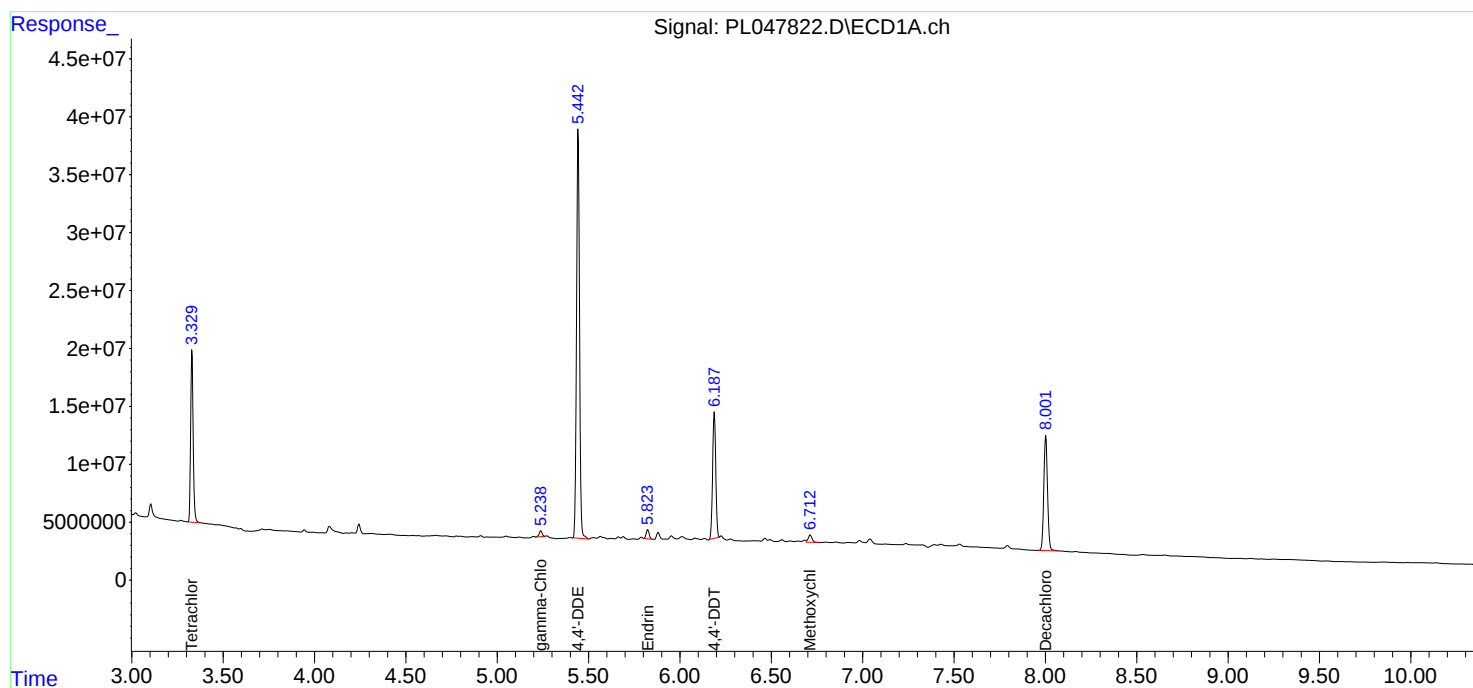


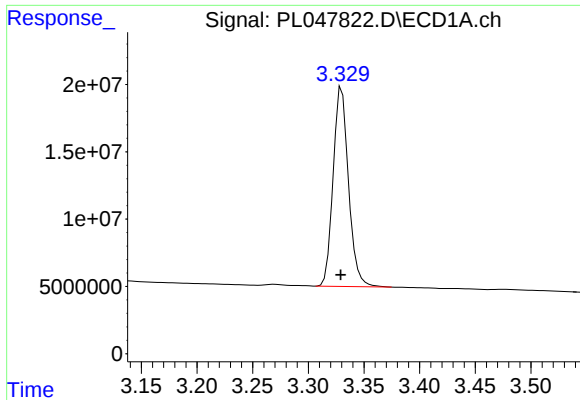

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 142301406
Conc: 15.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

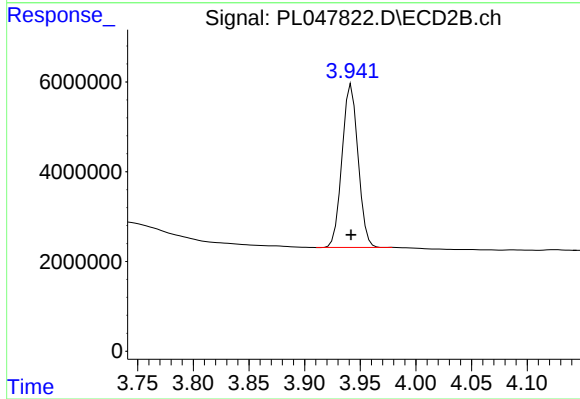


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 36421735
Conc: 15.26 ng/ml

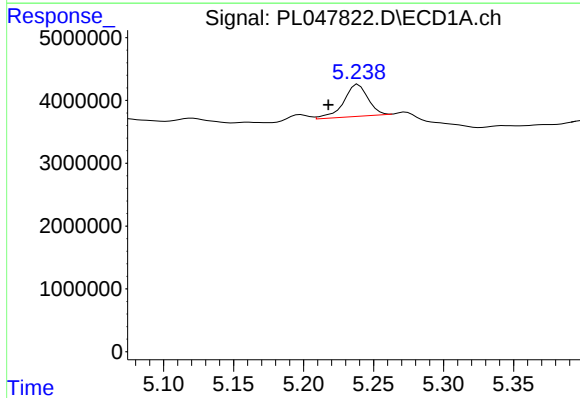


#10 gamma-Chlordane

R.T.: 5.239 min
Delta R.T.: 0.021 min
Response: 6119424
Conc: 0.46 ng/ml

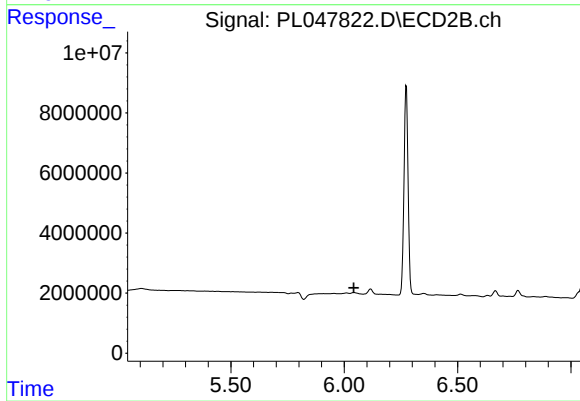

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.042 min
Response: 0
Conc: N.D.

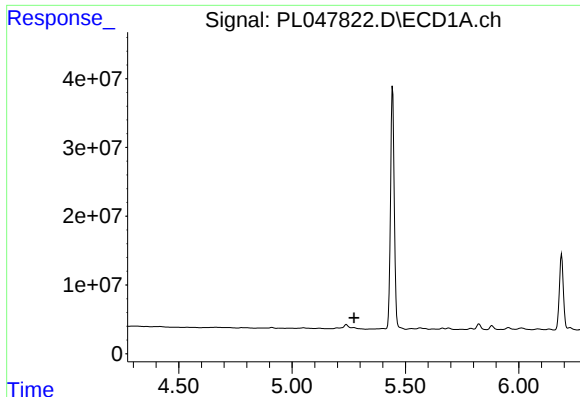

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

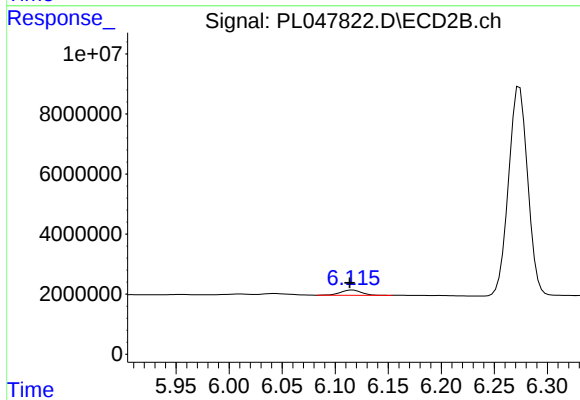


#11 alpha-Chlordane

R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 2343890
Conc: 0.77 ng/ml

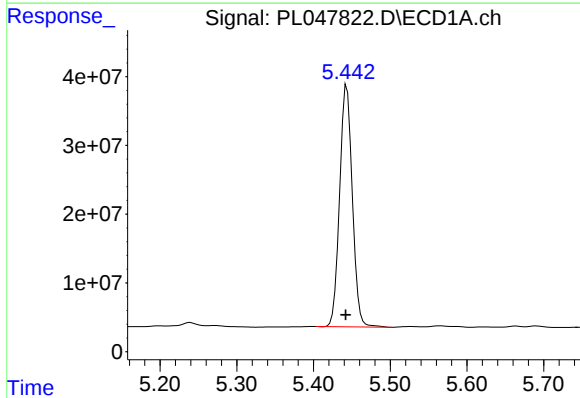


#12 4,4'-DDE

R.T.: 5.443 min
Delta R.T.: 0.001 min
Response: 404697459
Conc: 32.53 ng/ml

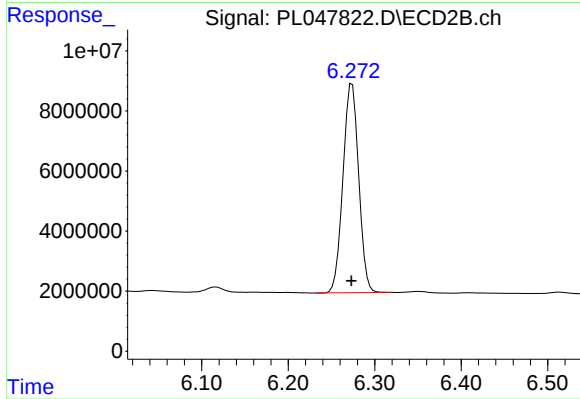

#12 4,4'-DDE


R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 87367251
Conc: 31.64 ng/ml

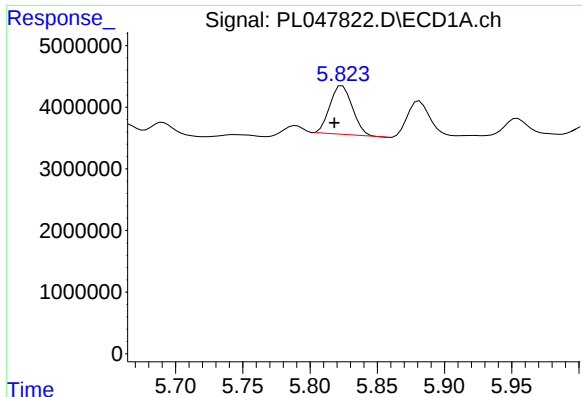

#14 Endrin


R.T.: 5.824 min
Delta R.T.: 0.006 min
Response: 9186726
Conc: 0.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

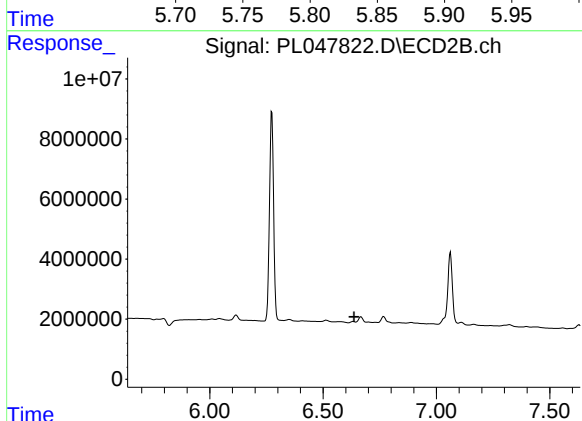


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

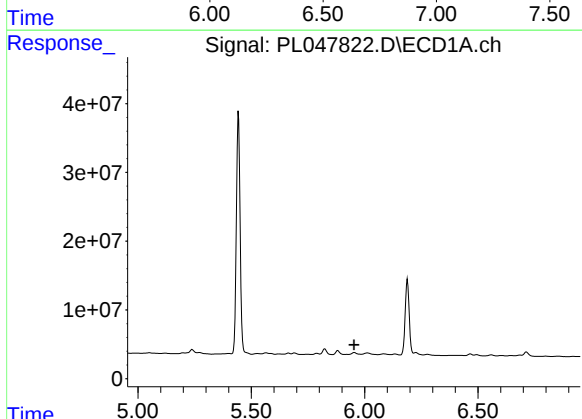


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

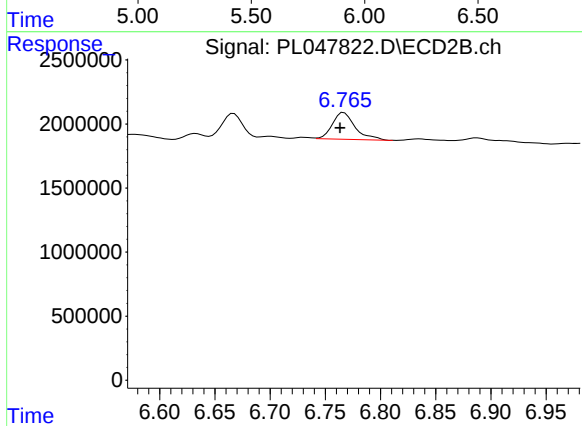

#16 4,4'-DDD


R.T.: 6.767 min
Delta R.T.: 0.004 min
Response: 2978396
Conc: 1.33 ng/ml

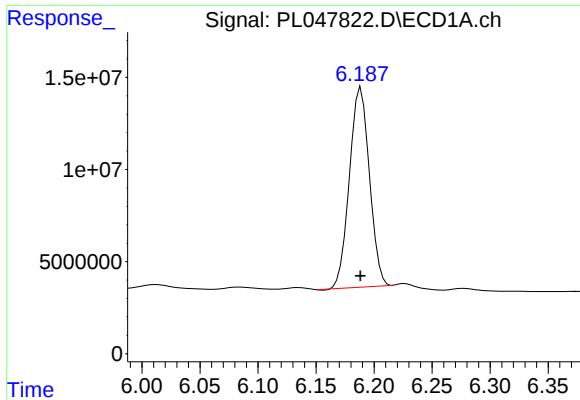

#17 4,4'-DDT


R.T.: 6.189 min
Delta R.T.: 0.000 min
Response: 129509462
Conc: 12.99 ng/ml

Instrument :
ECD_L
ClientSampleId :

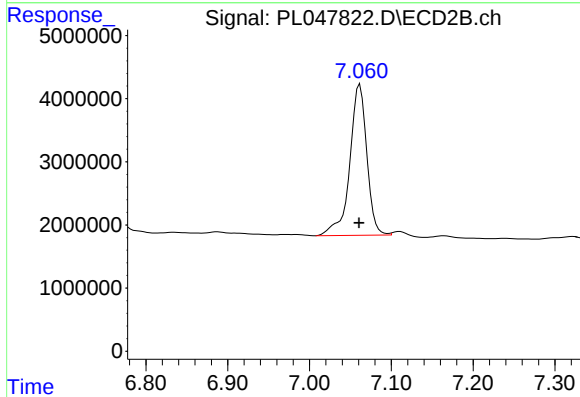


#17 4,4'-DDT

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 34628990
Conc: 14.54 ng/ml

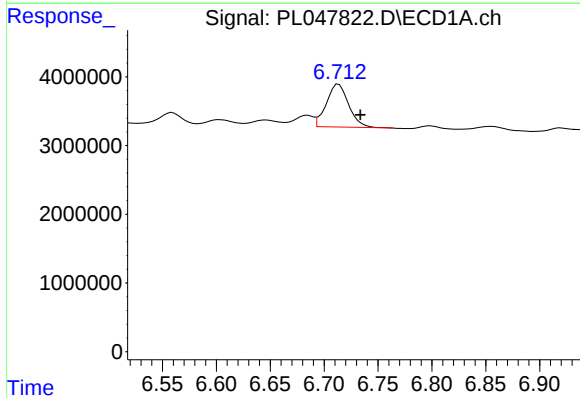


#20 Methoxychlor

R.T.: 6.714 min
Delta R.T.: -0.020 min
Response: 8975042
Conc: 1.69 ng/ml

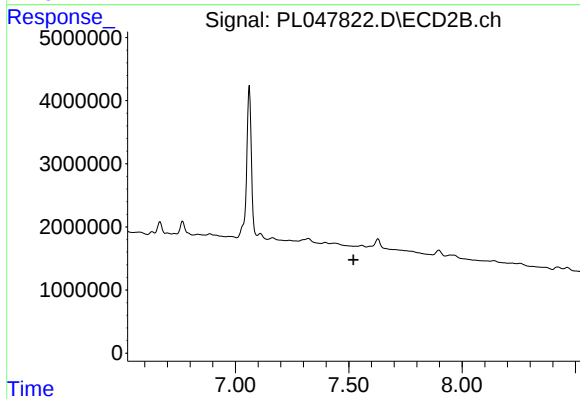

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.521 min
Response: 0
Conc: N.D.

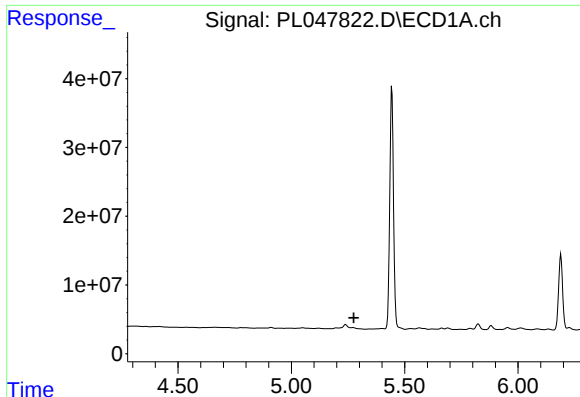

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

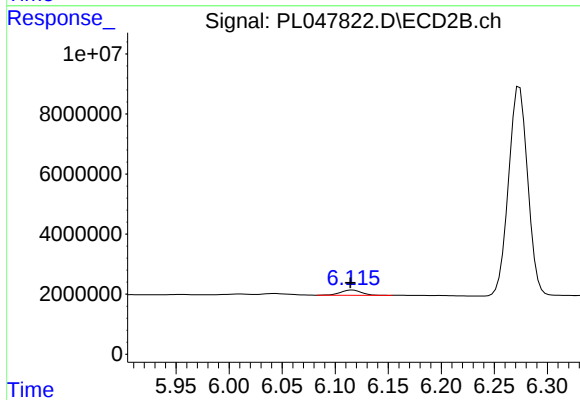


#25 Chlordane-3

R.T.: 6.116 min
Delta R.T.: 0.002 min
Response: 2343890
Conc: 7.91 ng/ml

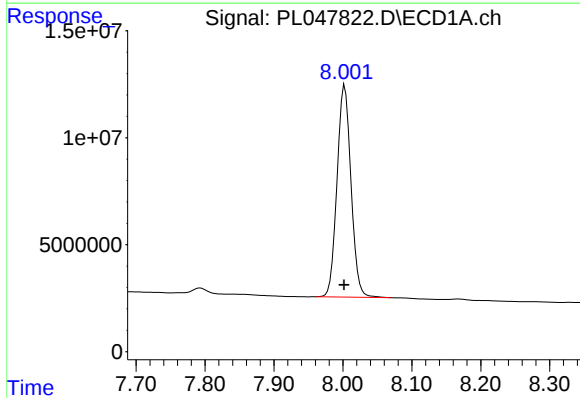

#28 Decachlorobiphenyl

R.T.: 8.003 min
Delta R.T.: 0.000 min
Response: 139611446
Conc: 12.47 ng/ml

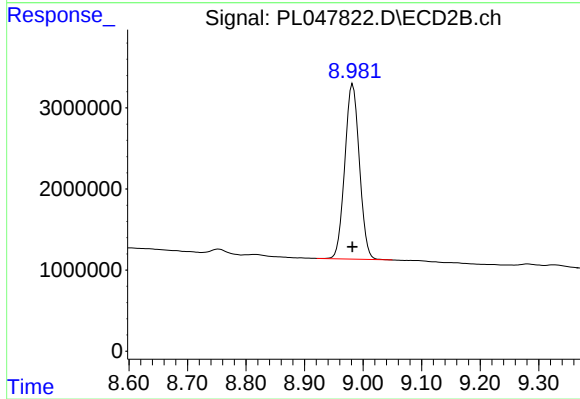

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: 0.000 min
Response: 37409185
Conc: 13.10 ng/ml