

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 06:23
 Operator : AJ\SJ
 Sample : K2568-16
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:55:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	215.8E6	48928967	23.338	20.496
28)	SA Decachlor...	8.004	8.983	112.7E6	34776504	10.065	12.183
Target Compounds							
2)	A alpha-BHC	0.000	4.303f	0	1804379	N.D.	0.544 #
10)	B gamma-Chl...	0.000	6.030	0	7546314	N.D.	2.494 #
12)	B 4,4'-DDE	5.444	6.273	17843313	4215116	1.434	1.526
13)	MA Dieldrin	5.557	0.000	33034642	0	2.545	N.D. #
15)	B Endosulfa...	0.000	6.867f	0	1854325	N.D.	0.707 #
16)	A 4,4'-DDD	0.000	6.761	0	3754538	N.D.	1.672 #
17)	MA 4,4'-DDT	6.188	7.066	8111284	1908017	0.814	0.801
19)	B Endosulfa...	6.499f	0.000	7934490	0	0.712	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 06:23
Operator : AJ\SJ
Sample : K2568-16
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:55:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

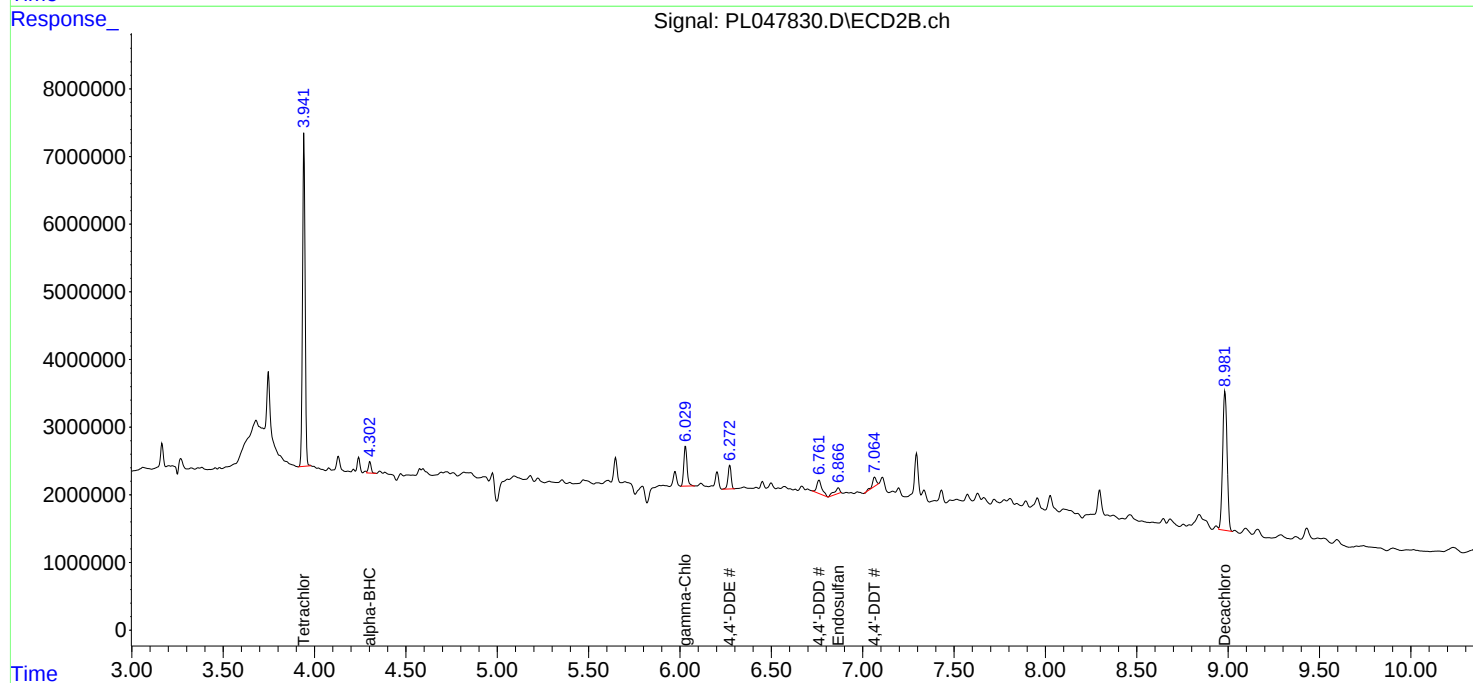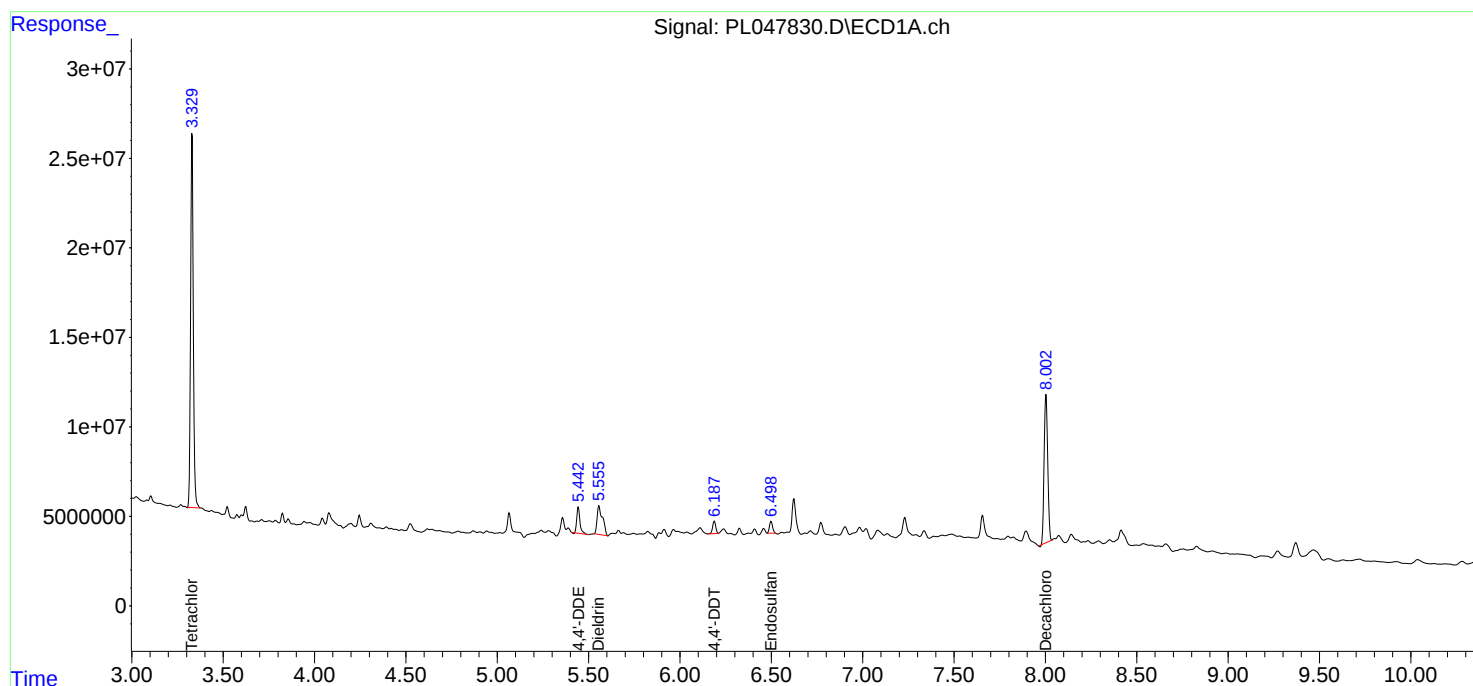


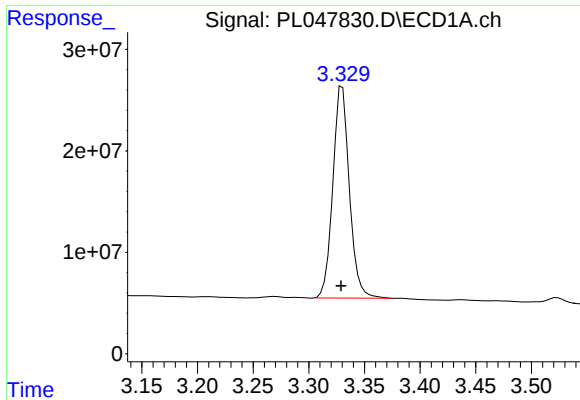

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 215831563
Conc: 23.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

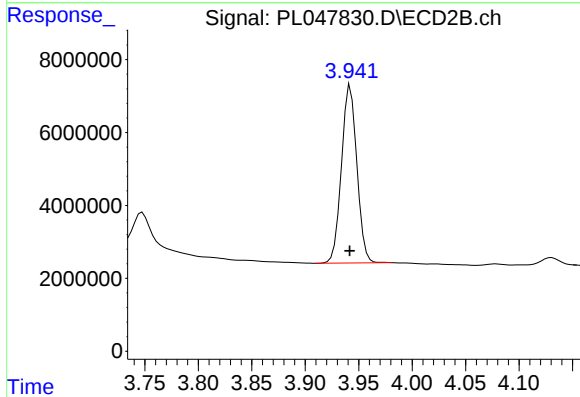


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 48928967
Conc: 20.50 ng/ml

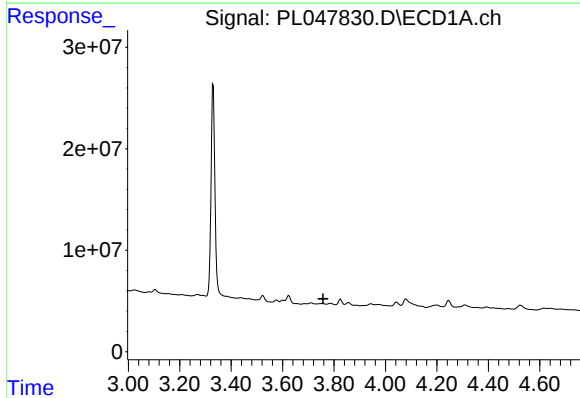


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.757 min
Response: 0
Conc: N.D.

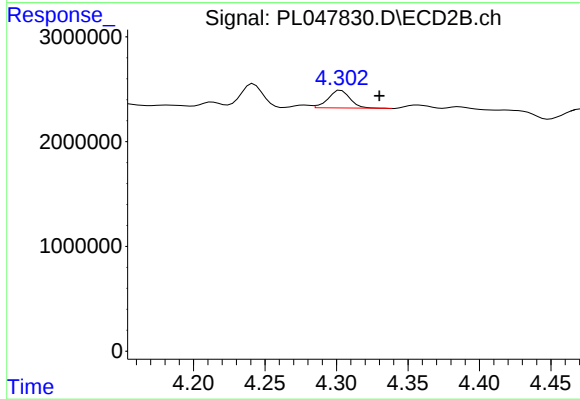

#2 alpha-BHC


R.T.: 4.303 min
Delta R.T.: -0.027 min
Response: 1804379
Conc: 0.54 ng/ml

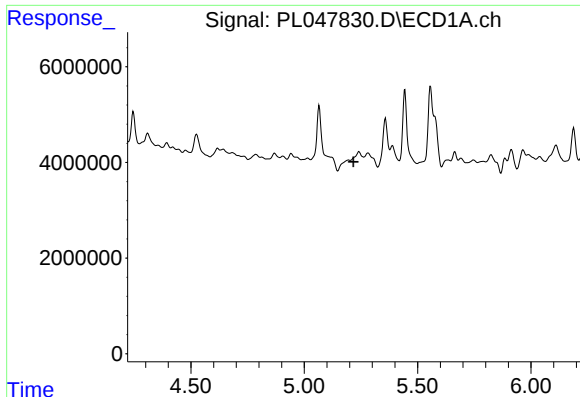

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

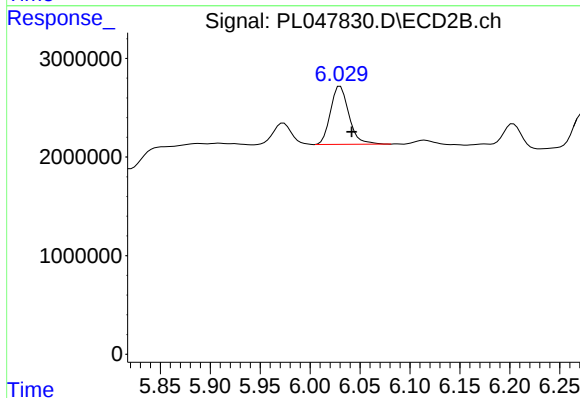


#10 gamma-Chlordane

R.T.: 6.030 min
Delta R.T.: -0.012 min
Response: 7546314
Conc: 2.49 ng/ml

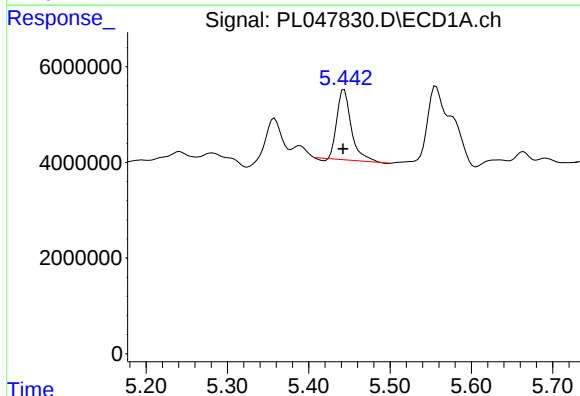


#12 4,4'-DDE

R.T.: 5.444 min
Delta R.T.: 0.002 min
Response: 17843313
Conc: 1.43 ng/ml

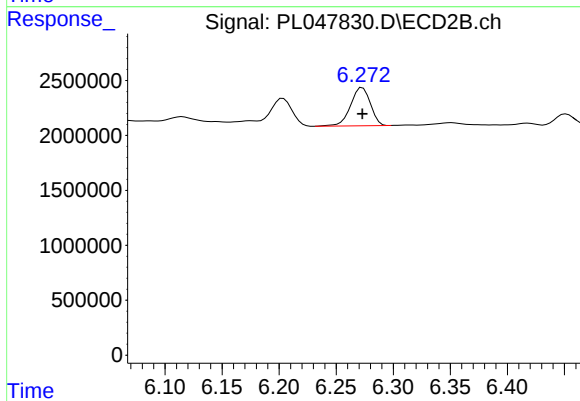

#12 4,4'-DDE


R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 4215116
Conc: 1.53 ng/ml

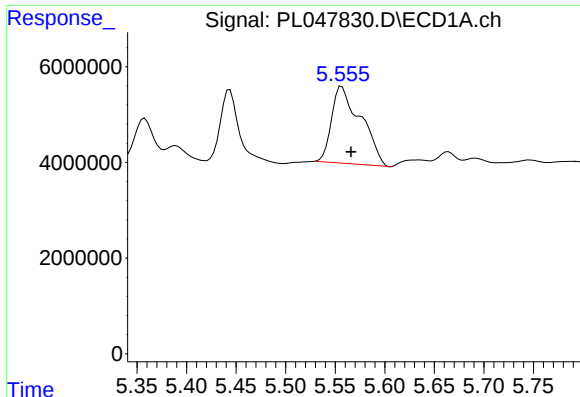

#13 Dieldrin


R.T.: 5.557 min
Delta R.T.: -0.009 min
Response: 33034642
Conc: 2.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

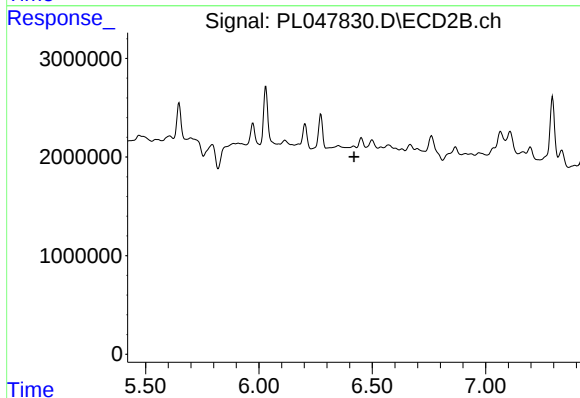


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.420 min
Response: 0
Conc: N.D.

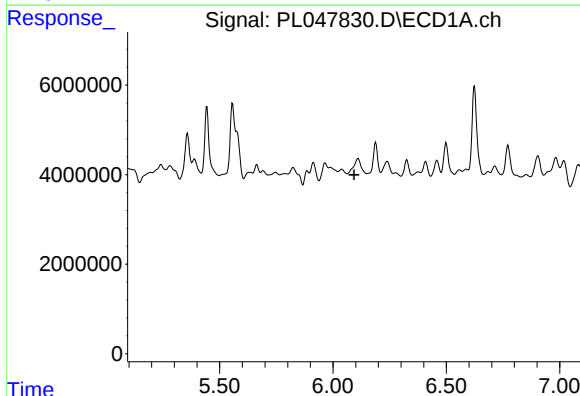


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.093 min
Response: 0
Conc: N.D.

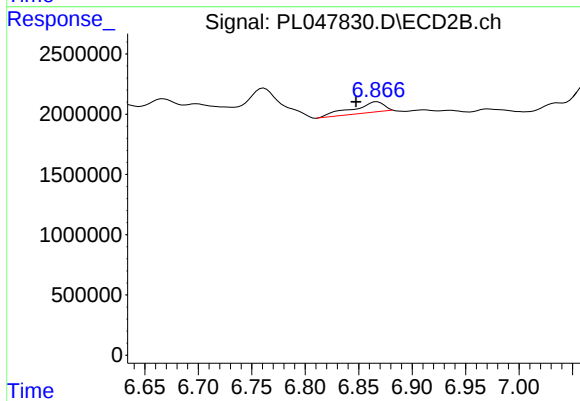

#15 Endosulfan II


R.T.: 6.867 min
Delta R.T.: 0.020 min
Response: 1854325
Conc: 0.71 ng/ml

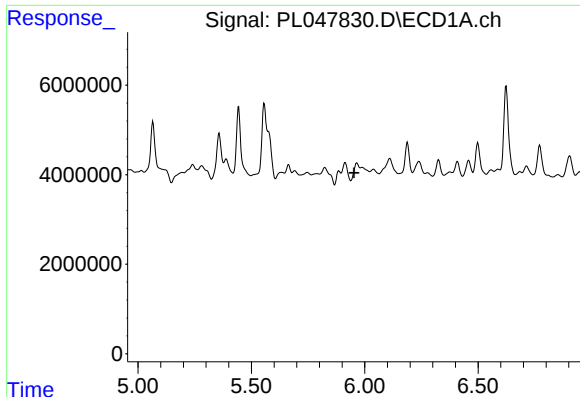

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.954 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

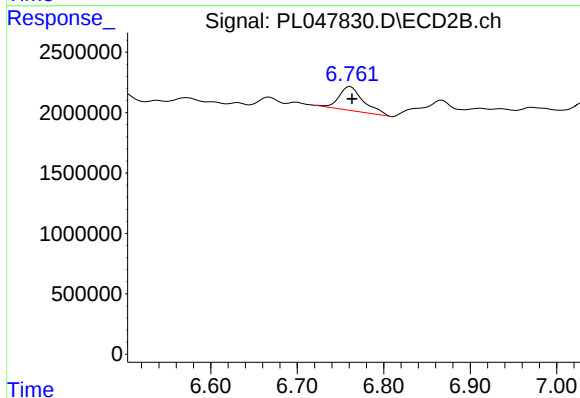


#16 4,4'-DDD

R.T.: 6.761 min
Delta R.T.: -0.002 min
Response: 3754538
Conc: 1.67 ng/ml

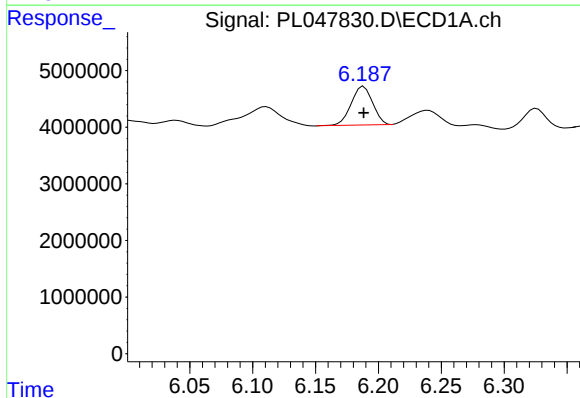


#17 4,4'-DDT

R.T.: 6.188 min
Delta R.T.: 0.000 min
Response: 8111284
Conc: 0.81 ng/ml

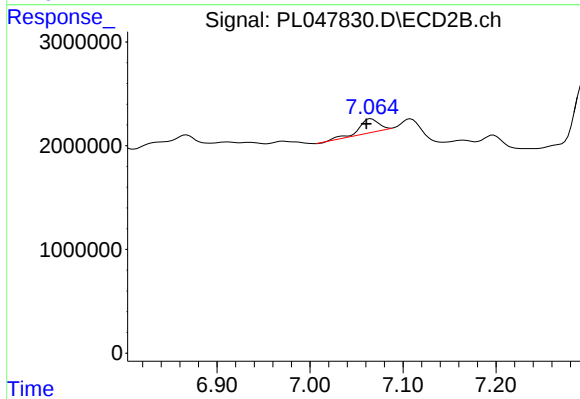

#17 4,4'-DDT


R.T.: 7.066 min
Delta R.T.: 0.005 min
Response: 1908017
Conc: 0.80 ng/ml

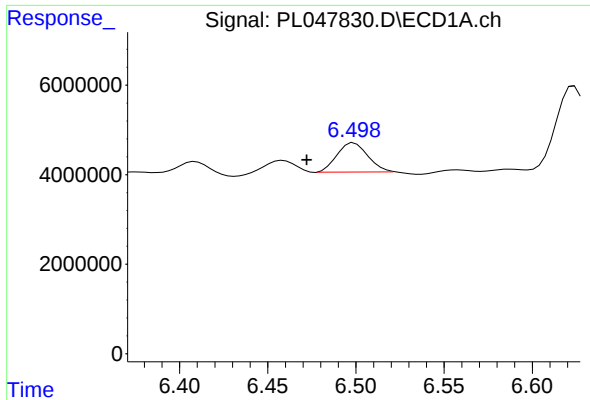

#19 Endosulfan Sulfate


R.T.: 6.499 min
Delta R.T.: 0.027 min
Response: 7934490
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

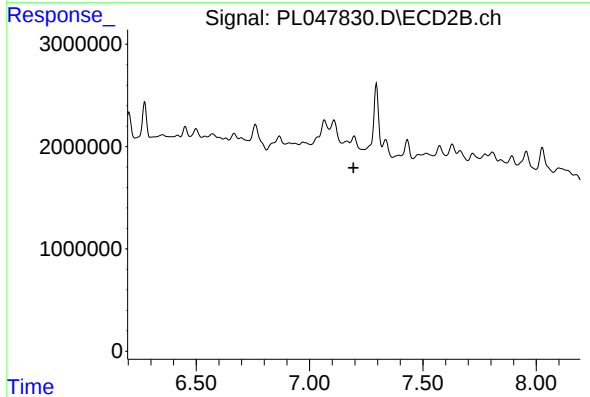


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.194 min
Response: 0
Conc: N.D.

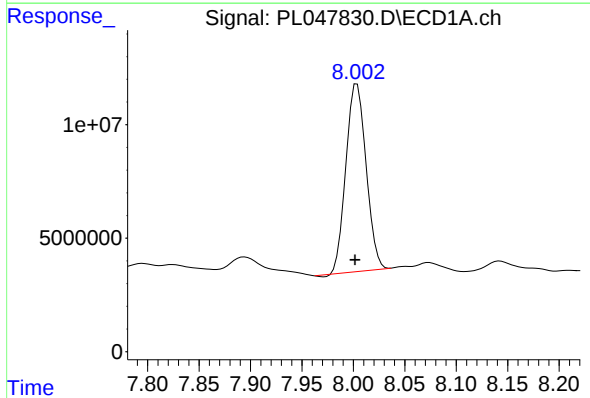

#28 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.002 min
Response: 112671323
Conc: 10.06 ng/ml

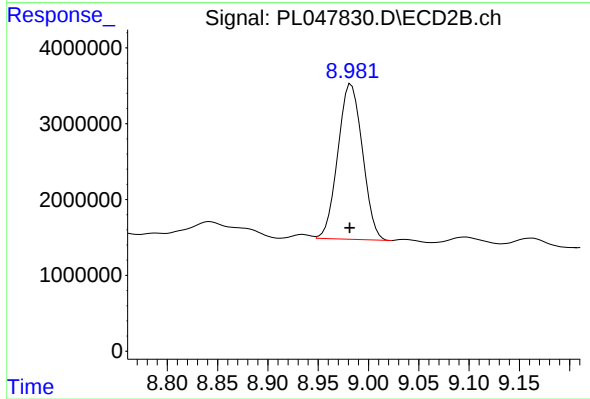

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: 0.001 min
Response: 34776504
Conc: 12.18 ng/ml