

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047834.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 07:23
 Operator : AJ\SJ
 Sample : K2568-20
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:56:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	189.9E6	45158003	20.538	18.916
28)	SA Decachlor...	8.003	8.984	173.9E6	47615690	15.531	16.680
Target Compounds							
10)	B gamma-Chl...	0.000	6.031	0	2670046	N.D.	0.882 #
12)	B 4,4'-DDE	5.443	6.273	25163938	5463493	2.023	1.979
13)	MA Dieldrin	5.576	0.000	15796714	0	1.217	N.D. #
15)	B Endosulfa...	6.114f	6.871f	6216657	340659	0.555	0.130 #
16)	A 4,4'-DDD	0.000	6.763	0	5260057	N.D.	2.343 #
17)	MA 4,4'-DDT	6.187	7.062	42204334	10768709	4.233	4.521
18)	B Endrin al...	6.287f	0.000	13786235	0	1.461	N.D. #
22)	Mirex	0.000	8.143f	0	8087706	N.D.	3.476 #
27)	Chlordane-5	6.114f	0.000	6216657	0	14.663	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047834.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 07:23
Operator : AJ\SJ
Sample : K2568-20
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:56:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

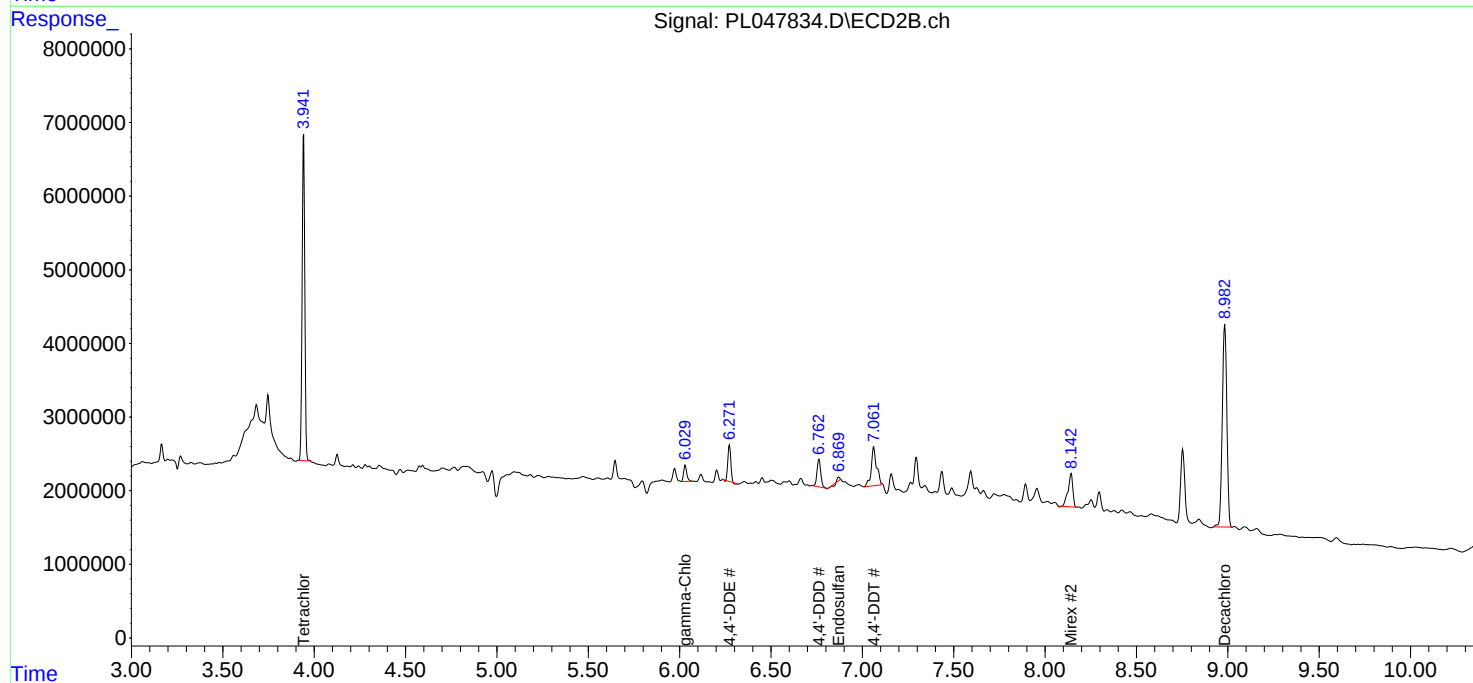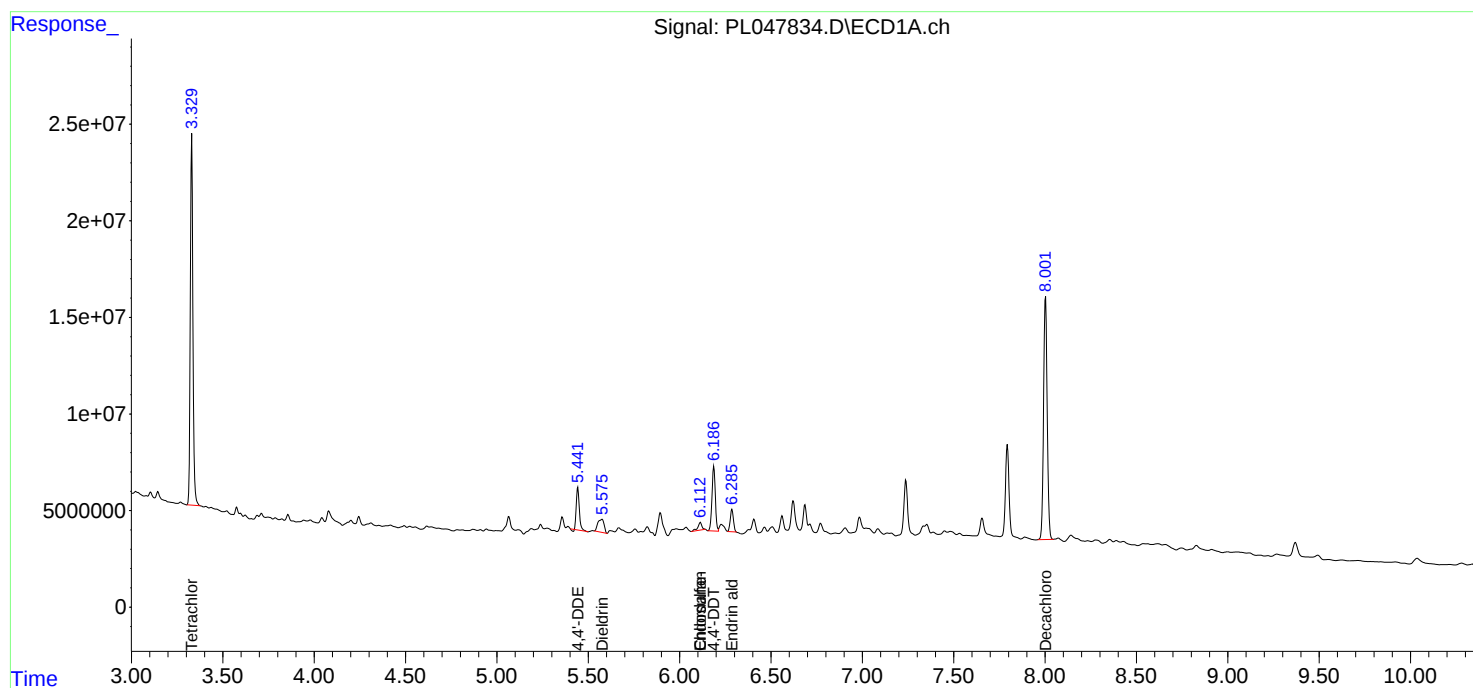


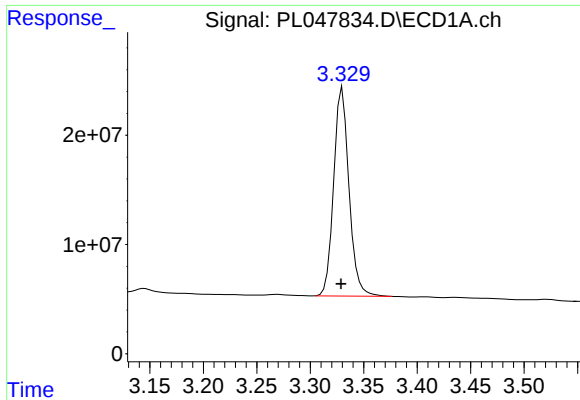

#1 Tetrachloro-m-xylene


R.T.: 3.330 min
Delta R.T.: 0.001 min
Response: 189937956
Conc: 20.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

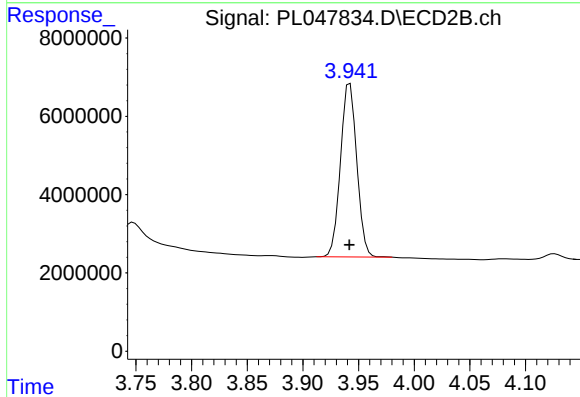


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 45158003
Conc: 18.92 ng/ml

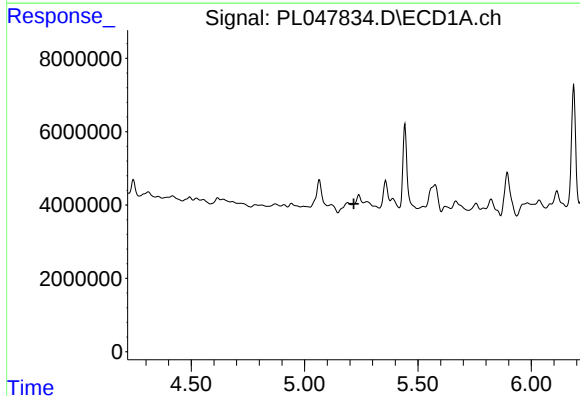


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.218 min
Response: 0
Conc: N.D.

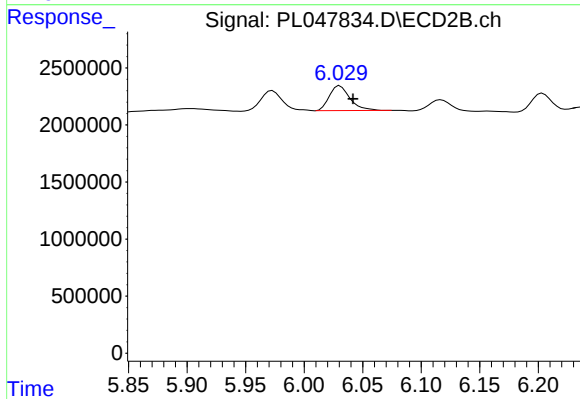

#10 gamma-Chlordane


R.T.: 6.031 min
Delta R.T.: -0.011 min
Response: 2670046
Conc: 0.88 ng/ml

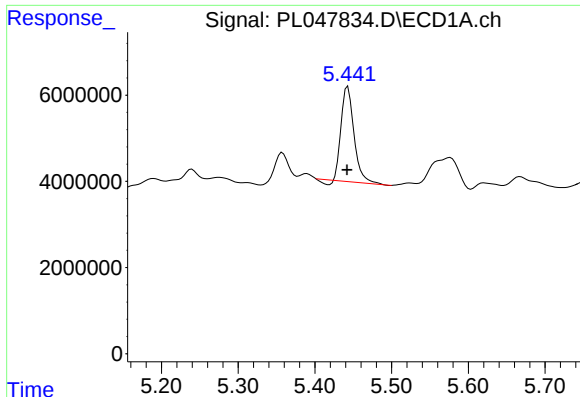

#12 4,4'-DDE


R.T.: 5.443 min
Delta R.T.: 0.000 min
Response: 25163938
Conc: 2.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

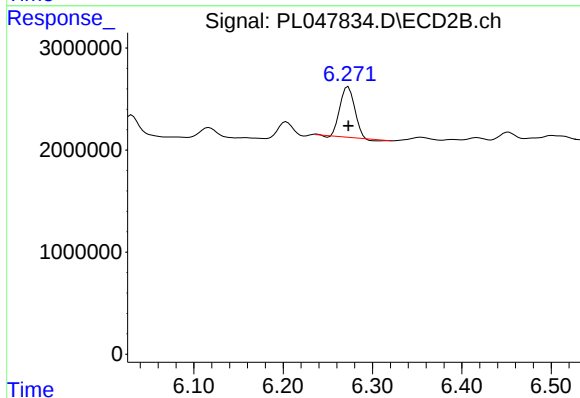


#12 4,4'-DDE

R.T.: 6.273 min
Delta R.T.: 0.000 min
Response: 5463493
Conc: 1.98 ng/ml

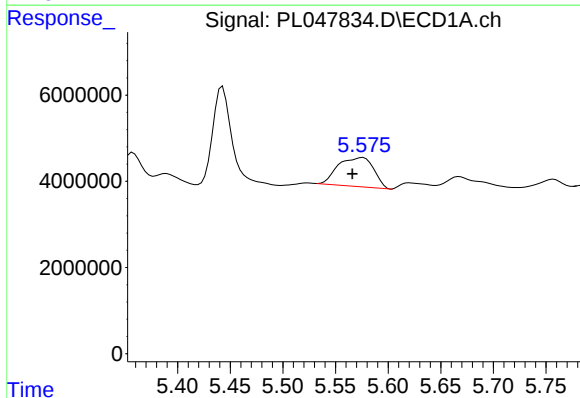


#13 Dieldrin

R.T.: 5.576 min
Delta R.T.: 0.010 min
Response: 15796714
Conc: 1.22 ng/ml

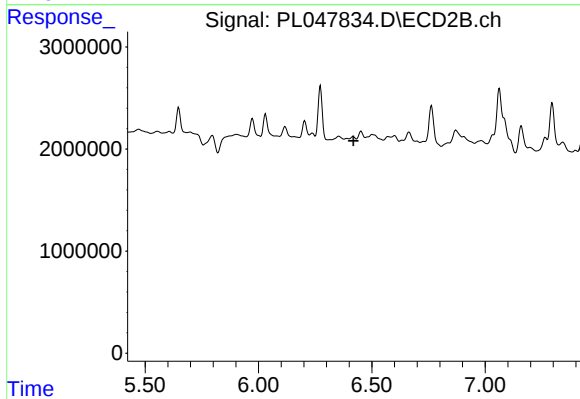

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.420 min
Response: 0
Conc: N.D.

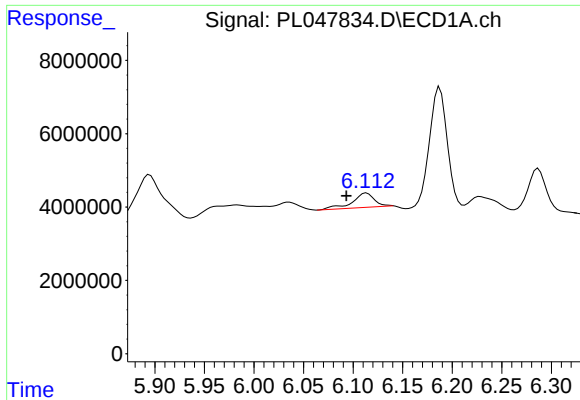

#15 Endosulfan II


R.T.: 6.114 min
Delta R.T.: 0.020 min
Response: 6216657
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

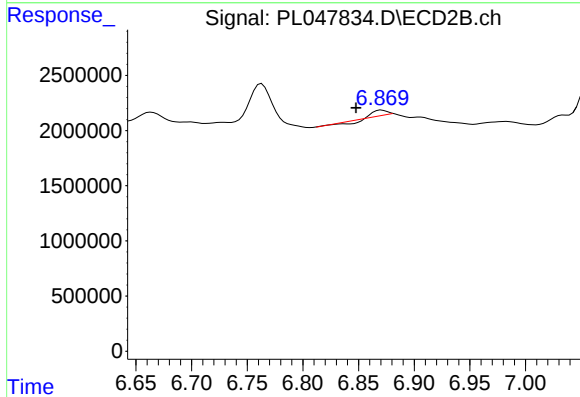


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.023 min
Response: 340659
Conc: 0.13 ng/ml

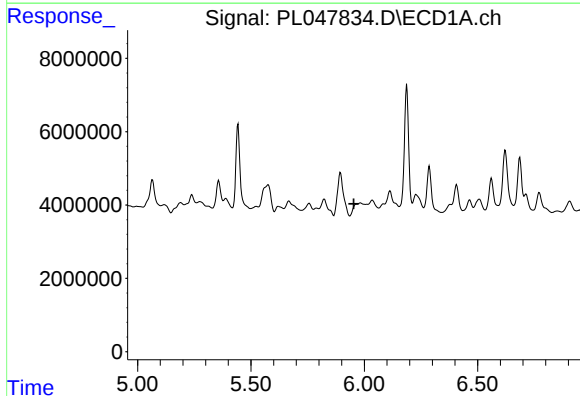


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.954 min
Response: 0
Conc: N.D.

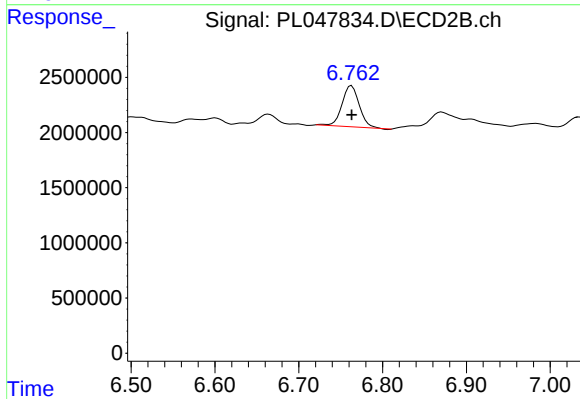

#16 4,4'-DDD


R.T.: 6.763 min
Delta R.T.: 0.000 min
Response: 5260057
Conc: 2.34 ng/ml

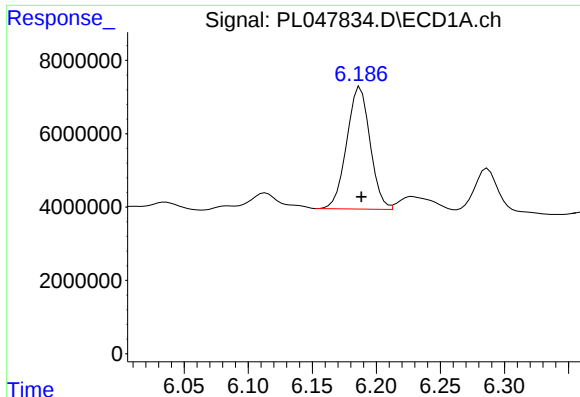

#17 4,4'-DDT


R.T.: 6.187 min
Delta R.T.: 0.000 min
Response: 42204334
Conc: 4.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

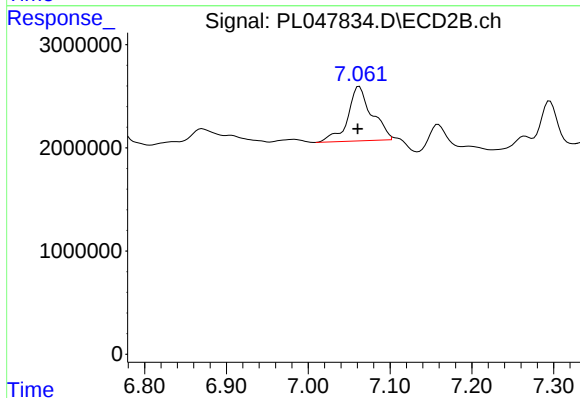


#17 4,4'-DDT

R.T.: 7.062 min
Delta R.T.: 0.002 min
Response: 10768709
Conc: 4.52 ng/ml

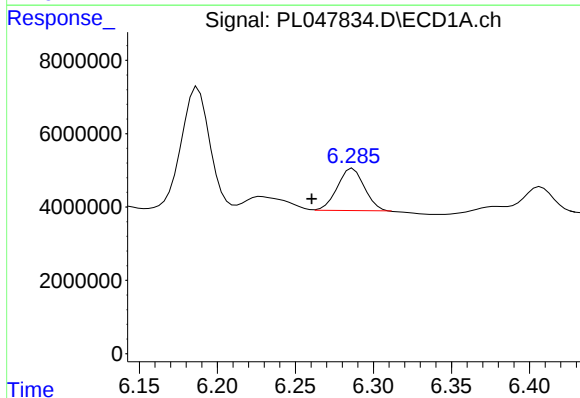


#18 Endrin aldehyde

R.T.: 6.287 min
Delta R.T.: 0.026 min
Response: 13786235
Conc: 1.46 ng/ml

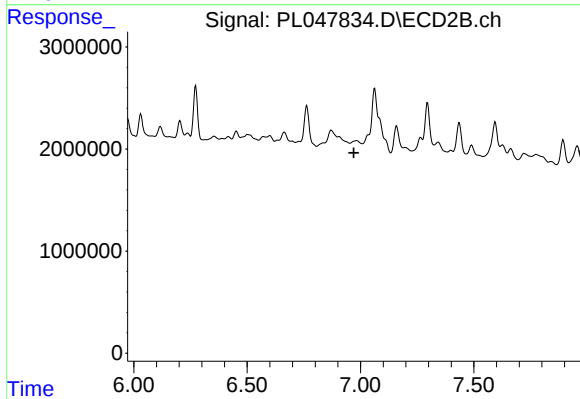

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 6.971 min
Response: 0
Conc: N.D.

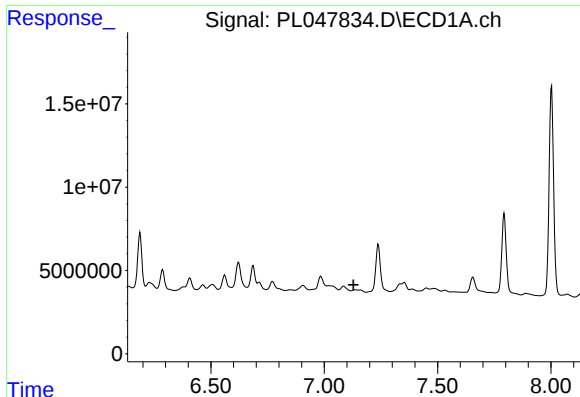

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

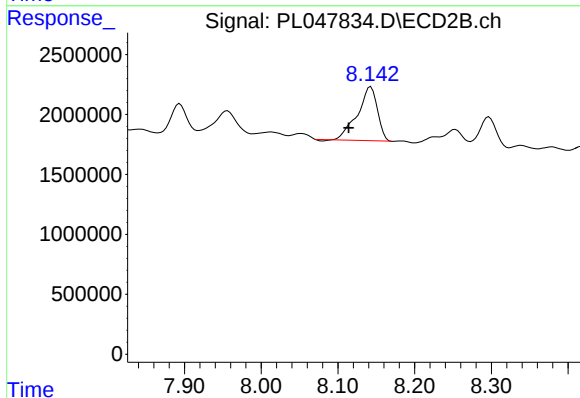


#22 Mirex

R.T.: 8.143 min
Delta R.T.: 0.029 min
Response: 8087706
Conc: 3.48 ng/ml

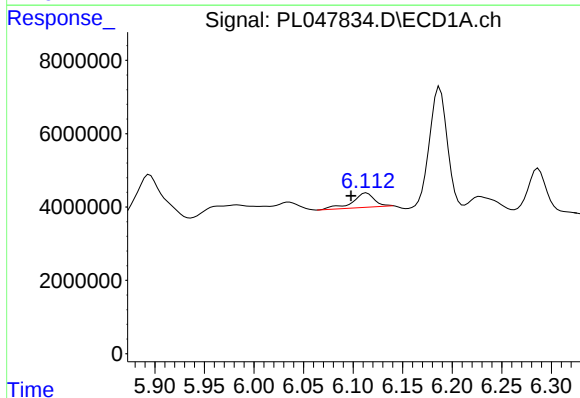


#27 Chlordane-5

R.T.: 6.114 min
Delta R.T.: 0.016 min
Response: 6216657
Conc: 14.66 ng/ml

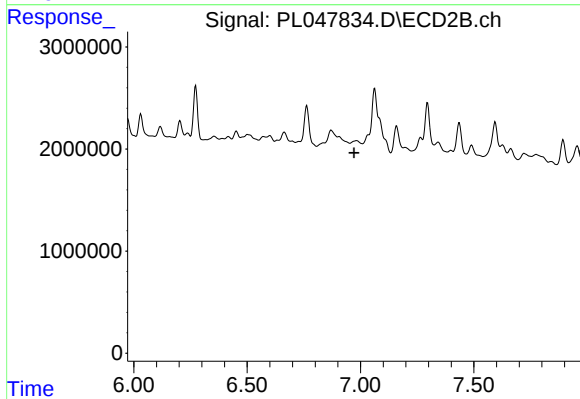

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.972 min
Response: 0
Conc: N.D.

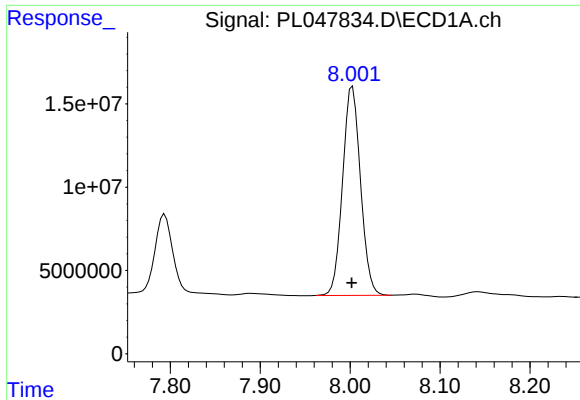

#28 Decachlorobiphenyl


R.T.: 8.003 min

Delta R.T.: 0.000 min

Response: 173863978

Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

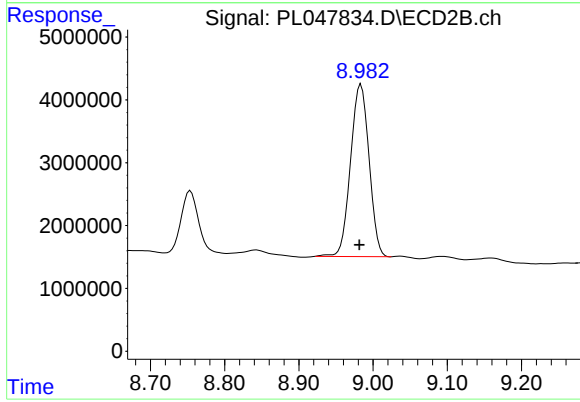

#28 Decachlorobiphenyl

R.T.: 8.984 min

Delta R.T.: 0.002 min

Response: 47615690

Conc: 16.68 ng/ml