

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
 Data File : PL047811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Apr 2019 00:36
 Operator : AJ\SJ
 Sample : K2203-17
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-03-042419-A

Manual Integrations
 APPROVED

mohammad
 4/26/2019 12:48:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 09:52:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 25 01:53:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.330	3.942	117.9E6	30420608	12.753	12.743
28)	SA Decachlor...	8.002	8.980	130.4E6	36768198	11.651	12.880
Target Compounds							
10)	B gamma-Chl...	5.219	6.040	4584806	2745055	0.344m	0.907m#
11)	B alpha-Chl...	5.274	6.115	15142880	3959589	1.160	1.309

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042519\
Data File : PL047811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Apr 2019 00:36
Operator : AJ\SJ
Sample : K2203-17
Misc :
ALS Vial : 42 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-03-042419-A


Manual Integrations
APPROVED

mohammad
4/26/2019 12:48:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 09:52:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL042419.M
Quant Title : GC Extractables
QLast Update : Thu Apr 25 01:53:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

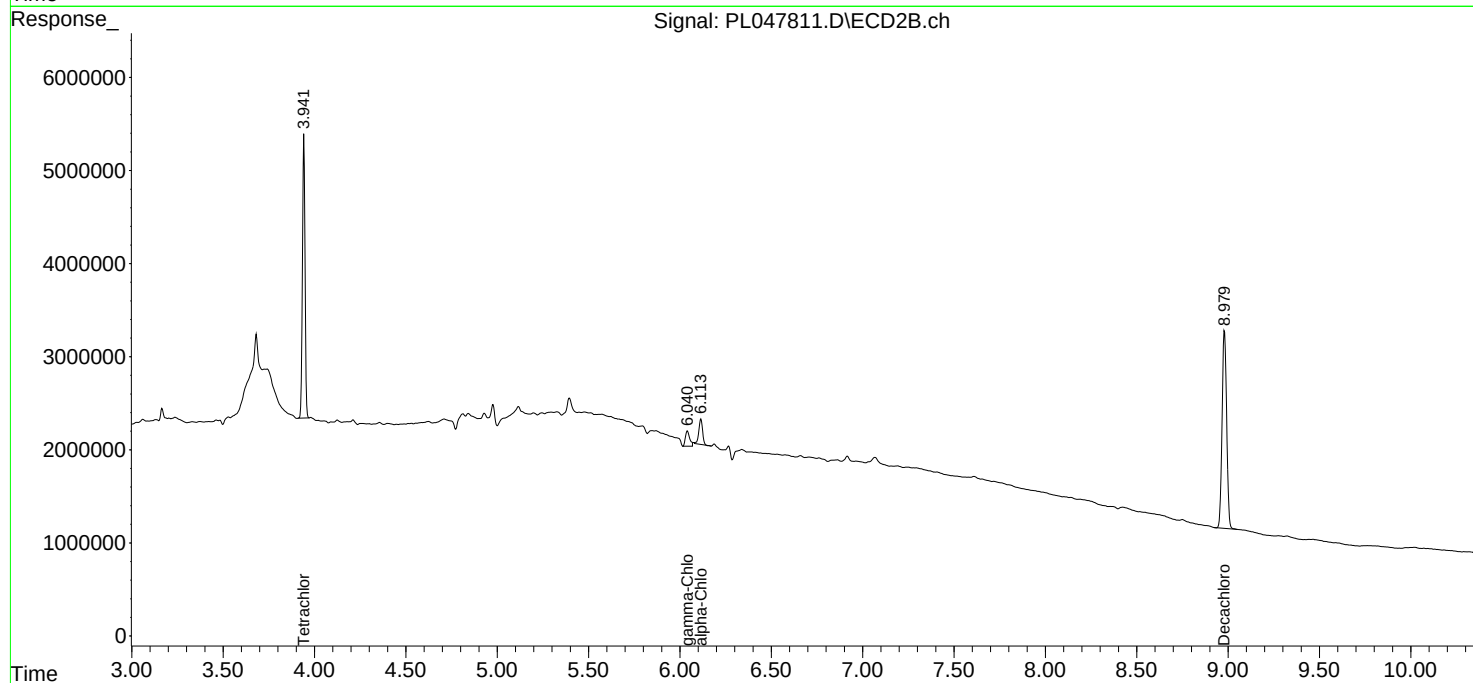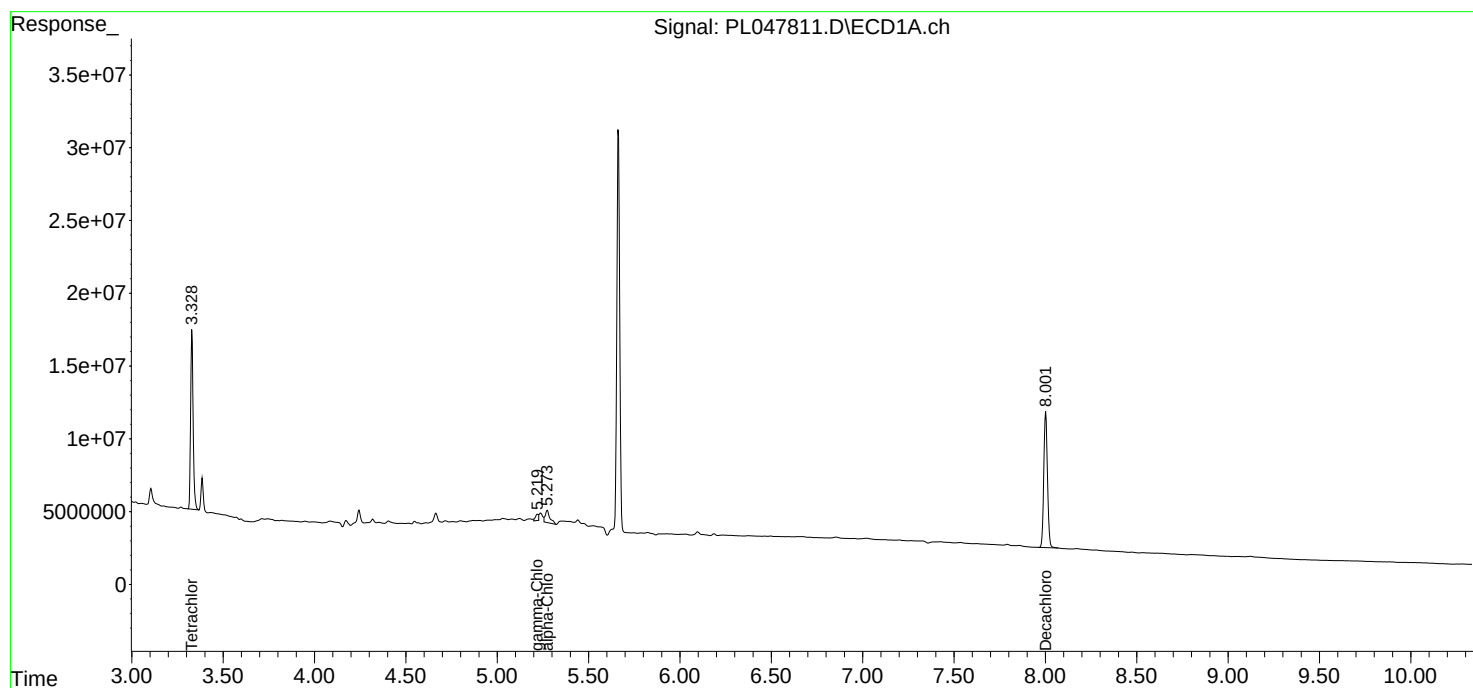

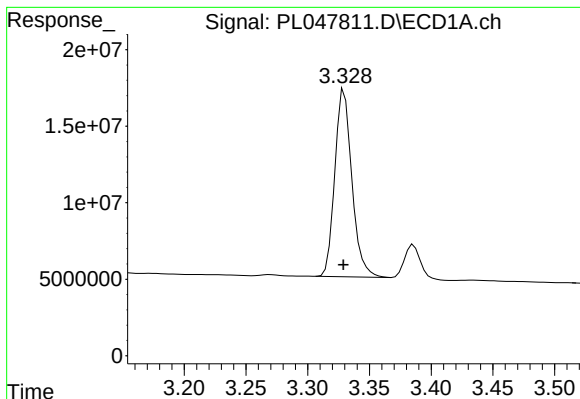


#1 Tetrachloro-m-xylene

R.T.: 3.330 min
Delta R.T.: 0.000 min
Response: 117939325
Conc: 12.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-042419-A


Manual Integrations
APPROVED

mohammad
4/26/2019 12:48:01 PM

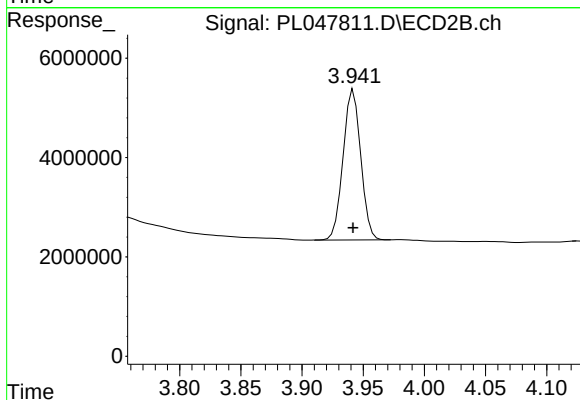


#1 Tetrachloro-m-xylene

R.T.: 3.942 min
Delta R.T.: 0.000 min
Response: 30420608
Conc: 12.74 ng/ml

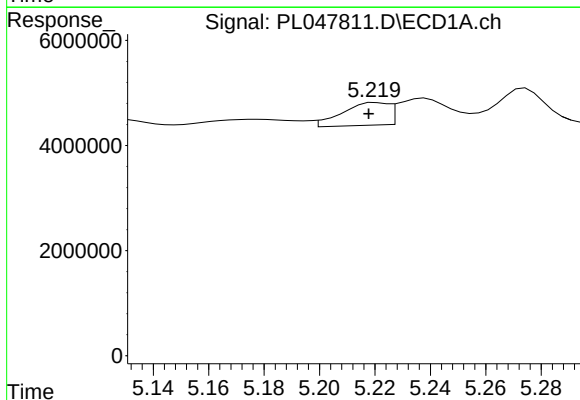


#10 gamma-Chlordane

R.T.: 5.219 min
Delta R.T.: 0.000 min
Response: 4584806
Conc: 0.34 ng/ml m

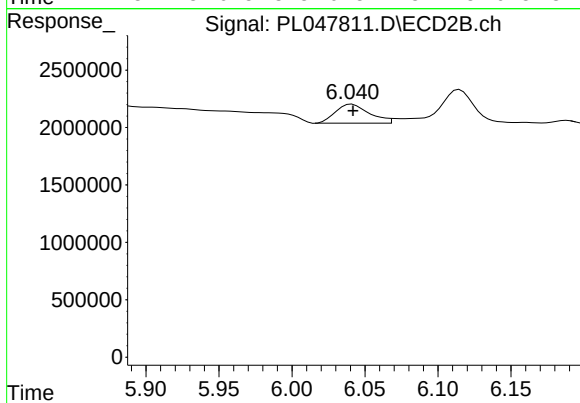

#10 gamma-Chlordane

R.T.: 6.040 min
Delta R.T.: -0.002 min
Response: 2745055
Conc: 0.91 ng/ml m

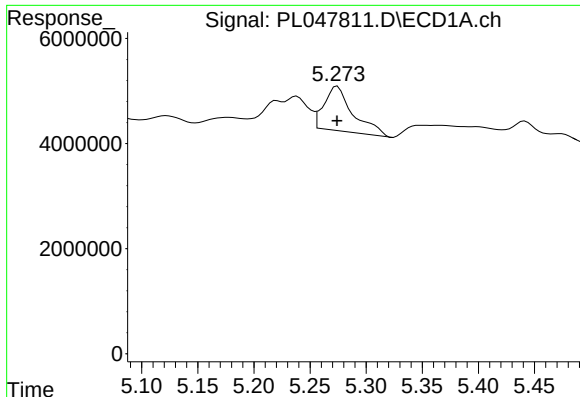


#11 alpha-Chlordane

R.T.: 5.274 min
Delta R.T.: 0.000 min
Response: 15142880
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-042419-A


Manual Integrations
APPROVED

mohammad
4/26/2019 12:48:01 PM

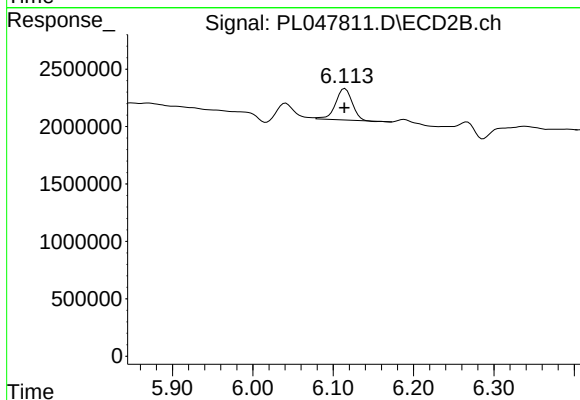


#11 alpha-Chlordane

R.T.: 6.115 min
Delta R.T.: 0.001 min
Response: 3959589
Conc: 1.31 ng/ml

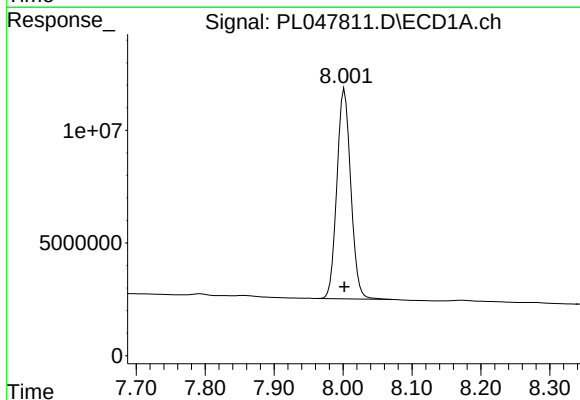

#28 Decachlorobiphenyl

R.T.: 8.002 min
Delta R.T.: 0.000 min
Response: 130420878
Conc: 11.65 ng/ml

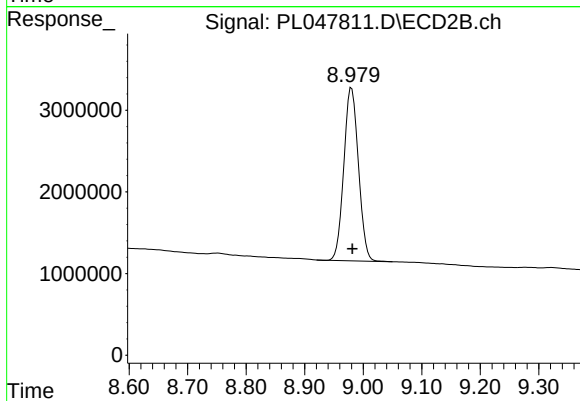

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.001 min
Response: 36768198
Conc: 12.88 ng/ml