

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
 Data File : PL074322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2022 09:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 01:56:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.636	5.489	7591975	38691195	23.497	21.700
28)	SA Decachlor...	10.407	11.331	11501398	37983196	22.117	21.504
Target Compounds							
2)	A alpha-BHC	5.370f	0.000	63593	0	0.152	N.D. #
5)	MB Aldrin	0.000	7.496f	0	241986	N.D.	0.103 #
6)	B beta-BHC	0.000	6.682	0	370318	N.D.	0.329 #
7)	B delta-BHC	0.000	6.941	0	1665426	N.D.	0.682 #
10)	B gamma-Chl...	0.000	8.196	0	536948	N.D.	0.241 #
11)	B alpha-Chl...	0.000	8.277	0	39187	N.D.	0.018 #
14)	MA Endrin	8.083f	0.000	74962	0	0.185	N.D. #
16)	A 4,4'-DDD	0.000	8.981	0	58823	N.D.	0.038 #
20)	A Methoxychlor	0.000	9.783	0	546057	N.D.	0.568 #
23)	Chlordane-1	0.000	6.852	0	629899	N.D.	7.893 #
25)	Chlordane-3	0.000	8.196	0	536948	N.D.	1.587 #
26)	Chlordane-4	0.000	8.277	0	39187	N.D.	0.099 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
Data File : PL074322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2022 09:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 01:56:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

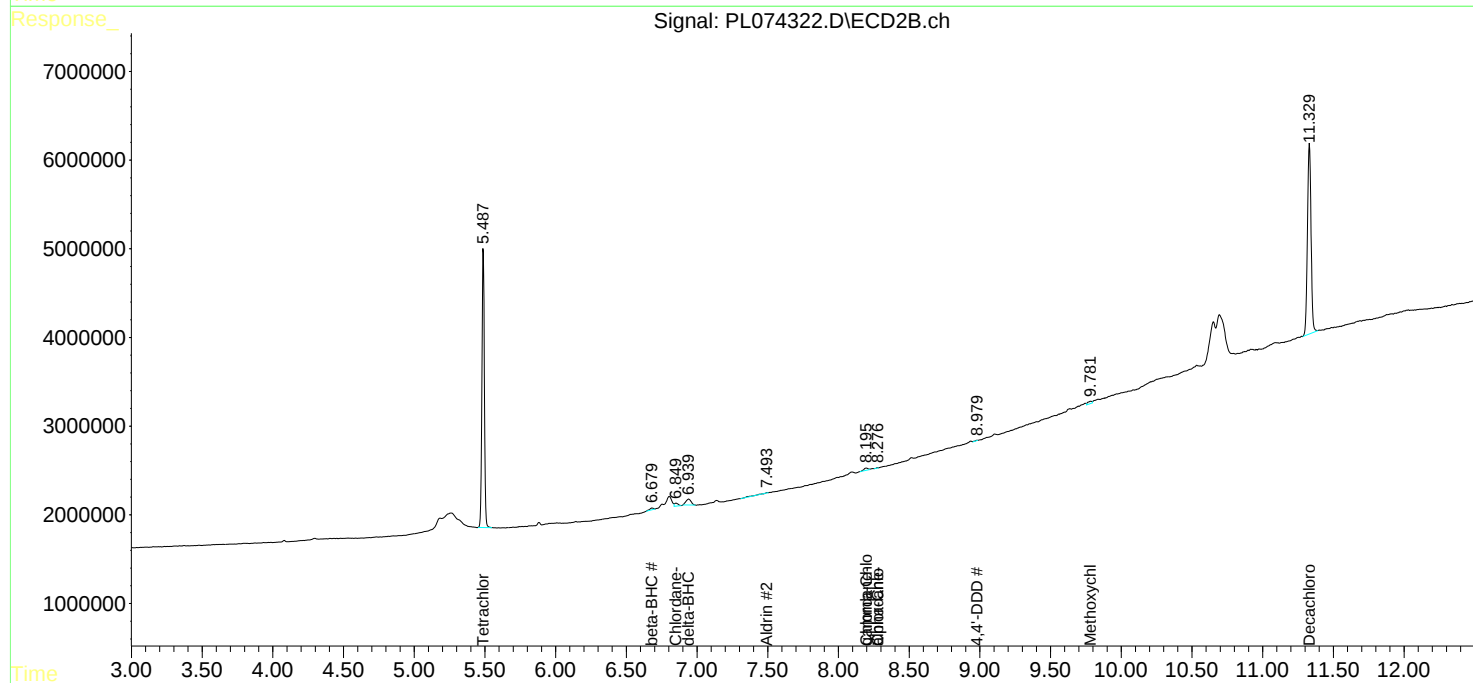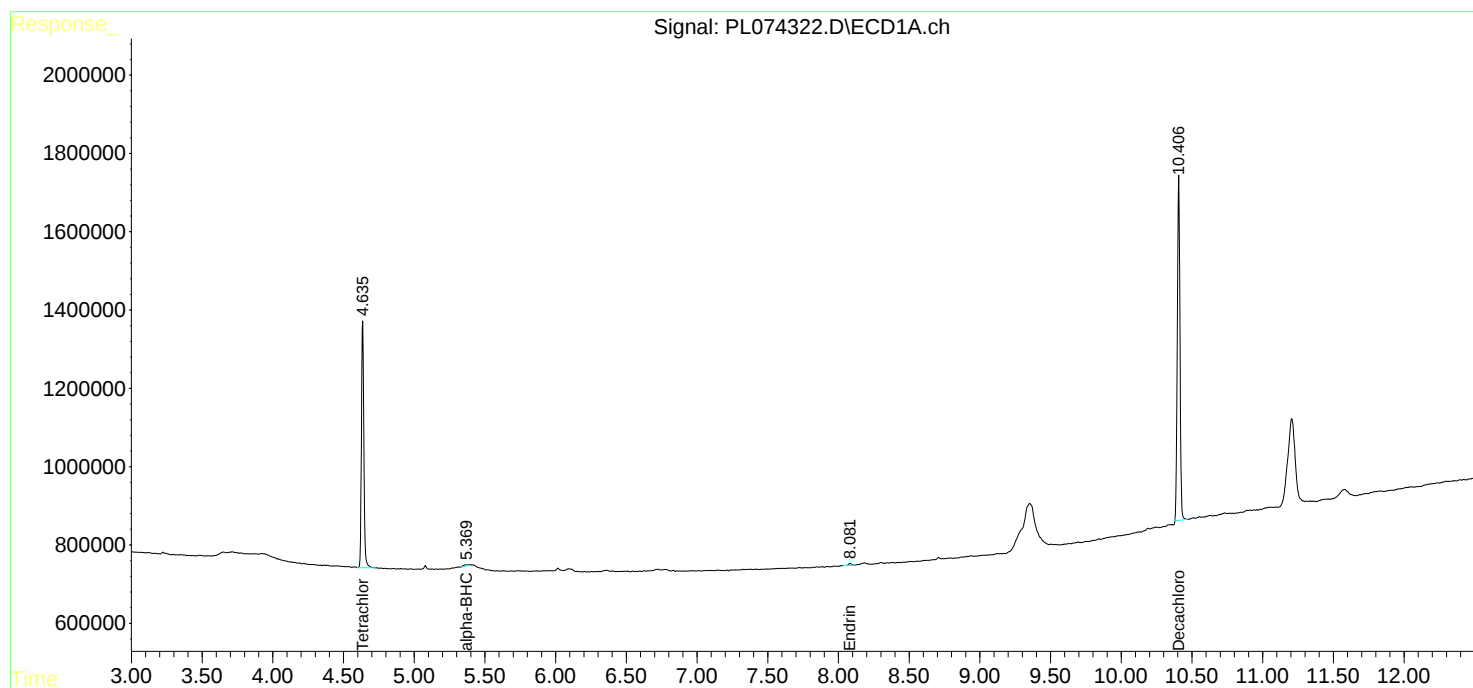


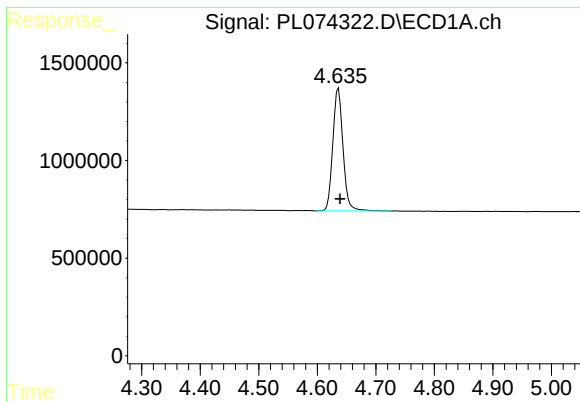

#1 Tetrachloro-m-xylene


R.T.: 4.636 min
Delta R.T.: -0.003 min
Response: 7591975
Conc: 23.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

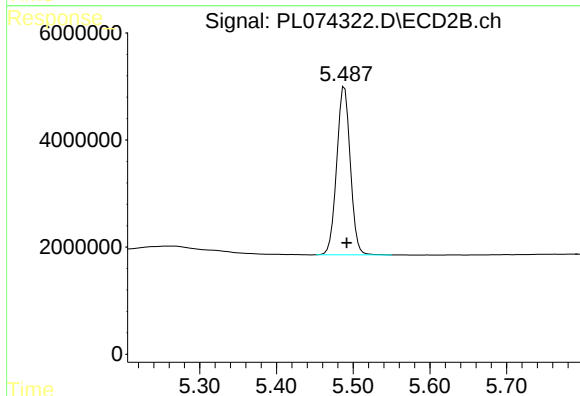


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.003 min
Response: 38691195
Conc: 21.70 ng/ml

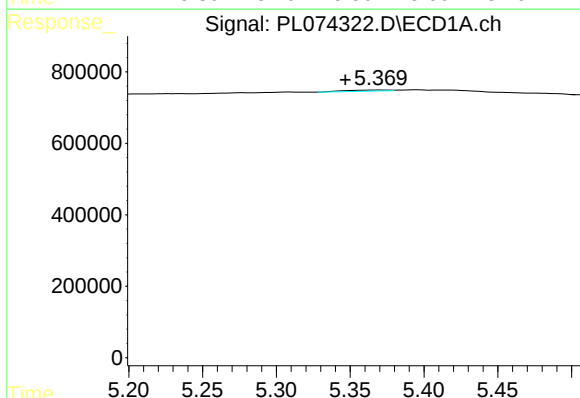


#2 alpha-BHC

R.T.: 5.370 min
Delta R.T.: 0.024 min
Response: 63593
Conc: 0.15 ng/ml

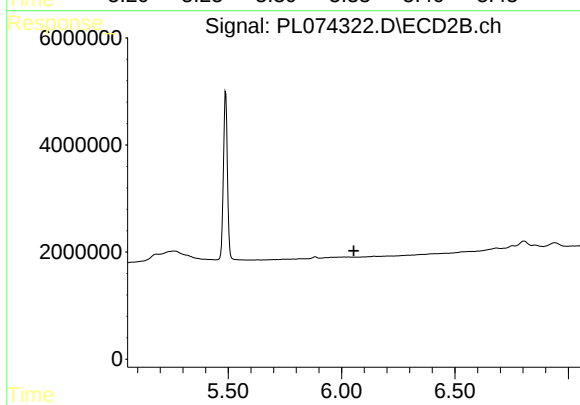

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

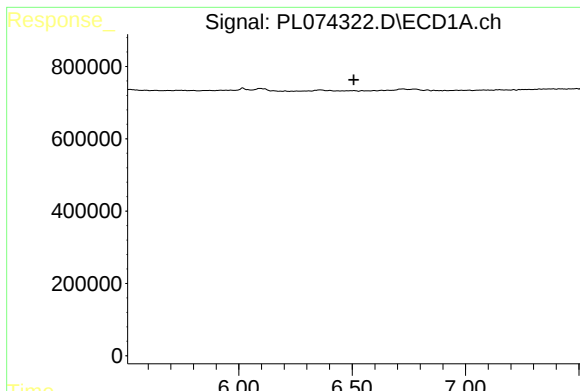

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 6.507 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

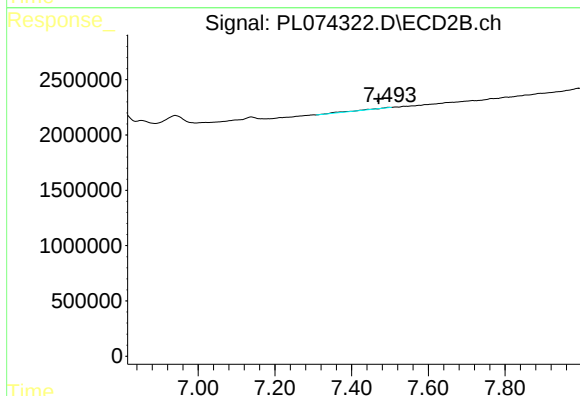


#5 Aldrin

R.T.: 7.496 min
Delta R.T.: 0.025 min
Response: 241986
Conc: 0.10 ng/ml

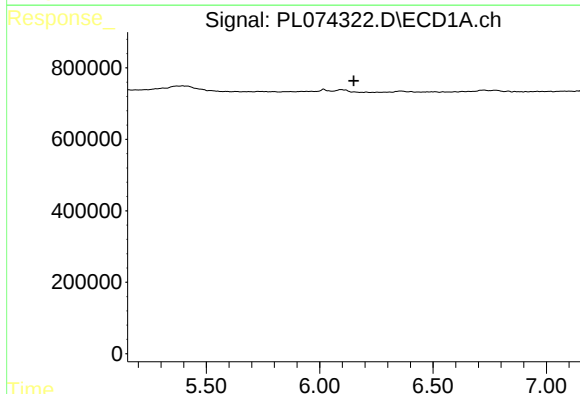


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

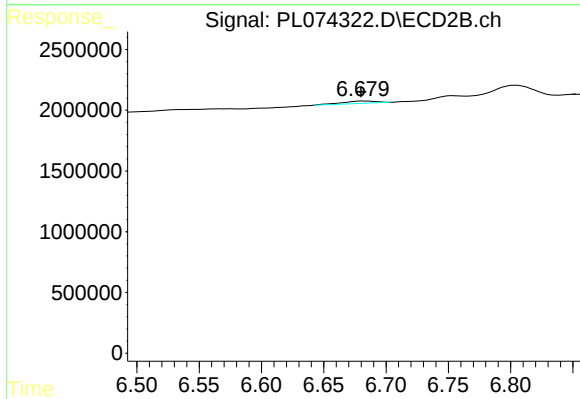

#6 beta-BHC


R.T.: 6.682 min
Delta R.T.: 0.002 min
Response: 370318
Conc: 0.33 ng/ml

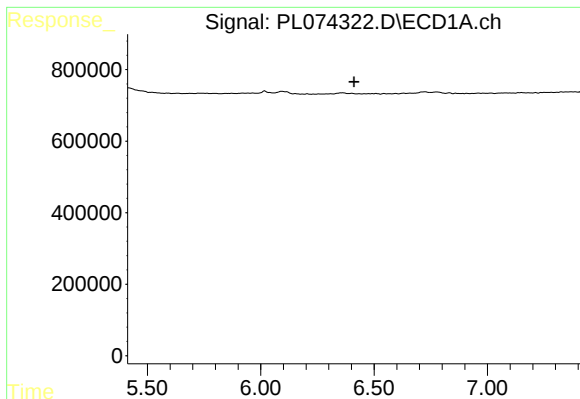

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

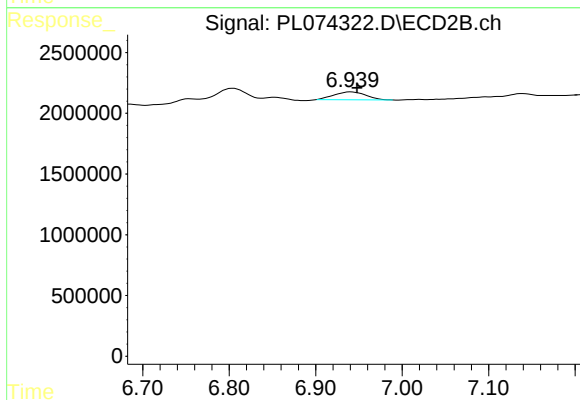


#7 delta-BHC

R.T.: 6.941 min
Delta R.T.: -0.007 min
Response: 1665426
Conc: 0.68 ng/ml

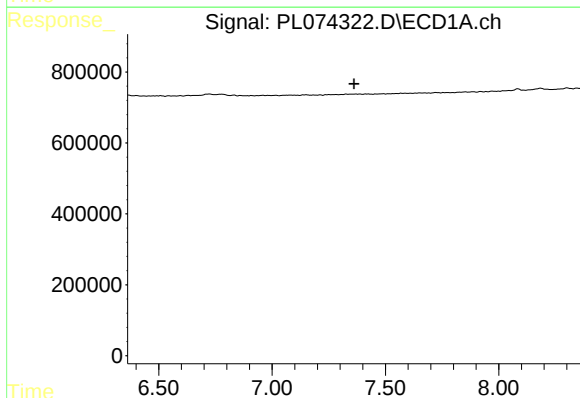


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

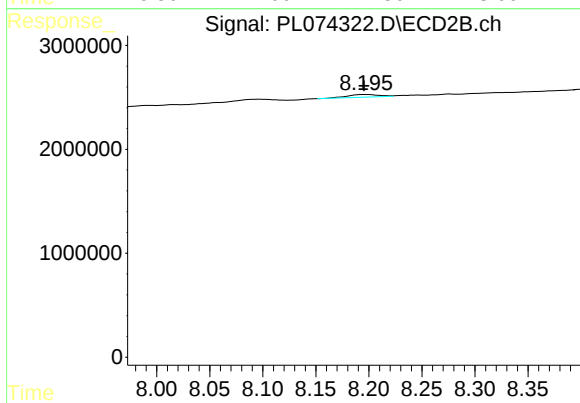

#10 gamma-Chlordane


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 536948
Conc: 0.24 ng/ml

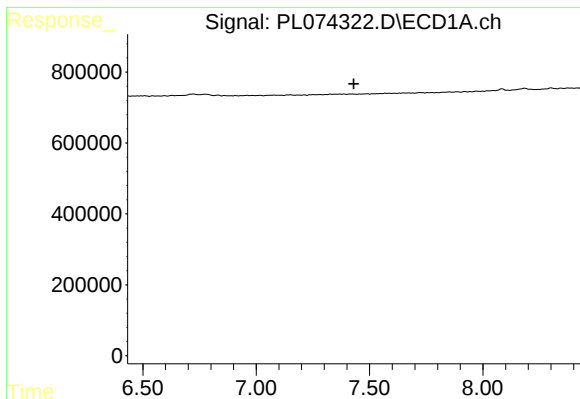

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.431 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

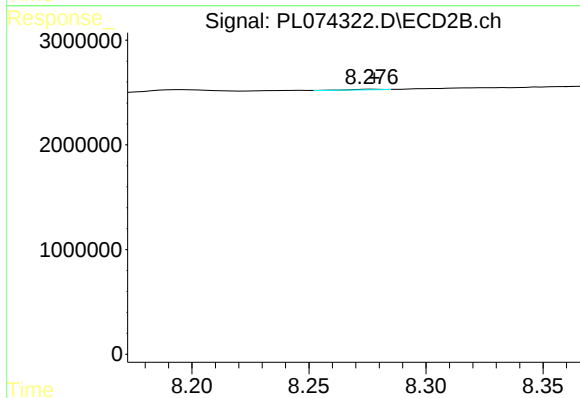


#11 alpha-Chlordane

R.T.: 8.277 min
Delta R.T.: -0.001 min
Response: 39187
Conc: 0.02 ng/ml

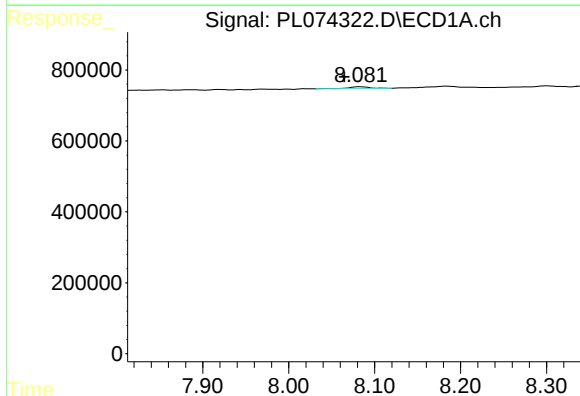


#14 Endrin

R.T.: 8.083 min
Delta R.T.: 0.018 min
Response: 74962
Conc: 0.18 ng/ml

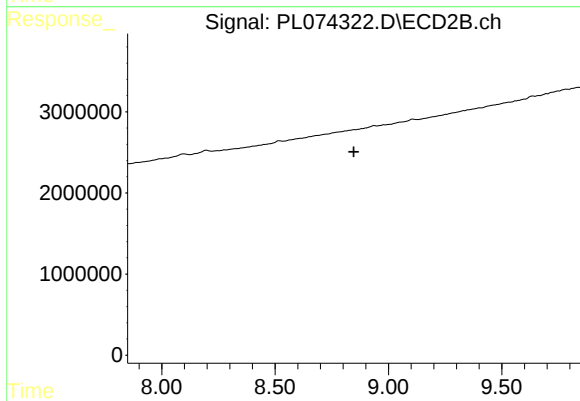

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.847 min
Response: 0
Conc: N.D.

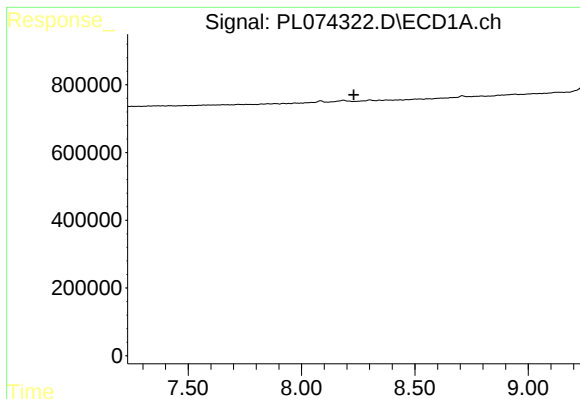

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.231 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

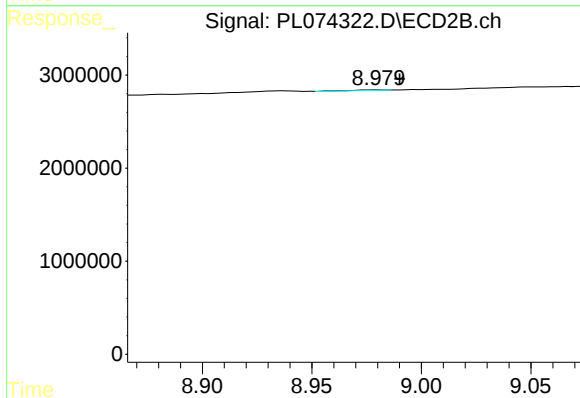


#16 4,4'-DDD

R.T.: 8.981 min
Delta R.T.: -0.009 min
Response: 58823
Conc: 0.04 ng/ml

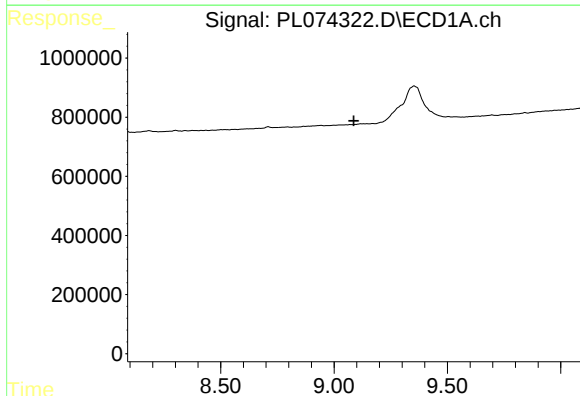


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

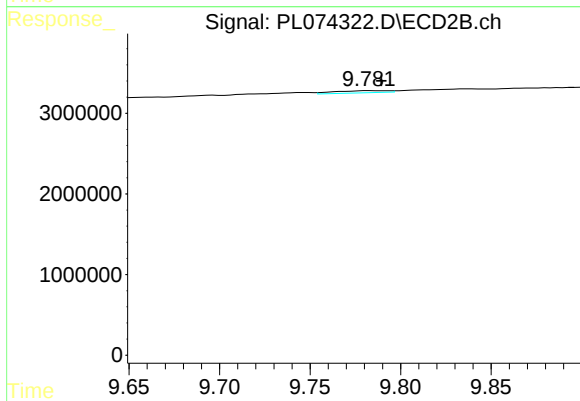

#20 Methoxychlor


R.T.: 9.783 min
Delta R.T.: -0.007 min
Response: 546057
Conc: 0.57 ng/ml

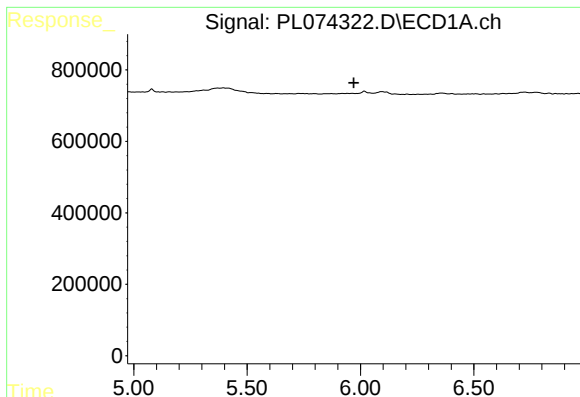

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

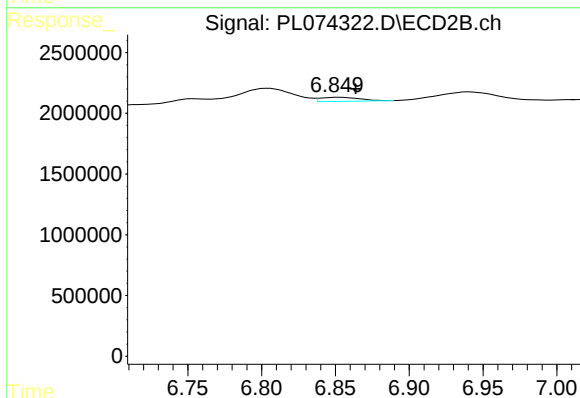


#23 Chlordane-1

R.T.: 6.852 min
Delta R.T.: -0.012 min
Response: 629899
Conc: 7.89 ng/ml

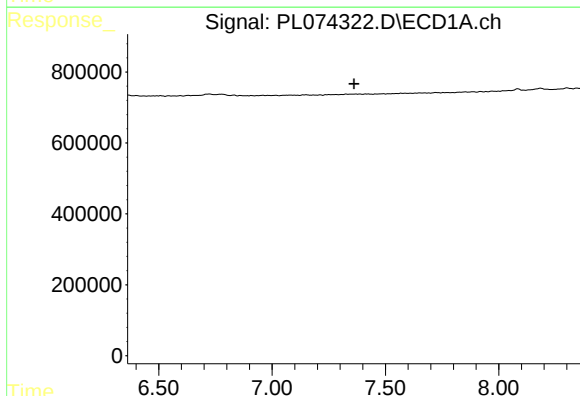


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

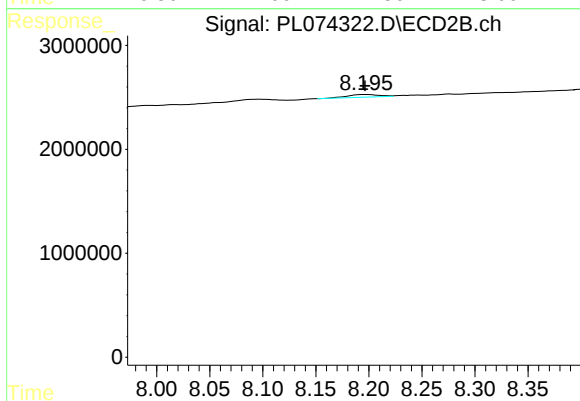

#25 Chlordane-3


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 536948
Conc: 1.59 ng/ml

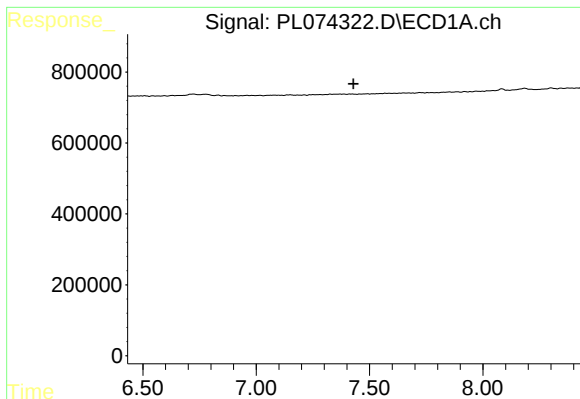

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.430 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

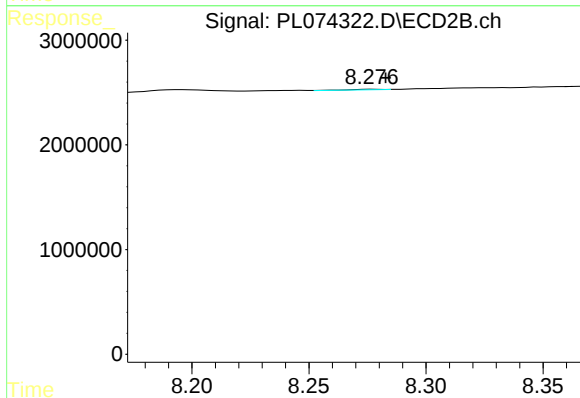


#26 Chlordane-4

R.T.: 8.277 min
Delta R.T.: -0.006 min
Response: 39187
Conc: 0.10 ng/ml

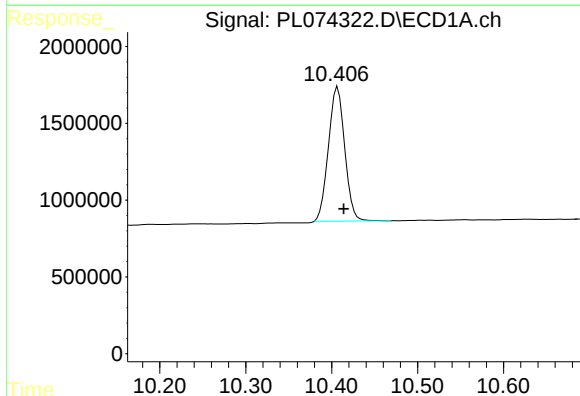

#28 Decachlorobiphenyl

R.T.: 10.407 min
Delta R.T.: -0.007 min
Response: 11501398
Conc: 22.12 ng/ml

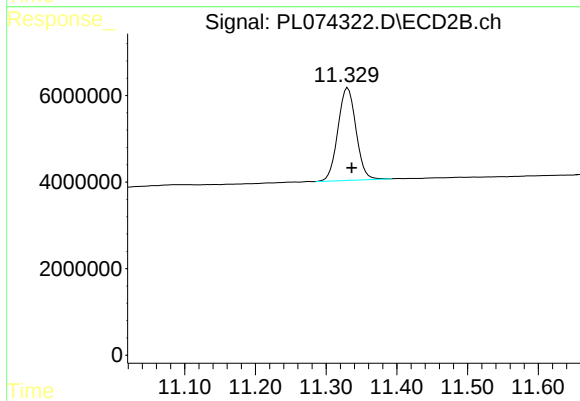

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: -0.005 min
Response: 37983196
Conc: 21.50 ng/ml