

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
 Data File : PL074344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Apr 2022 17:45
 Operator : AR\AJ
 Sample : N2448-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 02:04:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
 Quant Title : GC Extractables
 QLast Update : Thu Apr 14 09:29:23 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.635	5.489	6906619	37029629	21.375	20.769
28)	SA Decachlor...	10.404	11.331	10251893	38039328	19.714	21.536
Target Compounds							
2)	A alpha-BHC	5.355	0.000	11052	0	0.026	N.D. #
6)	B beta-BHC	0.000	6.678	0	1183569	N.D.	1.050 #
7)	B delta-BHC	0.000	6.957	0	2113472	N.D.	0.865 #
10)	B gamma-Chl...	0.000	8.195	0	651710	N.D.	0.292 #
14)	MA Endrin	0.000	8.844	0	121684	N.D.	0.072 #
17)	MA 4,4'-DDT	0.000	9.324f	0	99711	N.D.	0.056 #
20)	A Methoxychlor	0.000	9.800	0	247001	N.D.	0.257 #
21)	B Endrin ke...	0.000	9.927	0	722877	N.D.	0.418 #
23)	Chlordane-1	0.000	6.856	0	679754	N.D.	8.518 #
24)	Chlordane-2	0.000	7.426f	0	180039	N.D.	2.179 #
25)	Chlordane-3	0.000	8.195	0	651710	N.D.	1.926 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL042522\
Data File : PL074344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Apr 2022 17:45
Operator : AR\AJ
Sample : N2448-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 02:04:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL040822.M
Quant Title : GC Extractables
QLast Update : Thu Apr 14 09:29:23 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

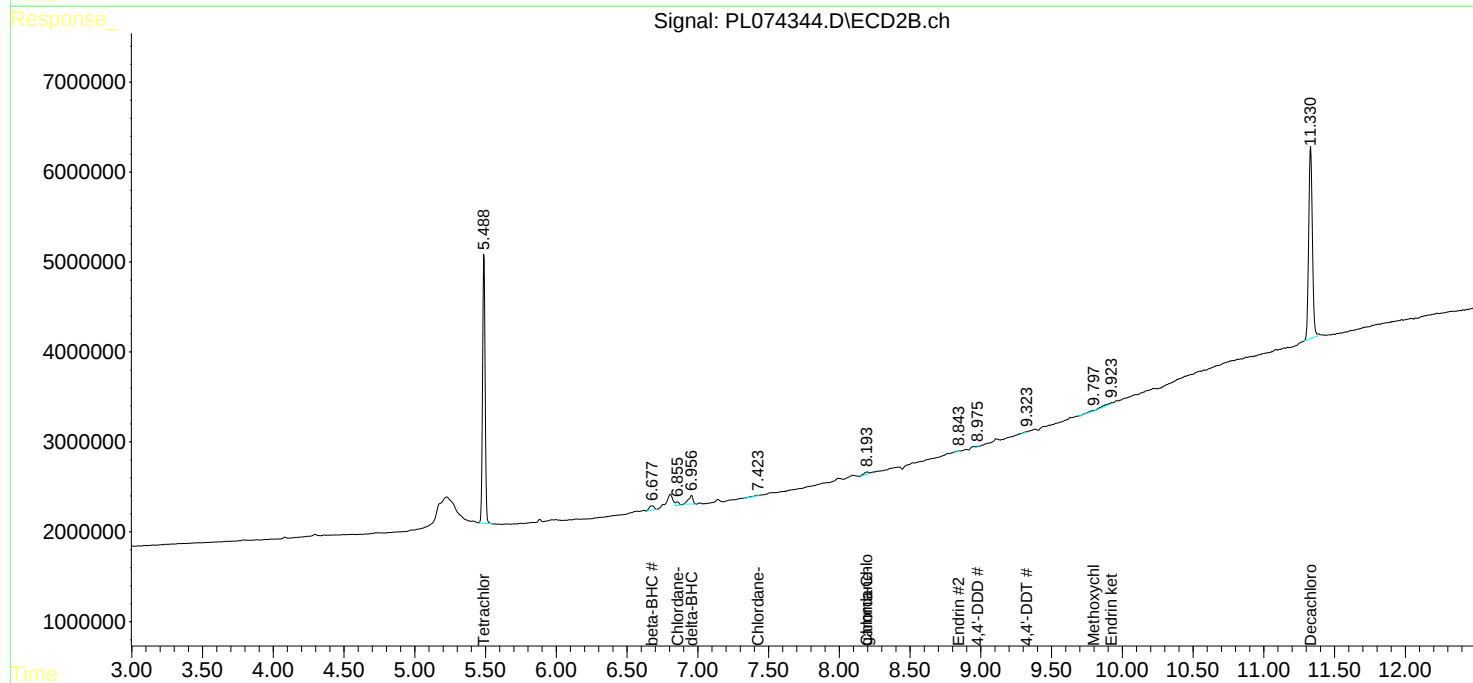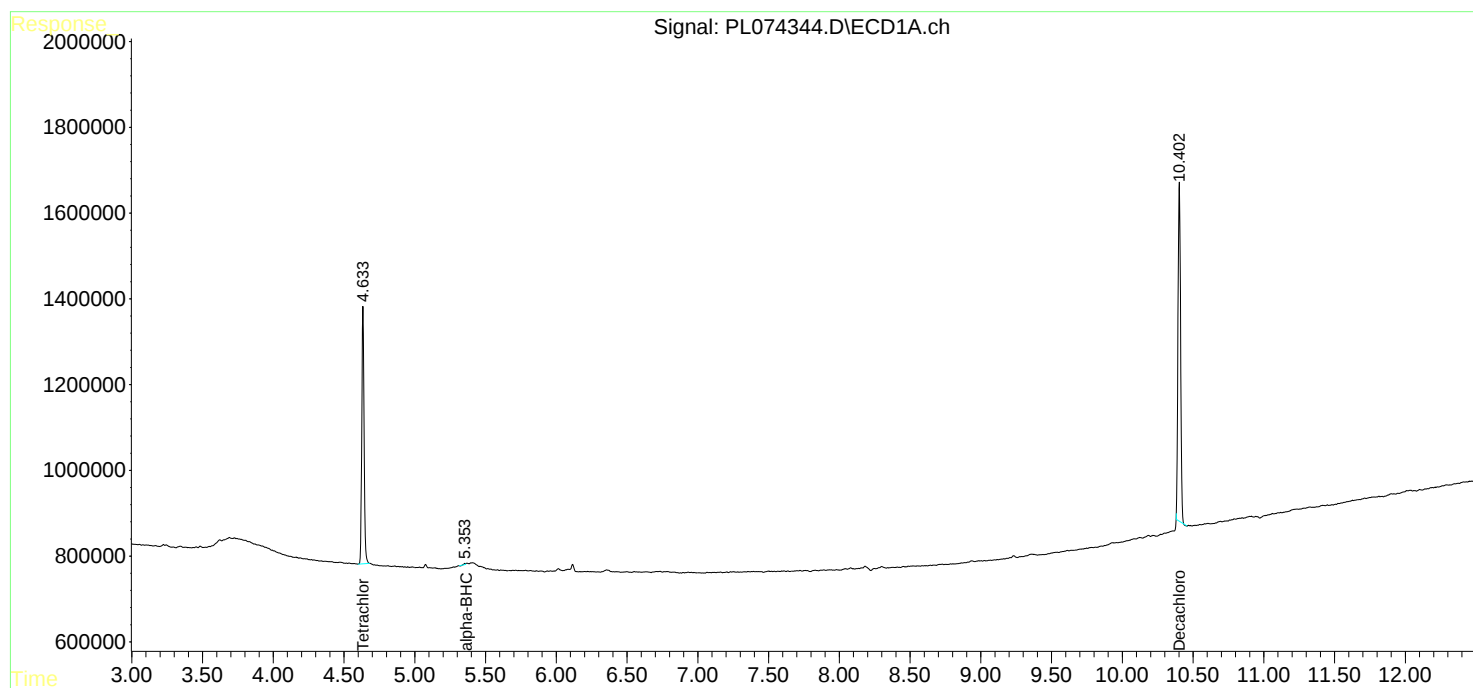


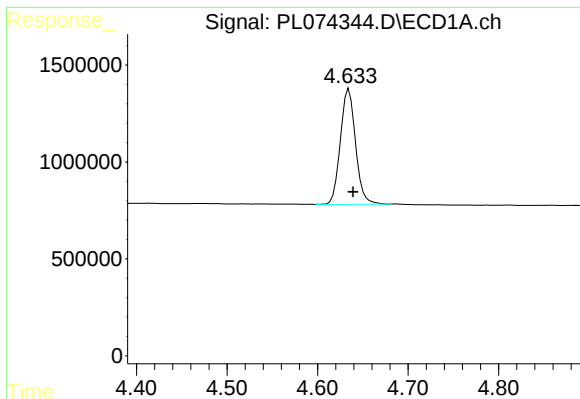

#1 Tetrachloro-m-xylene


R.T.: 4.635 min
Delta R.T.: -0.004 min
Response: 6906619
Conc: 21.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

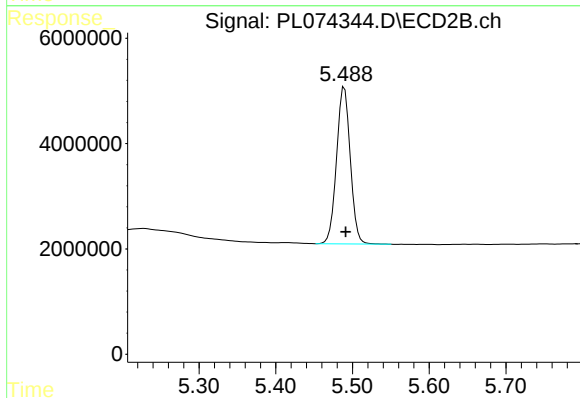


#1 Tetrachloro-m-xylene

R.T.: 5.489 min
Delta R.T.: -0.002 min
Response: 37029629
Conc: 20.77 ng/ml

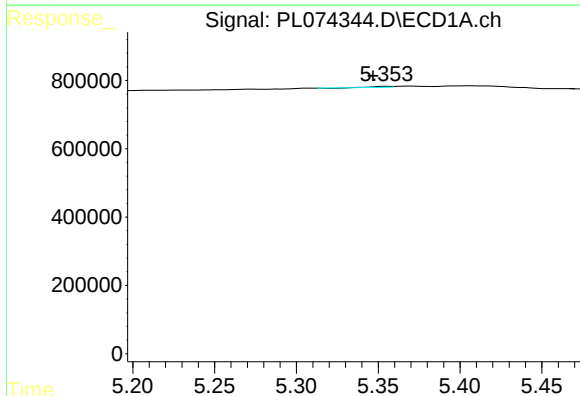


#2 alpha-BHC

R.T.: 5.355 min
Delta R.T.: 0.008 min
Response: 11052
Conc: 0.03 ng/ml

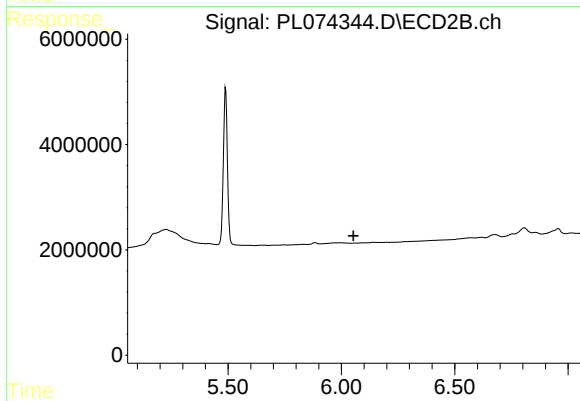

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.054 min
Response: 0
Conc: N.D.

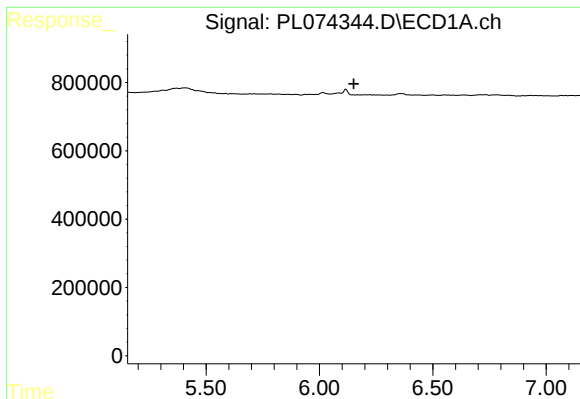

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

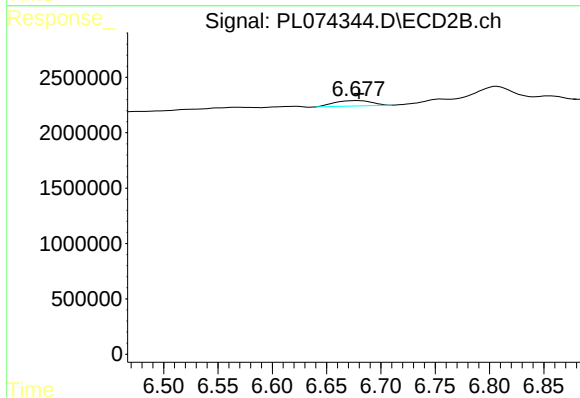


#6 beta-BHC

R.T.: 6.678 min
Delta R.T.: -0.002 min
Response: 1183569
Conc: 1.05 ng/ml

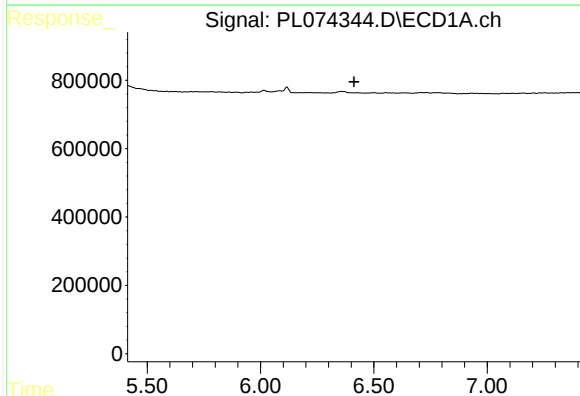


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 6.412 min
Response: 0
Conc: N.D.

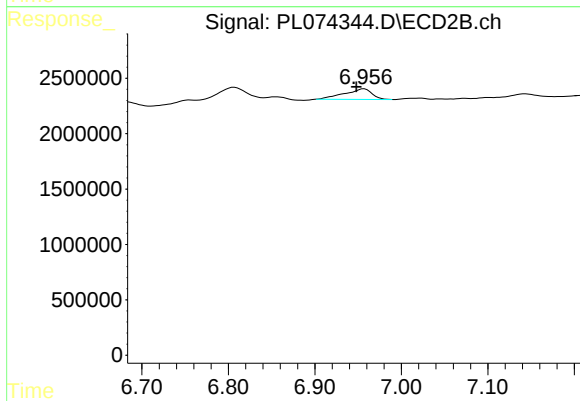

#7 delta-BHC


R.T.: 6.957 min
Delta R.T.: 0.009 min
Response: 2113472
Conc: 0.87 ng/ml

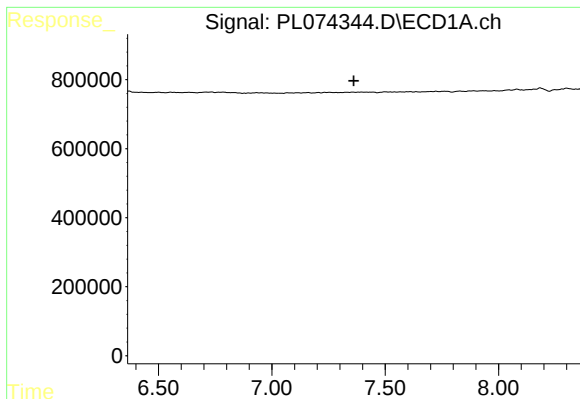

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

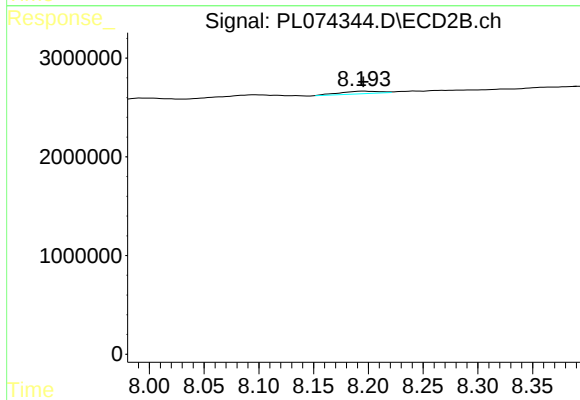


#10 gamma-Chlordane

R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 651710
Conc: 0.29 ng/ml

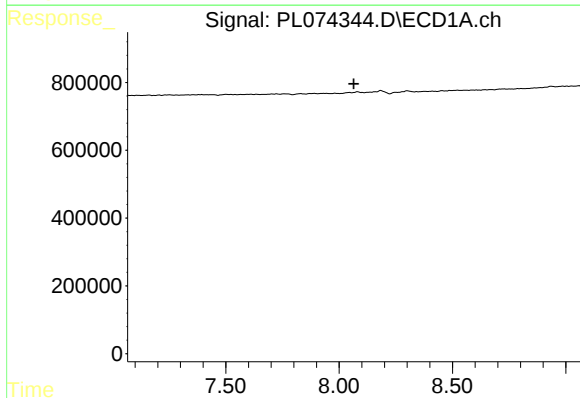


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 8.065 min
Response: 0
Conc: N.D.

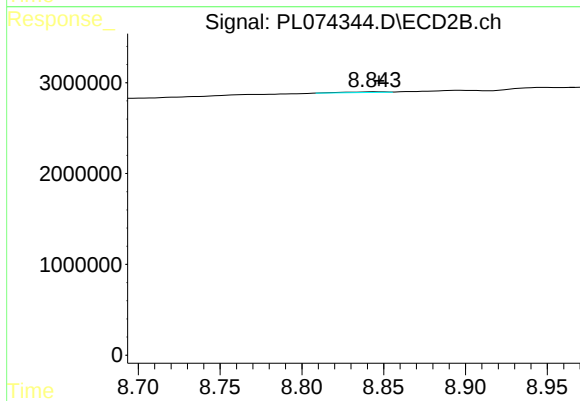

#14 Endrin


R.T.: 8.844 min
Delta R.T.: -0.003 min
Response: 121684
Conc: 0.07 ng/ml

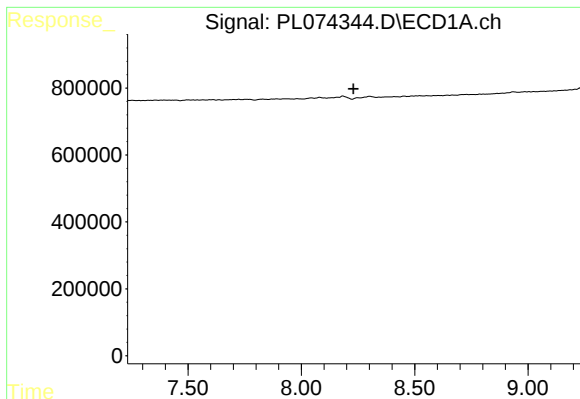

#16 4,4'-DDD


R.T.: 8.249 min
Delta R.T.: 0.019 min
Response: -46503
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

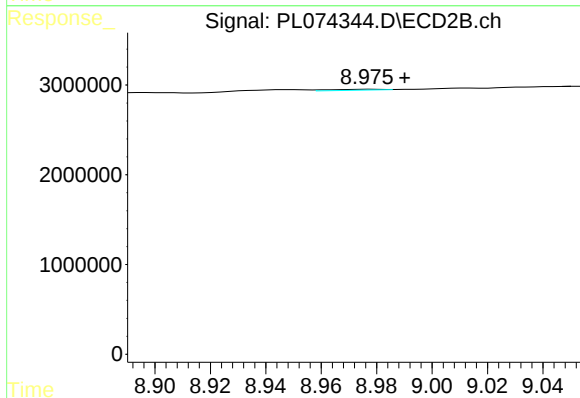


#16 4,4'-DDD

R.T.: 8.977 min
Delta R.T.: -0.013 min
Response: 147232
Conc: 0.10 ng/ml

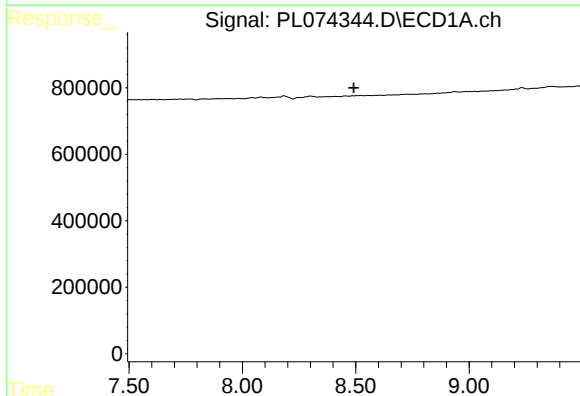


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.492 min
Response: 0
Conc: N.D.

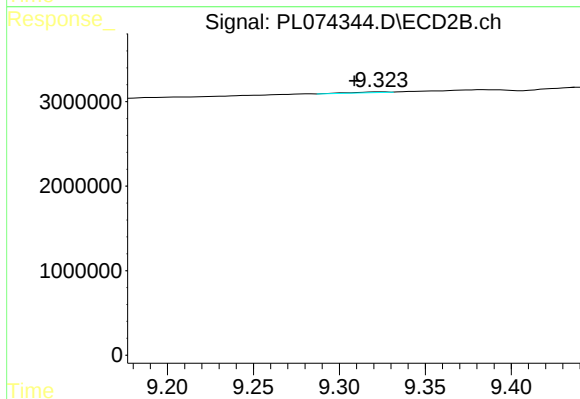

#17 4,4'-DDT


R.T.: 9.324 min
Delta R.T.: 0.016 min
Response: 99711
Conc: 0.06 ng/ml

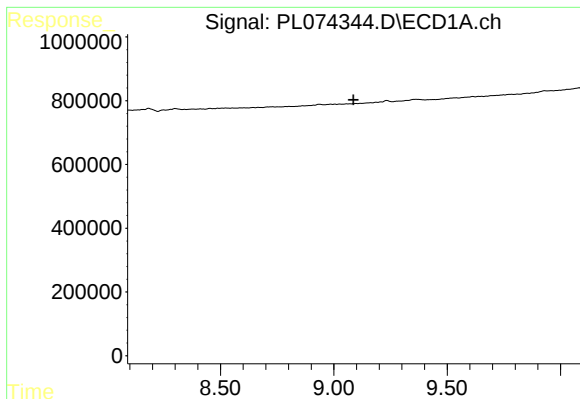

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.087 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

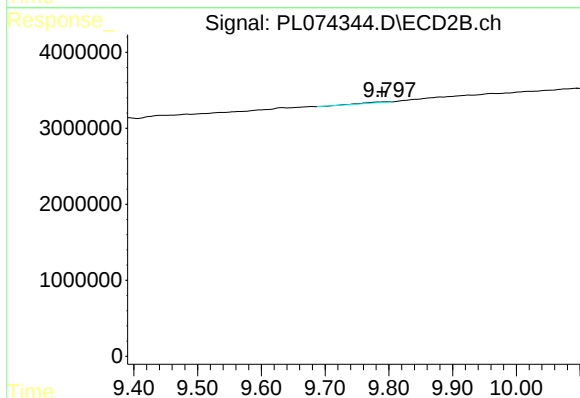


#20 Methoxychlor

R.T.: 9.800 min
Delta R.T.: 0.010 min
Response: 247001
Conc: 0.26 ng/ml

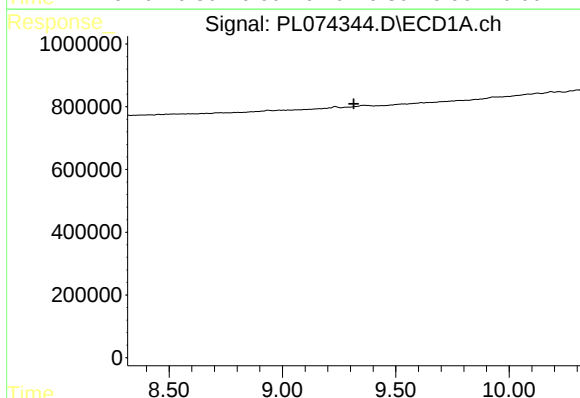


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.314 min
Response: 0
Conc: N.D.

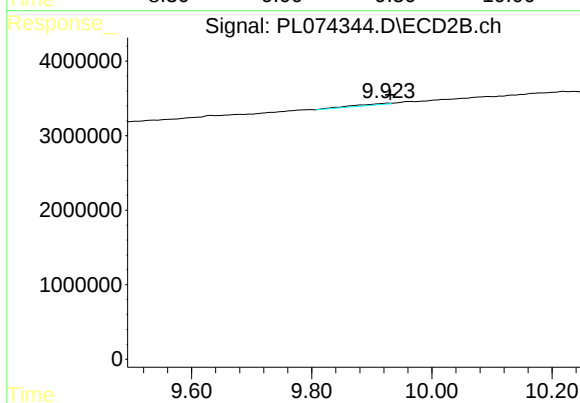

#21 Endrin ketone


R.T.: 9.927 min
Delta R.T.: -0.004 min
Response: 722877
Conc: 0.42 ng/ml

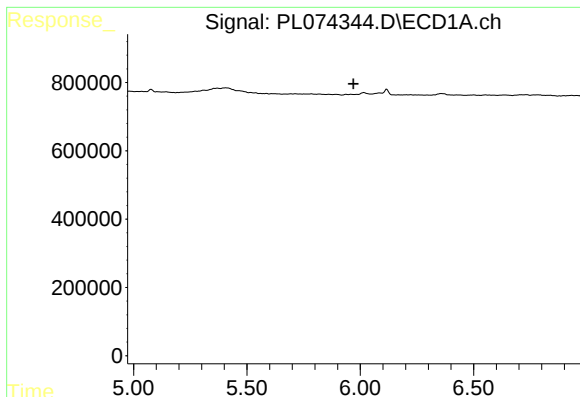

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.970 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

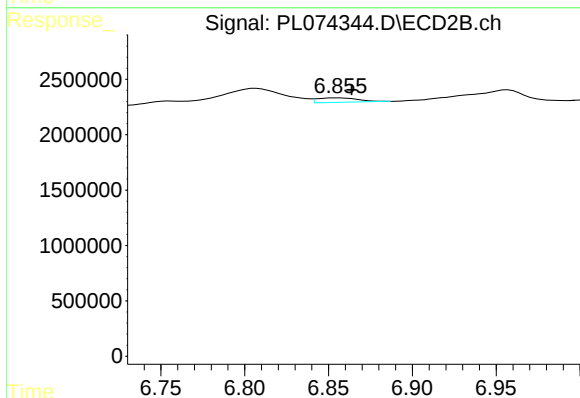


#23 Chlordane-1

R.T.: 6.856 min
Delta R.T.: -0.007 min
Response: 679754
Conc: 8.52 ng/ml

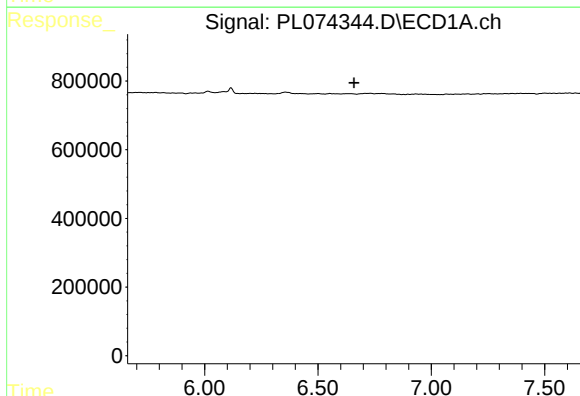


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 6.659 min
Response: 0
Conc: N.D.

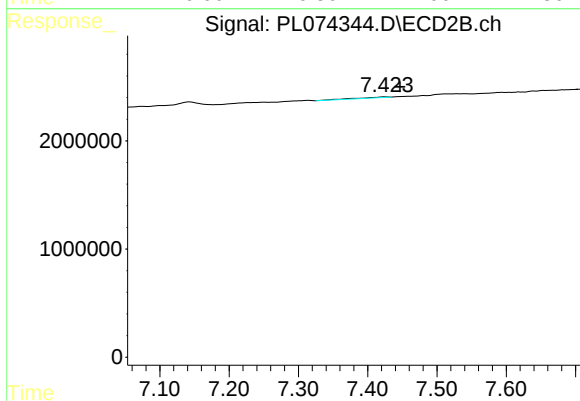

#24 Chlordane-2


R.T.: 7.426 min
Delta R.T.: -0.021 min
Response: 180039
Conc: 2.18 ng/ml

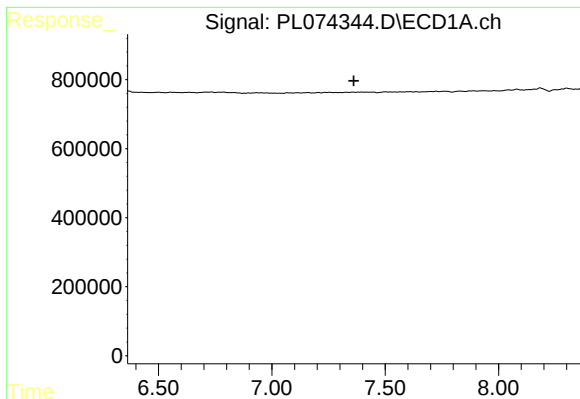

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

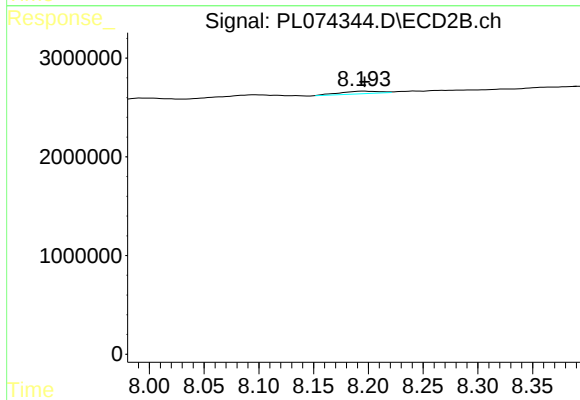


#25 Chlordane-3

R.T.: 8.195 min
Delta R.T.: -0.001 min
Response: 651710
Conc: 1.93 ng/ml

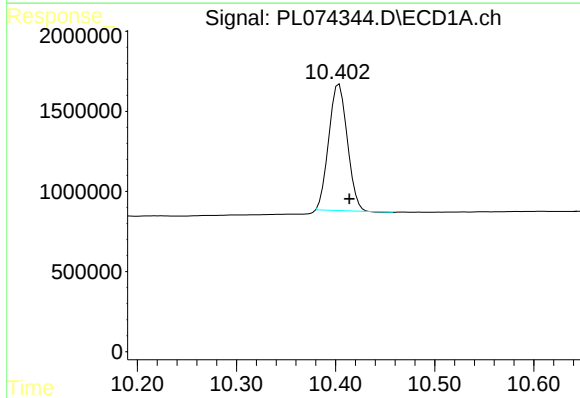

#28 Decachlorobiphenyl

R.T.: 10.404 min
Delta R.T.: -0.010 min
Response: 10251893
Conc: 19.71 ng/ml

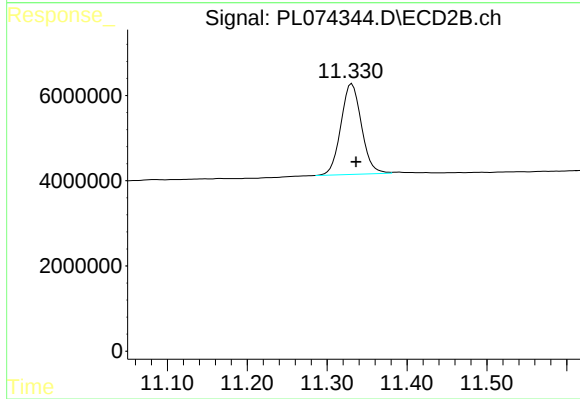

#28 Decachlorobiphenyl

R.T.: 11.331 min
Delta R.T.: -0.005 min
Response: 38039328
Conc: 21.54 ng/ml